

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
 Data File : BP014146.D
 Acq On : 20 Mar 2023 18:27
 Operator : CG/JU
 Sample : PB151508BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK508

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014146.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.417	35	39	45	rVB	45194	59083	1.07%	0.115%
2	3.852	109	113	134	rBV	410270	714908	12.89%	1.389%
3	4.181	165	169	175	rVB	10207	16019	0.29%	0.031%
4	7.158	670	675	677	rBV6	4242	7445	0.13%	0.014%
5	7.211	677	684	699	rVV	724863	1219933	22.00%	2.370%
6	7.375	705	712	722	rBV	586628	916431	16.52%	1.780%
7	7.581	738	747	763	rBV	761923	1225228	22.09%	2.380%
8	8.052	821	827	837	rBV	538996	871045	15.71%	1.692%
9	8.763	941	948	971	rBV	932447	1596502	28.79%	3.101%
10	9.228	1018	1027	1040	rBV	741104	1254670	22.62%	2.437%
11	9.952	1141	1150	1162	rBV	664867	1133123	20.43%	2.201%
12	10.493	1235	1242	1260	rBV	867177	1643550	29.63%	3.193%
13	10.875	1298	1307	1318	rBV	771000	1288652	23.23%	2.503%
14	11.016	1322	1331	1364	rBV	1068277	2000601	36.07%	3.886%
15	12.463	1572	1577	1586	rBV2	13627	25343	0.46%	0.049%
16	13.575	1760	1766	1772	rBV2	20261	35033	0.63%	0.068%
17	14.098	1847	1855	1866	rBV	1903896	2646721	47.72%	5.141%
18	14.387	1896	1904	1918	rBV	1941934	3007793	54.23%	5.843%
19	14.481	1918	1920	1926	rVB7	3583	5796	0.10%	0.011%
20	14.692	1948	1956	1966	rBV	1318907	1908630	34.41%	3.708%
21	14.898	1984	1991	2016	rBV	602503	1327850	23.94%	2.579%
22	15.687	2118	2125	2138	rBV	2755824	3935268	70.95%	7.644%
23	15.804	2139	2145	2158	rVV	1035565	1529008	27.57%	2.970%
24	15.928	2162	2166	2172	rVB2	16063	29525	0.53%	0.057%
25	16.469	2253	2258	2262	rBV7	4572	7385	0.13%	0.014%
26	17.128	2366	2370	2377	rVB10	6262	10201	0.18%	0.020%
27	17.239	2385	2389	2393	rVB6	3518	5840	0.11%	0.011%
28	17.451	2418	2425	2434	rBV	1719764	2467861	44.50%	4.794%
29	17.551	2435	2442	2452	rVV	3046080	4400355	79.34%	8.548%
30	18.092	2532	2534	2540	rVB7	6392	8232	0.15%	0.016%
31	18.316	2568	2572	2578	rBV6	30205	54486	0.98%	0.106%
32	19.351	2744	2748	2754	rBV2	46278	69451	1.25%	0.135%
33	19.416	2756	2759	2767	rVB	40091	63083	1.14%	0.123%
34	19.775	2814	2820	2830	rBV	4376327	5546179	100.00%	10.774%
35	21.527	3113	3118	3126	rBV	2179359	2984725	53.82%	5.798%
36	23.892	3512	3520	3530	rVB	2344478	4883238	88.05%	9.486%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014146.D
Acq On : 20 Mar 2023 18:27
Operator : CG/JU
Sample : PB151508BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK508

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Title : SVOA CALIBRATION

37	24.051	3541	3547	3557	rvB2	1234339	2580083	46.52%	5.012%
----	--------	------	------	------	------	---------	---------	--------	--------




Sum of corrected areas: 51479276

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014146.D
Acq On : 20 Mar 2023 18:27
Operator : CG/JU
Sample : PB151508BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK508

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

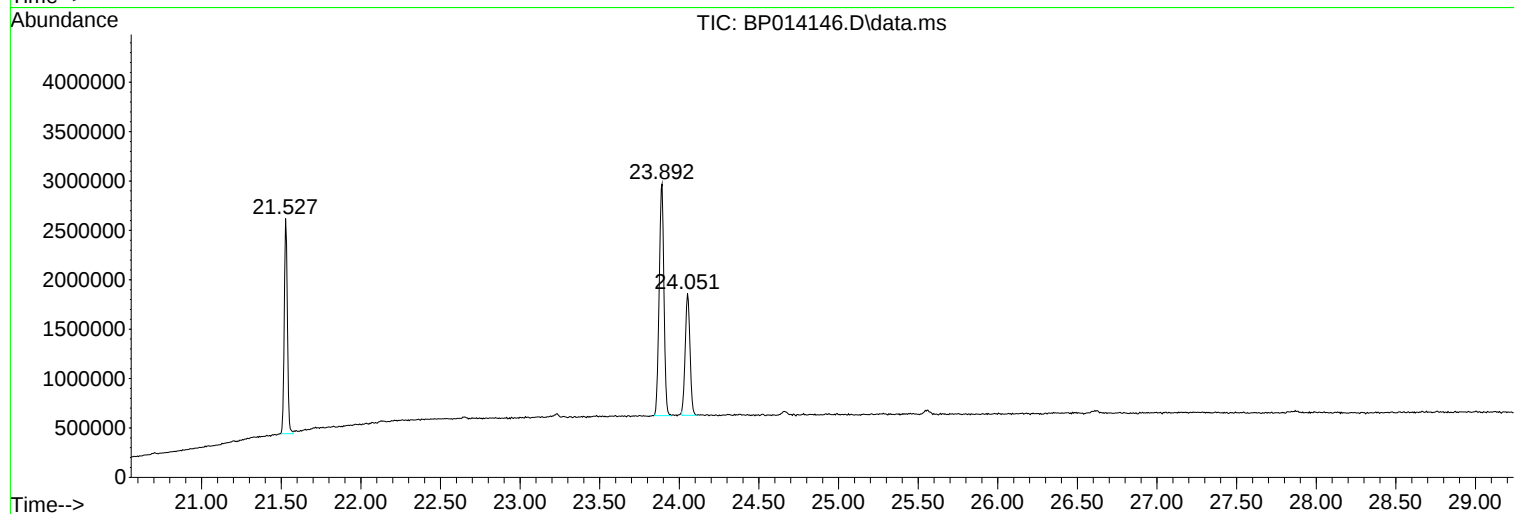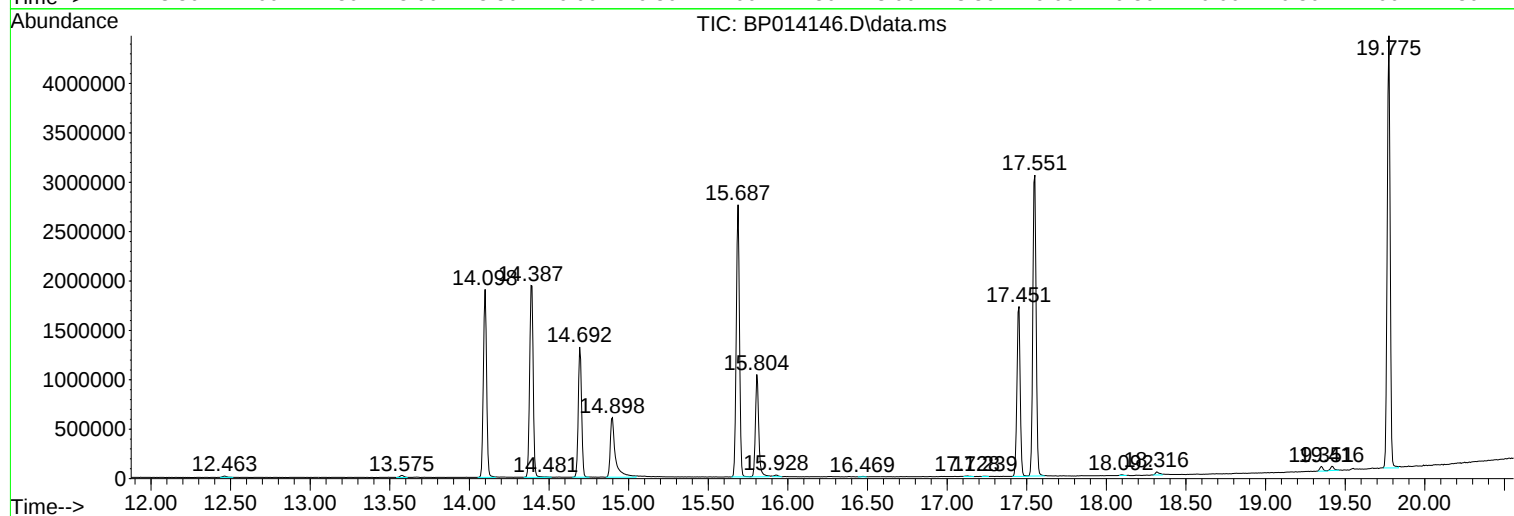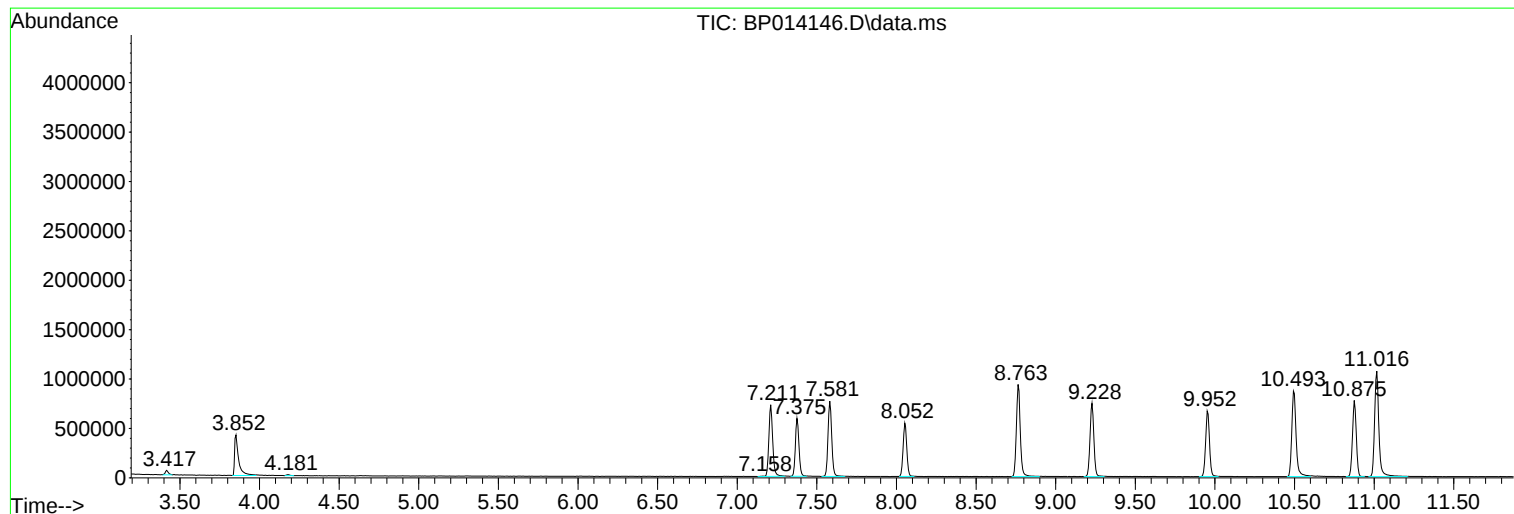

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014146.D
Acq On : 20 Mar 2023 18:27
Operator : CG/JU
Sample : PB151508BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK508

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014146.D
Acq On : 20 Mar 2023 18:27
Operator : CG/JU
Sample : PB151508BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK508

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc