

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
 Data File : BP014163.D
 Acq On : 21 Mar 2023 04:43
 Operator : CG/JU
 Sample : PB151522BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK522

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014163.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.417	35	39	46	rVB	53881	77863	1.28%	0.131%
2	3.846	110	112	131	rBV	512630	870325	14.26%	1.459%
3	4.175	164	168	175	rVB	16948	26558	0.44%	0.045%
4	7.211	677	684	701	rBV	840812	1419048	23.25%	2.379%
5	7.375	705	712	722	rBV	673359	1072670	17.58%	1.798%
6	7.575	739	746	759	rBV	848918	1420948	23.28%	2.382%
7	8.046	819	826	835	rBV	796499	1298829	21.28%	2.177%
8	8.763	941	948	966	rBV	1103426	1869285	30.63%	3.133%
9	9.222	1019	1026	1039	rBV	889383	1479958	24.25%	2.481%
10	9.952	1142	1150	1161	rBV	767858	1309412	21.45%	2.195%
11	10.493	1234	1242	1257	rBV	1031895	1931708	31.65%	3.238%
12	10.869	1298	1306	1316	rBV	1140057	1905638	31.22%	3.194%
13	11.010	1322	1330	1350	rBV	597573	1209520	19.82%	2.027%
14	12.457	1570	1576	1585	rBV2	17295	36813	0.60%	0.062%
15	13.569	1757	1765	1774	rBV	28868	48918	0.80%	0.082%
16	14.093	1847	1854	1870	rBV	2207050	3119178	51.11%	5.228%
17	14.387	1897	1904	1915	rBV	2359366	3510773	57.52%	5.885%
18	14.692	1948	1956	1964	rBV	1840114	2791787	45.74%	4.680%
19	14.892	1984	1990	2018	rBV	666548	1514659	24.82%	2.539%
20	15.681	2117	2124	2136	rBV	3120333	4500814	73.75%	7.544%
21	15.804	2139	2145	2162	rVV	1139956	1693673	27.75%	2.839%
22	15.922	2162	2165	2172	rVB3	16693	26054	0.43%	0.044%
23	17.116	2366	2368	2375	rVB6	5871	7482	0.12%	0.013%
24	17.228	2385	2387	2394	rVB7	5188	10180	0.17%	0.017%
25	17.445	2417	2424	2432	rBV	2534772	3599580	58.98%	6.034%
26	17.545	2434	2441	2454	rVV	3595552	5142087	84.25%	8.619%
27	18.322	2569	2573	2576	rBV5	10033	17738	0.29%	0.030%
28	19.345	2743	2747	2751	rBV2	52220	67895	1.11%	0.114%
29	19.416	2755	2759	2763	rVV	45581	61522	1.01%	0.103%
30	19.769	2813	2819	2826	rBV	4640497	6103145	100.00%	10.230%
31	21.522	3112	3117	3126	rBV	2625526	3771862	61.80%	6.323%
32	23.880	3511	3518	3527	rVB2	2316729	4684785	76.76%	7.853%
33	24.045	3539	3546	3556	rVB2	1484303	3056550	50.08%	5.124%




Sum of corrected areas: 59657257

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014163.D
Acq On : 21 Mar 2023 04:43
Operator : CG/JU
Sample : PB151522BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK522

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

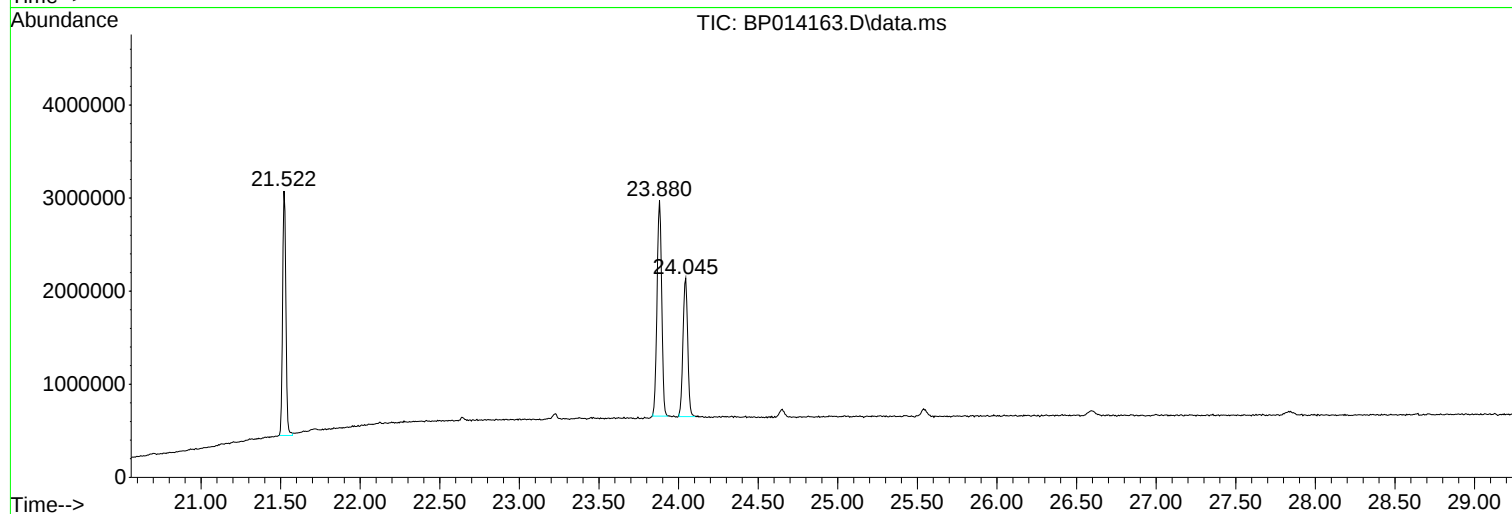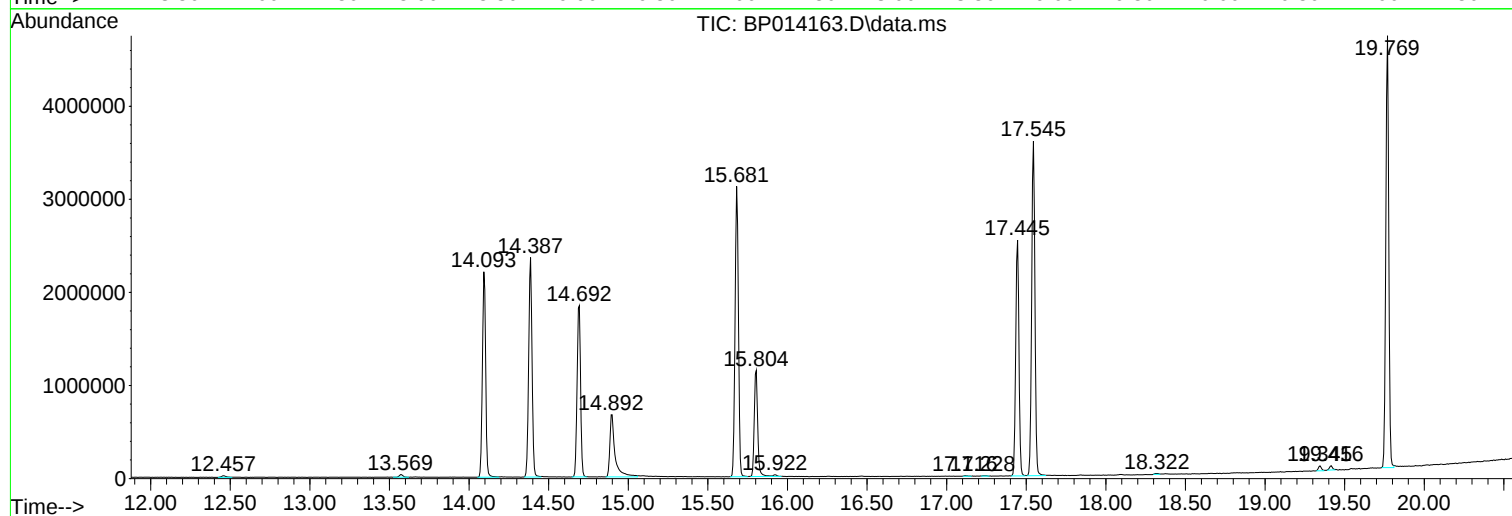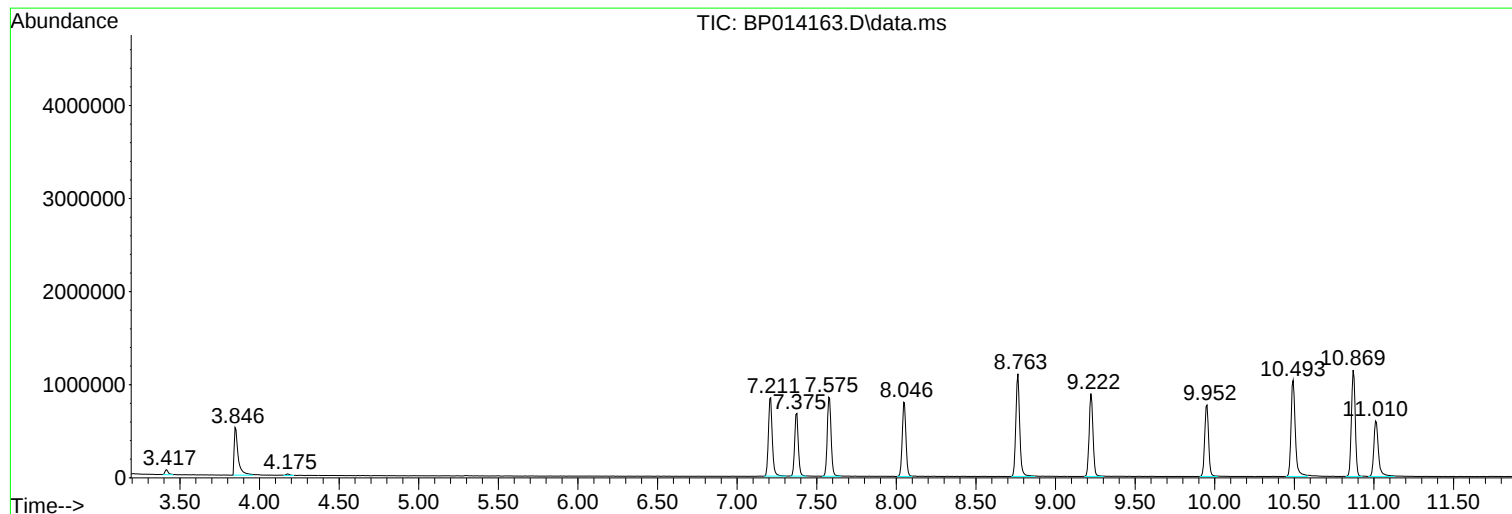

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014163.D
Acq On : 21 Mar 2023 04:43
Operator : CG/JU
Sample : PB151522BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK522

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014163.D
Acq On : 21 Mar 2023 04:43
Operator : CG/JU
Sample : PB151522BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK522

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc