

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
 Data File : BP014164.D
 Acq On : 21 Mar 2023 05:17
 Operator : CG/JU
 Sample : PB151524BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK524

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014164.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.417	35	39	49	rVB	53299	76137	1.25%	0.129%
2	3.852	110	113	133	rBV	492688	866671	14.19%	1.472%
3	4.175	164	168	174	rVB	14506	21695	0.36%	0.037%
4	4.640	243	247	254	rVB8	2706	6149	0.10%	0.010%
5	7.211	677	684	699	rBV	837276	1441568	23.60%	2.448%
6	7.375	705	712	725	rBV	681333	1088300	17.82%	1.848%
7	7.575	739	746	761	rBV	877452	1434239	23.48%	2.436%
8	8.046	819	826	838	rBV	719427	1191099	19.50%	2.023%
9	8.763	941	948	965	rBV	1094859	1851969	30.32%	3.145%
10	9.222	1018	1026	1039	rBV	888730	1477791	24.19%	2.510%
11	9.952	1141	1150	1161	rBV	756168	1322573	21.65%	2.246%
12	10.493	1235	1242	1268	rBV	1035686	1913289	31.32%	3.249%
13	10.869	1298	1306	1315	rBV	1040455	1751772	28.68%	2.975%
14	11.010	1321	1330	1348	rBV	716696	1405438	23.01%	2.387%
15	12.457	1569	1576	1588	rBV5	16711	40105	0.66%	0.068%
16	13.575	1759	1766	1775	rVB	22873	36178	0.59%	0.061%
17	14.093	1847	1854	1870	rBV	2336182	3179634	52.05%	5.400%
18	14.387	1897	1904	1916	rBV	2422490	3598620	58.91%	6.112%
19	14.687	1948	1955	1966	rBV	1740510	2627363	43.01%	4.462%
20	14.892	1984	1990	2018	rBV	724295	1594156	26.10%	2.707%
21	15.681	2116	2124	2135	rBV	3198926	4595176	75.23%	7.804%
22	15.798	2138	2144	2161	rVV	1179312	1764366	28.88%	2.996%
23	15.922	2161	2165	2170	rVB3	15872	25369	0.42%	0.043%
24	16.251	2216	2221	2226	rBV8	3538	7014	0.11%	0.012%
25	17.122	2362	2369	2375	rBV8	5493	12607	0.21%	0.021%
26	17.234	2383	2388	2392	rBV6	6064	10124	0.17%	0.017%
27	17.445	2417	2424	2434	rBV	2337953	3362718	55.05%	5.711%
28	17.545	2434	2441	2455	rVV	3637751	5226805	85.57%	8.877%
29	18.310	2568	2571	2580	rBV	14752	35620	0.58%	0.060%
30	19.345	2743	2747	2751	rBV4	51816	65896	1.08%	0.112%
31	19.410	2755	2758	2763	rBV	41356	60707	0.99%	0.103%
32	19.769	2813	2819	2831	rBV	4817010	6108267	100.00%	10.374%
33	21.522	3112	3117	3125	rBV	2556626	3386077	55.43%	5.751%
34	23.880	3511	3518	3528	rVB2	2185707	4505300	73.76%	7.651%
35	24.039	3539	3545	3558	rVB2	1287165	2791760	45.70%	4.741%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014164.D
Acq On : 21 Mar 2023 05:17
Operator : CG/JU
Sample : PB151524BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK524

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Title : SVOA CALIBRATION




Sum of corrected areas: 58882552

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014164.D
Acq On : 21 Mar 2023 05:17
Operator : CG/JU
Sample : PB151524BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK524

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

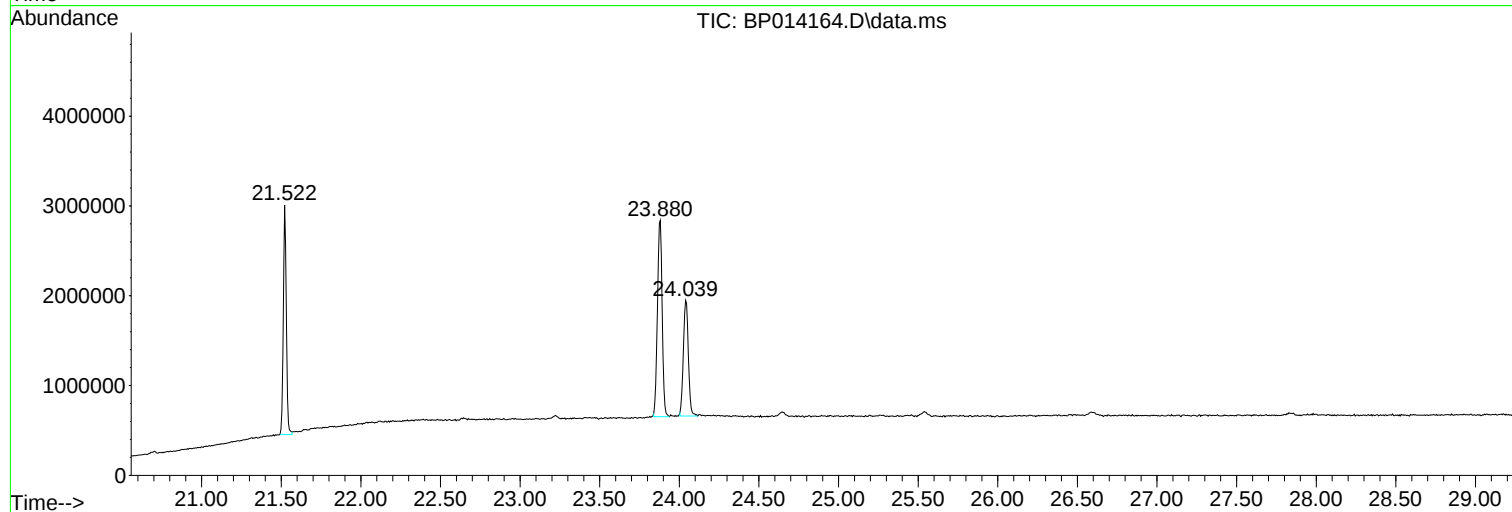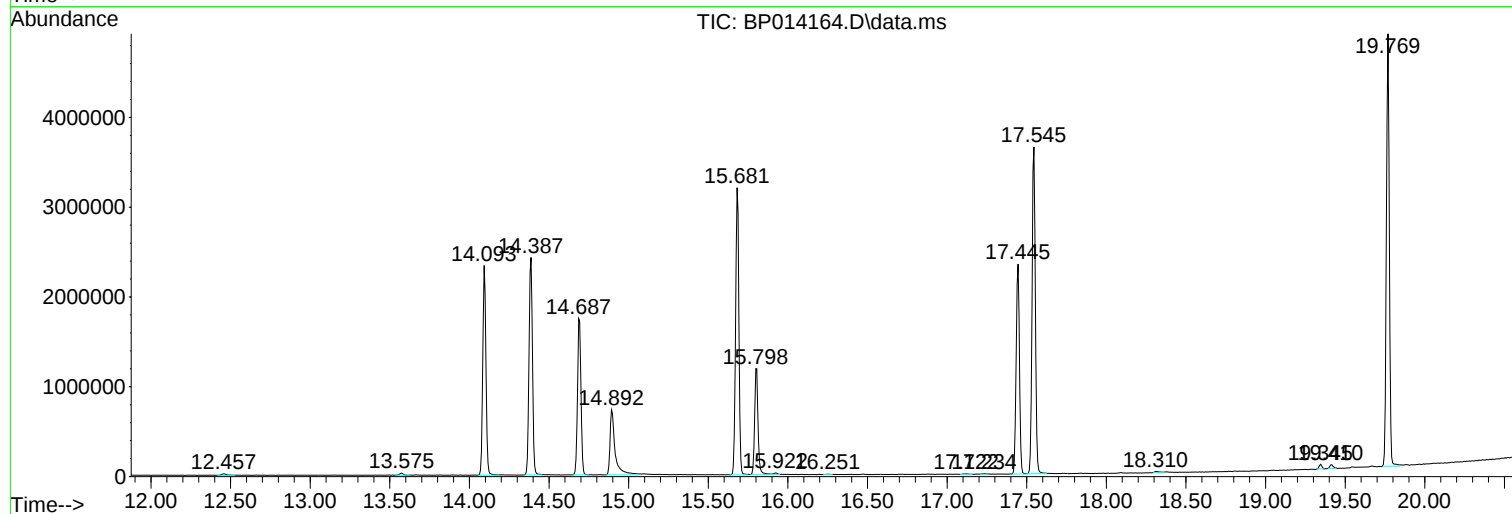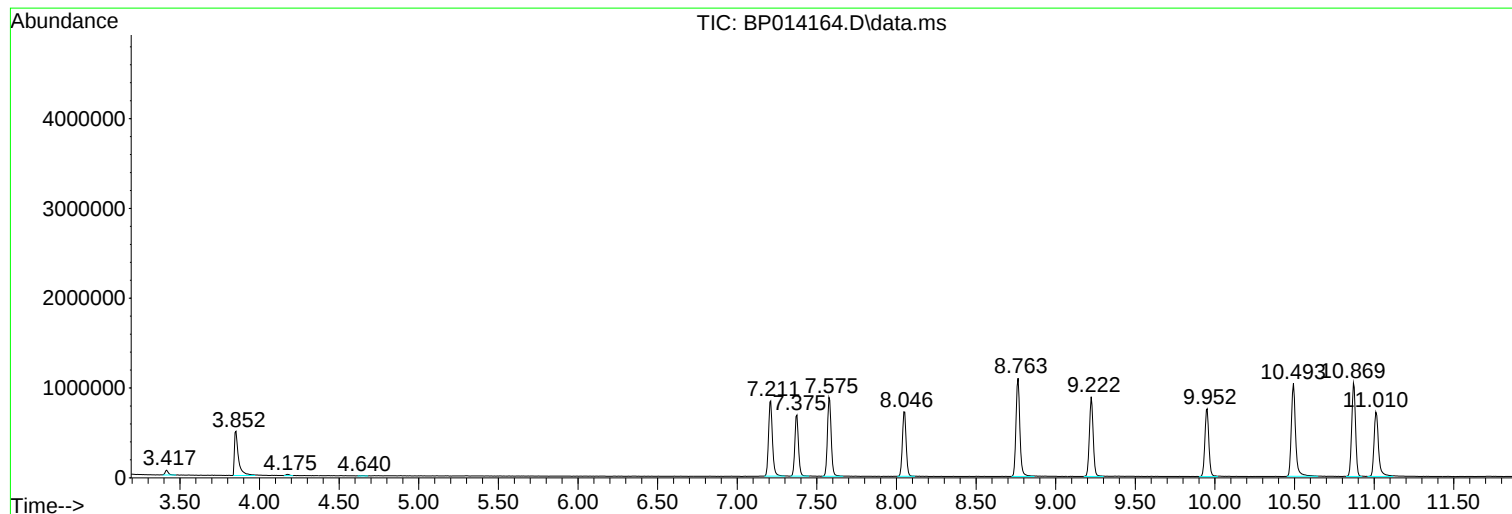

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014164.D
Acq On : 21 Mar 2023 05:17
Operator : CG/JU
Sample : PB151524BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK524

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014164.D
Acq On : 21 Mar 2023 05:17
Operator : CG/JU
Sample : PB151524BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK524

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------