

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
 Data File : BP014181.D
 Acq On : 21 Mar 2023 14:58
 Operator : CG/JU
 Sample : PB151552BL
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK552

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014181.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.411	34	38	46	rBV	53651	71727	1.18%	0.120%
2	3.846	108	112	138	rBV	674345	1128096	18.57%	1.893%
3	4.175	164	168	173	rBV	14475	20618	0.34%	0.035%
4	7.205	676	683	699	rBV	872848	1491364	24.55%	2.502%
5	7.369	704	711	723	rVV	705950	1121347	18.46%	1.881%
6	7.575	739	746	760	rBV	890788	1462509	24.07%	2.454%
7	8.046	820	826	839	rBV	745651	1201797	19.78%	2.016%
8	8.763	939	948	968	rBV	1102545	1921393	31.63%	3.224%
9	9.222	1019	1026	1042	rBV	924474	1525939	25.12%	2.560%
10	9.946	1141	1149	1161	rBV	791945	1358524	22.36%	2.279%
11	10.493	1234	1242	1261	rBV	1067647	1992238	32.79%	3.343%
12	10.869	1297	1306	1319	rBV	1063371	1775464	29.22%	2.979%
13	11.010	1322	1330	1354	rBV	1091915	2081374	34.26%	3.492%
14	12.457	1568	1576	1584	rBV4	15578	35810	0.59%	0.060%
15	13.569	1760	1765	1771	rBV7	6713	11276	0.19%	0.019%
16	13.663	1778	1781	1787	rBV7	4343	7403	0.12%	0.012%
17	14.092	1847	1854	1866	rBV	2312525	3177092	52.30%	5.331%
18	14.381	1896	1903	1919	rBV	2433141	3641071	59.93%	6.109%
19	14.686	1947	1955	1967	rBV	1751581	2615144	43.05%	4.388%
20	14.892	1983	1990	2014	rBV	679905	1491771	24.55%	2.503%
21	15.681	2117	2124	2136	rBV	3234338	4615001	75.96%	7.743%
22	15.798	2138	2144	2160	rVV	1176241	1705322	28.07%	2.861%
23	15.922	2161	2165	2170	rVB4	15934	26854	0.44%	0.045%
24	16.263	2219	2223	2225	rBV5	4147	6123	0.10%	0.010%
25	17.116	2365	2368	2374	rVB7	5330	9053	0.15%	0.015%
26	17.233	2385	2388	2395	rVB5	7517	13506	0.22%	0.023%
27	17.445	2417	2424	2434	rBV	2246730	3325398	54.74%	5.580%
28	17.545	2434	2441	2455	rVV	3512163	5225256	86.01%	8.767%
29	18.316	2569	2572	2580	rVB10	6685	14517	0.24%	0.024%
30	19.345	2743	2747	2754	rVB3	49113	59603	0.98%	0.100%
31	19.410	2755	2758	2763	rVB	42343	57976	0.95%	0.097%
32	19.769	2812	2819	2830	rBV	4421496	6075290	100.00%	10.194%
33	21.521	3112	3117	3127	rBV	2436472	3265346	53.75%	5.479%
34	23.874	3510	3517	3530	rVB2	2144880	4411260	72.61%	7.402%
35	24.039	3538	3545	3555	rVB2	1287822	2656278	43.72%	4.457%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014181.D
Acq On : 21 Mar 2023 14:58
Operator : CG/JU
Sample : PB151552BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK552

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Title : SVOA CALIBRATION




Sum of corrected areas: 59598740

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014181.D
Acq On : 21 Mar 2023 14:58
Operator : CG/JU
Sample : PB151552BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK552

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

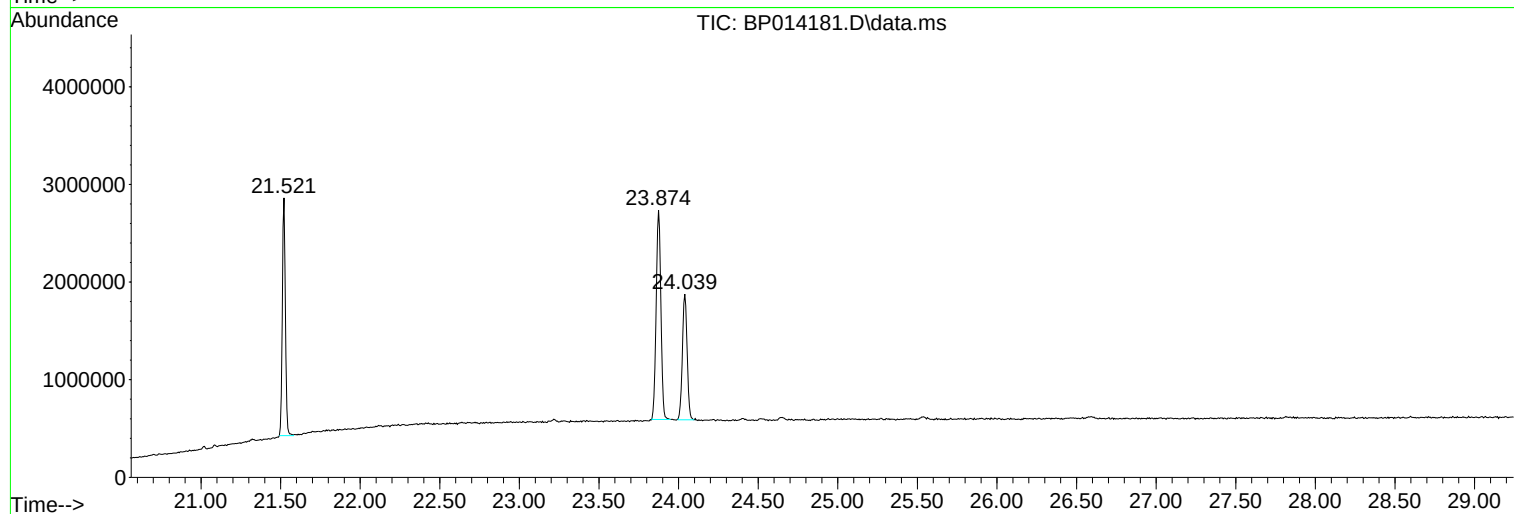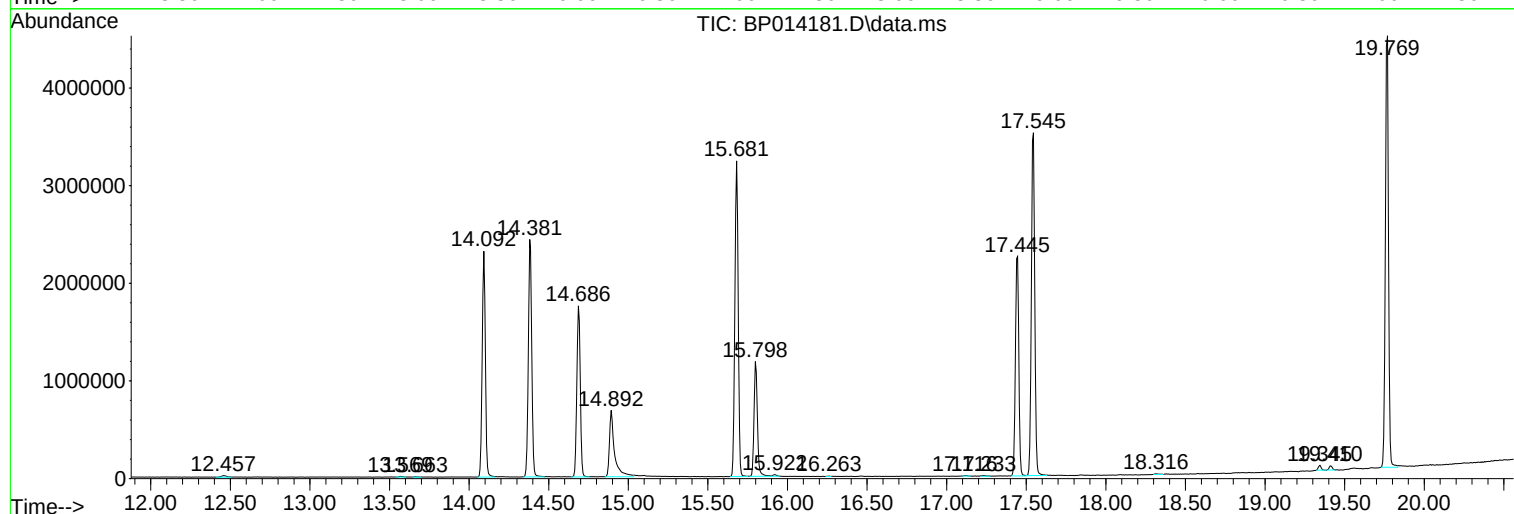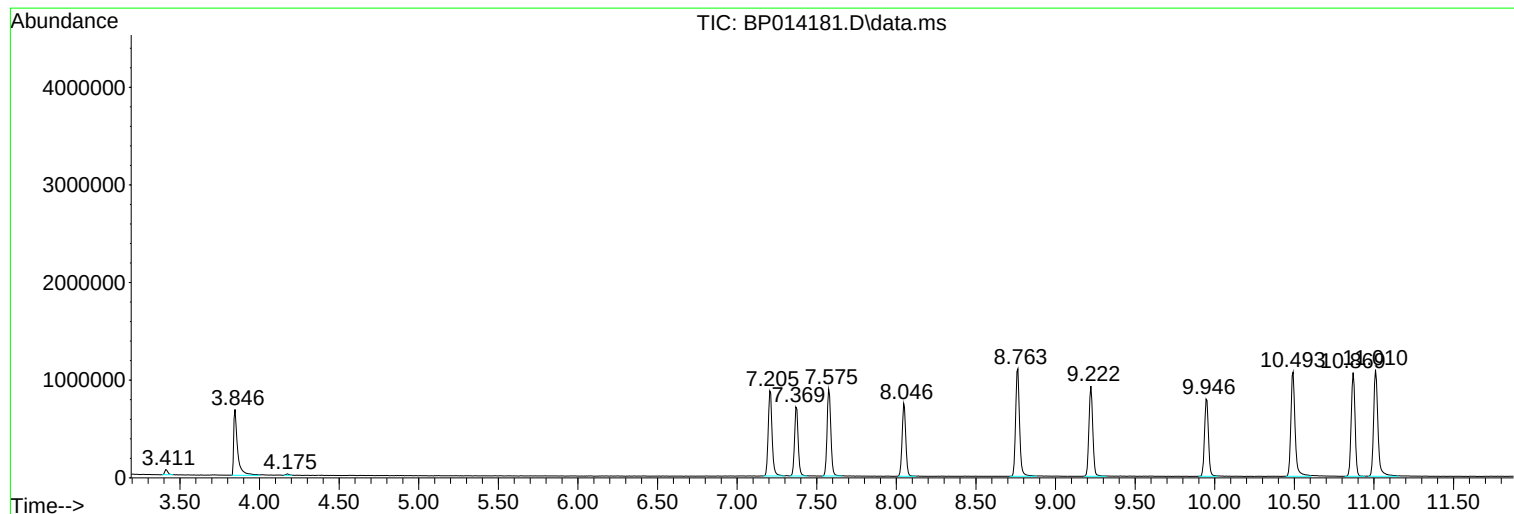

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014181.D
Acq On : 21 Mar 2023 14:58
Operator : CG/JU
Sample : PB151552BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK552

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014181.D
Acq On : 21 Mar 2023 14:58
Operator : CG/JU
Sample : PB151552BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK552

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc