

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
 Data File : BP014182.D
 Acq On : 21 Mar 2023 15:33
 Operator : CG/JU
 Sample : PB151554BL
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK554

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014182.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.411	34	38	46	rVB	51661	75360	1.28%	0.139%
2	3.846	109	112	133	rBV	660465	1057226	18.00%	1.947%
3	4.175	164	168	172	rVB2	10252	14012	0.24%	0.026%
4	7.205	677	683	697	rBV	846768	1427208	24.30%	2.628%
5	7.369	704	711	724	rVB	679517	1075857	18.32%	1.981%
6	7.575	739	746	761	rBV	879342	1404227	23.91%	2.585%
7	8.046	818	826	838	rBV	563794	916945	15.61%	1.688%
8	8.763	938	948	963	rBV	1044830	1840995	31.34%	3.390%
9	9.222	1017	1026	1038	rBV	876466	1460872	24.87%	2.690%
10	9.946	1142	1149	1165	rBV	754093	1307323	22.26%	2.407%
11	10.493	1233	1242	1262	rBV	1006432	1923668	32.75%	3.542%
12	10.869	1297	1306	1319	rBV	827436	1363001	23.20%	2.510%
13	11.010	1322	1330	1351	rBV	1031101	1986936	33.83%	3.658%
14	12.457	1570	1576	1587	rBV3	13996	34147	0.58%	0.063%
15	13.569	1761	1765	1772	rVB2	19200	31206	0.53%	0.057%
16	14.093	1847	1854	1868	rBV	2276986	3089528	52.60%	5.688%
17	14.381	1896	1903	1915	rBV	2337985	3521841	59.96%	6.484%
18	14.687	1947	1955	1966	rBV	1389829	1989723	33.87%	3.663%
19	14.892	1984	1990	2021	rBV	644215	1461294	24.88%	2.691%
20	15.681	2117	2124	2137	rBV	3154517	4477378	76.23%	8.244%
21	15.798	2138	2144	2159	rVV	1099668	1618255	27.55%	2.980%
22	15.922	2162	2165	2171	rVB4	15944	23978	0.41%	0.044%
23	16.251	2218	2221	2227	rBV8	4154	6316	0.11%	0.012%
24	17.228	2385	2387	2393	rVB5	4524	6117	0.10%	0.011%
25	17.439	2417	2423	2433	rBV	1740475	2505073	42.65%	4.612%
26	17.539	2434	2440	2452	rVV	3487071	5074580	86.39%	9.343%
27	19.345	2743	2747	2753	rBV3	44375	61746	1.05%	0.114%
28	19.410	2755	2758	2764	rVB	37167	57247	0.97%	0.105%
29	19.769	2812	2819	2827	rBV	4436360	5873845	100.00%	10.815%
30	21.522	3112	3117	3126	rBV	1781808	2489544	42.38%	4.584%
31	23.874	3510	3517	3530	rVB	2077212	4200320	71.51%	7.734%
32	24.039	3539	3545	3555	rVB	918912	1937031	32.98%	3.566%




Sum of corrected areas: 54312799

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014182.D
Acq On : 21 Mar 2023 15:33
Operator : CG/JU
Sample : PB151554BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK554

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

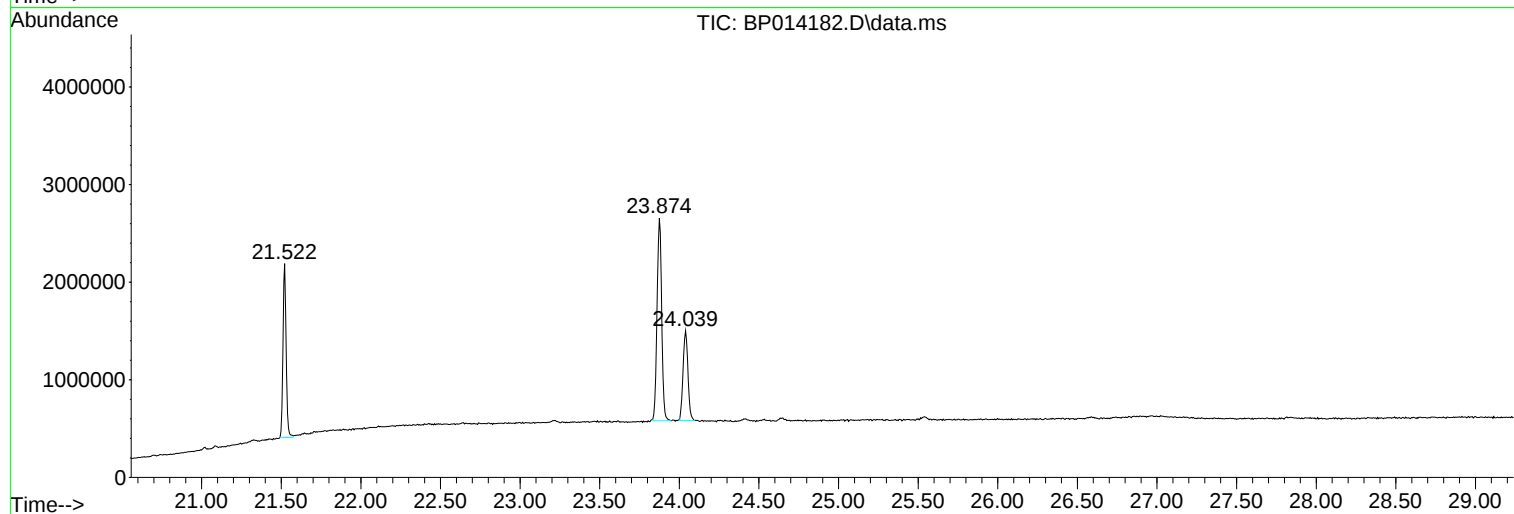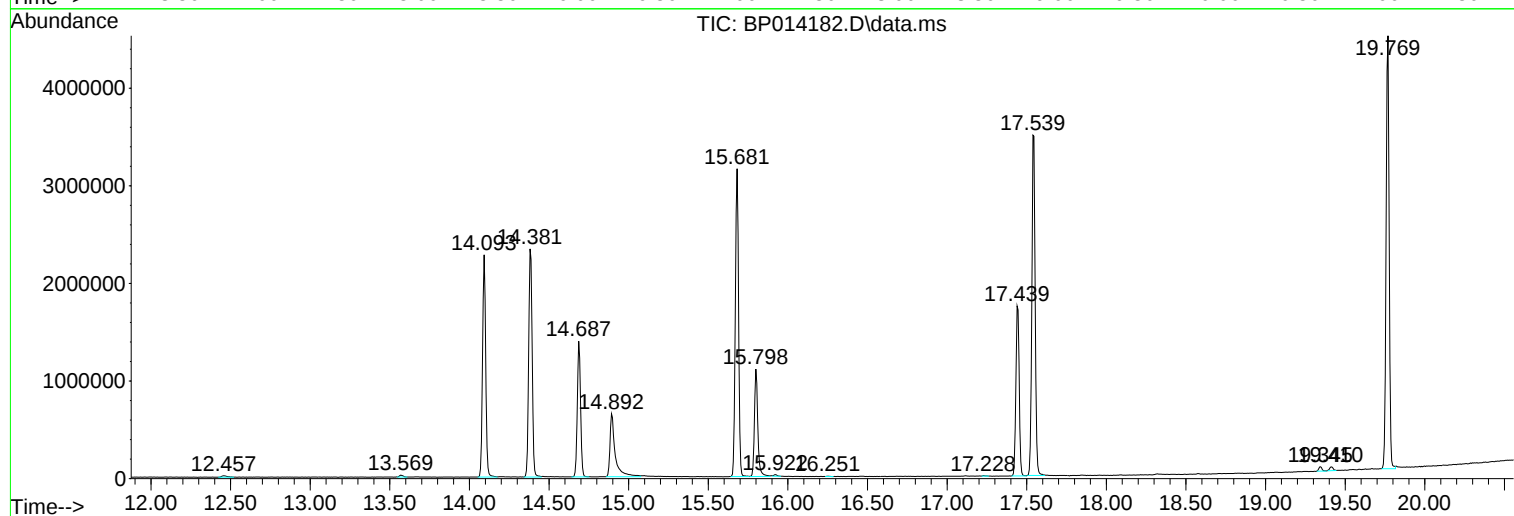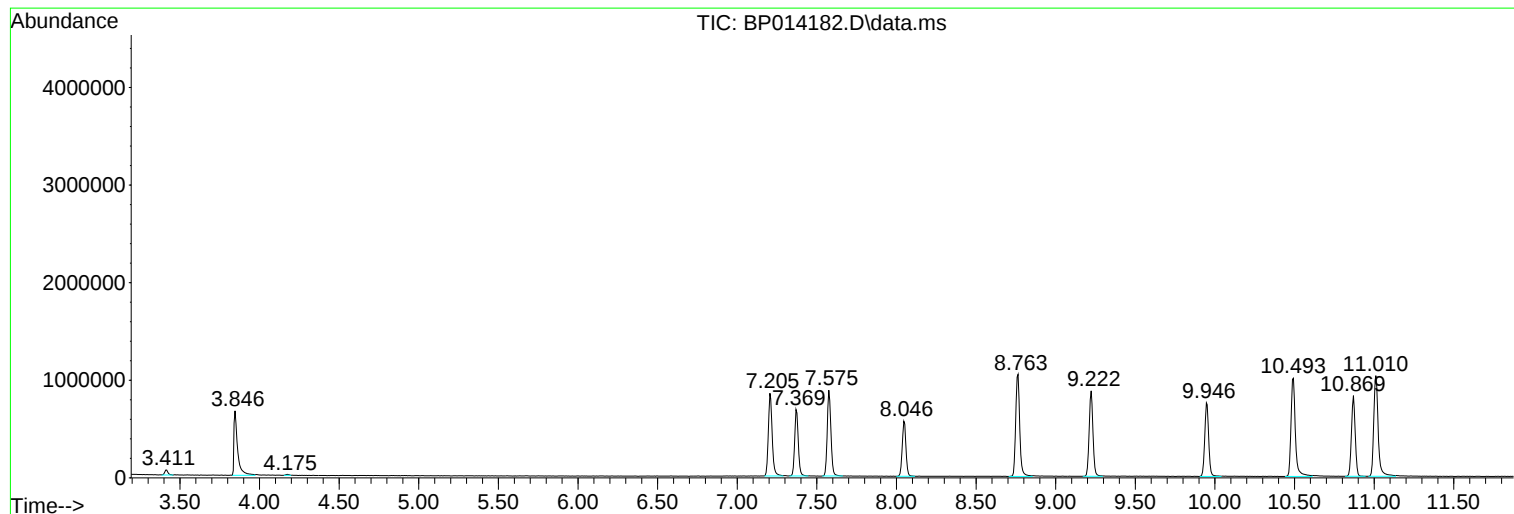

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014182.D
Acq On : 21 Mar 2023 15:33
Operator : CG/JU
Sample : PB151554BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK554

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014182.D
Acq On : 21 Mar 2023 15:33
Operator : CG/JU
Sample : PB151554BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK554

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc