

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
 Data File : BP014183.D
 Acq On : 21 Mar 2023 16:07
 Operator : CG/JU
 Sample : 01996-04DL 5X
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0A25DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014183.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	28	32	41	rBV	288136	464786	4.86%	1.116%
2	3.446	41	44	56	rVB	161450	220159	2.30%	0.529%
3	3.864	113	115	127	rBV	58931	104740	1.09%	0.251%
4	4.175	165	168	174	rVB	12384	17450	0.18%	0.042%
5	4.717	253	260	275	rBV	6347212	9571138	100.00%	22.982%
6	7.211	679	684	693	rBV	51731	107319	1.12%	0.258%
7	7.369	704	711	722	rBV	262805	429179	4.48%	1.031%
8	7.581	740	747	760	rBV	238058	421471	4.40%	1.012%
9	8.046	817	826	838	rBV	686610	1131691	11.82%	2.717%
10	8.763	941	948	960	rBV	188283	359262	3.75%	0.863%
11	9.222	1019	1026	1038	rBV	336421	584237	6.10%	1.403%
12	9.952	1143	1150	1161	rBV	260461	478279	5.00%	1.148%
13	10.493	1234	1242	1260	rBV	320124	706644	7.38%	1.697%
14	10.869	1297	1306	1319	rBV	1026554	1695569	17.72%	4.071%
15	11.016	1325	1331	1346	rBV	211362	473442	4.95%	1.137%
16	12.463	1571	1577	1583	rBV6	6939	14571	0.15%	0.035%
17	13.569	1758	1765	1774	rBV	32841	55780	0.58%	0.134%
18	14.093	1847	1854	1866	rBV	985332	1413291	14.77%	3.394%
19	14.381	1896	1903	1916	rBV	1045915	1528355	15.97%	3.670%
20	14.687	1948	1955	1971	rVB	1696006	2496123	26.08%	5.994%
21	14.940	1990	1998	2005	rBV6	20038	61229	0.64%	0.147%
22	15.681	2117	2124	2134	rBV	1449781	2088380	21.82%	5.015%
23	15.804	2138	2145	2157	rBV	373862	621502	6.49%	1.492%
24	15.922	2163	2165	2170	rVB5	9536	10828	0.11%	0.026%
25	16.045	2181	2186	2195	rVB3	14859	27972	0.29%	0.067%
26	17.439	2417	2423	2433	rBV	2255758	3200028	33.43%	7.684%
27	17.539	2433	2440	2451	rBV	1660699	2407467	25.15%	5.781%
28	18.304	2566	2570	2580	rBV3	34767	75358	0.79%	0.181%
29	18.398	2582	2586	2592	rVV	54928	84199	0.88%	0.202%
30	19.345	2744	2747	2752	rVB4	19134	25795	0.27%	0.062%
31	19.533	2776	2779	2786	rBV8	20674	37135	0.39%	0.089%
32	19.763	2813	2818	2824	rBV	2102116	2789814	29.15%	6.699%
33	21.522	3112	3117	3125	rBV	2389794	3206826	33.51%	7.700%
34	23.874	3511	3517	3528	rVB2	1037857	2146694	22.43%	5.155%
35	24.039	3539	3545	3555	rVB2	1224012	2589956	27.06%	6.219%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014183.D
Acq On : 21 Mar 2023 16:07
Operator : CG/JU
Sample : 01996-04DL 5X
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0A25DL

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Title : SVOA CALIBRATION




Sum of corrected areas: 41646669

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014183.D
Acq On : 21 Mar 2023 16:07
Operator : CG/JU
Sample : 01996-04DL 5X
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0A25DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

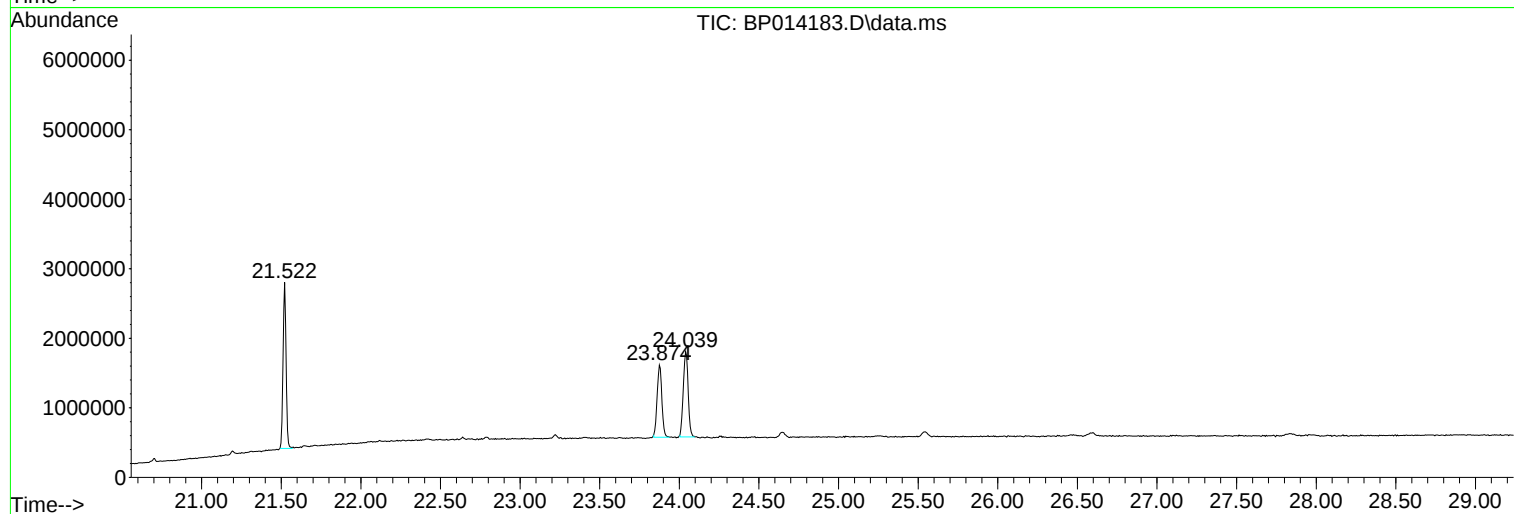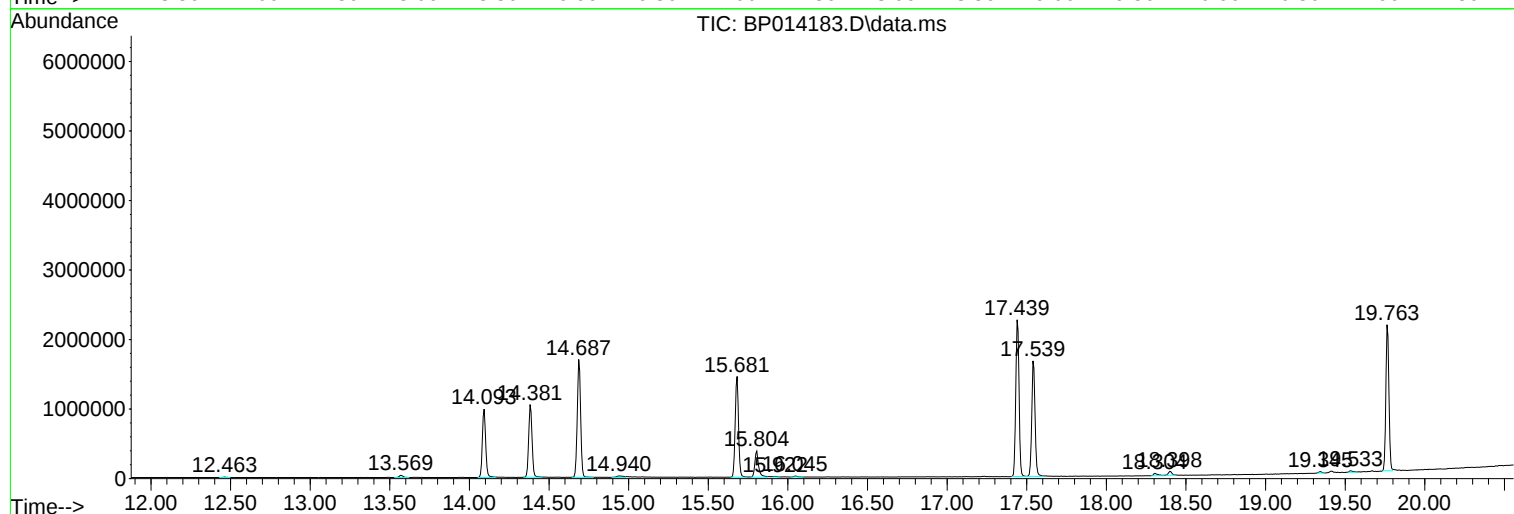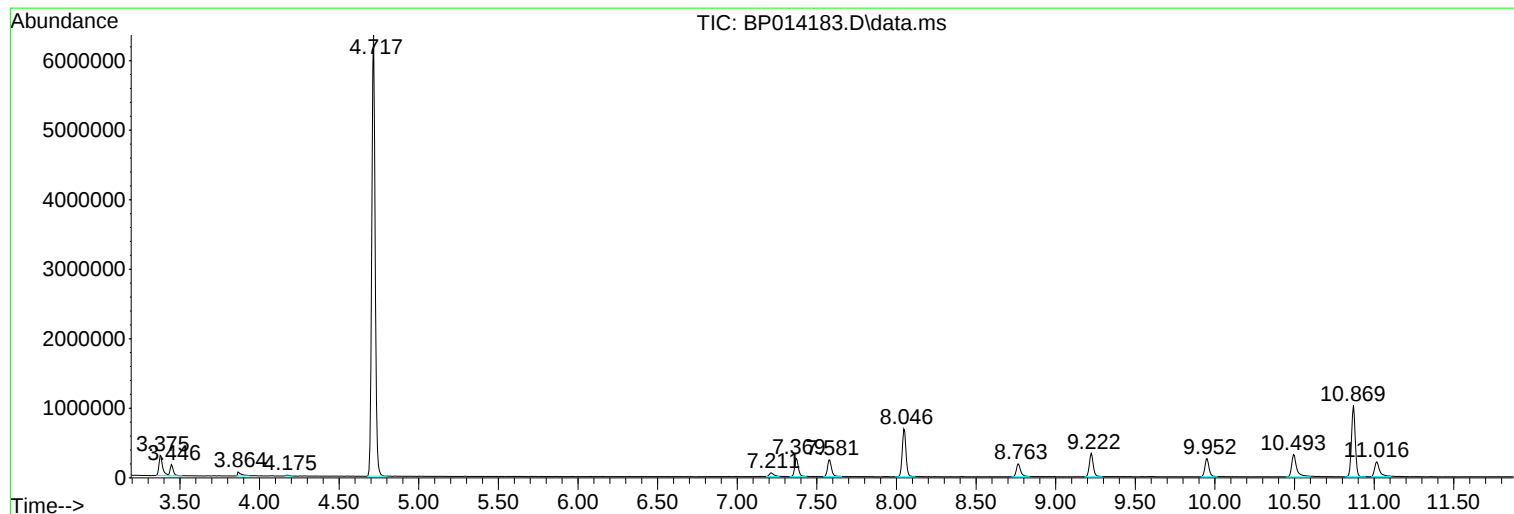

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014183.D
Acq On : 21 Mar 2023 16:07
Operator : CG/JU
Sample : 01996-04DL 5X
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0A25DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014183.D
Acq On : 21 Mar 2023 16:07
Operator : CG/JU
Sample : 01996-04DL 5X
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0A25DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc