

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
 Data File : BP014185.D
 Acq On : 21 Mar 2023 17:17
 Operator : CG/JU
 Sample : 01996-06DL 5X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0A27DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014185.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	27	32	40	rBV	411327	644833	6.21%	2.033%
2	3.446	40	44	54	rVB	197334	270714	2.61%	0.853%
3	3.887	116	119	130	rBV	16555	42618	0.41%	0.134%
4	4.175	164	168	172	rVB	10262	13352	0.13%	0.042%
5	4.716	253	260	274	rVB	6949567	10391536	100.00%	32.757%
6	7.216	679	685	699	rBV2	17828	49712	0.48%	0.157%
7	7.375	706	712	721	rBV	110860	188085	1.81%	0.593%
8	7.581	740	747	755	rBV	99566	181453	1.75%	0.572%
9	7.940	802	808	815	rVB6	9143	16626	0.16%	0.052%
10	8.046	819	826	841	rBV	579865	999305	9.62%	3.150%
11	8.405	881	887	898	rBV	25295	47329	0.46%	0.149%
12	8.769	943	949	964	rBV3	66891	142998	1.38%	0.451%
13	9.228	1019	1027	1043	rBV	129781	256805	2.47%	0.810%
14	9.951	1143	1150	1161	rBV	108738	201287	1.94%	0.635%
15	10.504	1236	1244	1265	rBV2	109146	310825	2.99%	0.980%
16	10.869	1297	1306	1318	rBV	839815	1456018	14.01%	4.590%
17	11.022	1324	1332	1347	rBV	59162	160364	1.54%	0.506%
18	13.569	1759	1765	1772	rBV	20279	36125	0.35%	0.114%
19	14.092	1846	1854	1866	rBV	445083	673005	6.48%	2.121%
20	14.387	1897	1904	1915	rBV	420683	661918	6.37%	2.087%
21	14.687	1948	1955	1966	rBV	1451357	2163851	20.82%	6.821%
22	14.969	1998	2003	2006	rBV7	7100	14527	0.14%	0.046%
23	15.510	2091	2095	2102	rVB5	7129	11794	0.11%	0.037%
24	15.681	2117	2124	2130	rBV	657215	965701	9.29%	3.044%
25	15.804	2140	2145	2157	rBV	132161	239027	2.30%	0.753%
26	16.045	2183	2186	2192	rBV4	10209	15239	0.15%	0.048%
27	16.728	2299	2302	2307	rBV7	6061	10411	0.10%	0.033%
28	17.445	2417	2424	2434	rBV	1918316	2765920	26.62%	8.719%
29	17.545	2434	2441	2450	rBV	750743	1133940	10.91%	3.574%
30	18.310	2566	2571	2580	rBV4	27587	57447	0.55%	0.181%
31	18.404	2582	2587	2592	rVV	54264	80548	0.78%	0.254%
32	19.339	2744	2746	2750	rBV5	12602	16173	0.16%	0.051%
33	19.763	2813	2818	2825	rBV	1017103	1396411	13.44%	4.402%
34	21.521	3112	3117	3129	rBV	2083006	2839360	27.32%	8.950%
35	23.874	3512	3517	3529	rVB2	500257	1043883	10.05%	3.291%
36	24.045	3539	3546	3557	rVB2	1041112	2224073	21.40%	7.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014185.D
Acq On : 21 Mar 2023 17:17
Operator : CG/JU
Sample : 01996-06DL 5X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0A27DL

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Title : SVOA CALIBRATION




Sum of corrected areas: 31723213

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014185.D
Acq On : 21 Mar 2023 17:17
Operator : CG/JU
Sample : 01996-06DL 5X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0A27DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

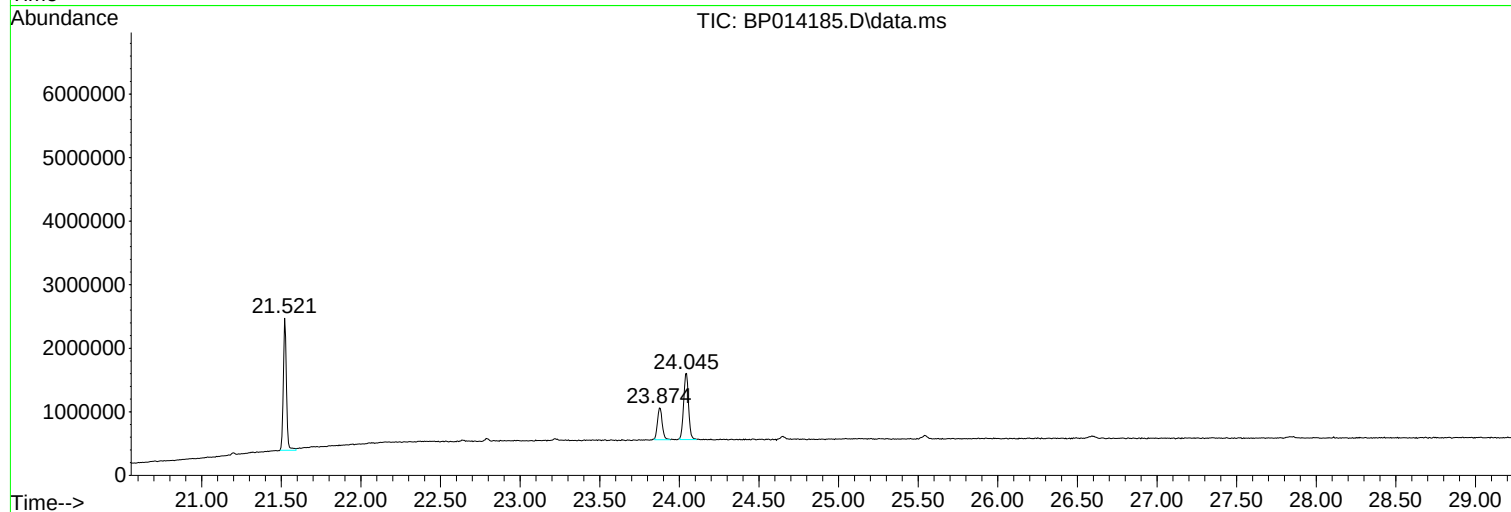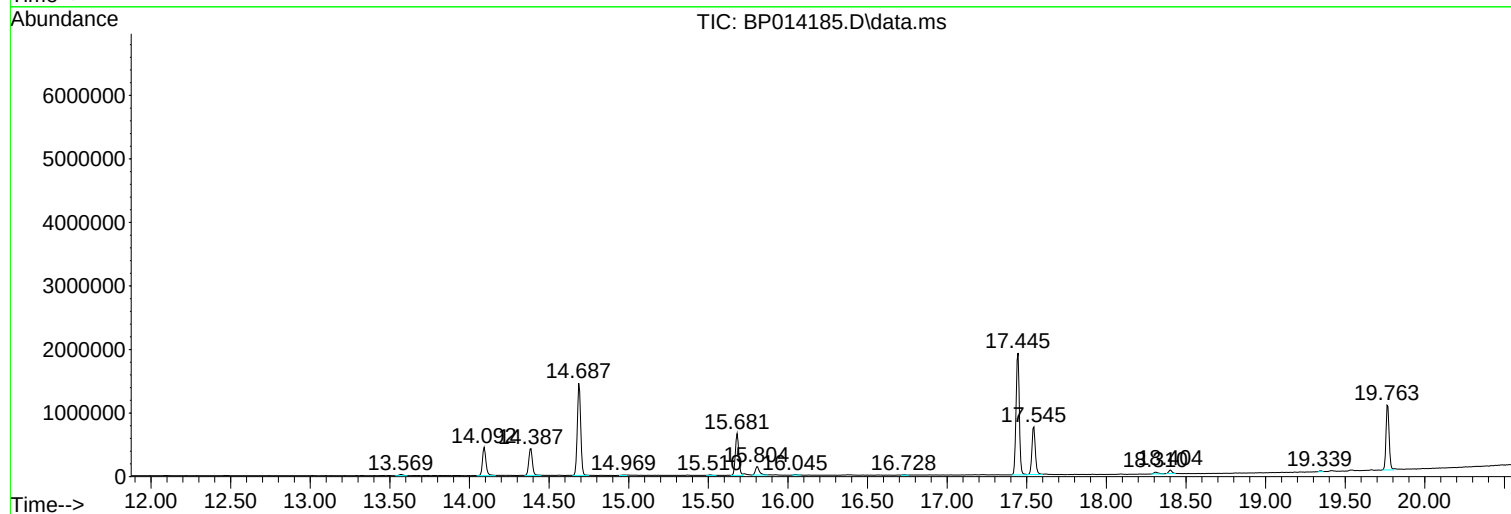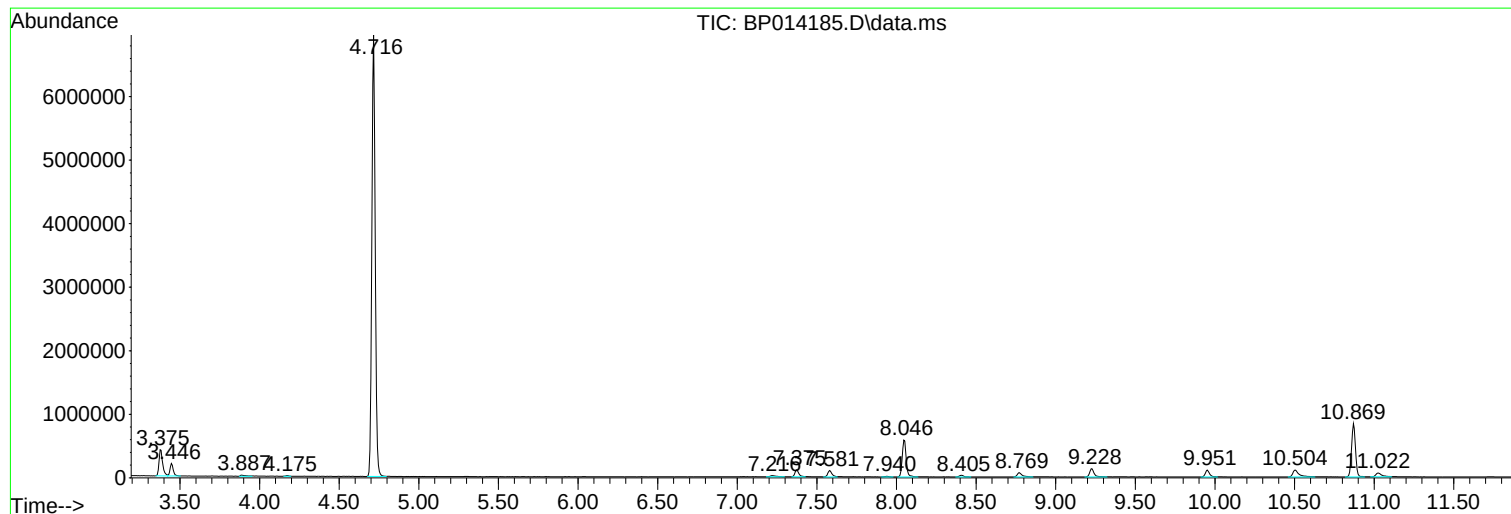

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014185.D
Acq On : 21 Mar 2023 17:17
Operator : CG/JU
Sample : 01996-06DL 5X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0A27DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014185.D
Acq On : 21 Mar 2023 17:17
Operator : CG/JU
Sample : 01996-06DL 5X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0A27DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc