

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
 Data File : BP014186.D
 Acq On : 21 Mar 2023 18:19
 Operator : CG/JU
 Sample : 01996-07DL 5X
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0A28DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014186.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	27	32	41	rBV	450904	708876	5.96%	1.760%
2	3.446	41	44	53	rVB	169984	221024	1.86%	0.549%
3	3.881	116	118	125	rBV	18883	32943	0.28%	0.082%
4	4.175	164	168	174	rVB	10629	14553	0.12%	0.036%
5	4.716	253	260	276	rBV	8006520	11884714	100.00%	29.510%
6	7.222	679	686	698	rBV2	20607	50100	0.42%	0.124%
7	7.375	706	712	722	rBV	123152	204532	1.72%	0.508%
8	7.581	740	747	757	rBV	104649	194938	1.64%	0.484%
9	7.940	804	808	817	rVB4	8719	14213	0.12%	0.035%
10	8.051	820	827	846	rVV	596401	986985	8.30%	2.451%
11	8.410	883	888	894	rVB	16480	28278	0.24%	0.070%
12	8.775	944	950	960	rBV	72849	148384	1.25%	0.368%
13	9.228	1020	1027	1039	rBV	135229	253413	2.13%	0.629%
14	9.951	1143	1150	1160	rBV	103575	196066	1.65%	0.487%
15	10.504	1234	1244	1263	rBV	123070	327438	2.76%	0.813%
16	10.875	1298	1307	1321	rBV	828006	1454841	12.24%	3.612%
17	11.028	1325	1333	1346	rBV	84392	206283	1.74%	0.512%
18	13.575	1760	1766	1773	rBV2	24325	40562	0.34%	0.101%
19	14.092	1847	1854	1868	rBV	429473	663154	5.58%	1.647%
20	14.386	1879	1904	1932	rBV2	612535	1980515	16.66%	4.918%
21	14.692	1949	1956	1968	rBV	1314932	1916640	16.13%	4.759%
22	14.980	1997	2005	2008	rBV10	6166	14623	0.12%	0.036%
23	15.516	2092	2096	2101	rVB4	10349	14054	0.12%	0.035%
24	15.680	2118	2124	2131	rBV	619006	953494	8.02%	2.368%
25	15.810	2139	2146	2157	rBV3	115812	230778	1.94%	0.573%
26	16.051	2181	2187	2195	rBV3	13979	28212	0.24%	0.070%
27	17.445	2417	2424	2435	rBV	1943451	2745802	23.10%	6.818%
28	17.545	2435	2441	2451	rVV	757684	1086416	9.14%	2.698%
29	18.104	2530	2536	2544	rVB3	44945	107491	0.90%	0.267%
30	18.310	2567	2571	2577	rBV5	37563	61979	0.52%	0.154%
31	18.404	2583	2587	2596	rVB	68462	100001	0.84%	0.248%
32	19.627	2787	2795	2808	rBV2	1382495	2780481	23.40%	6.904%
33	19.768	2814	2819	2830	rBV	971450	1307148	11.00%	3.246%
34	21.521	3112	3117	3125	rBV	1918334	2727855	22.95%	6.773%
35	22.627	3299	3305	3313	rVB2	422036	944662	7.95%	2.346%
36	22.798	3328	3334	3350	rVB2	1216310	2508832	21.11%	6.230%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014186.D
Acq On : 21 Mar 2023 18:19
Operator : CG/JU
Sample : 01996-07DL 5X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0A28DL

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Title : SVOA CALIBRATION

37	23.880	3513	3518	3528	rVB2	464962	948018	7.98%	2.354%
38	24.045	3539	3546	3559	rBV2	1005774	2184594	18.38%	5.424%




Sum of corrected areas: 40272892

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014186.D
Acq On : 21 Mar 2023 18:19
Operator : CG/JU
Sample : 01996-07DL 5X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0A28DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

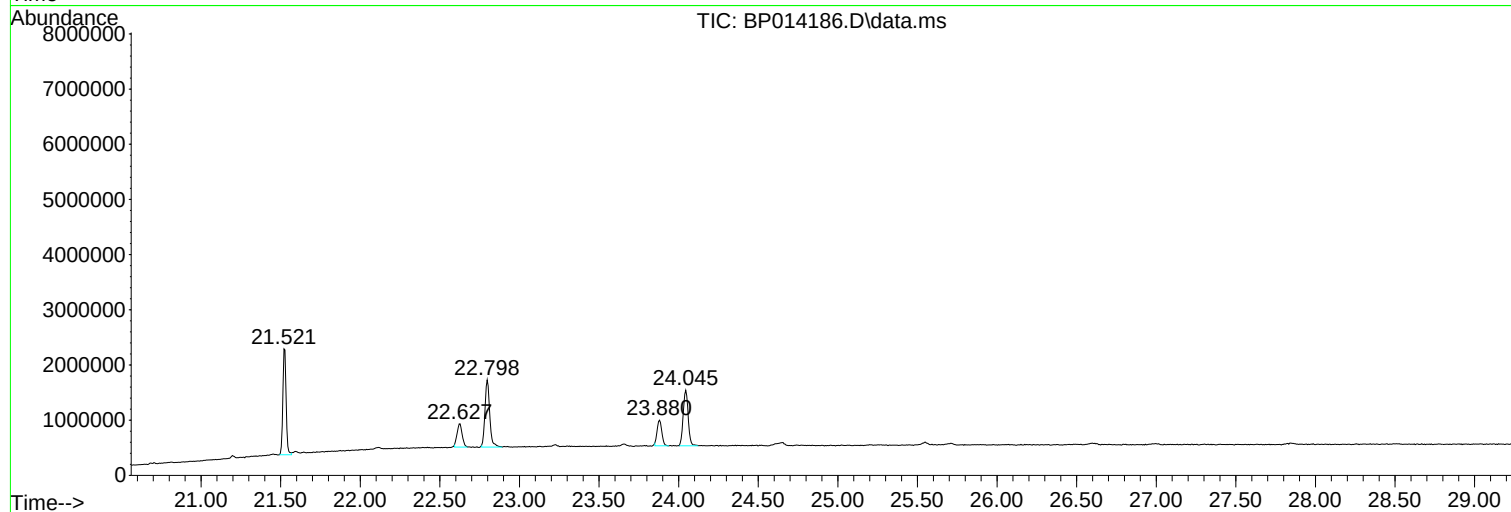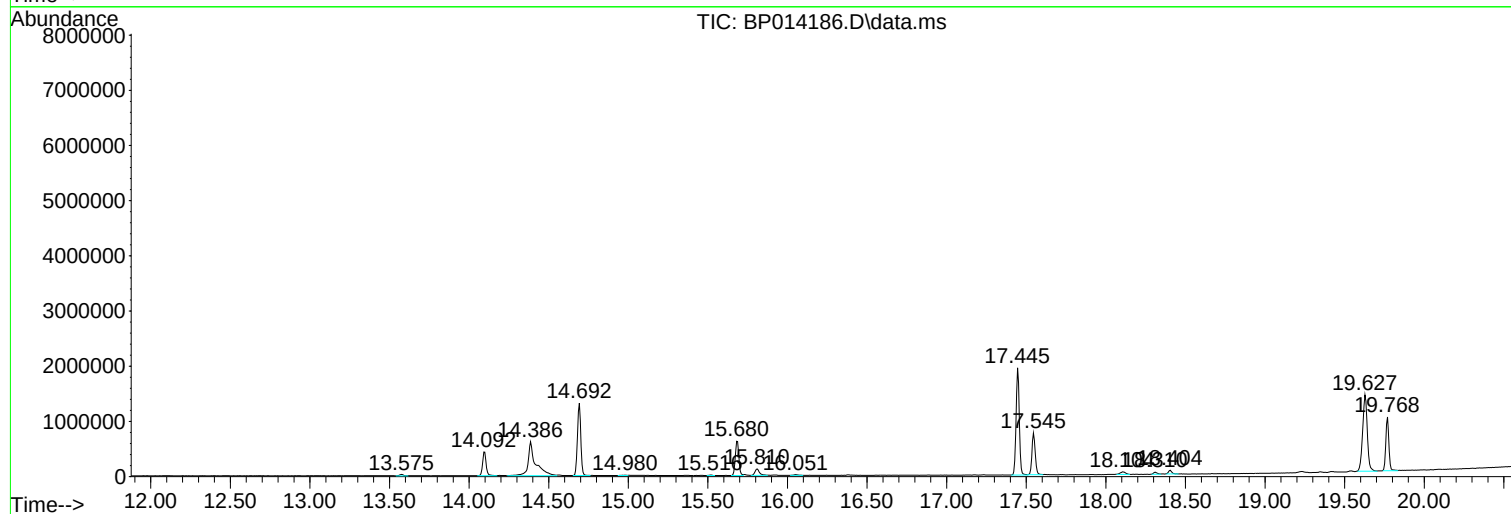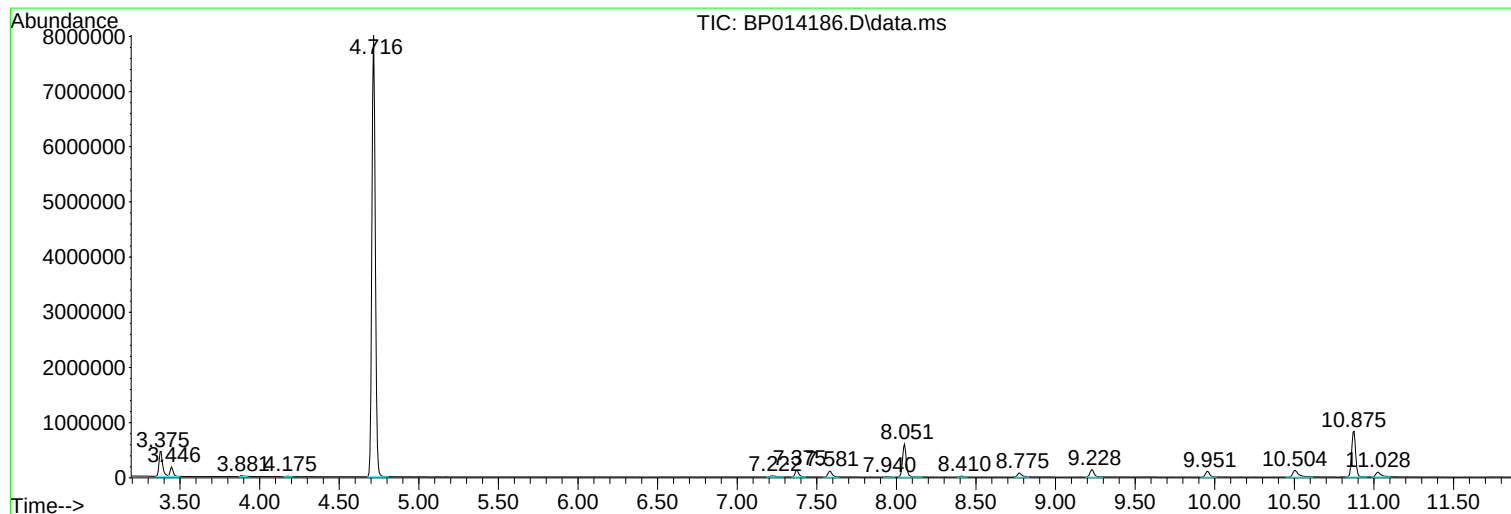

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014186.D
Acq On : 21 Mar 2023 18:19
Operator : CG/JU
Sample : 01996-07DL 5X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0A28DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014186.D
Acq On : 21 Mar 2023 18:19
Operator : CG/JU
Sample : 01996-07DL 5X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0A28DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
