

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
 Data File : BP014187.D
 Acq On : 21 Mar 2023 18:54
 Operator : CG/JU
 Sample : 01996-08DL 5X
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0A29DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014187.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	29	33	36	rBV	15773	22979	0.71%	0.094%
2	3.411	36	38	41	rVV	14893	19585	0.60%	0.080%
3	3.446	41	44	55	rVB	96709	139178	4.30%	0.571%
4	3.705	85	88	97	rBV	24103	43403	1.34%	0.178%
5	4.170	164	167	172	rVB	11367	16783	0.52%	0.069%
6	4.711	253	259	269	rVB	372040	585981	18.09%	2.405%
7	7.064	655	659	661	rVB5	2890	3705	0.11%	0.015%
8	7.146	668	673	678	rVB6	7009	11096	0.34%	0.046%
9	7.211	678	684	696	rBV	70345	141030	4.35%	0.579%
10	7.369	705	711	723	rBV	146362	245300	7.57%	1.007%
11	7.575	738	746	757	rBV	165039	289231	8.93%	1.187%
12	8.046	817	826	835	rBV	685607	1125242	34.74%	4.619%
13	8.764	941	948	964	rBV	125642	260891	8.05%	1.071%
14	9.222	1017	1026	1040	rBV	171021	315507	9.74%	1.295%
15	9.605	1086	1091	1097	rVB2	15089	23939	0.74%	0.098%
16	9.952	1143	1150	1162	rBV	137144	258696	7.99%	1.062%
17	10.499	1234	1243	1262	rBV	153511	414710	12.80%	1.702%
18	10.869	1297	1306	1318	rBV	973460	1675417	51.72%	6.877%
19	11.046	1331	1336	1340	rBV6	6851	11904	0.37%	0.049%
20	11.722	1445	1451	1452	rBV6	2537	5145	0.16%	0.021%
21	11.887	1474	1479	1481	rBV6	1939	3579	0.11%	0.015%
22	12.099	1511	1515	1521	rVB7	6854	10602	0.33%	0.044%
23	12.469	1571	1578	1582	rBV8	3590	8071	0.25%	0.033%
24	13.569	1758	1765	1772	rBV	30599	51614	1.59%	0.212%
25	14.093	1846	1854	1869	rBV	489603	744454	22.98%	3.056%
26	14.193	1869	1871	1878	rVB8	2357	4557	0.14%	0.019%
27	14.381	1896	1903	1916	rBV	542488	811228	25.04%	3.330%
28	14.687	1948	1955	1970	rVB	1695611	2442685	75.40%	10.027%
29	14.934	1987	1997	2006	rBV7	25529	88208	2.72%	0.362%
30	15.093	2022	2024	2028	rVB5	3351	4121	0.13%	0.017%
31	15.416	2076	2079	2082	rBV5	2885	3271	0.10%	0.013%
32	15.675	2117	2123	2136	rBV	717586	1106743	34.16%	4.543%
33	15.804	2138	2145	2155	rBV	150041	262572	8.11%	1.078%
34	15.916	2162	2164	2171	rVB7	5156	7390	0.23%	0.030%
35	16.045	2181	2186	2192	rVB	23758	34183	1.06%	0.140%
36	16.363	2237	2240	2243	rBV5	3001	4635	0.14%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
 Data File : BP014187.D
 Acq On : 21 Mar 2023 18:54
 Operator : CG/JU
 Sample : 01996-08DL 5X
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0A29DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

37	16.834	2316	2320	2324	rVB7	5788	9272	0.29%	0.038%
38	17.104	2365	2366	2371	rVB5	3458	4624	0.14%	0.019%
39	17.169	2374	2377	2378	rBV3	3818	3474	0.11%	0.014%
40	17.228	2384	2387	2394	rVB6	6585	10268	0.32%	0.042%
41	17.440	2416	2423	2434	rBV	2216372	3099493	95.68%	12.723%
42	17.540	2434	2440	2448	rBV	835807	1186872	36.64%	4.872%
43	18.187	2546	2550	2554	rBV7	9027	15349	0.47%	0.063%
44	18.298	2565	2569	2578	rBV	122636	202020	6.24%	0.829%
45	18.398	2583	2586	2593	rVB3	25263	39437	1.22%	0.162%
46	19.528	2774	2778	2788	rBV2	88679	155237	4.79%	0.637%
47	19.763	2813	2818	2824	rBV	1075105	1432754	44.23%	5.881%
48	21.522	3111	3117	3126	rBV	2315036	3239500	100.00%	13.298%
49	23.874	3511	3517	3527	rVB	560275	1134551	35.02%	4.657%
50	24.039	3538	3545	3555	rVB2	1250019	2631100	81.22%	10.800%




Sum of corrected areas: 24361586

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014187.D
Acq On : 21 Mar 2023 18:54
Operator : CG/JU
Sample : 01996-08DL 5X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0A29DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

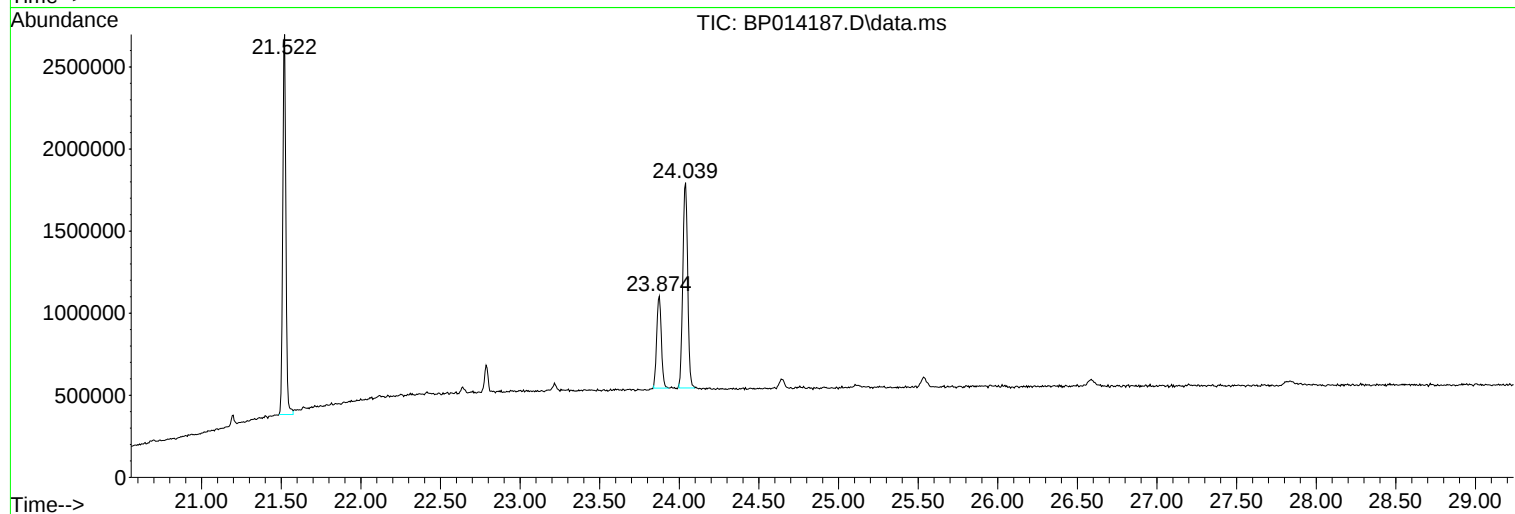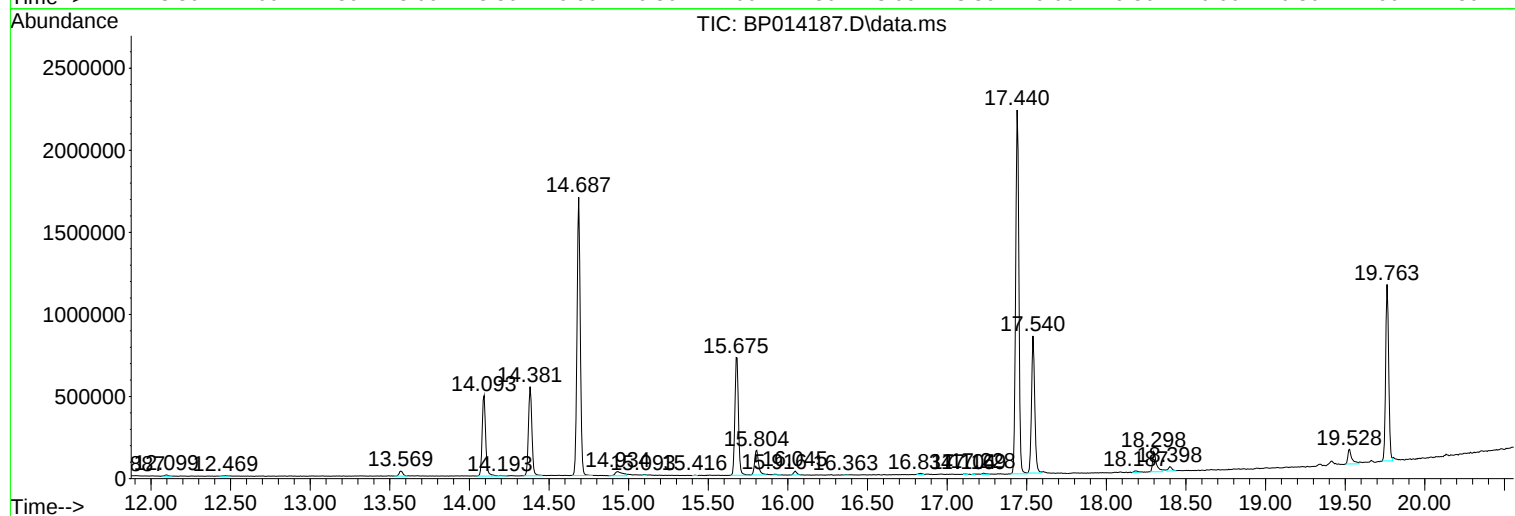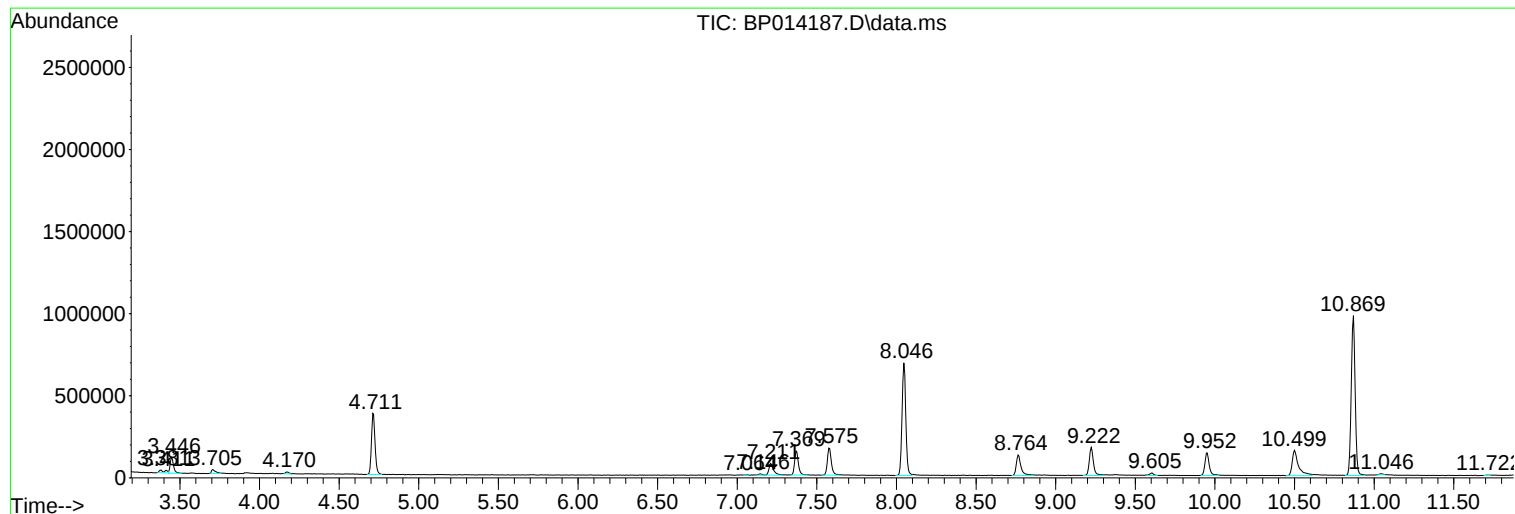

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014187.D
Acq On : 21 Mar 2023 18:54
Operator : CG/JU
Sample : 01996-08DL 5X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0A29DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014187.D
Acq On : 21 Mar 2023 18:54
Operator : CG/JU
Sample : 01996-08DL 5X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0A29DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc