

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
 Data File : BP014198.D
 Acq On : 22 Mar 2023 01:44
 Operator : CG/JU
 Sample : PB151552BL
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK552

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014198.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.411	34	38	46	rVB	62445	83224	1.14%	0.118%
2	3.840	108	111	143	rBV	764673	1330502	18.30%	1.888%
3	4.169	163	167	173	rVB	14329	22455	0.31%	0.032%
4	7.205	676	683	700	rBV	1067067	1770371	24.34%	2.512%
5	7.369	703	711	724	rVV	850126	1331343	18.31%	1.889%
6	7.575	738	746	763	rBV	1063891	1764463	24.26%	2.504%
7	8.046	816	826	840	rBV	856452	1427000	19.62%	2.025%
8	8.757	940	947	964	rBV	1353161	2259430	31.07%	3.206%
9	9.216	1018	1025	1038	rBV	1066397	1781608	24.50%	2.528%
10	9.946	1141	1149	1160	rBV	925126	1586882	21.82%	2.252%
11	10.487	1233	1241	1262	rBV	1253182	2361687	32.47%	3.351%
12	10.863	1296	1305	1315	rBV	1242018	2097516	28.84%	2.976%
13	11.004	1322	1329	1347	rBV	1304323	2406176	33.09%	3.414%
14	12.451	1568	1575	1583	rBV3	20630	43803	0.60%	0.062%
15	13.569	1759	1765	1772	rVB6	13373	22448	0.31%	0.032%
16	13.657	1772	1780	1786	rBV6	5528	13370	0.18%	0.019%
17	14.087	1845	1853	1865	rBV	2564216	3682048	50.63%	5.225%
18	14.381	1896	1903	1916	rBV	2888202	4219470	58.02%	5.988%
19	14.681	1947	1954	1969	rBV	2048470	3023296	41.57%	4.290%
20	14.892	1983	1990	2015	rBV	768986	1736847	23.88%	2.465%
21	15.675	2116	2123	2134	rBV	3782178	5415524	74.47%	7.685%
22	15.798	2137	2144	2160	rVV	1264825	1863206	25.62%	2.644%
23	15.916	2160	2164	2171	rVB3	19323	36210	0.50%	0.051%
24	16.245	2217	2220	2224	rBV6	6186	8310	0.11%	0.012%
25	17.110	2363	2367	2374	rVB8	7614	12359	0.17%	0.018%
26	17.439	2416	2423	2431	rBV	2713266	3811183	52.41%	5.408%
27	17.539	2433	2440	2453	rVV	4312262	6132420	84.32%	8.702%
28	19.339	2742	2746	2751	rBV2	61107	83586	1.15%	0.119%
29	19.410	2754	2758	2765	rVB2	51475	75226	1.03%	0.107%
30	19.763	2811	2818	2831	rBV	5505930	7272439	100.00%	10.320%
31	21.516	3111	3116	3124	rBV	2900122	3942435	54.21%	5.594%
32	23.868	3508	3516	3525	rBV2	2696973	5591540	76.89%	7.935%
33	24.033	3537	3544	3552	rVB2	1499120	3262562	44.86%	4.630%




Sum of corrected areas: 70470939

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014198.D
Acq On : 22 Mar 2023 01:44
Operator : CG/JU
Sample : PB151552BL
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK552

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

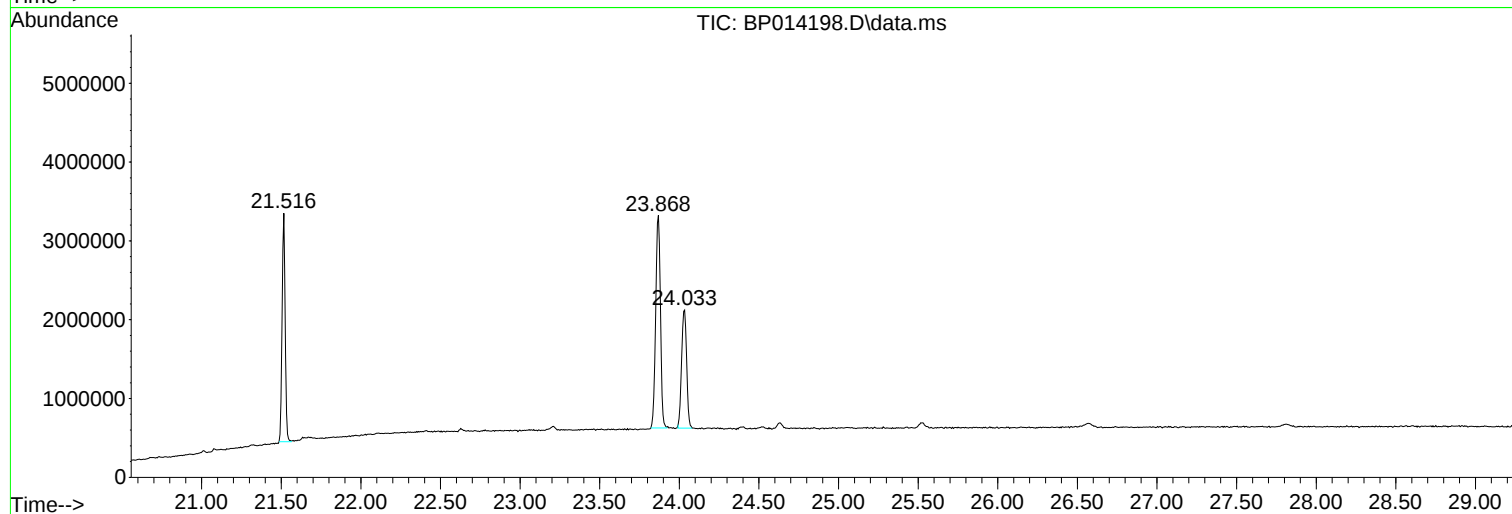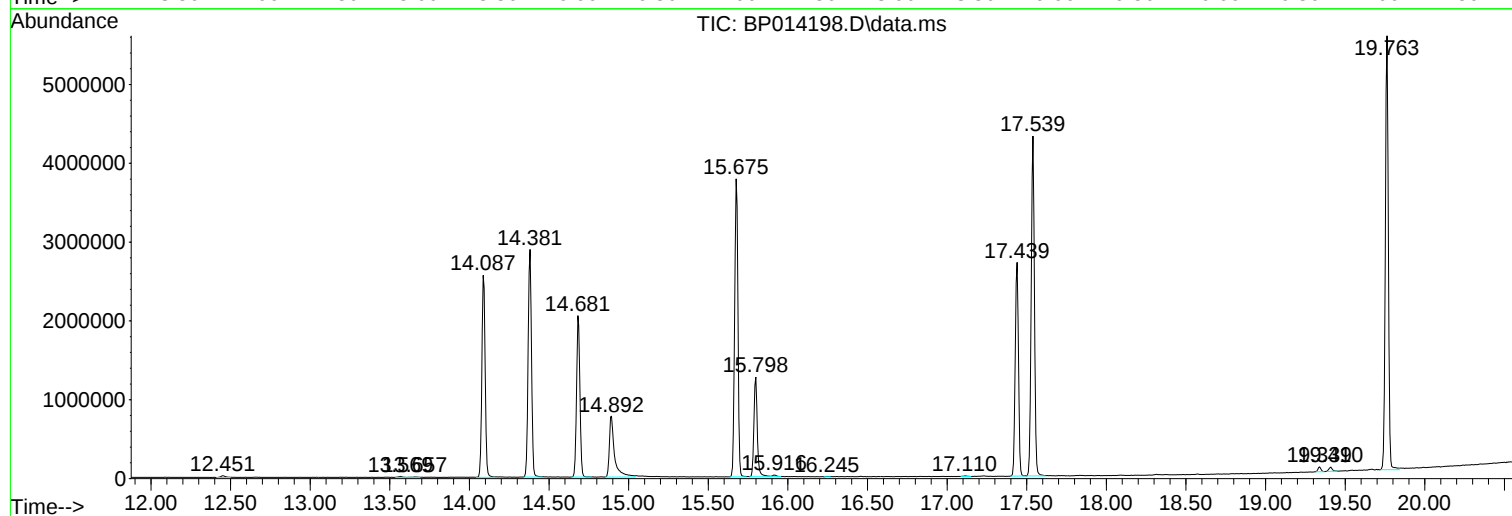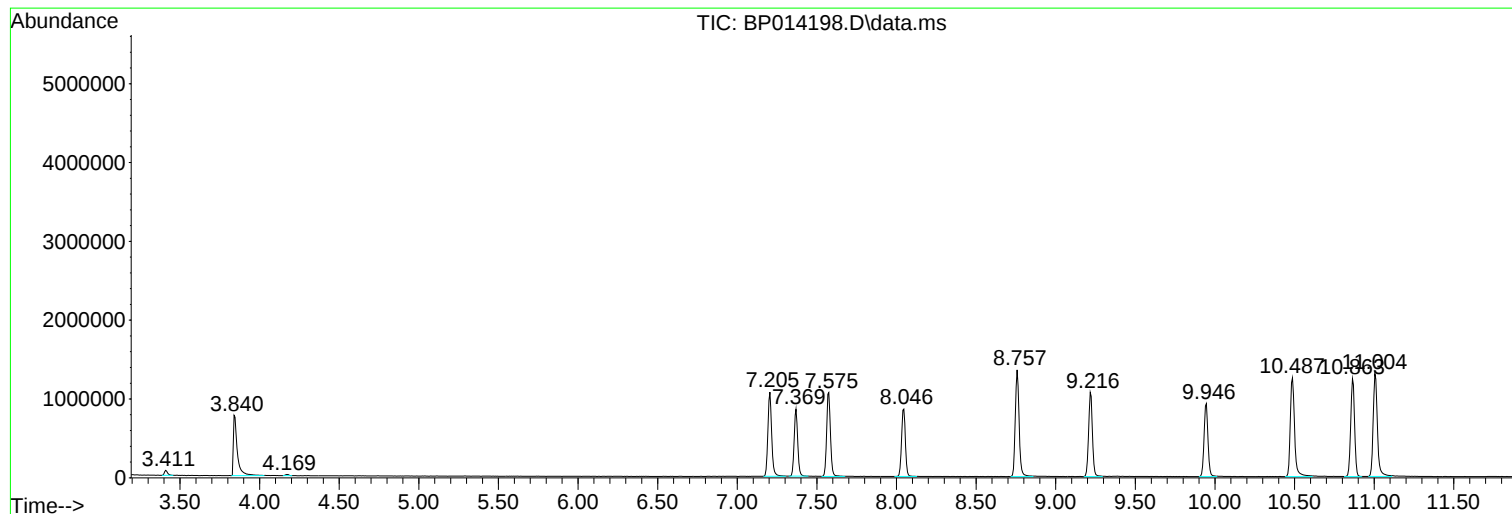

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014198.D
Acq On : 22 Mar 2023 01:44
Operator : CG/JU
Sample : PB151552BL
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK552

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014198.D
Acq On : 22 Mar 2023 01:44
Operator : CG/JU
Sample : PB151552BL
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK552

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc