

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
 Data File : BP014201.D
 Acq On : 22 Mar 2023 03:26
 Operator : CG/JU
 Sample : PB151558BL
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK558

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014201.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.411	34	38	44	rBV	53120	68266	1.14%	0.118%
2	3.840	109	111	129	rBV	656924	1122578	18.69%	1.935%
3	4.175	163	168	172	rBV2	11113	18210	0.30%	0.031%
4	7.205	676	683	697	rBV	882122	1471884	24.51%	2.537%
5	7.369	704	711	726	rVB	696571	1110706	18.49%	1.914%
6	7.575	737	746	760	rBV	870813	1465768	24.40%	2.526%
7	8.046	816	826	835	rBV	695367	1144996	19.06%	1.973%
8	8.758	940	947	962	rBV	1108016	1882354	31.34%	3.244%
9	9.216	1017	1025	1041	rBV	913039	1506679	25.08%	2.597%
10	9.940	1141	1148	1166	rBV	758842	1317814	21.94%	2.271%
11	10.487	1232	1241	1262	rBV	1069936	1988836	33.11%	3.428%
12	10.863	1294	1305	1316	rVB	1018822	1705262	28.39%	2.939%
13	11.005	1322	1329	1351	rBV	1068983	2032831	33.84%	3.504%
14	12.452	1569	1575	1585	rBV2	15719	33601	0.56%	0.058%
15	13.569	1758	1765	1772	rBV2	32251	53001	0.88%	0.091%
16	14.087	1846	1853	1868	rBV	2192854	3080972	51.29%	5.310%
17	14.381	1894	1903	1918	rBV	2379122	3555382	59.19%	6.128%
18	14.681	1947	1954	1963	rBV	1702119	2454020	40.86%	4.230%
19	14.893	1983	1990	2015	rBV	607689	1405064	23.39%	2.422%
20	15.675	2116	2123	2137	rBV	3209279	4545782	75.68%	7.835%
21	15.793	2137	2143	2159	rVV	1003493	1518275	25.28%	2.617%
22	15.916	2160	2164	2169	rVB3	15248	23506	0.39%	0.041%
23	17.228	2383	2387	2394	rBV7	5054	10878	0.18%	0.019%
24	17.439	2416	2423	2432	rBV	2177382	3088932	51.43%	5.324%
25	17.539	2432	2440	2453	rBV2	3501571	5163899	85.97%	8.900%
26	19.339	2742	2746	2750	rBV3	47032	65873	1.10%	0.114%
27	19.404	2754	2757	2762	rVB	40761	56863	0.95%	0.098%
28	19.757	2812	2817	2828	rBV	4358348	6006463	100.00%	10.353%
29	21.516	3111	3116	3125	rBV	2166785	3097344	51.57%	5.339%
30	23.863	3508	3515	3528	rBV2	2183456	4514923	75.17%	7.782%
31	24.027	3537	3543	3553	rVB2	1168646	2507921	41.75%	4.323%




Sum of corrected areas: 58018883

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014201.D
Acq On : 22 Mar 2023 03:26
Operator : CG/JU
Sample : PB151558BL
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK558

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

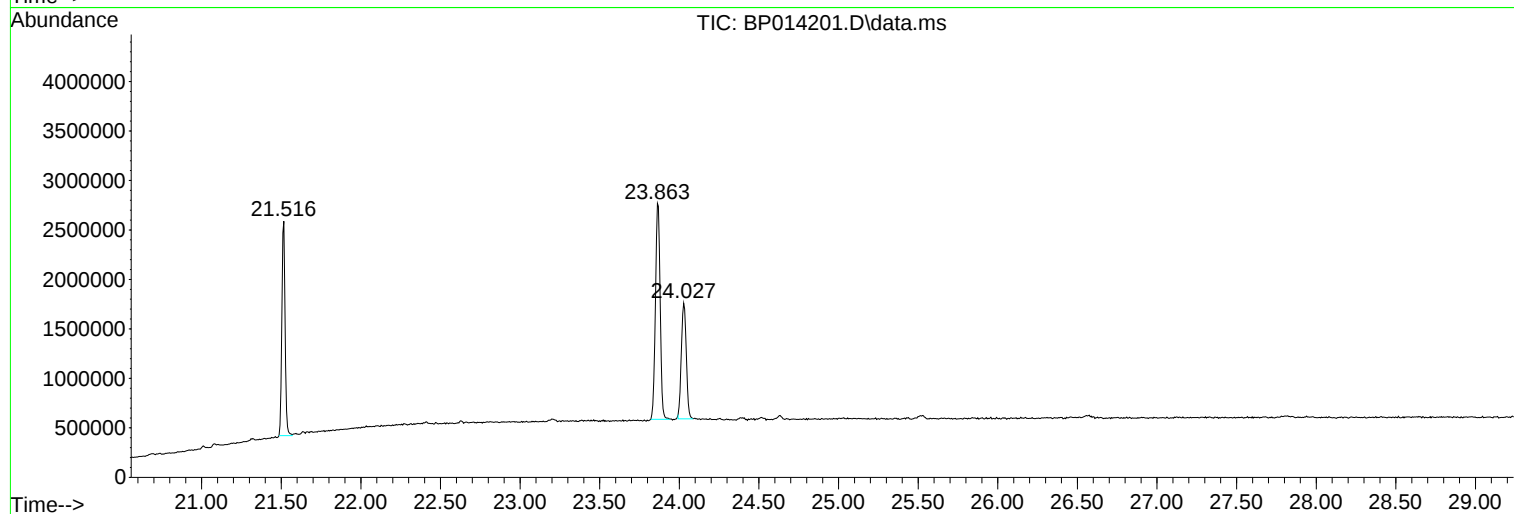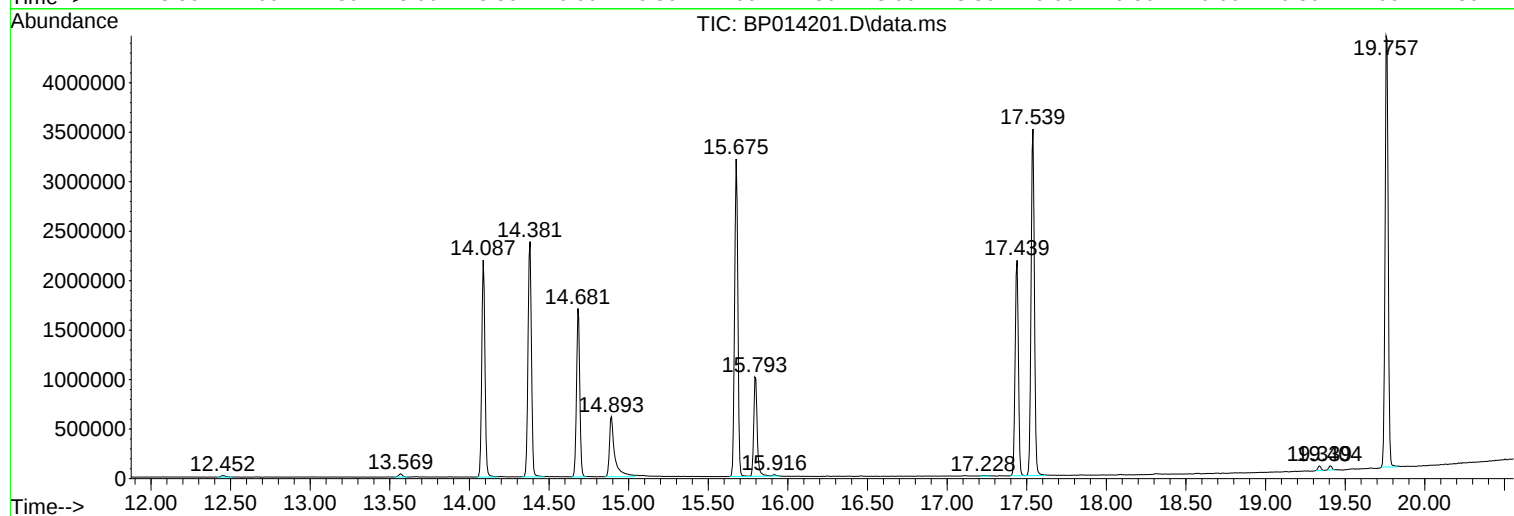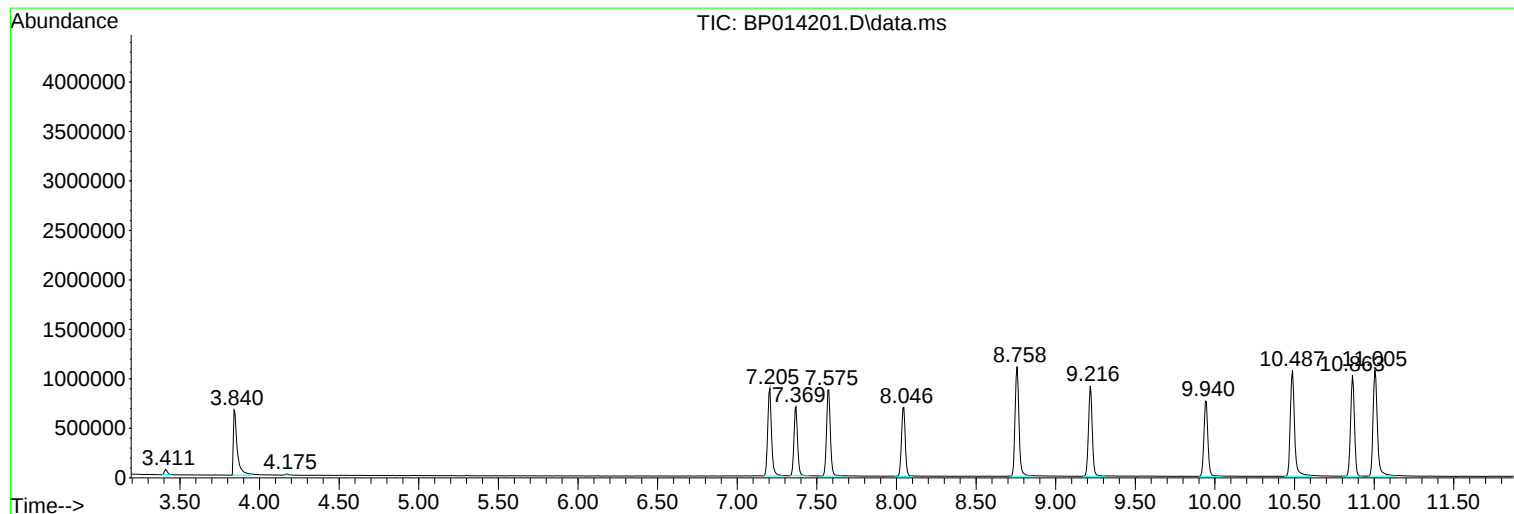

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014201.D
Acq On : 22 Mar 2023 03:26
Operator : CG/JU
Sample : PB151558BL
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK558

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014201.D
Acq On : 22 Mar 2023 03:26
Operator : CG/JU
Sample : PB151558BL
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK558

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc