

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
 Data File : BP014211.D
 Acq On : 22 Mar 2023 09:43
 Operator : CG/JU
 Sample : PB151541BL
 Misc :
 ALS Vial : 83 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK541

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014211.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	4	7	15	rVB2	14633	22926	0.41%	0.042%
2	3.411	34	38	44	rBV	51962	67526	1.20%	0.125%
3	3.846	110	112	127	rBV	416008	672945	11.91%	1.244%
4	4.175	162	168	173	rBV2	13068	23384	0.41%	0.043%
5	7.205	676	683	695	rBV	869551	1435819	25.41%	2.655%
6	7.369	704	711	723	rVB	683311	1076006	19.04%	1.990%
7	7.575	739	746	759	rVB	845720	1405936	24.88%	2.600%
8	8.046	814	826	841	rBV	657231	1074397	19.01%	1.987%
9	8.758	939	947	964	rBV	1089166	1851443	32.76%	3.423%
10	9.216	1018	1025	1039	rBV	856947	1451922	25.69%	2.685%
11	9.946	1141	1149	1161	rBV	765950	1289071	22.81%	2.384%
12	10.487	1233	1241	1268	rBV	1023193	1961168	34.71%	3.626%
13	10.863	1298	1305	1315	rBV	962484	1601960	28.35%	2.962%
14	11.004	1322	1329	1349	rBV	667225	1299642	23.00%	2.403%
15	12.457	1568	1576	1582	rBV2	13675	30352	0.54%	0.056%
16	13.569	1760	1765	1772	rBV2	12542	22040	0.39%	0.041%
17	13.663	1776	1781	1787	rVB8	3418	6350	0.11%	0.012%
18	14.087	1847	1853	1868	rBV	2126477	2977686	52.70%	5.506%
19	14.381	1895	1903	1916	rBV	2298488	3459619	61.22%	6.397%
20	14.681	1947	1954	1968	rVB	1571684	2324552	41.14%	4.298%
21	14.892	1984	1990	2020	rBV	567863	1363116	24.12%	2.520%
22	15.675	2116	2123	2132	rBV	3085360	4375923	77.44%	8.091%
23	15.798	2137	2144	2156	rVV	944684	1411894	24.99%	2.611%
24	15.916	2160	2164	2170	rVB3	17826	28284	0.50%	0.052%
25	16.457	2254	2256	2262	rVB7	4401	6393	0.11%	0.012%
26	17.116	2365	2368	2373	rVB7	4373	6396	0.11%	0.012%
27	17.234	2384	2388	2389	rBV4	5135	5817	0.10%	0.011%
28	17.439	2416	2423	2433	rBV	2034632	2944193	52.10%	5.444%
29	17.539	2433	2440	2455	rVV	3520273	4973838	88.02%	9.197%
30	18.086	2529	2533	2538	rVB7	13437	21256	0.38%	0.039%
31	19.339	2742	2746	2750	rBV2	49353	67090	1.19%	0.124%
32	19.410	2754	2758	2762	rVV	36649	52607	0.93%	0.097%
33	19.763	2812	2818	2829	rBV	4196068	5650705	100.00%	10.448%
34	21.516	3111	3116	3125	rBV	1962387	2737459	48.44%	5.062%
35	23.868	3509	3516	3526	rVB2	2015008	4055061	71.76%	7.498%
36	24.033	3537	3544	3555	rVB2	1063098	2328171	41.20%	4.305%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014211.D
Acq On : 22 Mar 2023 09:43
Operator : CG/JU
Sample : PB151541BL
Misc :
ALS Vial : 83 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK541

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Title : SVOA CALIBRATION




Sum of corrected areas: 54082947

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014211.D
Acq On : 22 Mar 2023 09:43
Operator : CG/JU
Sample : PB151541BL
Misc :
ALS Vial : 83 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK541

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

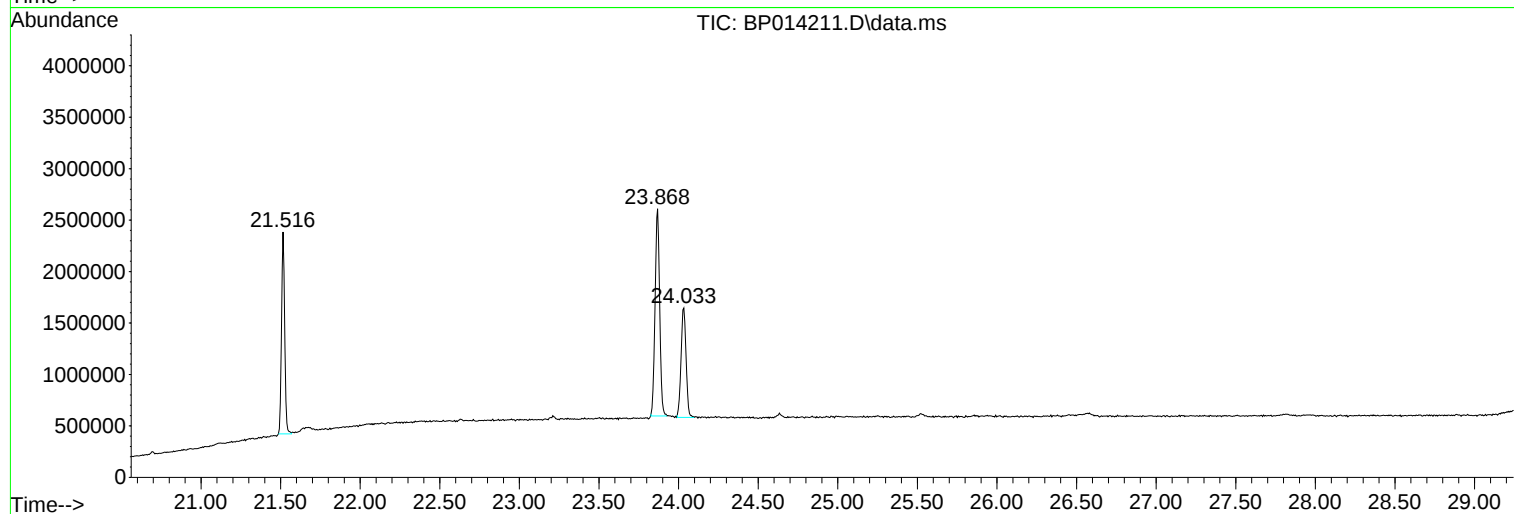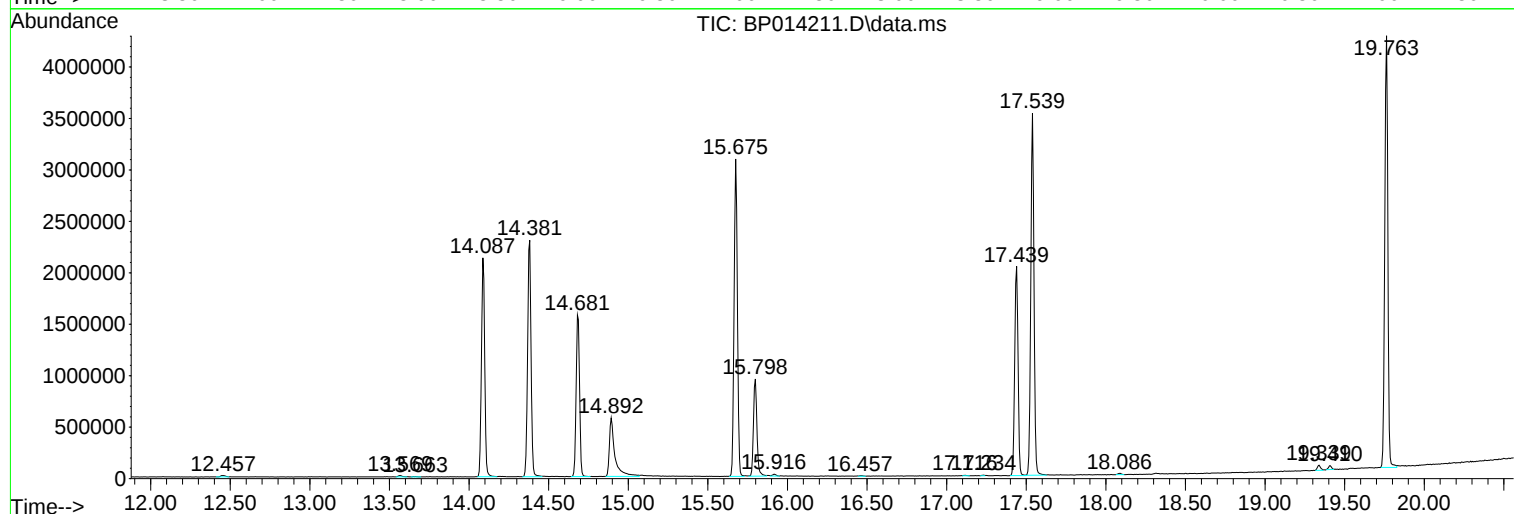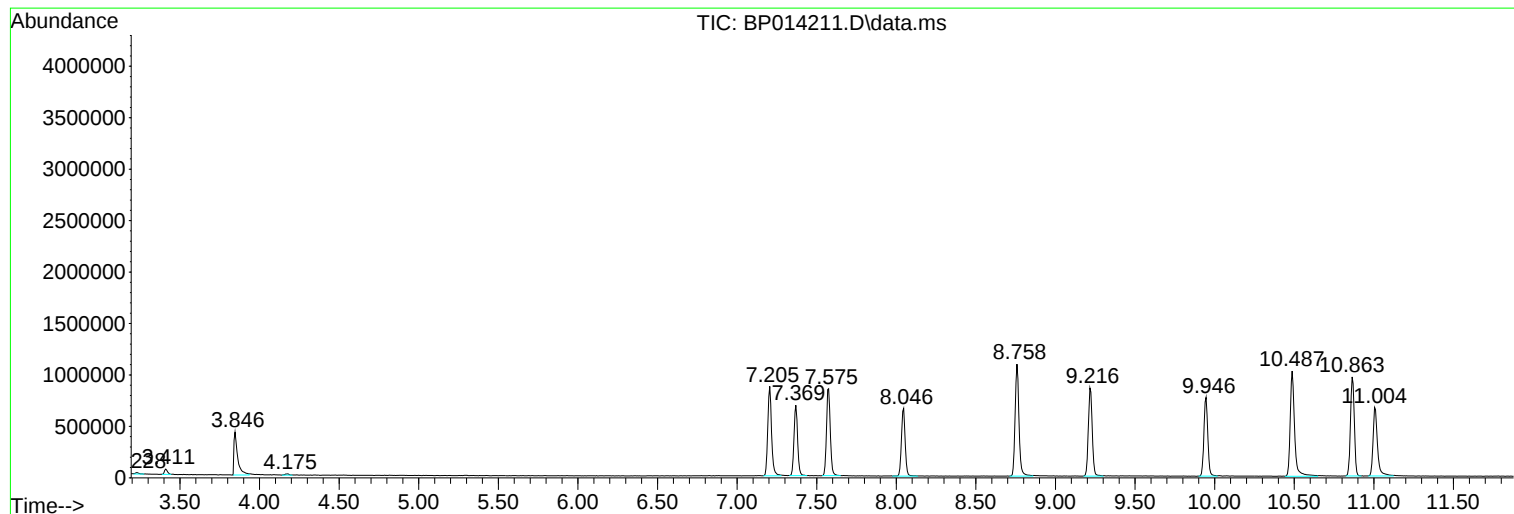

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014211.D
Acq On : 22 Mar 2023 09:43
Operator : CG/JU
Sample : PB151541BL
Misc :
ALS Vial : 83 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK541

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032023\
Data File : BP014211.D
Acq On : 22 Mar 2023 09:43
Operator : CG/JU
Sample : PB151541BL
Misc :
ALS Vial : 83 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK541

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc