

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032421\
 Data File : BP005035.D
 Acq On : 24 Mar 2021 14:00
 Operator : CG/JU
 Sample : M1557-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PT-ACIDS-WP

Quant Time: Mar 24 14:33:33 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 24 10:16:52 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.722	152	24454	20.00	ng	# 0.00
21) Naphthalene-d8	10.516	136	93049	20.00	ng	# 0.00
39) Acenaphthene-d10	14.375	164	62761	20.00	ng	0.00
64) Phenanthrene-d10	17.133	188	135043	20.00	ng	# 0.00
76) Chrysene-d12	21.227	240	139972	20.00	ng	0.00
86) Perylene-d12	23.515	264	138677	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.316	112	219574	138.18	ng	0.00
7) Phenol-d6	6.904	99	294028	129.18	ng	0.00
23) Nitrobenzene-d5	8.881	82	197015	90.85	ng	0.00
42) 2,4,6-Tribromophenol	15.874	330	113339	138.60	ng	0.00
45) 2-Fluorobiphenyl	12.992	172	407351	87.80	ng	0.00
79) Terphenyl-d14	19.710	244	692185	90.02	ng	0.00
Target Compounds						Qvalue
6) Aniline	6.928	93	6480	2.51	ng	# 1
8) 2-Chlorophenol	7.293	128	83753	49.97	ng	85
9) Benzaldehyde	6.934	77	3493	Below Cal		# 1
10) Phenol	6.928	94	264975	113.59	ng	79
15) Benzyl Alcohol	8.169	79	122048	69.50	ng	# 12
17) 2-Methylphenol	8.175	107	227790	153.01	ng	# 90
26) 2-Nitrophenol	9.634	139	136154	153.61	ng	# 63
27) 2,4-Dimethylphenol	9.698	122	88546	62.12	ng	# 84
28) bis(2-Chloroethoxy)met...	9.698	93	5162	2.55	ng	# 1
29) 2,4-Dichlorophenol	10.163	162	102434	64.23	ng	92
31) Naphthalene	10.698	128	14504	2.76	ng	# 83
32) Benzoic acid	9.698	122	88546	83.68	ng	# 26
36) 4-Chloro-3-methylphenol	11.810	107	150758	78.25	ng	# 81
43) 2,4,6-Trichlorophenol	12.798	196	51545	36.49	ng	100
44) 2,4,5-Trichlorophenol	12.869	196	112603	73.59	ng	# 93
52) Acenaphthene	14.498	154	49223	13.20	ng	# 4
53) 3-Nitroaniline	14.492	138	2206	2.10	ng	# 1
54) 2,4-Dinitrophenol	14.498	184	74801	108.42	ng	# 74
56) 4-Nitrophenol	14.604	139	118600	137.88	ng	# 41
59) 2,3,4,6-Tetrachlorophenol	15.010	232	3153	2.23	ng	# 95
63) Azobenzene	15.516	77	41118	7.61	ng	# 1
65) 4,6-Dinitro-2-methylph...	15.516	198	143383	145.49	ng	88
69) Atrazine	16.786	200	27622	19.16	ng	# 36
70) Pentachlorophenol	16.786	266	145359	125.12	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032421\
Data File : BP005035.D
Acq On : 24 Mar 2021 14:00
Operator : CG/JU
Sample : M1557-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PT-ACIDS-WP

Quant Time: Mar 24 14:33:33 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 24 10:16:52 2021
Response via : Initial Calibration




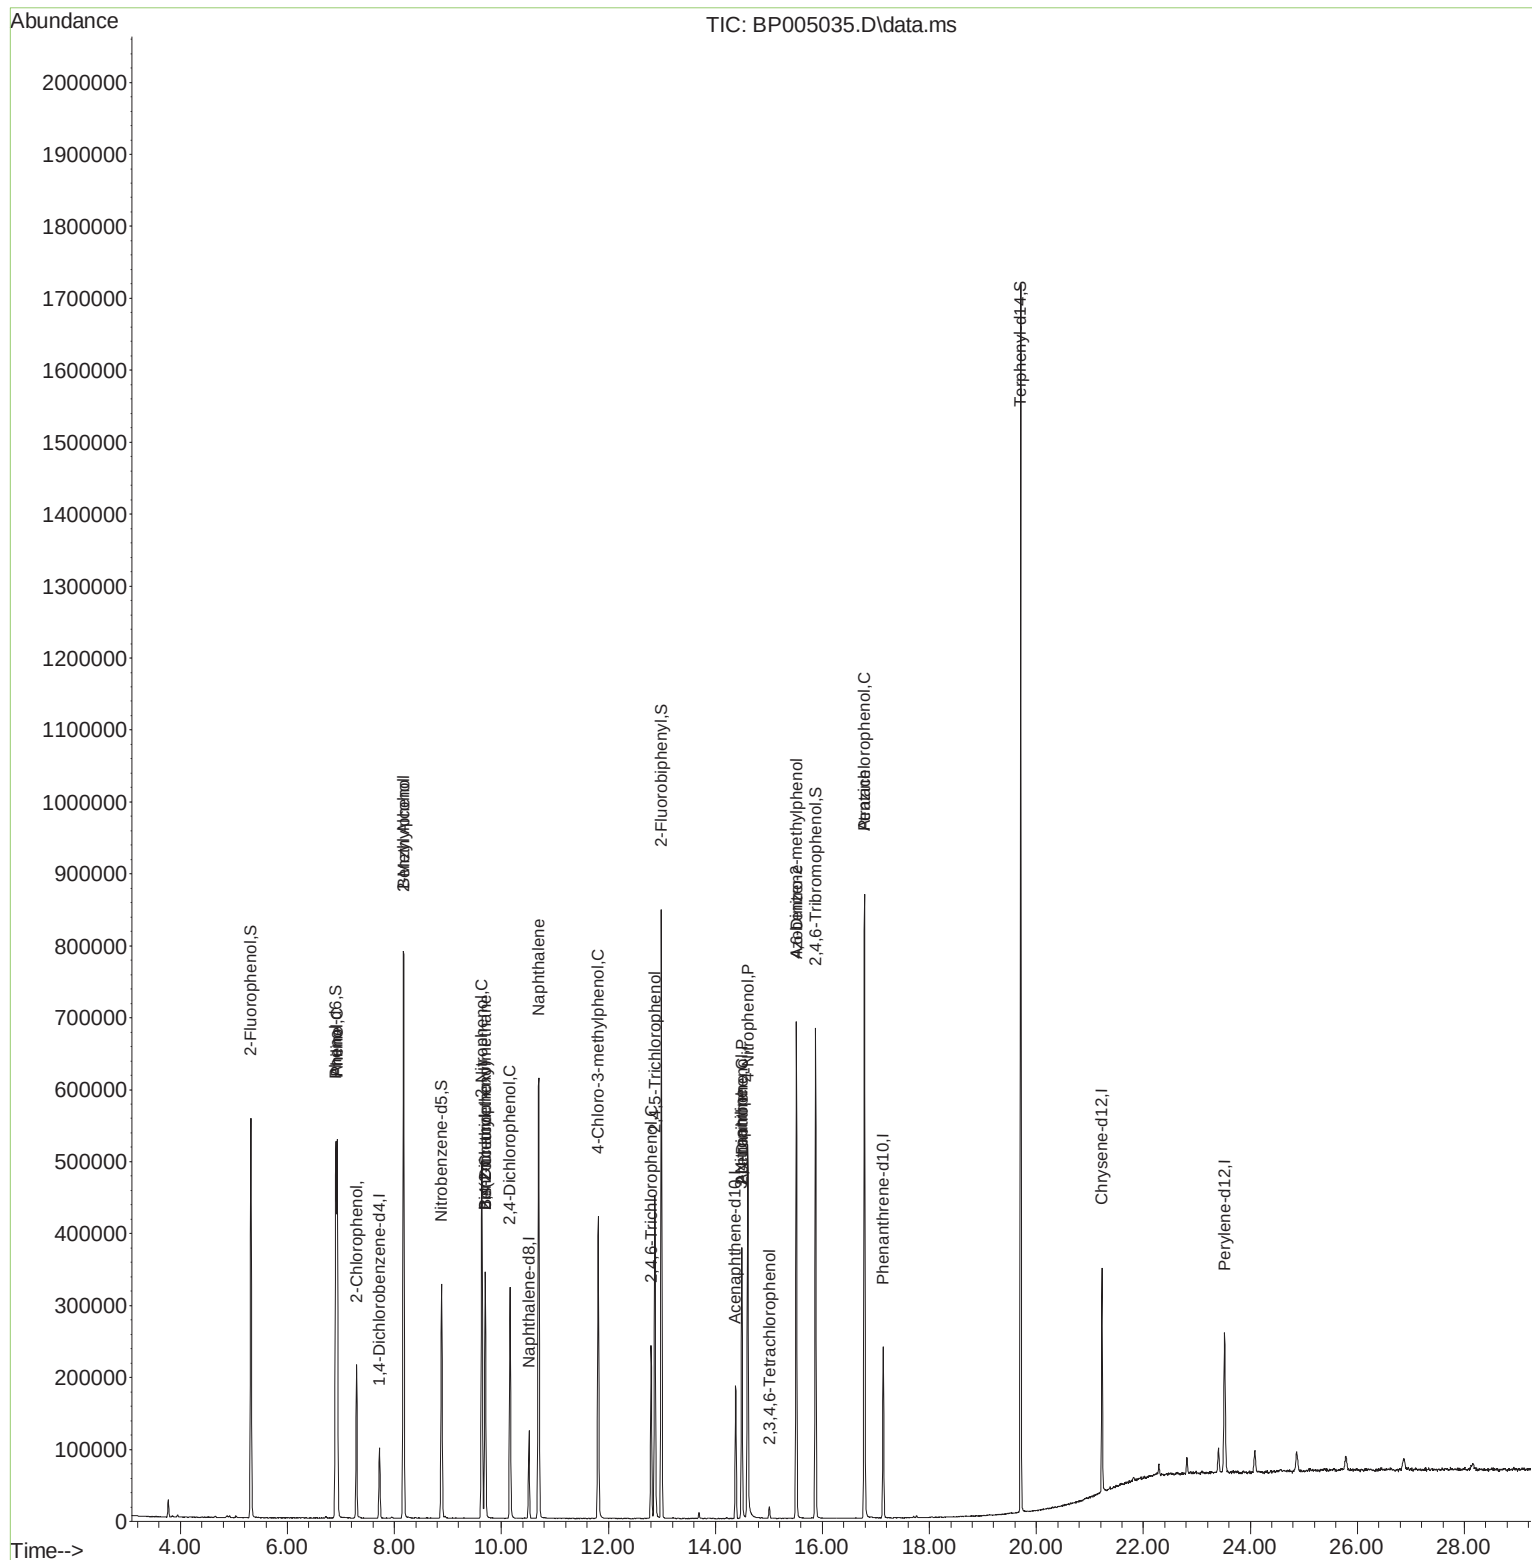


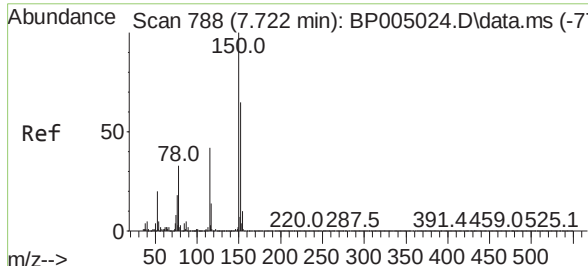

1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 7.722 min Scan# 788
 Delta R.T. -0.000 min
 Lab File: BP005035.D
 Acq: 24 Mar 2021 14:00




Instrument :
 BNA_P
 ClientSampleId :
 PT-ACIDS-WP


Tgt Ion:	152	Resp:	24454
Ion	Ratio	Lower	Upper
152	100		
150	158.8	123.8	185.6
115	66.9	43.8	65.6#

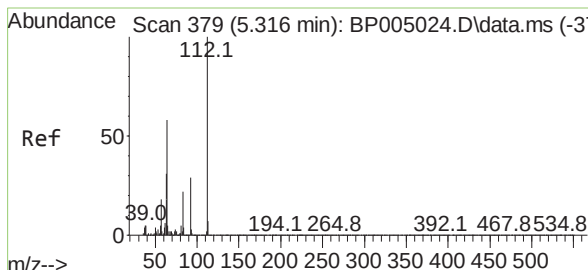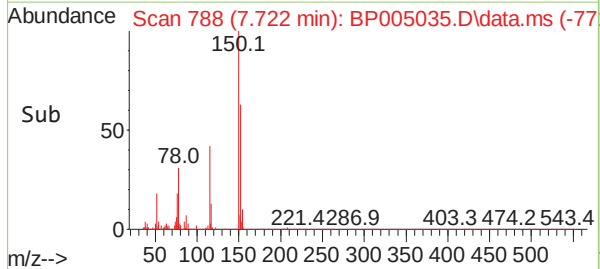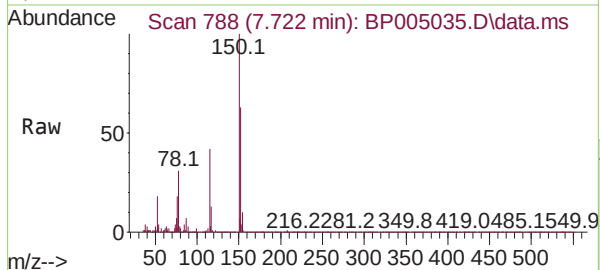

2-Fluorophenol
 Concen: 138.18 ng
 RT: 5.316 min Scan# 379
 Delta R.T. 0.005 min
 Lab File: BP005035.D
 Acq: 24 Mar 2021 14:00

Tgt Ion:	112	Resp:	219574
Ion	Ratio	Lower	Upper
112	100		
64	56.7	32.8	49.2#
63	33.9	17.0	25.4#







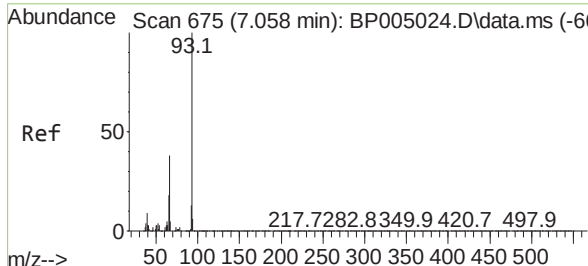

Aniline
 Concen: 2.51 ng
 RT: 6.928 min Scan# 653
 Delta R.T. -0.130 min
 Lab File: BP005035.D
 Acq: 24 Mar 2021 14:00




Instrument :
 BNA_P
 ClientSampleId :
 PT-ACIDS-WP


Tgt Ion:	93	Resp:	6480
Ion	Ratio	Lower	Upper
93	100		
66	1749.6	25.4	38.0#
65	1141.7	12.5	18.7#

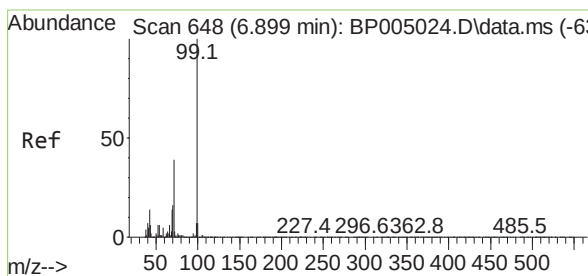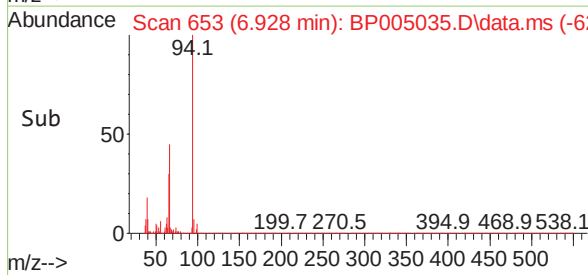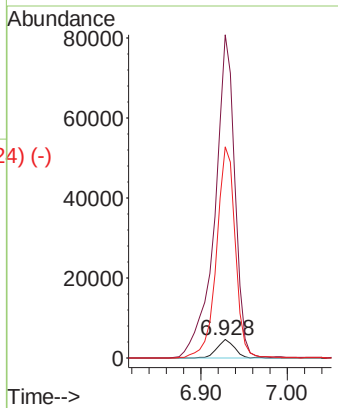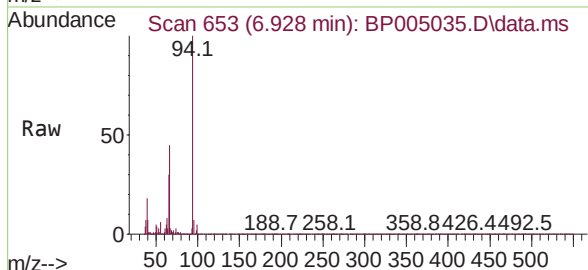

Phenol-d6
 Concen: 129.18 ng
 RT: 6.904 min Scan# 649
 Delta R.T. 0.005 min
 Lab File: BP005035.D
 Acq: 24 Mar 2021 14:00

Tgt Ion:	99	Resp:	294028
Ion	Ratio	Lower	Upper
99	100		
42	15.5	8.6	13.0#
71	39.5	23.4	35.2#


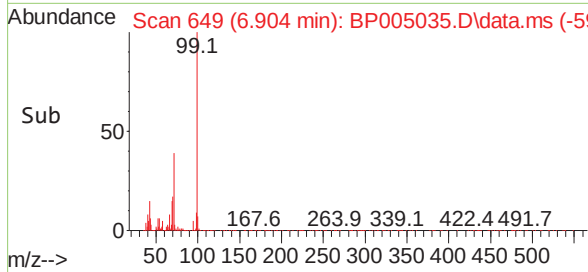
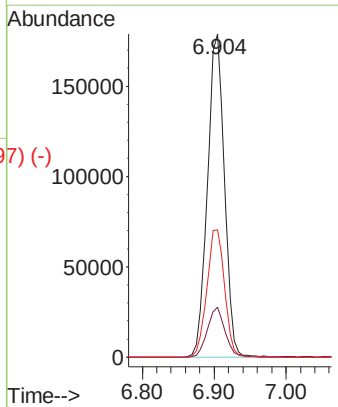



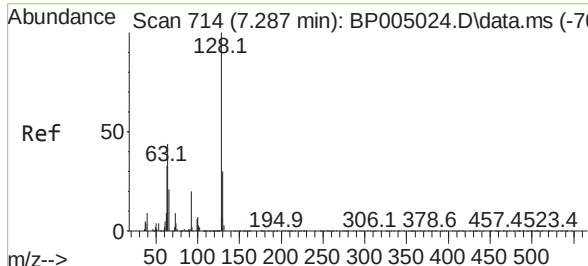

2-Chlorophenol
 Concen: 49.97 ng
 RT: 7.293 min Scan# 715
 Delta R.T. 0.005 min
 Lab File: BP005035.D
 Acq: 24 Mar 2021 14:00




Instrument :
 BNA_P
 ClientSampleId :
 PT-ACIDS-WP


Tgt Ion:	128	Resp:	83753
Ion	Ratio	Lower	Upper
128	100		
130	33.0	13.0	53.0
64	47.5	10.4	50.4

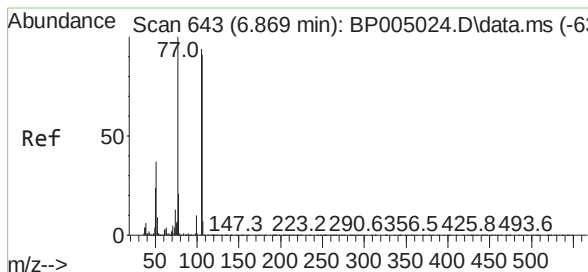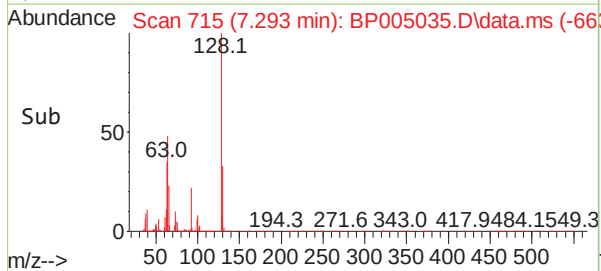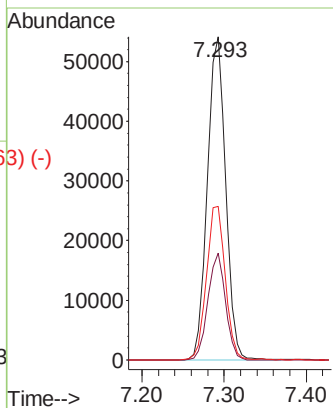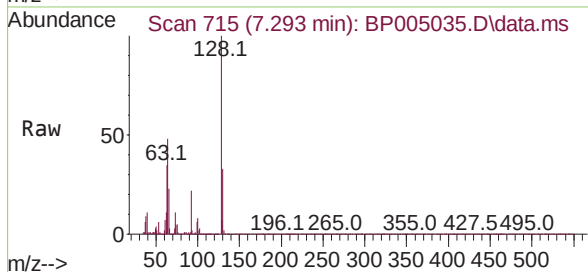

Benzaldehyde
 Concen: Below Cal
 RT: 6.934 min Scan# 654
 Delta R.T. 0.064 min
 Lab File: BP005035.D
 Acq: 24 Mar 2021 14:00

Tgt Ion:	77	Resp:	3493
Ion	Ratio	Lower	Upper
77	100		
105	1.1	97.1	137.1#
106	1.4	93.7	133.7#


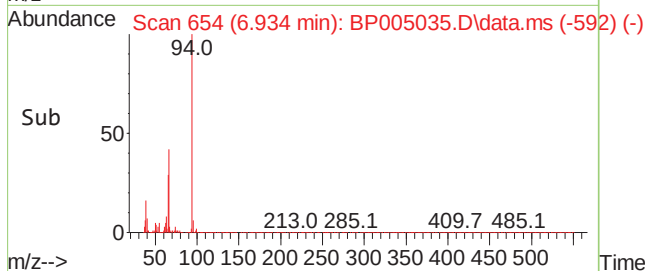




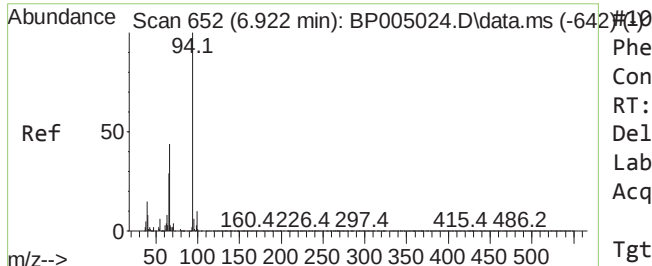

Phenol
 Concen: 113.59 ng
 RT: 6.928 min Scan# 653
 Delta R.T. 0.005 min
 Lab File: BP005035.D
 Acq: 24 Mar 2021 14:00




Instrument :
 BNA_P
 ClientSampleId :
 PT-ACIDS-WP


Tgt Ion:	94	Resp:	264975
Ion	Ratio	Lower	Upper
94	100		
65	29.5	2.3	42.3
66	45.2	10.9	50.9

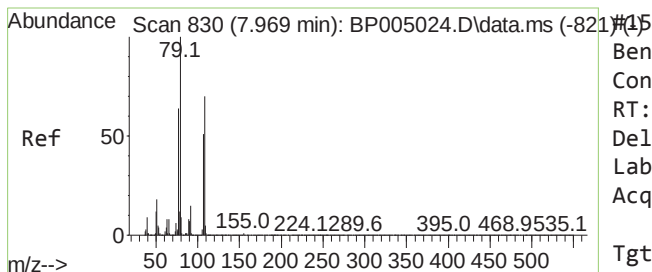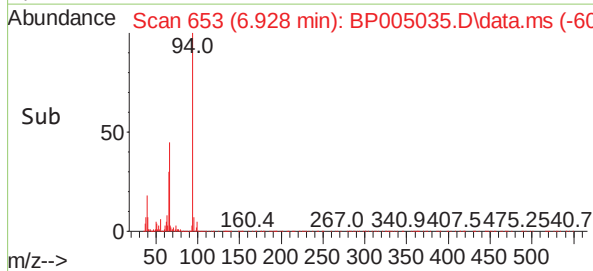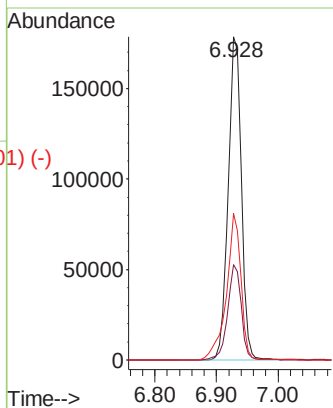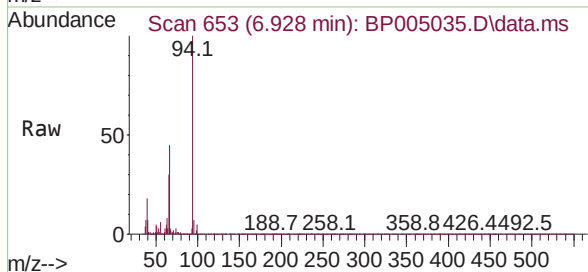

Benzyl Alcohol
 Concen: 69.50 ng
 RT: 8.169 min Scan# 864
 Delta R.T. 0.205 min
 Lab File: BP005035.D
 Acq: 24 Mar 2021 14:00

Tgt Ion:	79	Resp:	122048
Ion	Ratio	Lower	Upper
79	100		
108	199.4	73.5	110.3#
77	103.1	50.3	75.5#


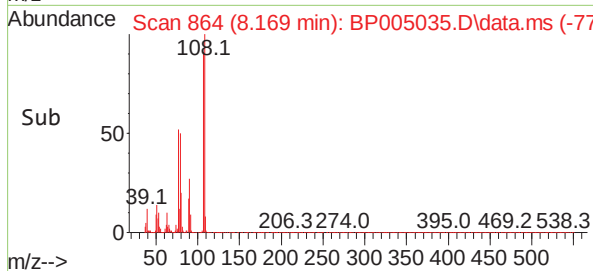




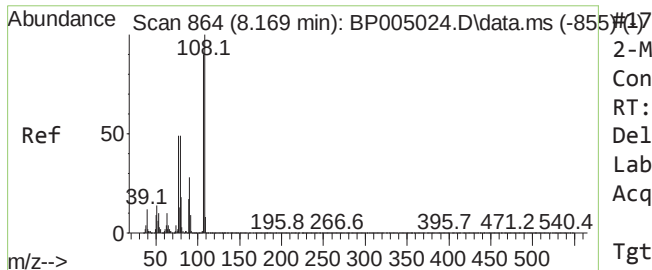

2-Methylphenol
 Concen: 153.01 ng
 RT: 8.175 min Scan# 865
 Delta R.T. 0.005 min
 Lab File: BP005035.D
 Acq: 24 Mar 2021 14:00




Instrument :
 BNA_P
 ClientSampleId :
 PT-ACIDS-WP


Tgt Ion:	107	Resp:	227790
Ion	Ratio	Lower	Upper
107	100		
108	113.5	89.6	134.4
77	52.9	31.8	47.6#
79	53.2	31.1	46.7#

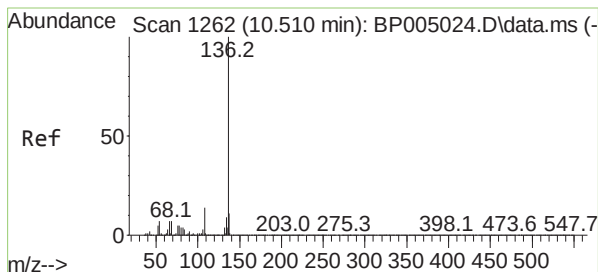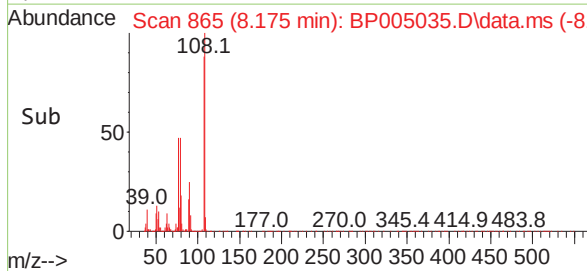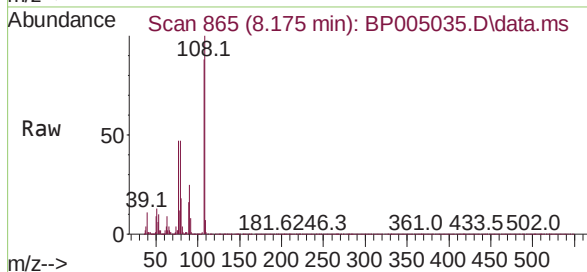

Naphthalene-d8
 Concen: 20.00 ng
 RT: 10.516 min Scan# 1263
 Delta R.T. 0.005 min
 Lab File: BP005035.D
 Acq: 24 Mar 2021 14:00

Tgt Ion:	136	Resp:	93049
Ion	Ratio	Lower	Upper
136	100		
137	10.7	8.6	13.0
54	5.1	3.6	5.4
68	6.6	3.3	4.9#


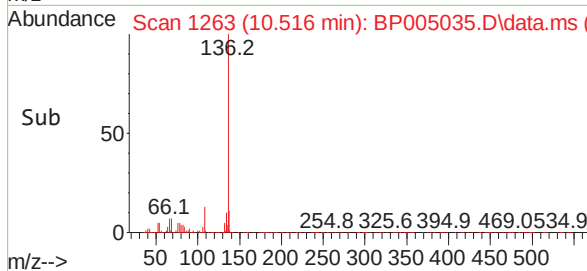
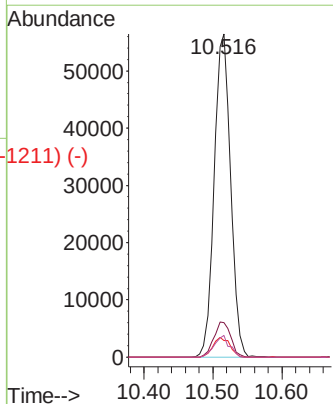
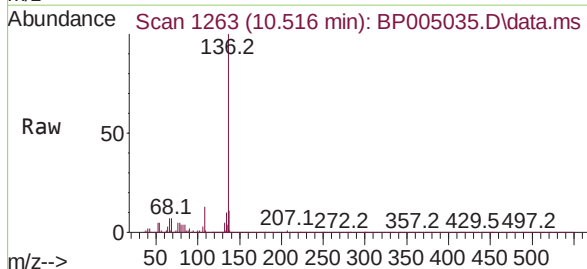


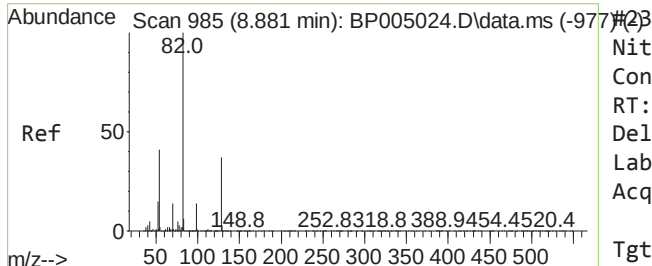

Nitrobenzene-d5
 Concen: 90.85 ng
 RT: 8.881 min Scan# 985
 Delta R.T. -0.000 min
 Lab File: BP005035.D
 Acq: 24 Mar 2021 14:00




Instrument :
 BNA_P
 ClientSampleId :
 PT-ACIDS-WP

Tgt Ion:	82	Resp:	197015
Ion	Ratio	Lower	Upper
82	100		
128	36.2	45.6	68.4#
54	40.1	30.1	45.1

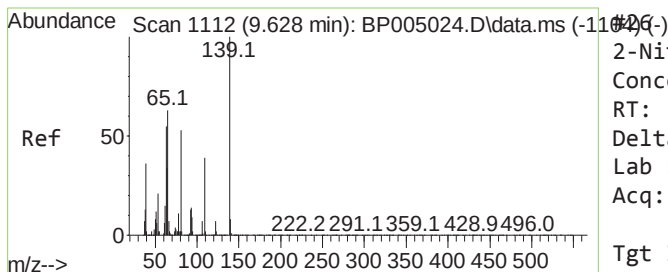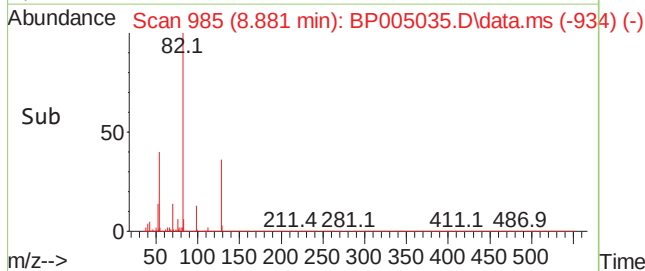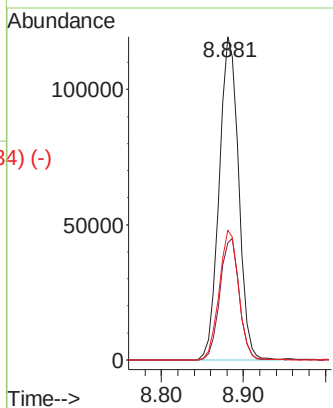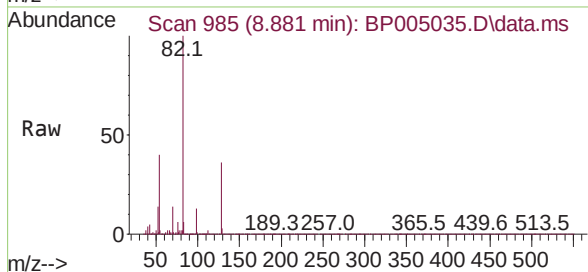


2-Nitrophenol
 Concen: 153.61 ng
 RT: 9.634 min Scan# 1113
 Delta R.T. 0.005 min
 Lab File: BP005035.D
 Acq: 24 Mar 2021 14:00

Tgt Ion:	139	Resp:	136154
Ion	Ratio	Lower	Upper
139	100		
109	41.1	22.1	33.1#
65	59.6	26.5	39.7#

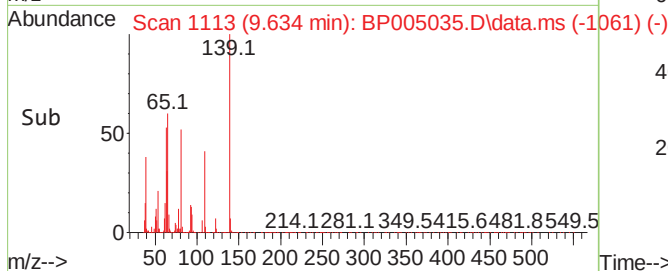



Abundance Scan 1123 (9.693 min): BP005024.D\data.ms (-1127-)




2,4-Dimethylphenol
Concen: 62.12 ng
RT: 9.698 min Scan# 1124
Delta R.T. 0.005 min
Lab File: BP005035.D
Acq: 24 Mar 2021 14:00

Instrument :
BNA_P
ClientSampleId :
PT-ACIDS-WP


Tgt Ion:	122	Resp:	88546
Ion	Ratio	Lower	Upper
122	100		
107	132.1	87.3	130.9#
121	63.3	47.3	70.9

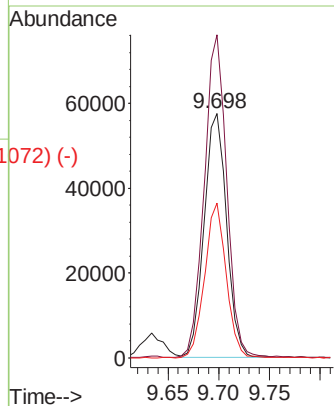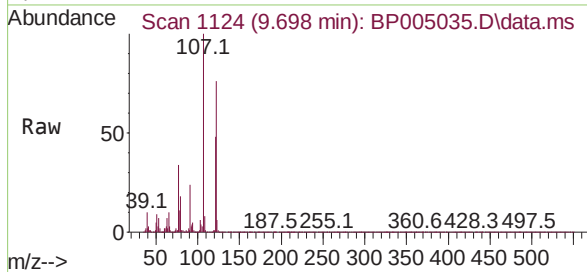

Abundance Scan 1124 (9.698 min): BP005035.D\data.ms (-1072-)





Abundance Scan 1164 (9.934 min): BP005024.D\data.ms (-1128-)





bis(2-Chloroethoxy)methane
Concen: 2.55 ng
RT: 9.698 min Scan# 1124
Delta R.T. -0.236 min
Lab File: BP005035.D
Acq: 24 Mar 2021 14:00

Tgt Ion:	93	Resp:	5162
Ion	Ratio	Lower	Upper
93	100		
95	19.1	26.7	40.1#
123	145.1	10.5	15.7#

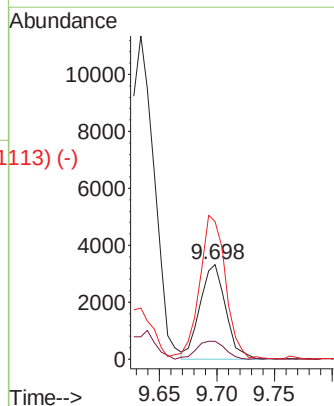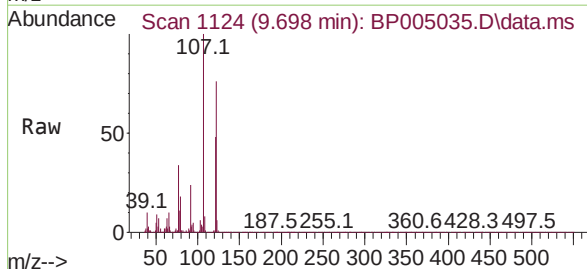

Abundance Scan 1124 (9.698 min): BP005035.D\data.ms (-1113-)




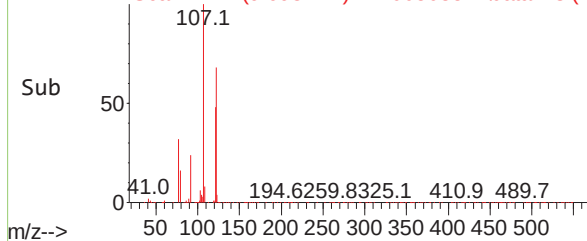


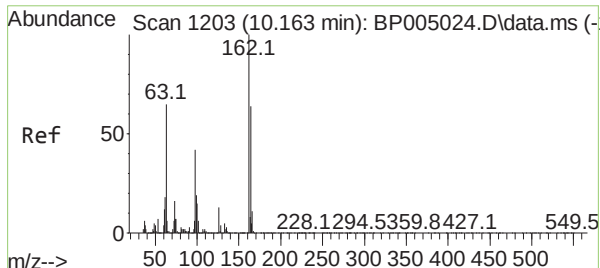

2,4-Dichlorophenol
Concen: 64.23 ng
RT: 10.163 min Scan# 1203
Delta R.T. -0.000 min
Lab File: BP005035.D
Acq: 24 Mar 2021 14:00




Instrument :
BNA_P
ClientSampleId :
PT-ACIDS-WP

Tgt Ion:	162	Resp:	102434
Ion	Ratio	Lower	Upper
162	100		
164	67.3	45.8	85.8
98	41.6	10.2	50.2

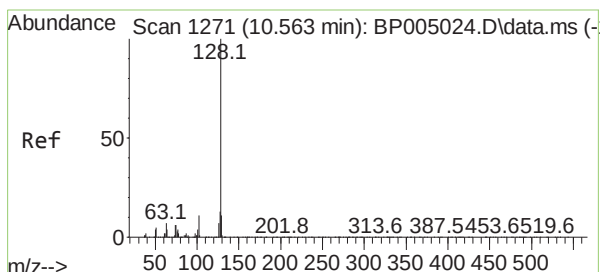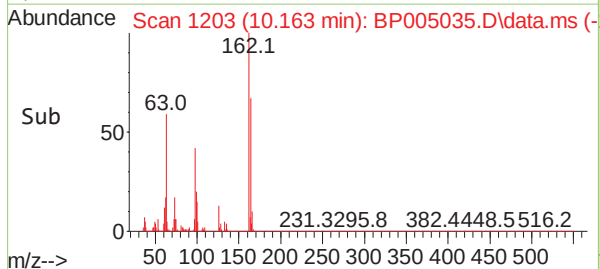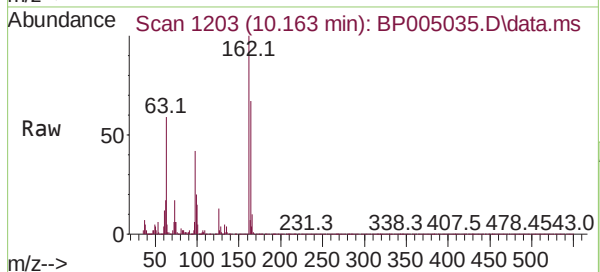


Naphthalene
Concen: 2.76 ng
RT: 10.698 min Scan# 1294
Delta R.T. 0.135 min
Lab File: BP005035.D
Acq: 24 Mar 2021 14:00

Tgt Ion:	128	Resp:	14504
Ion	Ratio	Lower	Upper
128	100		
129	7.1	8.8	13.2#
127	22.2	10.6	15.8#

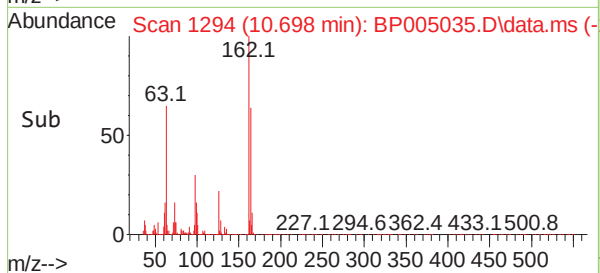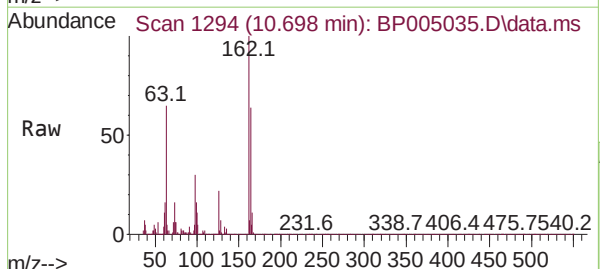




Abundance Scan 1147 (9.834 min): BP005024.D\data.ms (-11302-)




Benzoic acid
Concen: 83.68 ng
RT: 9.698 min Scan# 1124
Delta R.T. -0.136 min
Lab File: BP005035.D
Acq: 24 Mar 2021 14:00

Instrument :
BNA_P
ClientSampleId :
PT-ACIDS-WP

Tgt Ion:122 Resp: 88546
Ion Ratio Lower Upper
122 100
105 4.4 94.1 134.1#
77 45.3 50.1 90.1#

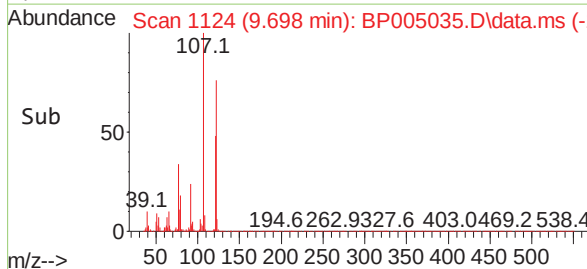
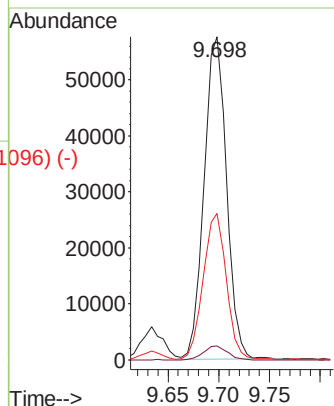
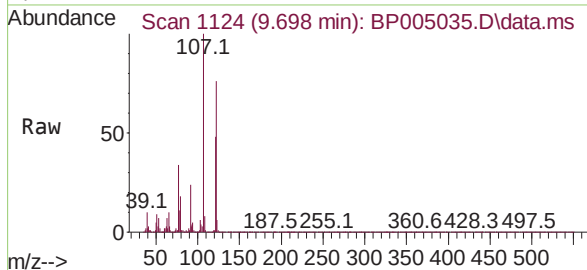


Abundance Scan 1483 (11.810 min): BP005024.D\data.ms (-1426-)




4-Chloro-3-methylphenol
Concen: 78.25 ng
RT: 11.810 min Scan# 1483
Delta R.T. -0.000 min
Lab File: BP005035.D
Acq: 24 Mar 2021 14:00

Tgt Ion:107 Resp: 150758
Ion Ratio Lower Upper
107 100
144 21.6 22.7 34.1#
142 69.0 70.7 106.1#

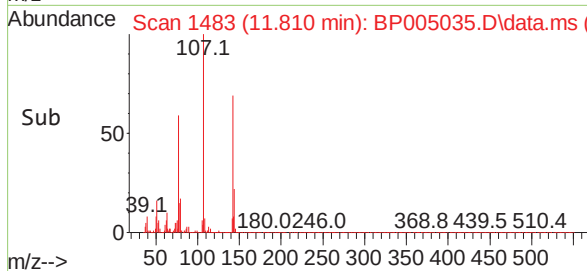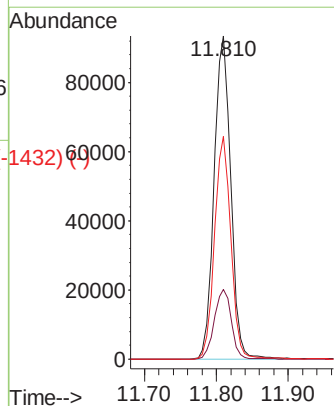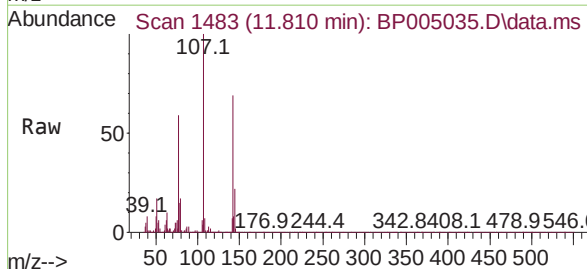



Abundance Scan 1919 (14.375 min): BP005024.D\data.ms (-1868) (-)

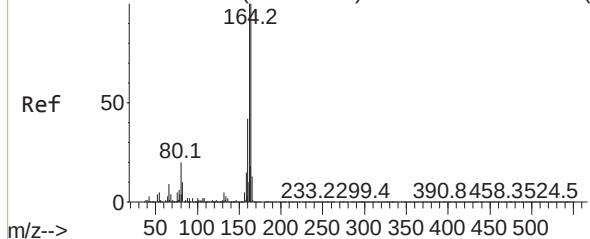


Acenaphthene-d10
Concen: 20.00 ng
RT: 14.375 min Scan# 1919
Delta R.T. -0.000 min
Lab File: BP005035.D
Acq: 24 Mar 2021 14:00

Instrument :
BNA_P
ClientSampleId :
PT-ACIDS-WP


Tgt Ion:164 Resp: 62761
Ion Ratio Lower Upper
164 100
162 100.5 79.4 119.2
160 43.5 36.1 54.1

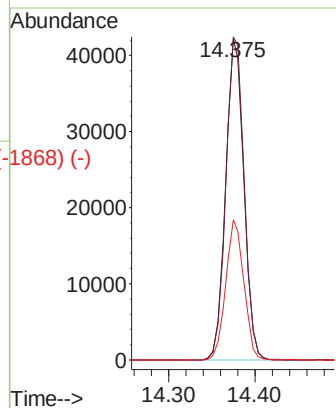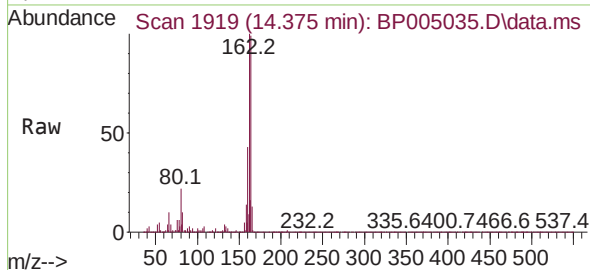

Abundance Scan 1919 (14.375 min): BP005035.D\data.ms (-1868) (-)


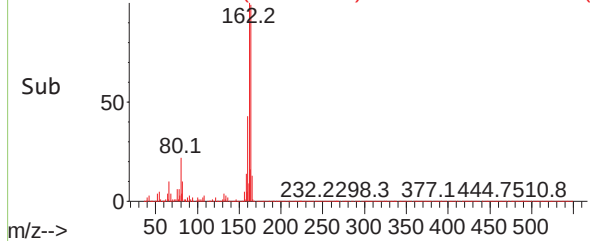


Abundance Scan 2174 (15.875 min): BP005024.D\data.ms (-2122) (-)

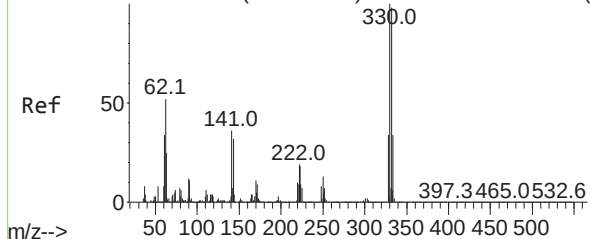



2,4,6-Tribromophenol
Concen: 138.60 ng
RT: 15.874 min Scan# 2174
Delta R.T. 0.005 min
Lab File: BP005035.D
Acq: 24 Mar 2021 14:00

Tgt Ion:330 Resp: 113339
Ion Ratio Lower Upper
330 100
332 96.3 77.1 115.7
141 34.9 23.4 35.2

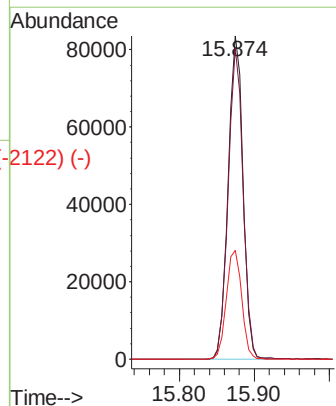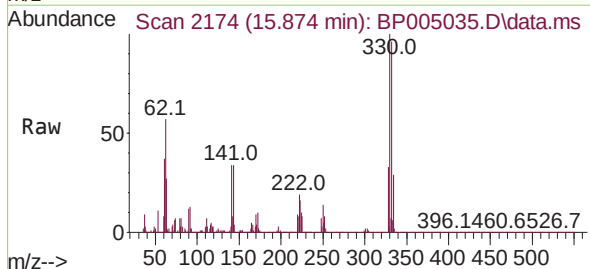

Abundance Scan 2174 (15.874 min): BP005035.D\data.ms (-2122) (-)




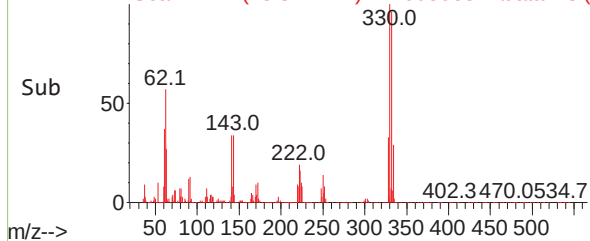


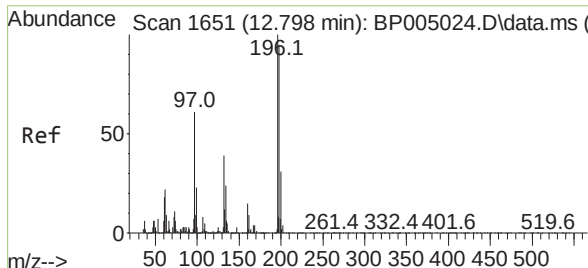

Scan 1651 (12.798 min): BP005024.D\data.ms (-1643) (-)
 2,4,6-Trichlorophenol
 Concen: 36.49 ng
 RT: 12.798 min Scan# 1651
 Delta R.T. -0.000 min
 Lab File: BP005035.D
 Acq: 24 Mar 2021 14:00




Instrument :
 BNA_P
 ClientSampleId :
 PT-ACIDS-WP

Tgt Ion:	196	Resp:	51545
Ion	Ratio	Lower	Upper
196	100		
198	96.1	77.0	115.6
200	31.4	25.1	37.7

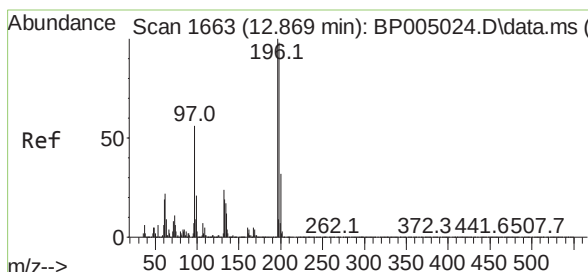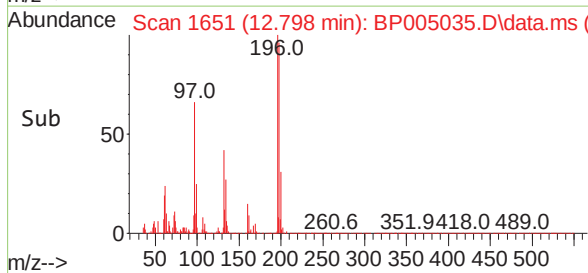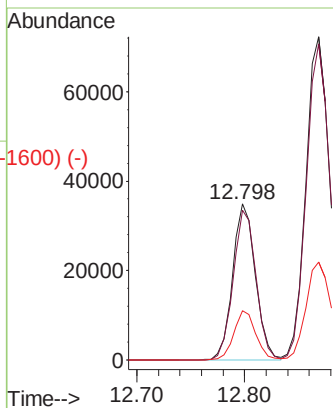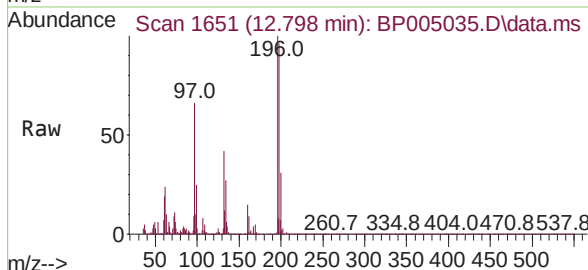


Scan 1663 (12.869 min): BP005024.D\data.ms (-1647) (-)
 2,4,5-Trichlorophenol
 Concen: 73.59 ng
 RT: 12.869 min Scan# 1663
 Delta R.T. -0.000 min
 Lab File: BP005035.D
 Acq: 24 Mar 2021 14:00

Tgt Ion:	196	Resp:	112603
Ion	Ratio	Lower	Upper
196	100		
198	97.9	77.3	115.9
97	53.5	31.0	46.4#
132	25.7	20.9	31.3

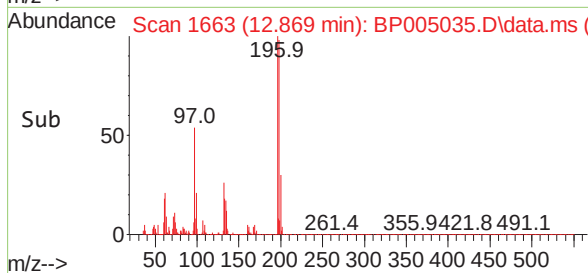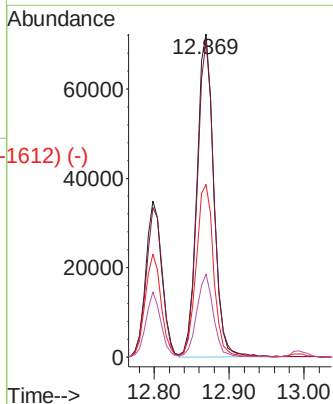




Abundance Scan 1684 (12.993 min): BP005024.D\data.ms (-1675) (-)

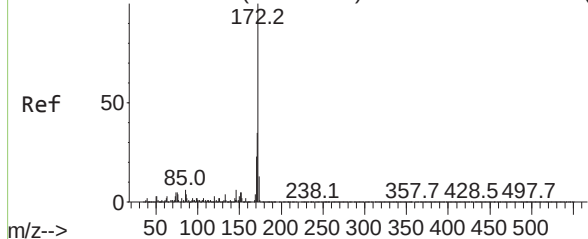


2-Fluorobiphenyl
Concen: 87.80 ng
RT: 12.992 min Scan# 1684
Delta R.T. -0.000 min
Lab File: BP005035.D
Acq: 24 Mar 2021 14:00

Instrument :
BNA_P
ClientSampleId :
PT-ACIDS-WP

Tgt Ion:	172	Resp:	407351
Ion	Ratio	Lower	Upper
172	100		
171	34.5	28.5	42.7
170	21.8	19.2	28.8

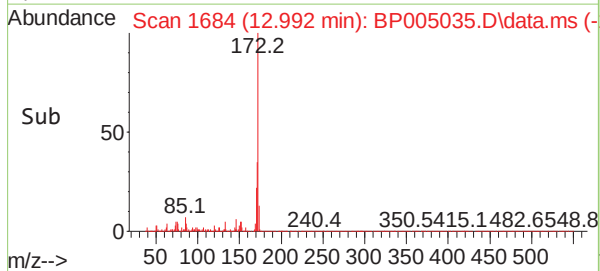
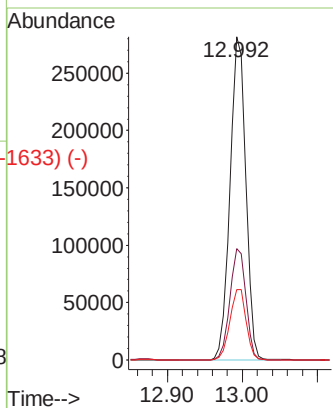
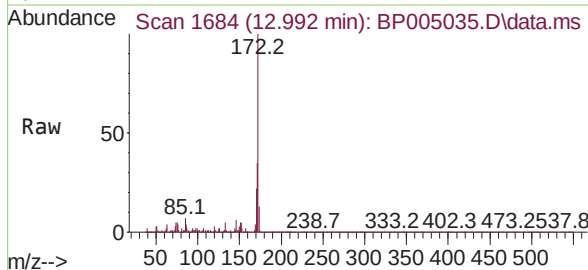


Abundance Scan 1930 (14.439 min): BP005024.D\data.ms (-1529) (-)

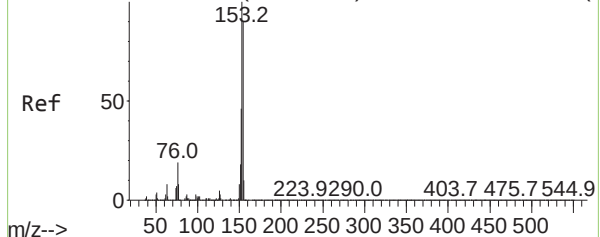

Acenaphthene
Concen: 13.20 ng
RT: 14.498 min Scan# 1940
Delta R.T. 0.058 min
Lab File: BP005035.D
Acq: 24 Mar 2021 14:00


Tgt Ion:	154	Resp:	49223
Ion	Ratio	Lower	Upper
154	100		
153	0.0	91.0	136.6#
152	0.5	43.0	64.6#

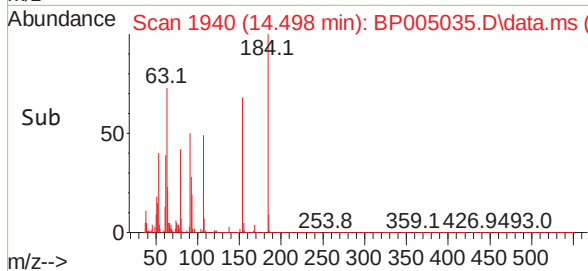



Abundance Scan 1904 (14.287 min): BP005024.D\data.ms (-1853) (-)

3-Nitroaniline
Concen: 2.10 ng
RT: 14.492 min Scan# 1939
Delta R.T. 0.205 min
Lab File: BP005035.D
Acq: 24 Mar 2021 14:00


Instrument :
BNA_P
ClientSampled :
PT-ACIDS-WP

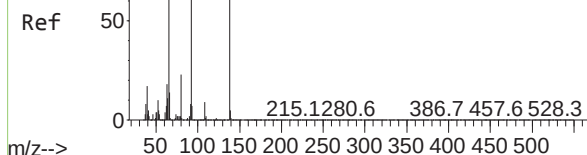

Tgt Ion:	138	Resp:	2206
Ion	Ratio	Lower	Upper
138	100		
108	200.3	7.5	11.3#
92	812.9	75.0	112.6#

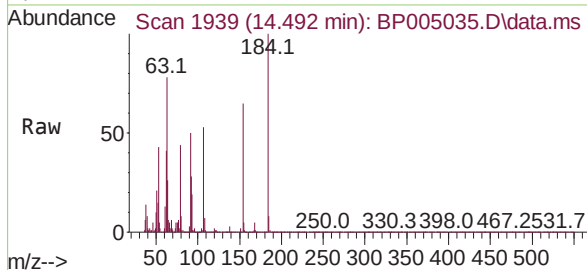


Abundance Scan 1939 (14.492 min): BP005035.D\data.ms (-1853) (-)





Abundance Scan 1939 (14.492 min): BP005024.D\data.ms (-1851) (-)


2,4-Dinitrophenol
Concen: 108.42 ng
RT: 14.498 min Scan# 1940
Delta R.T. 0.005 min
Lab File: BP005035.D
Acq: 24 Mar 2021 14:00




Tgt Ion:	184	Resp:	74801
Ion	Ratio	Lower	Upper
184	100		
63	73.1	32.3	48.5#
154	68.2	49.1	73.7

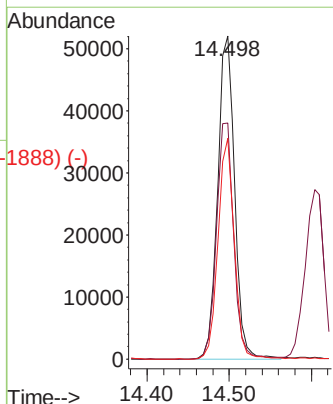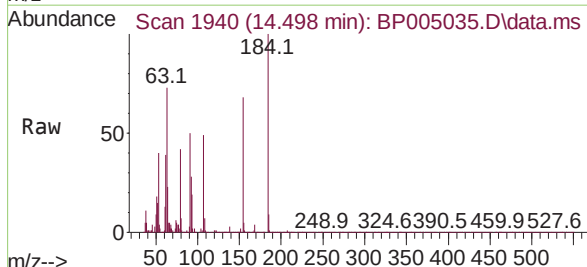

Abundance Scan 1940 (14.498 min): BP005035.D\data.ms (-1888) (-)







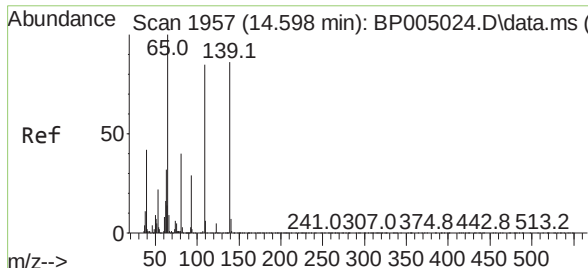

4-Nitrophenol
Concen: 137.88 ng
RT: 14.604 min Scan# 1958
Delta R.T. 0.005 min
Lab File: BP005035.D
Acq: 24 Mar 2021 14:00




Instrument :
BNA_P
ClientSampleId :
PT-ACIDS-WP

Tgt Ion:	139	Resp:	118600
Ion	Ratio	Lower	Upper
139	100		
109	101.2	44.6	84.6#
65	117.3	41.6	81.6#

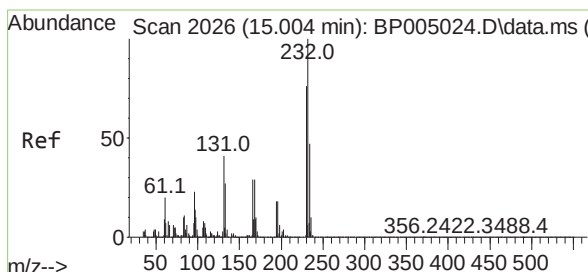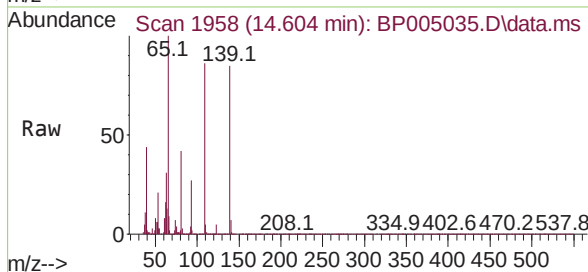


2,3,4,6-Tetrachlorophenol
Concen: 2.23 ng
RT: 15.010 min Scan# 2027
Delta R.T. 0.006 min
Lab File: BP005035.D
Acq: 24 Mar 2021 14:00

Tgt Ion:	232	Resp:	3153
Ion	Ratio	Lower	Upper
232	100		
131	46.3	34.1	51.1
130	1.8	1.8	2.8#
166	32.5	24.6	36.8

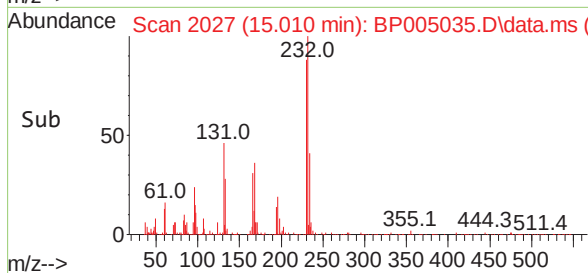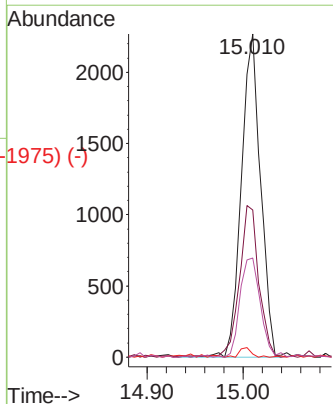




Abundance Scan 2148 (15.722 min): BP005024.D\data.ms (-2361) (-)

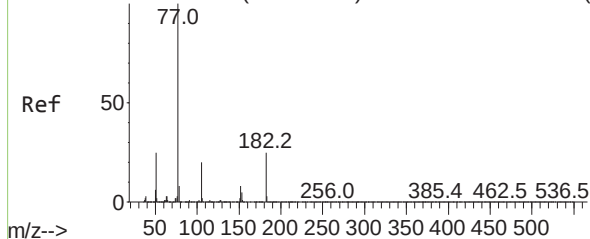


Azobenzene
Concen: 7.61 ng
RT: 15.516 min Scan# 2113
Delta R.T. -0.206 min
Lab File: BP005035.D
Acq: 24 Mar 2021 14:00

Instrument :
BNA_P
ClientSampleId :
PT-ACIDS-WP

Tgt Ion: 77 Resp: 41118
Ion Ratio Lower Upper
77 100
182 9.3 16.9 56.9#
105 147.0 5.6 45.6#
51 125.1 2.9 42.9#

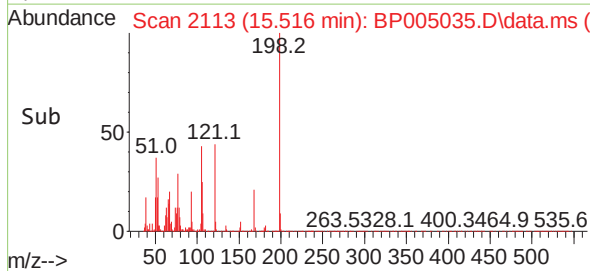

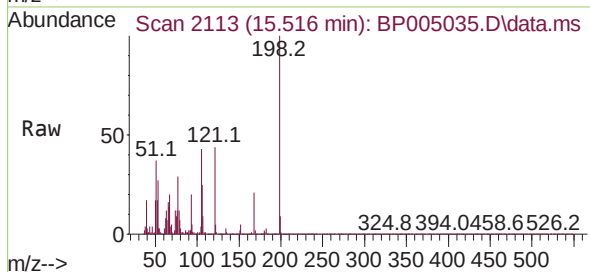


Abundance Scan 2388 (17.133 min): BP005024.D\data.ms (-2358) (-)

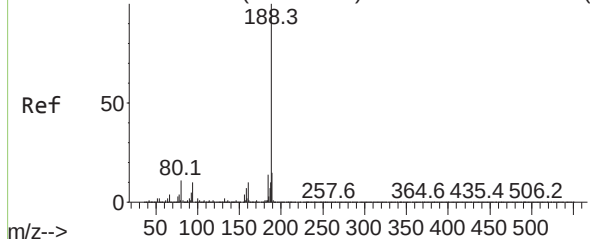


Phenanthrene-d10
Concen: 20.00 ng
RT: 17.133 min Scan# 2388
Delta R.T. -0.000 min
Lab File: BP005035.D
Acq: 24 Mar 2021 14:00

Tgt Ion:188 Resp: 135043
Ion Ratio Lower Upper
188 100
94 8.1 6.2 9.2
80 10.7 6.2 9.2#

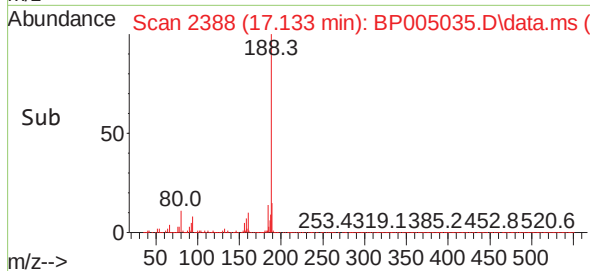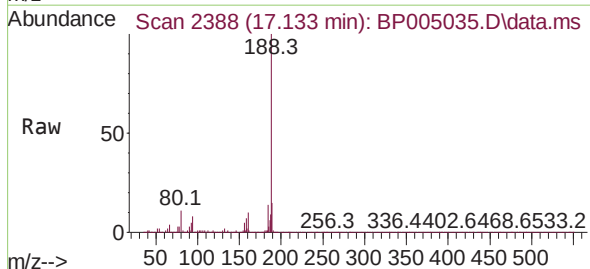

Abundance Scan 2112 (15.510 min): BP005024.D\data.ms (-2165) (-)





4,6-Dinitro-2-methylphenol
Concen: 145.49 ng
RT: 15.516 min Scan# 2113
Delta R.T. 0.005 min
Lab File: BP005035.D
Acq: 24 Mar 2021 14:00


Instrument :
BNA_P
ClientSampleId :
PT-ACIDS-WP

Tgt Ion:	198	Resp:	143383
Ion	Ratio	Lower	Upper
198	100		
51	36.6	6.4	46.4
105	43.0	18.9	58.9


Abundance Scan 2113 (15.516 min): BP005035.D\data.ms

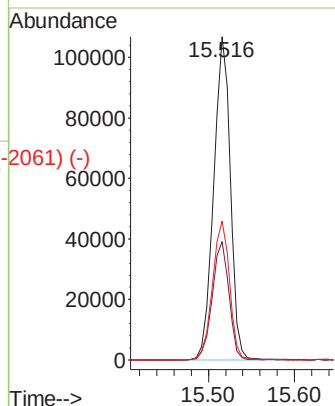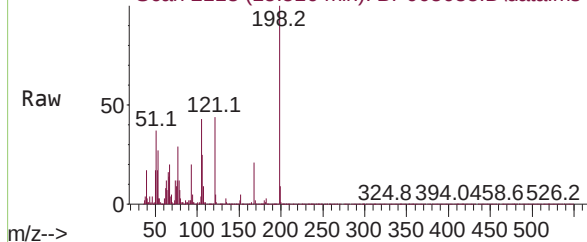

Abundance Scan 2113 (15.516 min): BP005035.D\data.ms (-2061) (-)





Abundance Scan 2298 (16.604 min): BP005024.D\data.ms (-2165) (-)




Atrazine
Concen: 19.16 ng
RT: 16.786 min Scan# 2329
Delta R.T. 0.182 min
Lab File: BP005035.D
Acq: 24 Mar 2021 14:00

Tgt Ion:	200	Resp:	27622
Ion	Ratio	Lower	Upper
200	100		
173	0.0	5.9	45.9#
215	0.1	28.4	68.4#


Abundance Scan 2329 (16.786 min): BP005035.D\data.ms

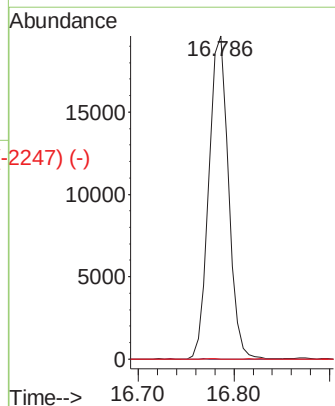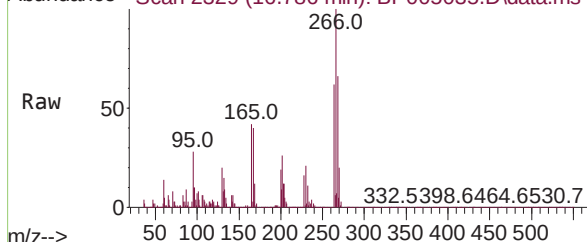

Abundance Scan 2329 (16.786 min): BP005035.D\data.ms (-2247) (-)

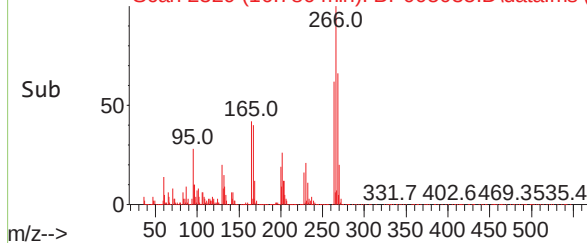

Abundance Scan 2328 (16.781 min): BP005024.D\data.ms (-2319) (-)





Pentachlorophenol
Concen: 125.12 ng
RT: 16.786 min Scan# 2329
Delta R.T. 0.006 min
Lab File: BP005035.D
Acq: 24 Mar 2021 14:00


Tgt Ion:	266	Resp:	145359
Ion	Ratio	Lower	Upper
266	100		
268	65.9	51.1	76.7
264	62.2	50.6	76.0

Instrument :
BNA_P
ClientSampleId :
PT-ACIDS-WP


Abundance Scan 2329 (16.786 min): BP005035.D\data.ms

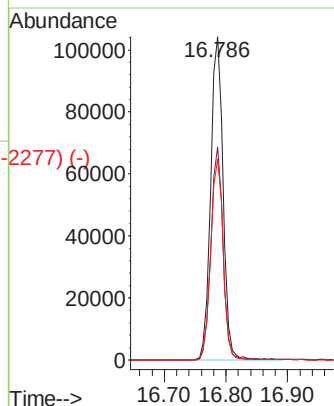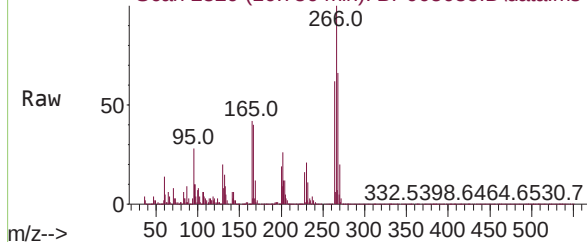

Abundance Scan 2329 (16.786 min): BP005035.D\data.ms (-2277) (-)

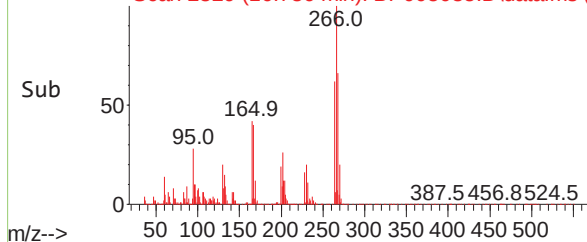



Abundance Scan 3084 (21.227 min): BP005024.D\data.ms (-3075) (-)

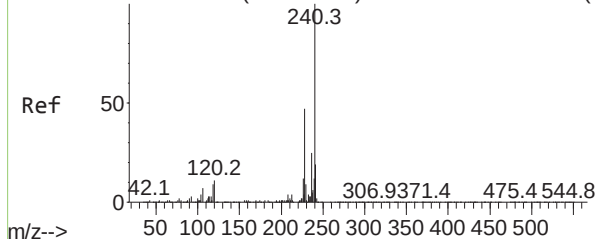


Chrysene-d12
Concen: 20.00 ng
RT: 21.227 min Scan# 3084
Delta R.T. -0.000 min
Lab File: BP005035.D
Acq: 24 Mar 2021 14:00

Tgt Ion:	240	Resp:	139972
Ion	Ratio	Lower	Upper
240	100		
120	9.1	7.8	11.6
236	24.5	20.8	31.2


Abundance Scan 3084 (21.227 min): BP005035.D\data.ms

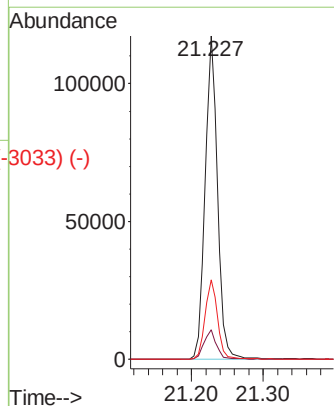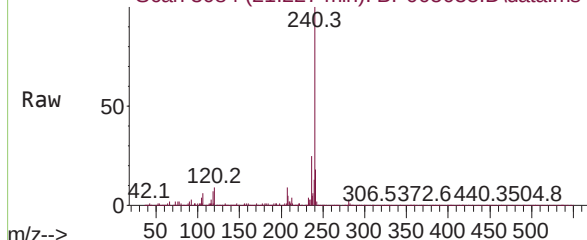

Abundance Scan 3084 (21.227 min): BP005035.D\data.ms (-3033) (-)

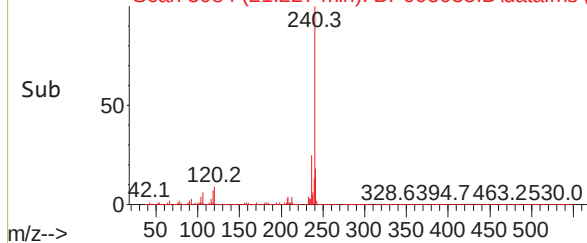




Abundance Scan 2825 (19.704 min): BP005024.D\data.ms (-2819) (-)




Terphenyl-d14
Concen: 90.02 ng
RT: 19.710 min Scan# 2826
Delta R.T. 0.006 min
Lab File: BP005035.D
Acq: 24 Mar 2021 14:00

Instrument :
BNA_P
ClientSampleId :
PT-ACIDS-WP

Tgt Ion:	244	Resp:	692185
Ion	Ratio	Lower	Upper
244	100		
212	6.9	5.8	8.6
122	9.4	7.8	11.8

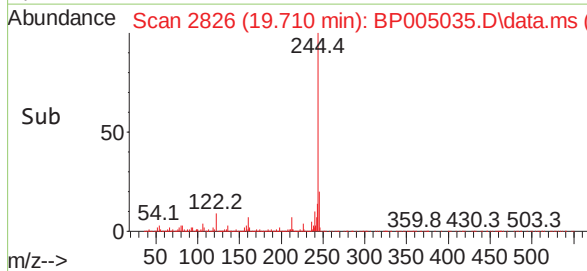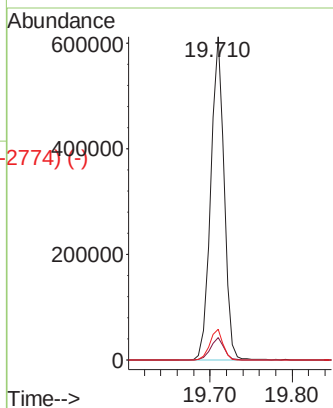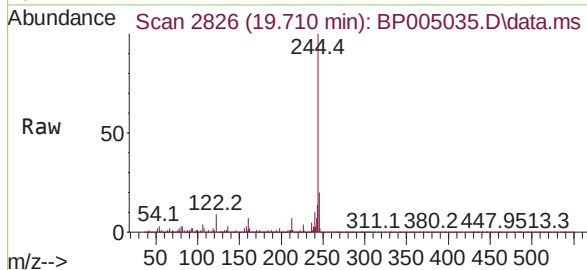

Abundance Scan 3473 (23.515 min): BP005024.D\data.ms (-3485) (-)



Perylene-d12
Concen: 20.00 ng
RT: 23.515 min Scan# 3473
Delta R.T. 0.006 min
Lab File: BP005035.D
Acq: 24 Mar 2021 14:00

Tgt Ion:	264	Resp:	138677
Ion	Ratio	Lower	Upper
264	100		
260	24.5	18.8	28.2
265	21.9	17.4	26.2

