

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032421\
 Data File : BP005032.D
 Acq On : 24 Mar 2021 09:53
 Operator : CG/JU
 Sample : PB135047BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB135047BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP005032.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.317	373	379	392	rBV	671746	928699	41.64%	10.281%
2	6.899	641	648	662	rBV	608871	938273	42.07%	10.387%
3	7.722	780	788	796	rBV	118388	183630	8.23%	2.033%
4	8.881	977	985	996	rBV	359498	592913	26.58%	6.564%
5	10.510	1255	1262	1271	rBV	136887	236491	10.60%	2.618%
6	12.993	1676	1684	1694	rBV	898370	1325785	59.44%	14.677%
7	14.375	1913	1919	1931	rBV	214111	315282	14.14%	3.490%
8	15.869	2166	2173	2189	rBV	734379	1027399	46.07%	11.374%
9	17.134	2378	2388	2398	rBV	281881	402724	18.06%	4.458%
10	19.704	2819	2825	2835	rBV	1920411	2230273	100.00%	24.691%
11	21.228	3079	3084	3091	rBV	346954	438603	19.67%	4.856%
12	23.510	3466	3472	3480	rVB2	213674	412760	18.51%	4.570%




Sum of corrected areas: 9032832

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032421\
Data File : BP005032.D
Acq On : 24 Mar 2021 09:53
Operator : CG/JU
Sample : PB135047BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB135047BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

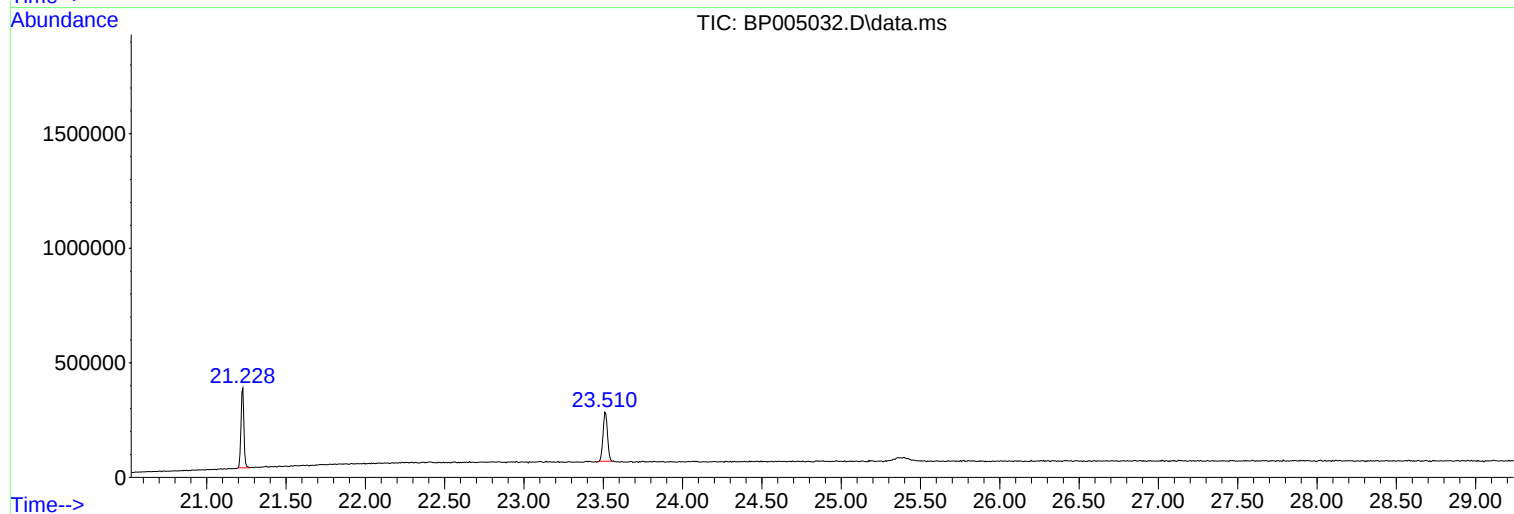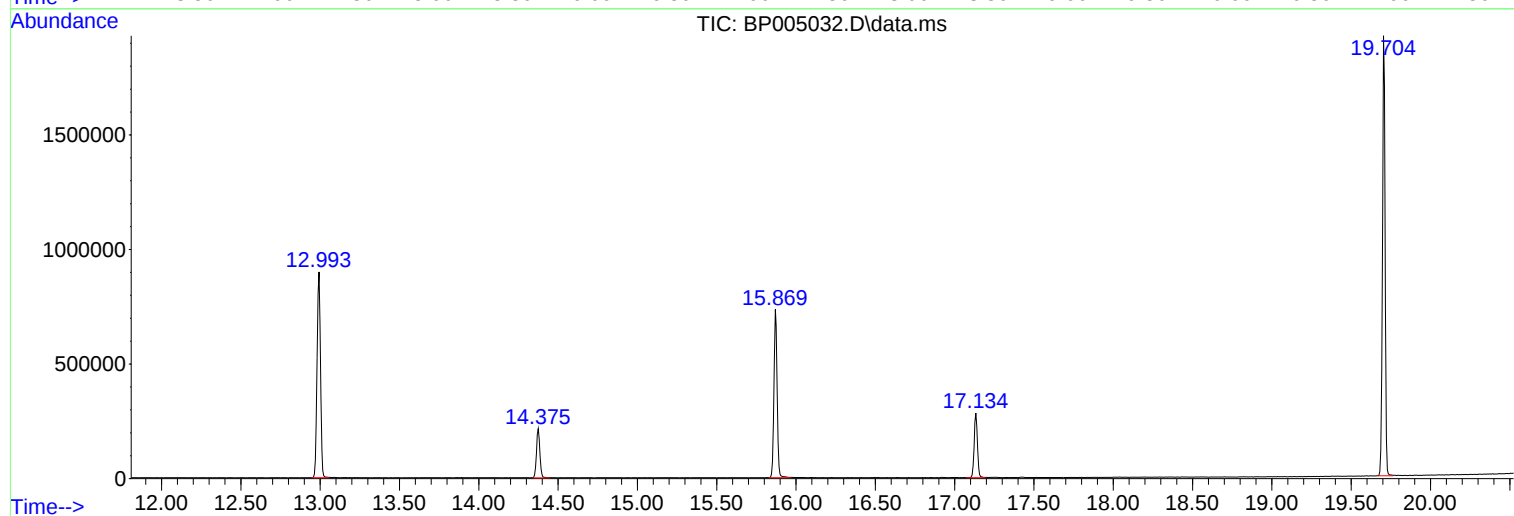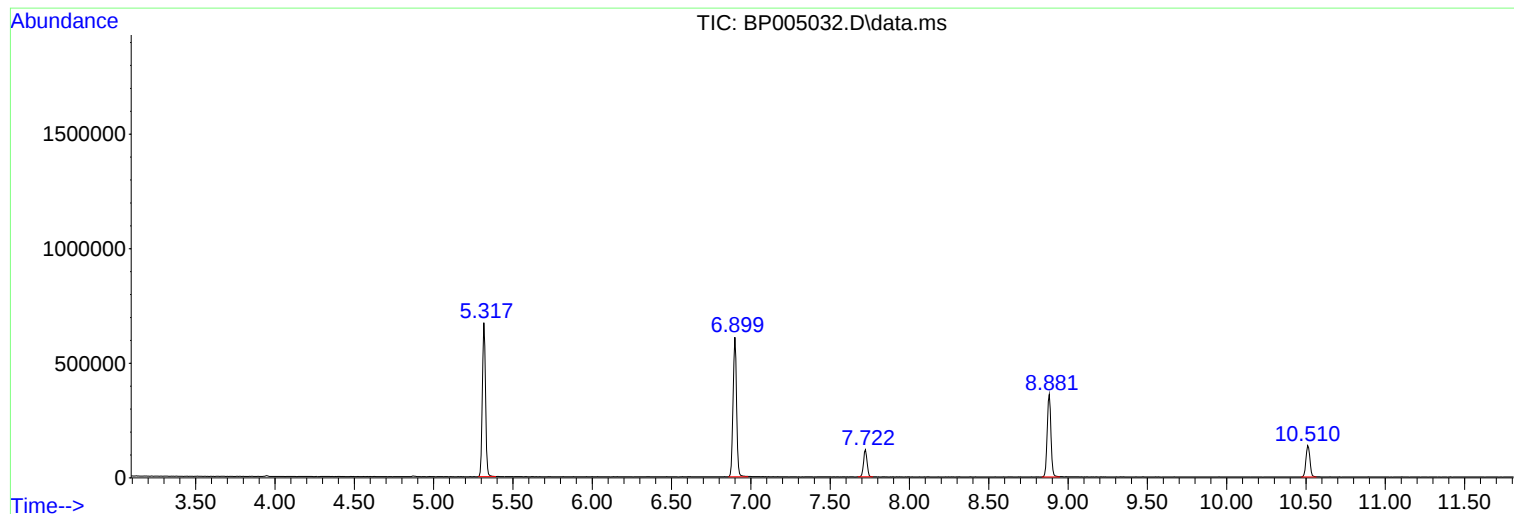

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032421\
Data File : BP005032.D
Acq On : 24 Mar 2021 09:53
Operator : CG/JU
Sample : PB135047BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB135047BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032421\
Data File : BP005032.D
Acq On : 24 Mar 2021 09:53
Operator : CG/JU
Sample : PB135047BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB135047BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------