
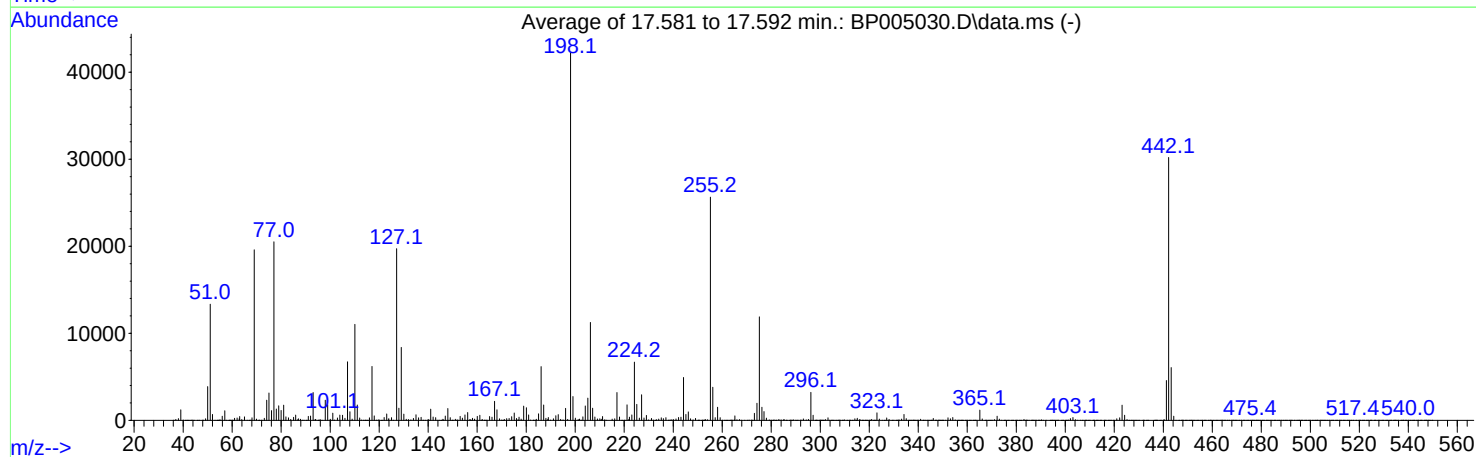


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032421\
 Data File : BP005030.D
 Acq On : 24 Mar 2021 08:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 25 10:21:09 2021

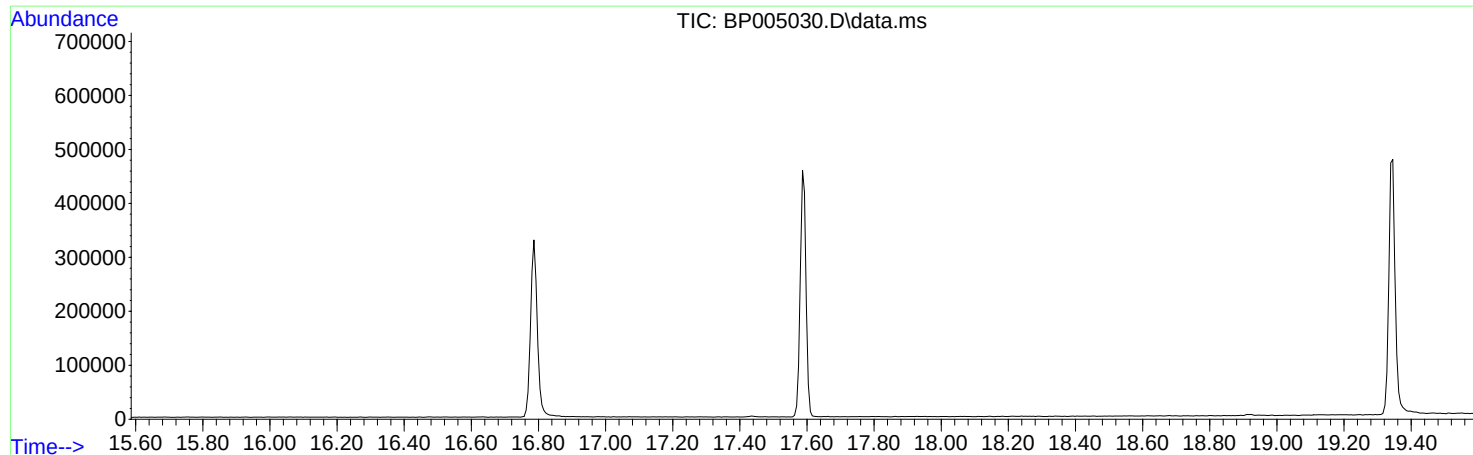




AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.6	13343	PASS
68	69	0.00	2	1.5	288	PASS
69	198	0.00	100	46.4	19601	PASS
70	69	0.00	2	0.7	141	PASS
127	198	10	80	46.7	19735	PASS
197	198	0.00	2	0.3	113	PASS
198	198	100	100	100.0	42263	PASS
199	198	5	9	6.5	2742	PASS
275	198	10	60	28.2	11903	PASS
365	198	1	100	2.8	1168	PASS
441	198	0.01	100	10.8	4584	PASS
442	442	100	100	100.0	30199	PASS
443	442	15	24	20.1	6073	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032421\
Data File : BP005030.D
Acq On : 24 Mar 2021 08:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 25 08:25:21 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 24 10:16:52 2021
Response via : Initial Calibration

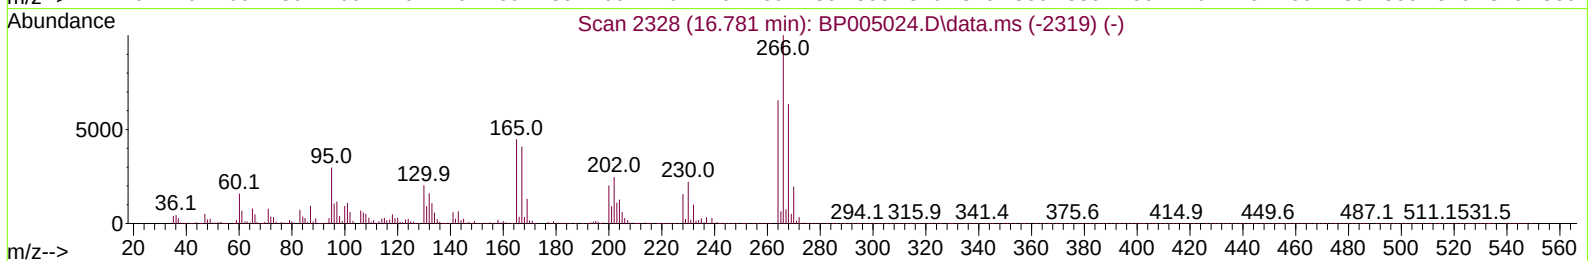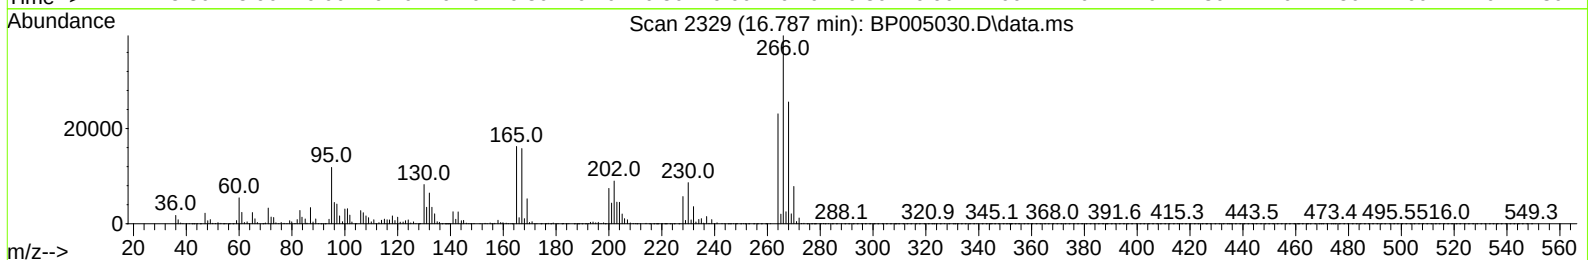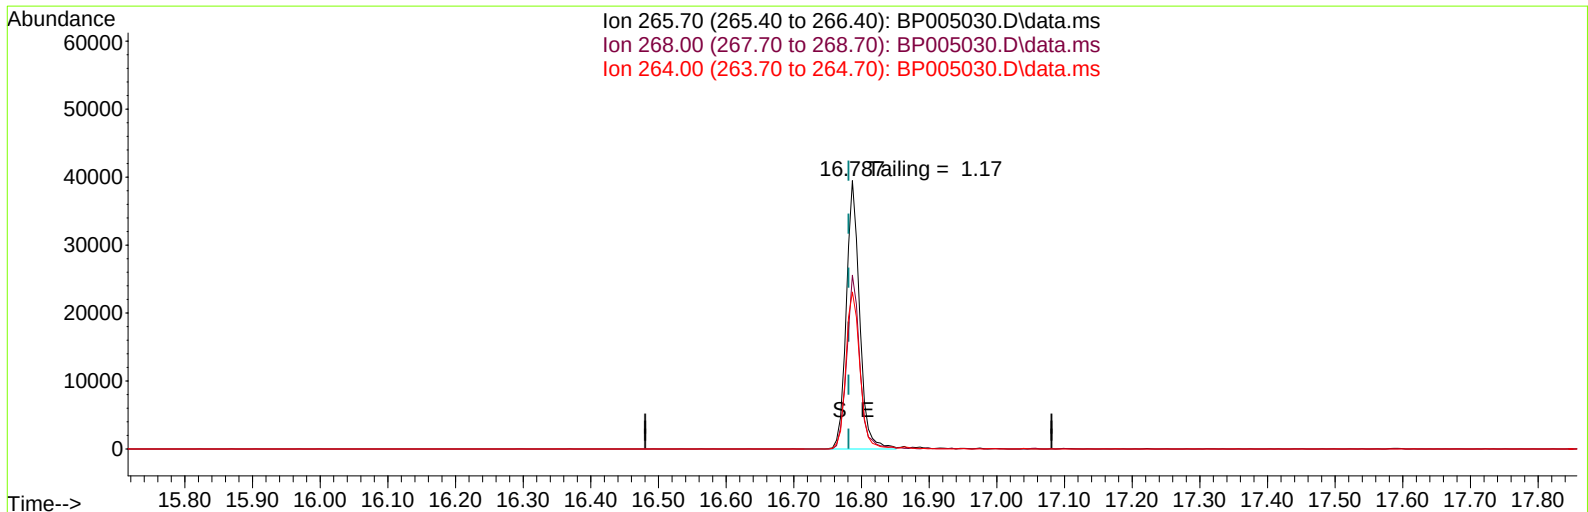

TIC: BP005030.D\data.ms

(70) Pentachlorophenol (C)

16.787min (+ 0.006) 525192.26 ng




response 54218

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	64.78
264.00	63.30	58.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032421\
 Data File : BP005030.D
 Acq On : 24 Mar 2021 08:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Mar 25 08:25:21 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 24 10:16:52 2021
 Response via : Initial Calibration

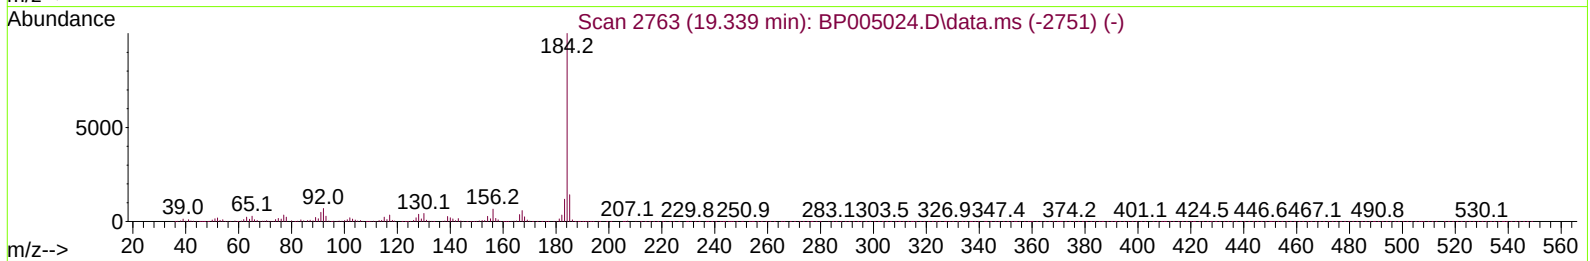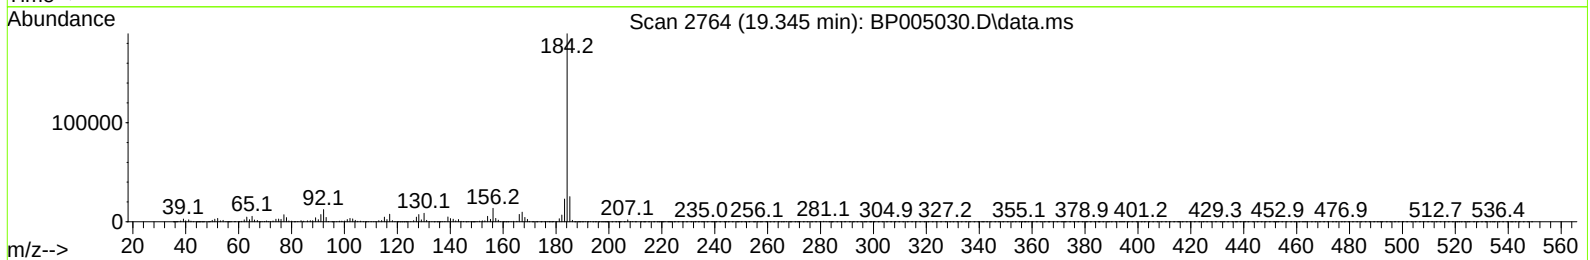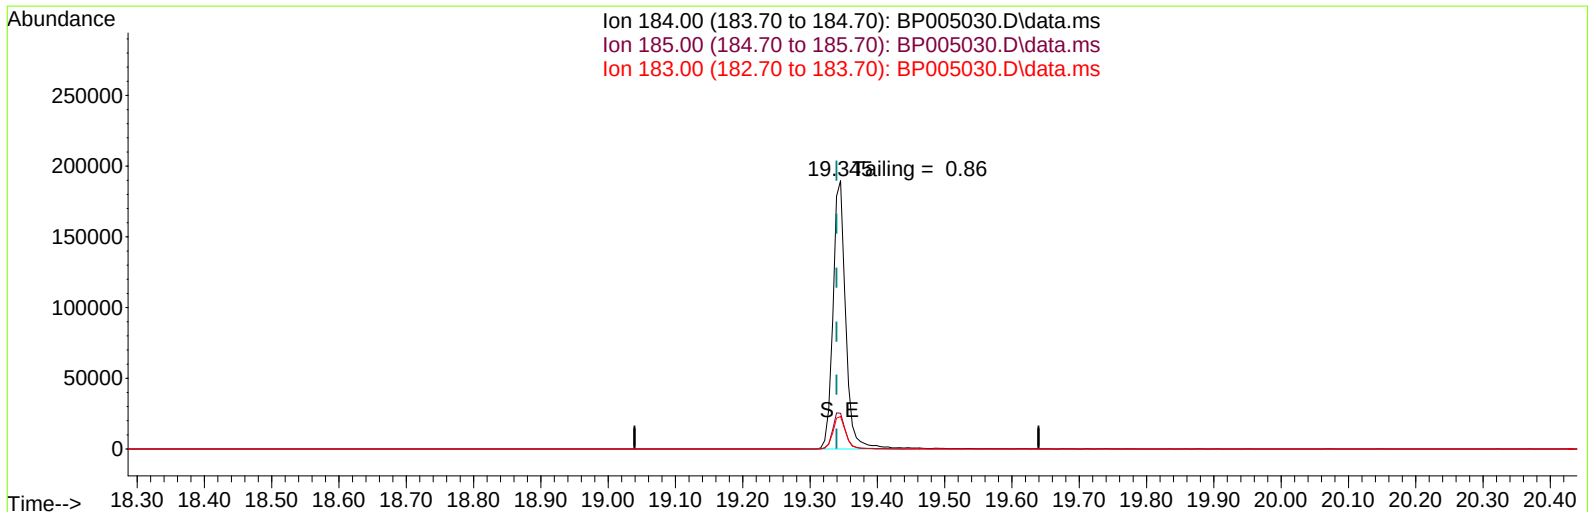

TIC: BP005030.D\data.ms

(77) Benzidine

19.345min (+ 0.006) 627598.75 ng

response 247854

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.33
183.00	12.00	12.12
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_P
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
03/24/2021	BNA_P	BP005030.D
Compound Name	Response	Retention Time
DDT	154871	20.545
DDD	2832	20.116
DDE	510	19.622
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3342	158213	2.11

Instrument :
BNA_P
ClientSampleId :
DFTPP