

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032423\
 Data File : BP014282.D
 Acq On : 24 Mar 2023 09:45
 Operator : CG/JU
 Sample : PB151650BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK650

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014282.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.405	33	37	43	rBV	46323	64484	1.10%	0.116%
2	3.834	108	110	132	rBV	561603	968426	16.46%	1.741%
3	4.164	162	166	173	rVB2	11960	18017	0.31%	0.032%
4	7.193	674	681	697	rBV	756887	1293139	21.98%	2.324%
5	7.358	703	709	724	rBV	608981	1000064	17.00%	1.798%
6	7.563	737	744	762	rBV	773667	1264128	21.49%	2.272%
7	8.034	815	824	836	rBV	644933	1037776	17.64%	1.865%
8	8.746	939	945	962	rBV	937692	1666214	28.32%	2.995%
9	9.210	1016	1024	1040	rBV	823016	1355165	23.04%	2.436%
10	9.940	1138	1148	1161	rBV	679667	1199386	20.39%	2.156%
11	10.481	1232	1240	1261	rBV	891241	1740254	29.58%	3.128%
12	10.857	1294	1304	1314	rBV	947976	1600989	27.21%	2.878%
13	11.004	1321	1329	1358	rBV	878465	1770482	30.10%	3.183%
14	12.457	1567	1576	1583	rBV3	12429	29989	0.51%	0.054%
15	13.563	1760	1764	1771	rVB8	5680	11116	0.19%	0.020%
16	14.087	1846	1853	1870	rBV	2123175	2993706	50.89%	5.381%
17	14.375	1895	1902	1916	rBV	2269207	3332760	56.65%	5.991%
18	14.681	1947	1954	1964	rBV	1610540	2426918	41.25%	4.363%
19	14.887	1982	1989	2014	rBV	600780	1355599	23.04%	2.437%
20	15.675	2116	2123	2138	rBV	3020162	4343141	73.83%	7.807%
21	15.798	2138	2144	2159	rVV	1003385	1490365	25.33%	2.679%
22	15.916	2161	2164	2173	rVB5	19688	37629	0.64%	0.068%
23	17.110	2363	2367	2372	rBV7	4169	6437	0.11%	0.012%
24	17.228	2382	2387	2393	rBV5	6035	14465	0.25%	0.026%
25	17.439	2416	2423	2433	rBV	2221942	3105956	52.80%	5.583%
26	17.539	2434	2440	2456	rVV	3380980	4895833	83.22%	8.801%
27	19.345	2743	2747	2753	rBV3	44655	58446	0.99%	0.105%
28	19.416	2754	2759	2763	rBV	40870	62737	1.07%	0.113%
29	19.763	2812	2818	2830	rBV	4337283	5882868	100.00%	10.575%
30	21.522	3112	3117	3130	rBV	2364461	3294858	56.01%	5.923%
31	23.880	3511	3518	3528	rVB2	2247626	4619456	78.52%	8.304%
32	24.039	3539	3545	3560	rVB2	1280872	2690307	45.73%	4.836%




Sum of corrected areas: 55631110

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032423\
Data File : BP014282.D
Acq On : 24 Mar 2023 09:45
Operator : CG/JU
Sample : PB151650BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK650

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

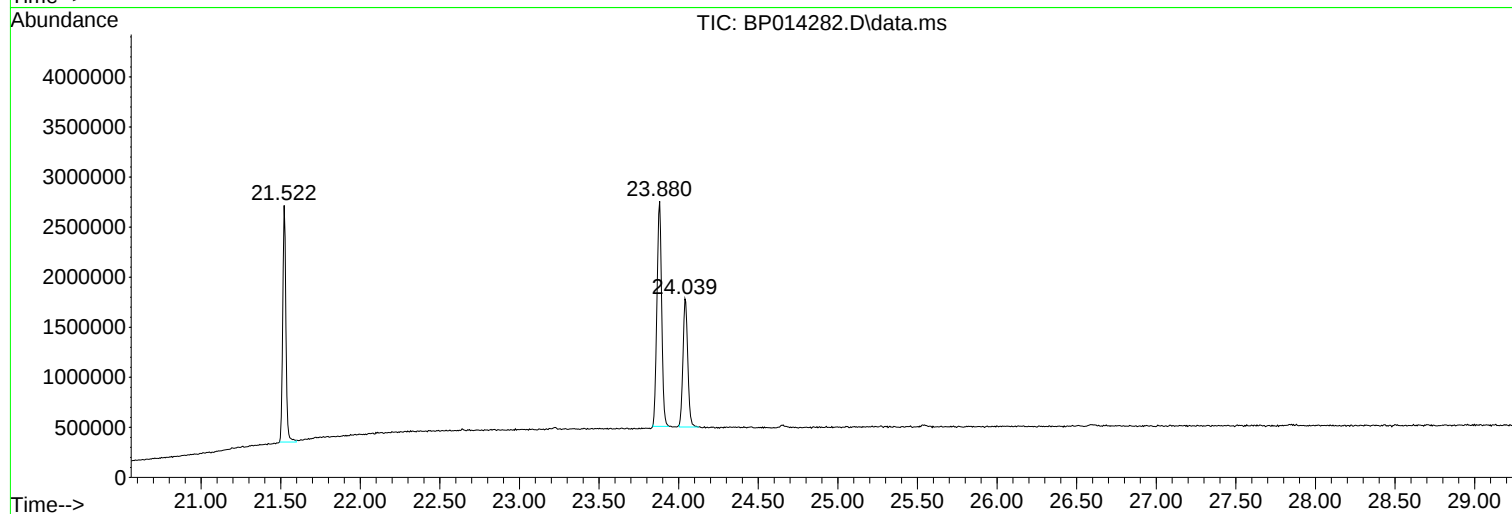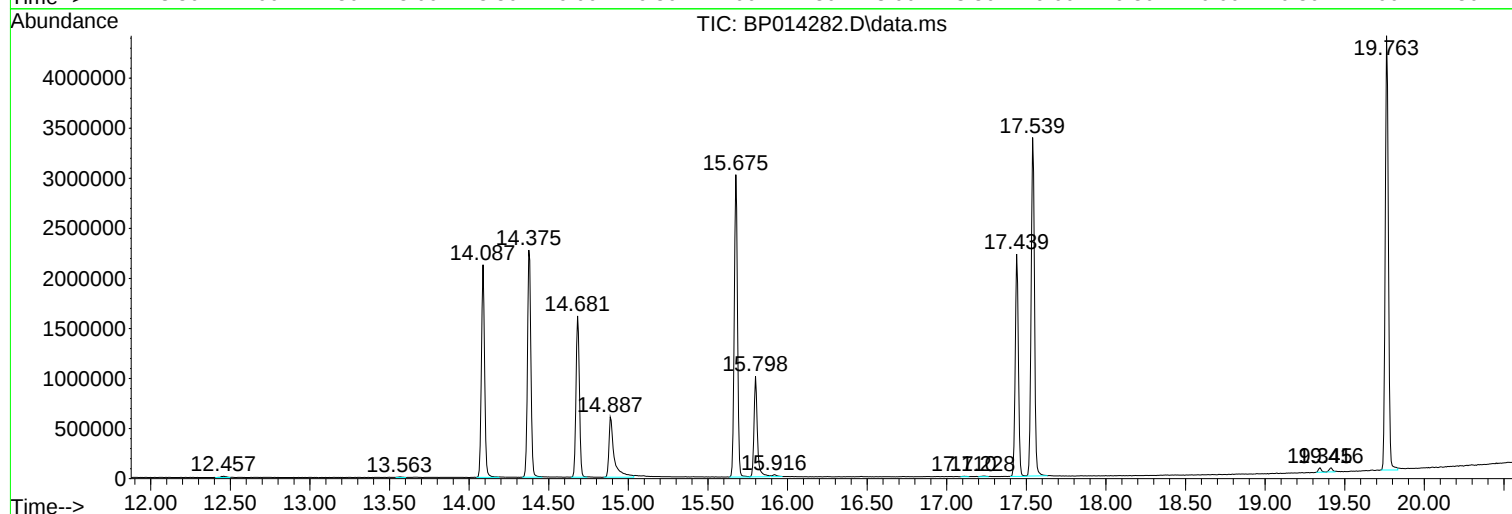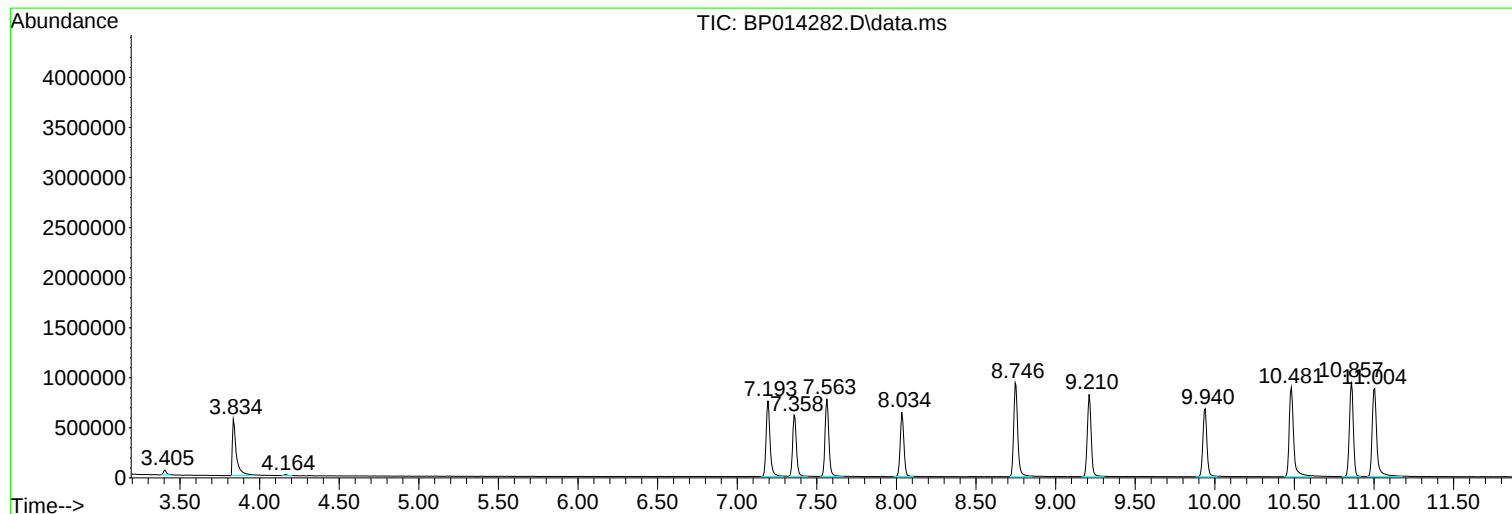

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032423\
Data File : BP014282.D
Acq On : 24 Mar 2023 09:45
Operator : CG/JU
Sample : PB151650BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK650

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032423\
Data File : BP014282.D
Acq On : 24 Mar 2023 09:45
Operator : CG/JU
Sample : PB151650BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK650

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------