


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032523\
 Data File : BP014294.D
 Acq On : 24 Mar 2023 18:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 25 03:19:01 2023

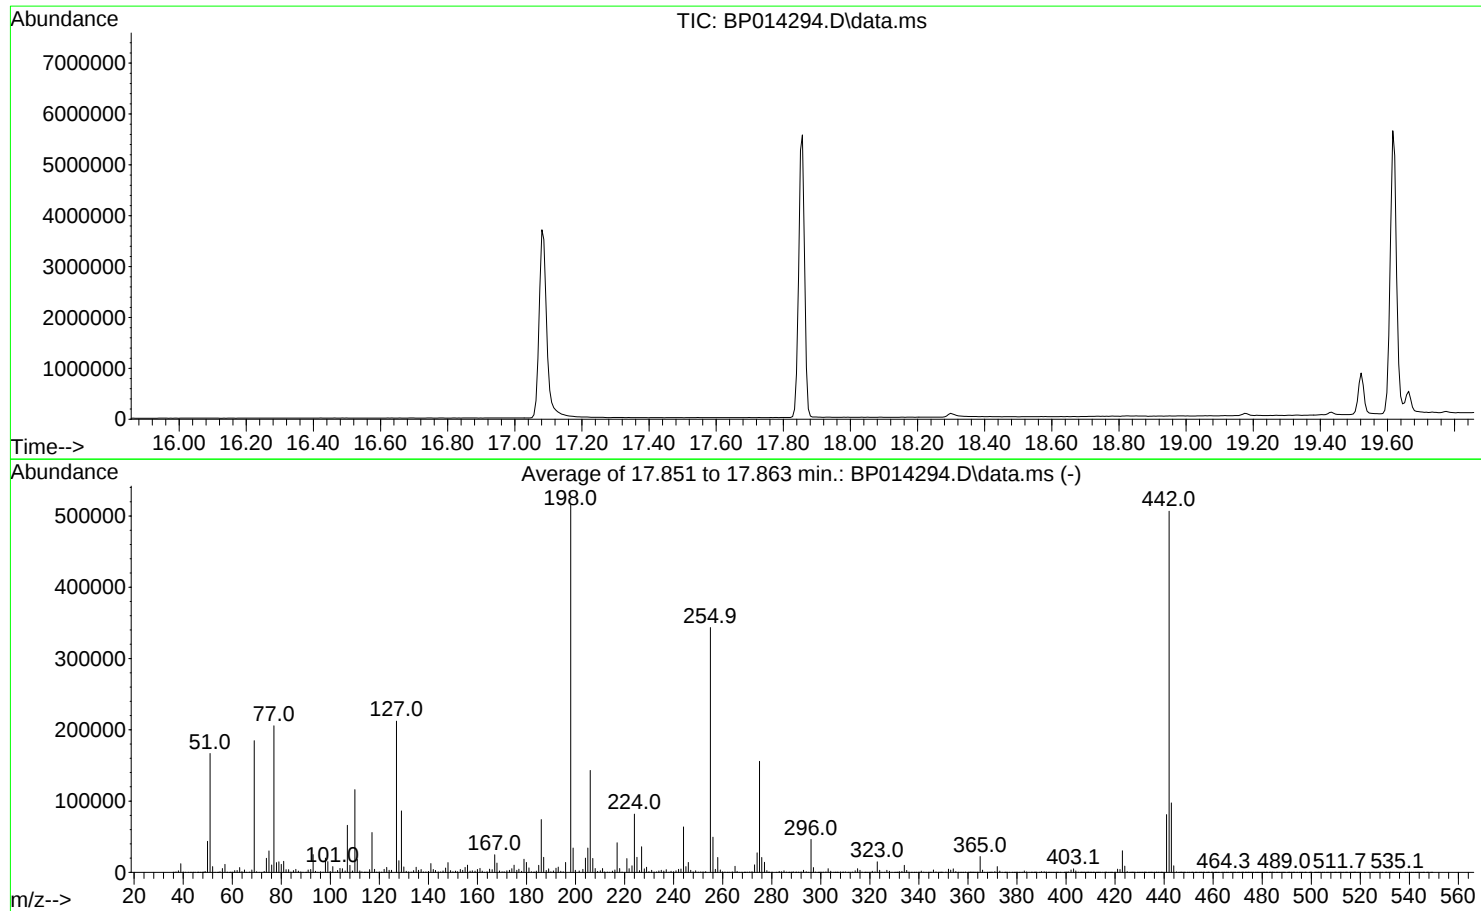




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.3	166746	PASS
68	69	0.00	2	1.9	3443	PASS
69	198	0.00	100	35.8	184799	PASS
70	69	0.00	2	0.6	1020	PASS
127	198	10	80	41.1	212158	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	516111	PASS
199	198	5	9	6.6	34173	PASS
275	198	10	60	30.2	155720	PASS
365	198	1	100	4.3	22155	PASS
441	198	0.01	100	15.7	81066	PASS
442	442	100	100	100.0	506773	PASS
443	442	15	24	19.2	97430	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032523\
Data File : BP014294.D
Acq On : 24 Mar 2023 18:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 25 04:32:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 25 03:19:01 2023
Response via : Initial Calibration

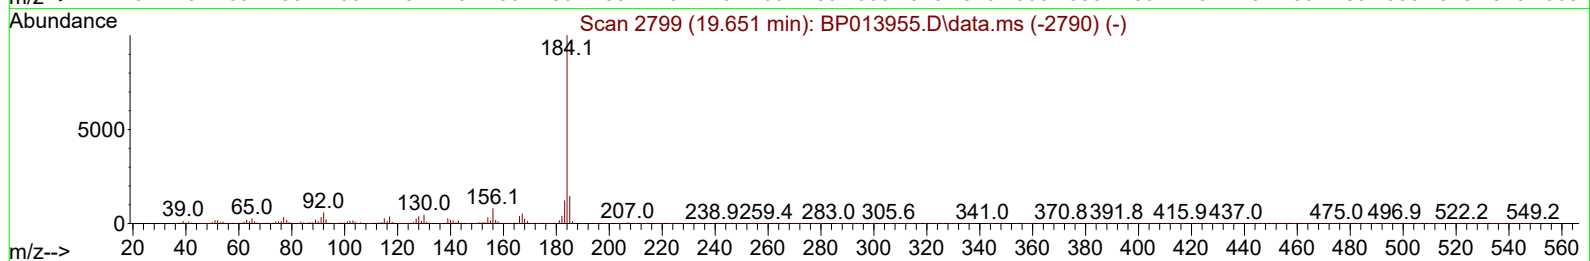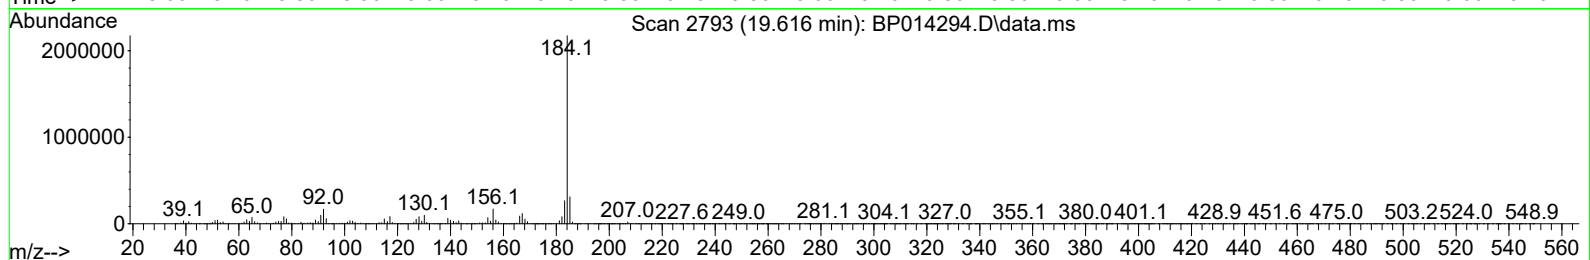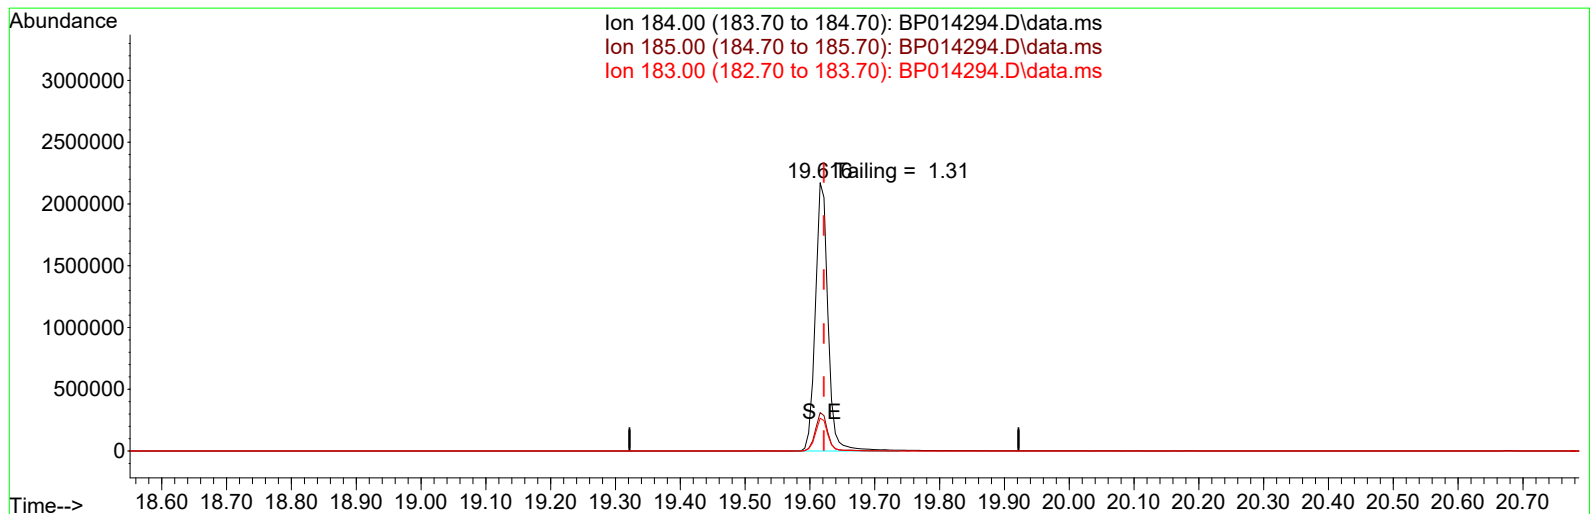

TIC: BP014294.D\data.ms

(77) Benzidine

19.616min (-0.006) -20.00 ng




response 2961293

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.33
183.00	12.10	12.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032523\
 Data File : BP014294.D
 Acq On : 24 Mar 2023 18:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Mar 25 04:32:53 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 25 03:19:01 2023
 Response via : Initial Calibration

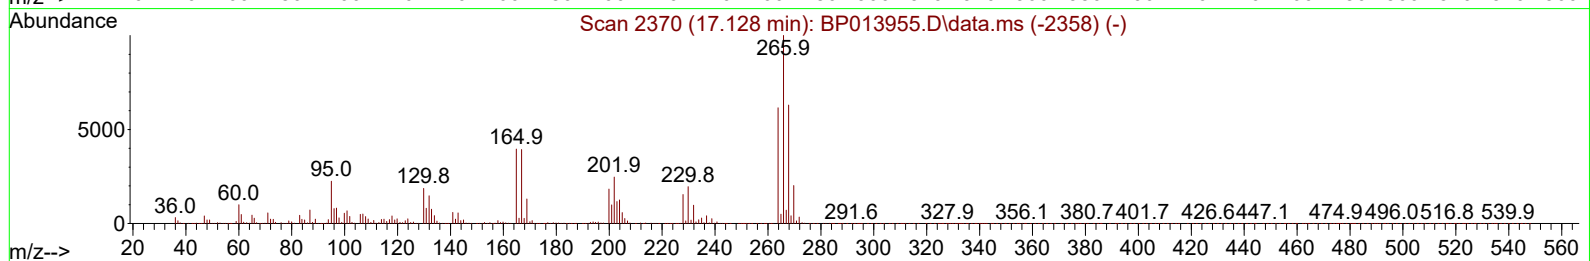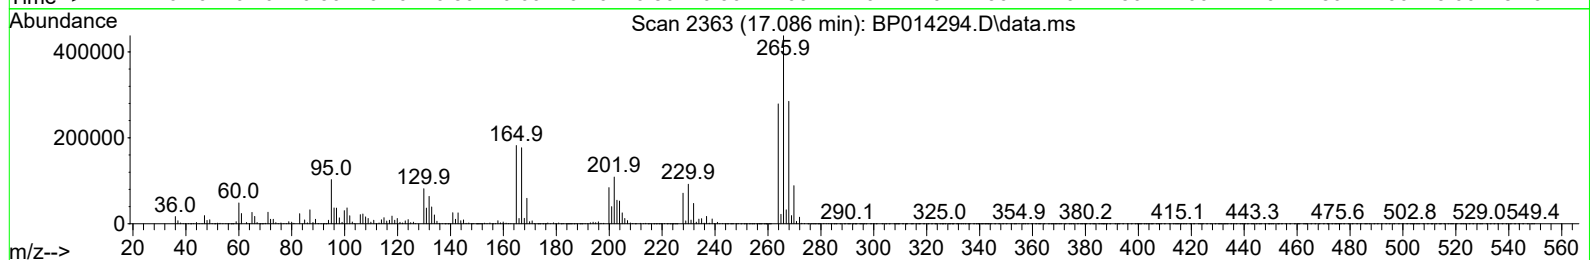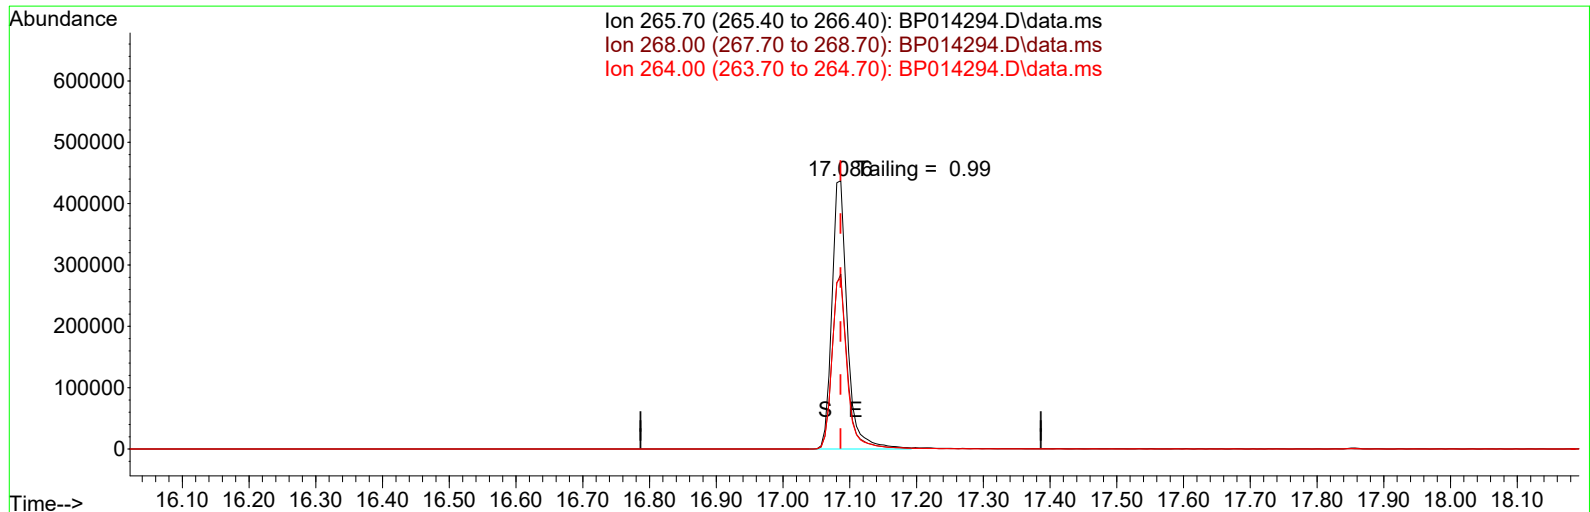

TIC: BP014294.D\data.ms

(70) Pentachlorophenol (C)

17.086min (-0.000) 1910234.30 ng

response 703186

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	65.11
264.00	61.50	63.77
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/25/2023	BNA_P	<u>BP014294.D</u>
Compound Name	Response	Retention Time
DDT	1723128	20.81
DDD	26587	20.427
DDE	1034	19.886
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27621	1750749	1.58

Instrument :
BNA_P
ClientSampleId :
DFTPP