

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
 Data File : BP014354.D
 Acq On : 29 Mar 2023 09:44
 Operator : CG/JU
 Sample : 02087-01DL 5X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QF8DL

Quant Time: Mar 30 01:00:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 30 00:56:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.022	152	154116	20.000	ng/ul	0.00
20) Naphthalene-d8	10.846	136	673960	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.675	164	465467	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.439	188	1054189	20.000	ng/ul	0.00
79) Chrysene-d12	21.521	240	911342	20.000	ng/ul	0.00
88) Perylene-d12	24.045	264	819490	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	2211	0.556	ng/uL	0.00
4) Pyridine-d5	3.817	84	293	0.029	ng/ul	0.00
7) Phenol-d5	7.199	99	17293	1.217	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	7.346	67	62250	6.826	ng/ul	0.00
11) 2-Chlorophenol-d4	7.552	132	51382	5.002	ng/ul	0.00
15) 4-Methylphenol-d8	8.746	113	35946	3.135	ng/ul	0.01
21) Nitrobenzene-d5	9.204	128	31885	5.860	ng/ul	0.00
24) 2-Nitrophenol-d4	9.928	143	33211	5.331	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.481	165	56392	4.970	ng/ul	0.02
31) 4-Chloroaniline-d4	10.999	131	50467	3.377	ng/ul	0.01
46) Dimethylphthalate-d6	14.081	166	274421	7.271	ng/ul	0.00
49) Acenaphthylene-d8	14.369	160	278145	6.642	ng/ul	0.00
54) 4-Nitrophenol-d4	14.892	143	241	0.042	ng/ul	0.01
60) Fluorene-d10	15.669	176	230861	7.335	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.798	200	37994	4.898	ng/ul	0.00
73) Anthracene-d10	17.539	188	371150	7.275	ng/ul	0.00
81) Pyrene-d10	19.763	212	443683	7.248	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.880	264	307397	7.060	ng/ul	0.00
Target Compounds					Qvalue	
30) Naphthalene	10.899	128	224218	5.973	ng/ul	99
36) 2-Methylnaphthalene	12.504	142	84096	3.305	ng/ul	99
37) 1-Methylnaphthalene	12.722	142	63403	2.513	ng/ul	92
66) 4,6-Dinitro-2-methylph...	15.822	198	15813	2.104	ng/ul#	73
71) Pentachlorophenol	17.086	266	319161	36.562	ng/ul	98
72) Phenanthrene	17.481	178	119024	2.029	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014354.D
Acq On : 29 Mar 2023 09:44
Operator : CG/JU
Sample : 02087-01DL 5X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QF8DL

Quant Time: Mar 30 01:00:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 30 00:56:20 2023
Response via : Initial Calibration

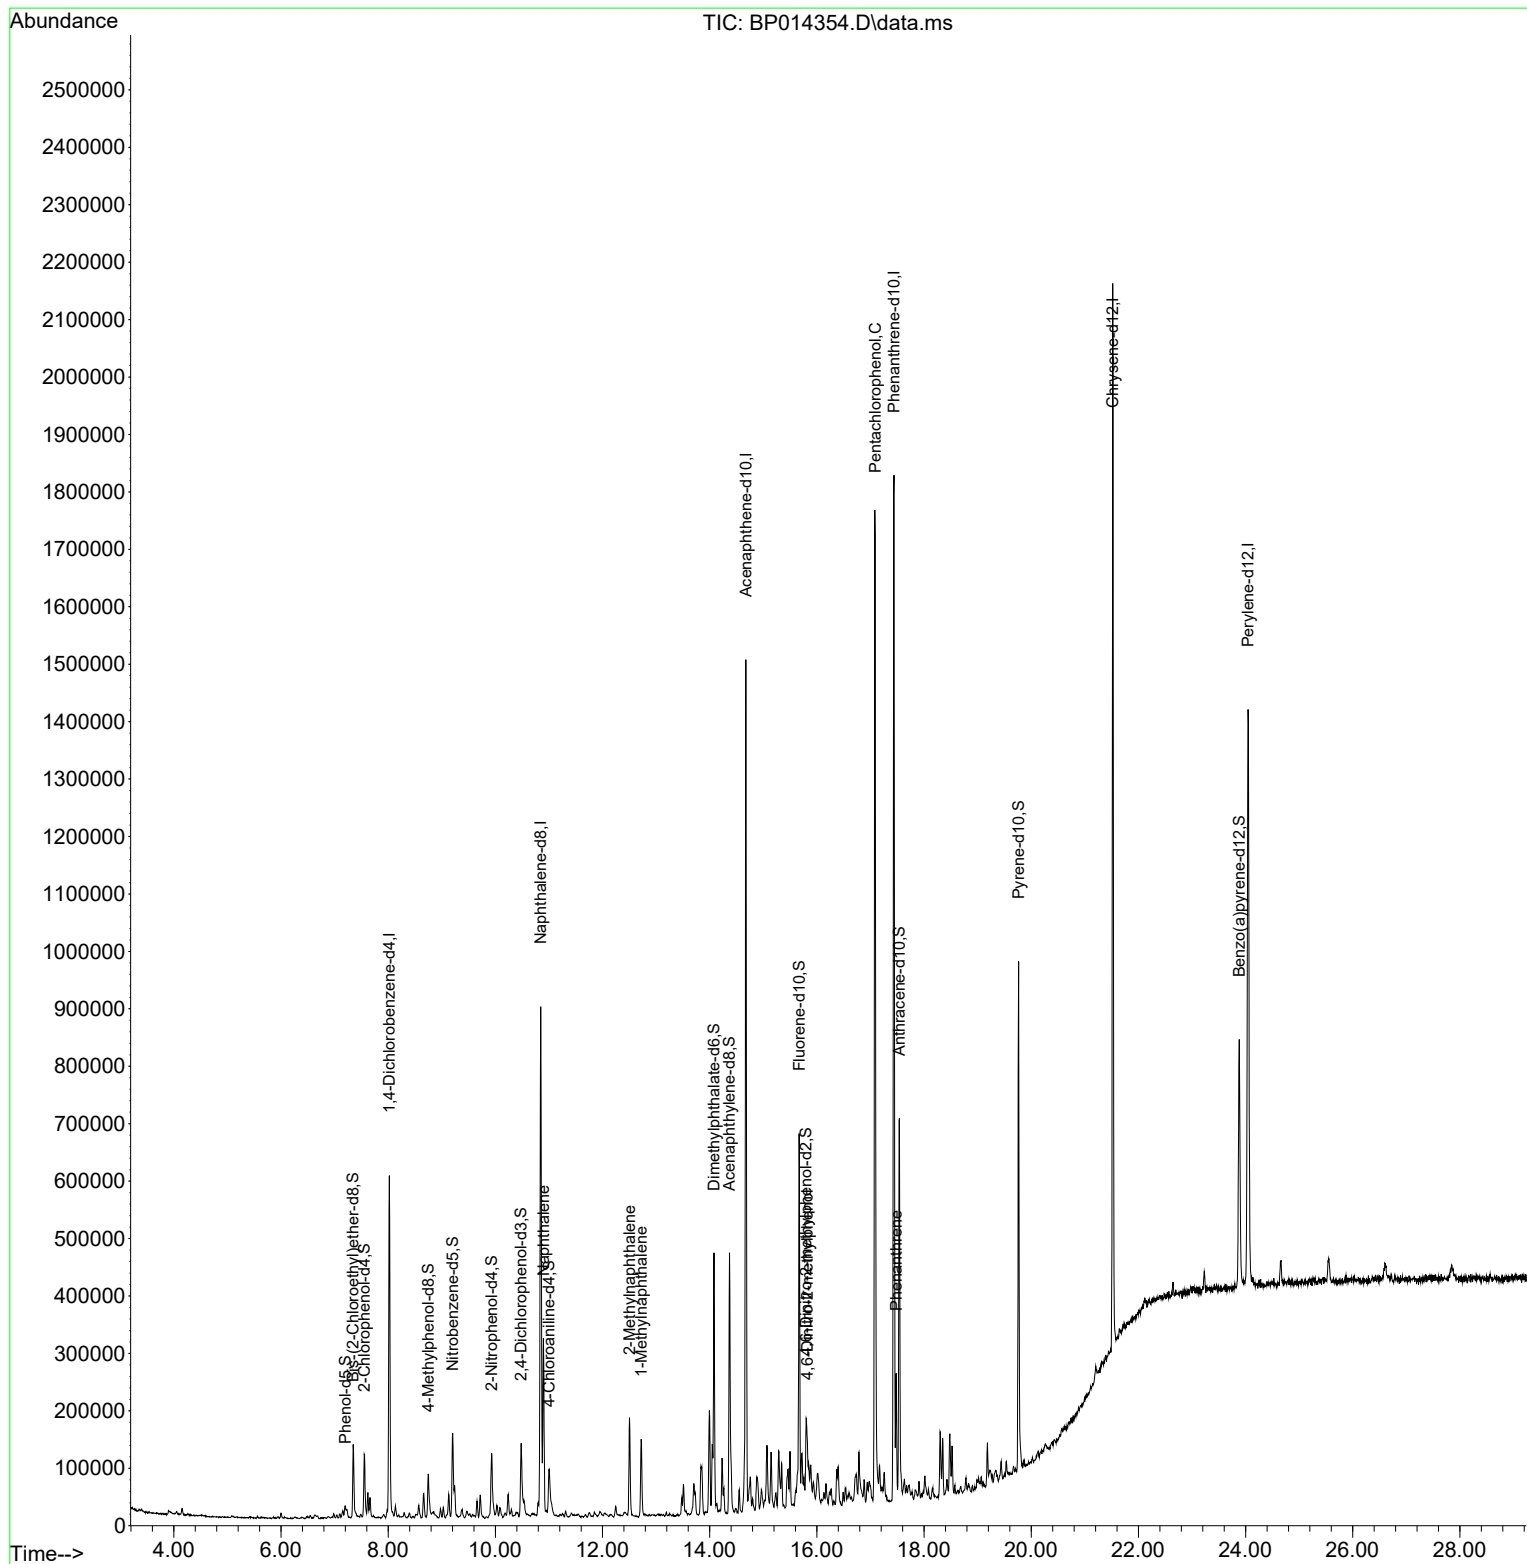

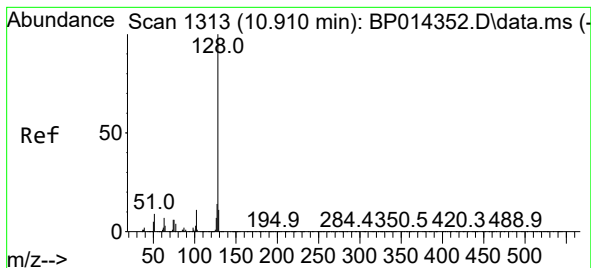

#30

Naphthalene

Concen: 5.973 ng/ul

RT: 10.899 min Scan# 1

Delta R.T. 0.006 min

Lab File: BP014354.D

Acq: 29 Mar 2023 09:44

Instrument :

BNA_P

ClientSampleId :

C0QF8DL





Tgt Ion:128 Resp: 224218

Ion Ratio Lower Upper

128 100

129 11.6 8.9 13.3

127 13.3 11.0 16.6

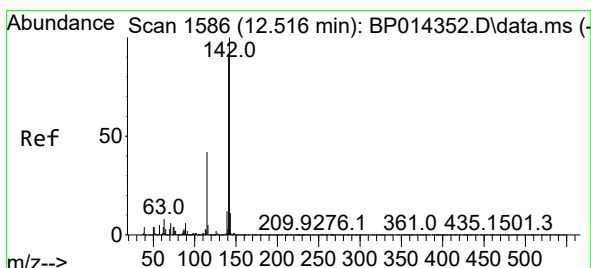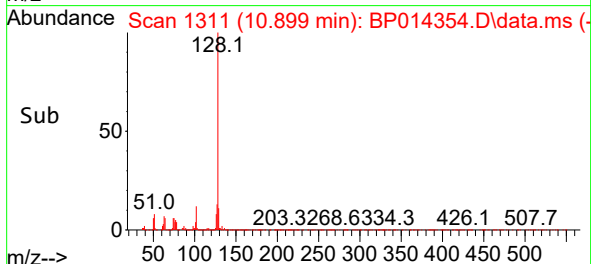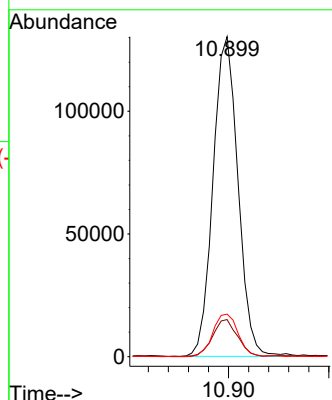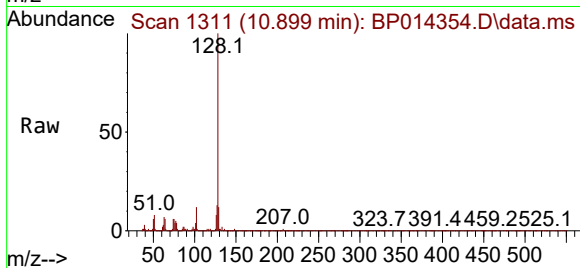

#36

2-Methylnaphthalene

Concen: 3.305 ng/ul

RT: 12.504 min Scan# 1584

Delta R.T. 0.006 min

Lab File: BP014354.D




Acq: 29 Mar 2023 09:44


Tgt Ion:142 Resp: 84096

Ion Ratio Lower Upper

142 100

141 88.1 71.6 107.4


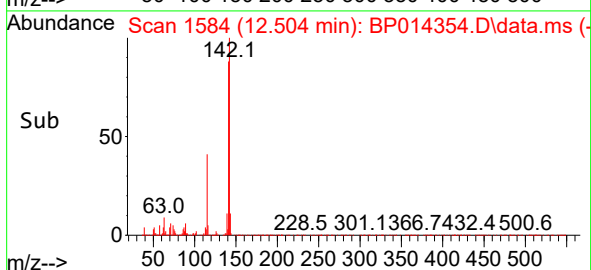
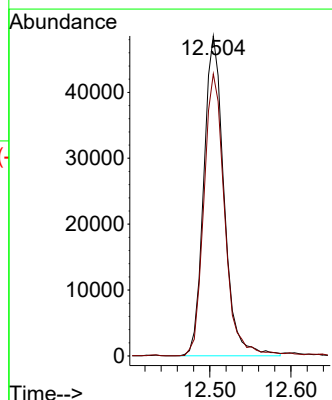
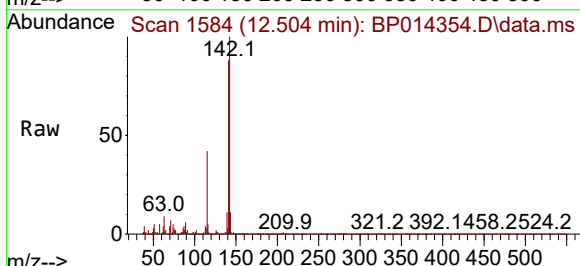


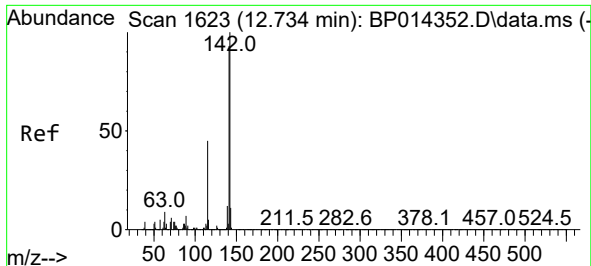

#37
1-Methylnaphthalene
Concen: 2.513 ng/ul
RT: 12.722 min Scan# 1621
Delta R.T. 0.006 min
Lab File: BP014354.D
Acq: 29 Mar 2023 09:44




Instrument :
BNA_P
ClientSampleId :
C0QF8DL


Tgt Ion:142 Resp: 63403
Ion Ratio Lower Upper
142 100
141 87.7 76.6 114.8
116 4.5 3.6 5.4

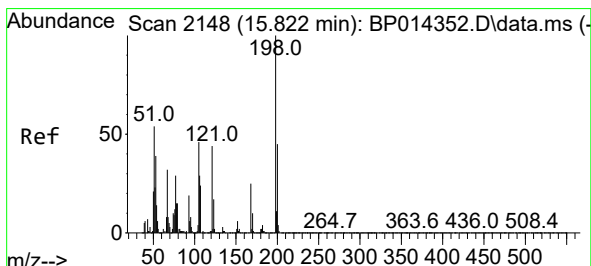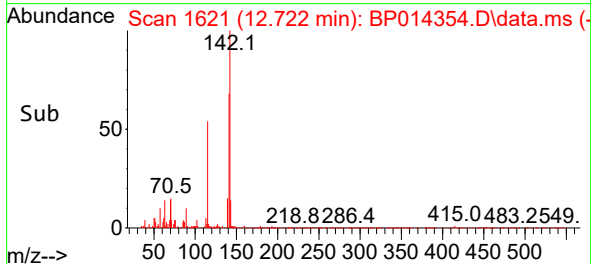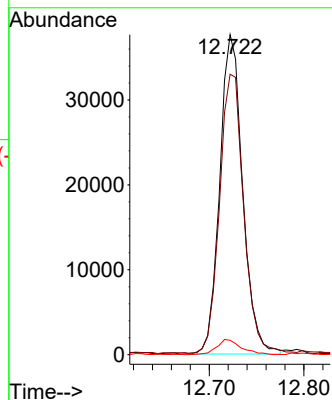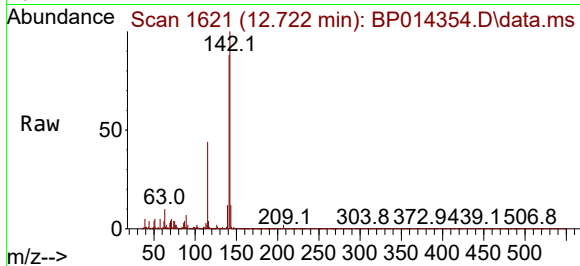

#66
4,6-Dinitro-2-methylphenol
Concen: 2.104 ng/ul
RT: 15.822 min Scan# 2148
Delta R.T. 0.012 min
Lab File: BP014354.D
Acq: 29 Mar 2023 09:44

Tgt Ion:198 Resp: 15813
Ion Ratio Lower Upper
198 100
182 3.9 3.5 5.3
77 14.0 24.4 36.6#

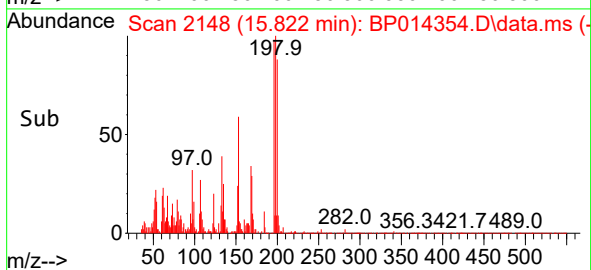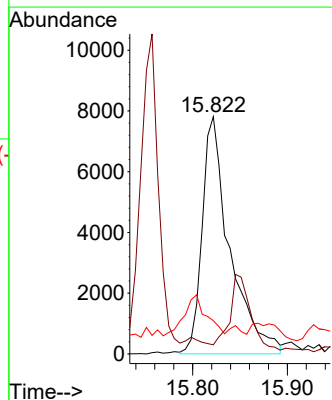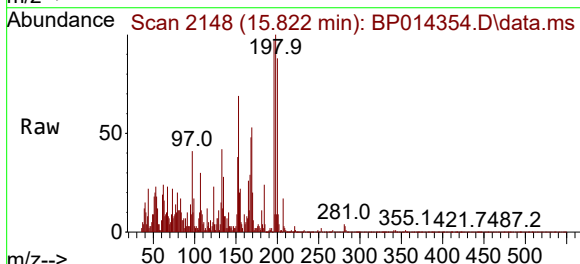

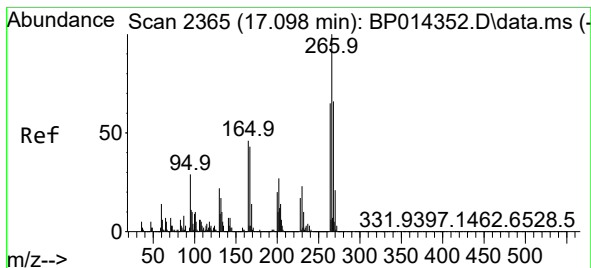

#71

Pentachlorophenol

Concen: 36.562 ng/ul

RT: 17.086 min Scan# 21

Delta R.T. 0.000 min

Lab File: BP014354.D

Acq: 29 Mar 2023 09:44

Instrument :

BNA_P

ClientSampleId :

C0QF8DL





Tgt Ion:266 Resp: 319161

Ion Ratio Lower Upper

266 100

264 61.0 51.0 76.4

268 64.6 51.4 77.2

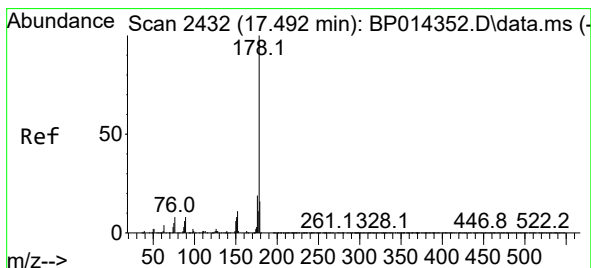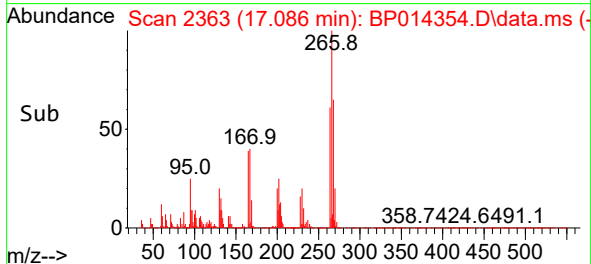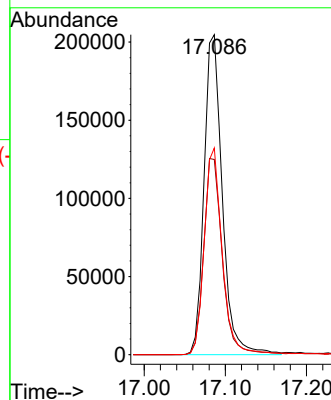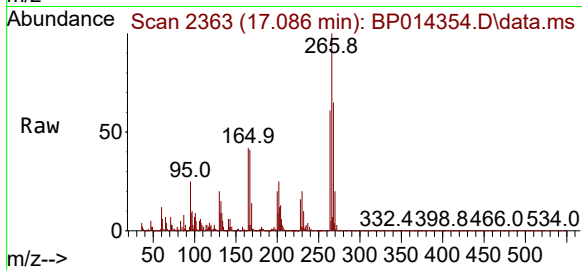

#72

Phenanthrene

Concen: 2.029 ng/ul

RT: 17.481 min Scan# 2430

Delta R.T. 0.000 min

Lab File: BP014354.D

Acq: 29 Mar 2023 09:44

Tgt Ion:178 Resp: 119024

Ion Ratio Lower Upper

178 100

179 16.0 12.2 18.4

176 18.7 15.3 22.9

