

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
 Data File : BP014378.D
 Acq On : 29 Mar 2023 23:48
 Operator : CG/JU
 Sample : 02041-02
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB956

Quant Time: Mar 30 01:06:11 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 30 00:56:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	165613	20.000	ng/u1	0.00
20) Naphthalene-d8	10.840	136	707420	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.675	164	475063	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.434	188	1076035	20.000	ng/u1	0.00
79) Chrysene-d12	21.522	240	945439	20.000	ng/u1	0.00
88) Perylene-d12	24.039	264	863918	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	18265	4.277	ng/uL	0.00
4) Pyridine-d5	3.828	84	95981	8.770	ng/u1	0.00
7) Phenol-d5	7.181	99	85311	5.586	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.340	67	292569	29.855	ng/u1	0.00
11) 2-Chlorophenol-d4	7.546	132	250566	22.698	ng/u1	0.00
15) 4-Methylphenol-d8	8.734	113	180724	14.669	ng/u1	0.00
21) Nitrobenzene-d5	9.193	128	172276	30.166	ng/u1	0.00
24) 2-Nitrophenol-d4	9.922	143	192233	29.396	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.463	165	334758	28.109	ng/u1	0.00
31) 4-Chloroaniline-d4	10.987	131	382805	24.402	ng/u1	0.00
46) Dimethylphthalate-d6	14.081	166	1357395	35.240	ng/u1	0.00
49) Acenaphthylene-d8	14.369	160	1363272	31.896	ng/u1	0.00
54) 4-Nitrophenol-d4	14.910	143	26400	4.537	ng/u1	0.03
60) Fluorene-d10	15.669	176	1081305	33.662	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.793	200	208067	26.279	ng/u1	0.00
73) Anthracene-d10	17.534	188	1878007	36.063	ng/u1	0.00
81) Pyrene-d10	19.763	212	2229261	35.104	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.880	264	1743602	37.987	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.428	88	18909	4.029 ng/uL	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014378.D
Acq On : 29 Mar 2023 23:48
Operator : CG/JU
Sample : 02041-02
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB956

Quant Time: Mar 30 01:06:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 30 00:56:20 2023
Response via : Initial Calibration

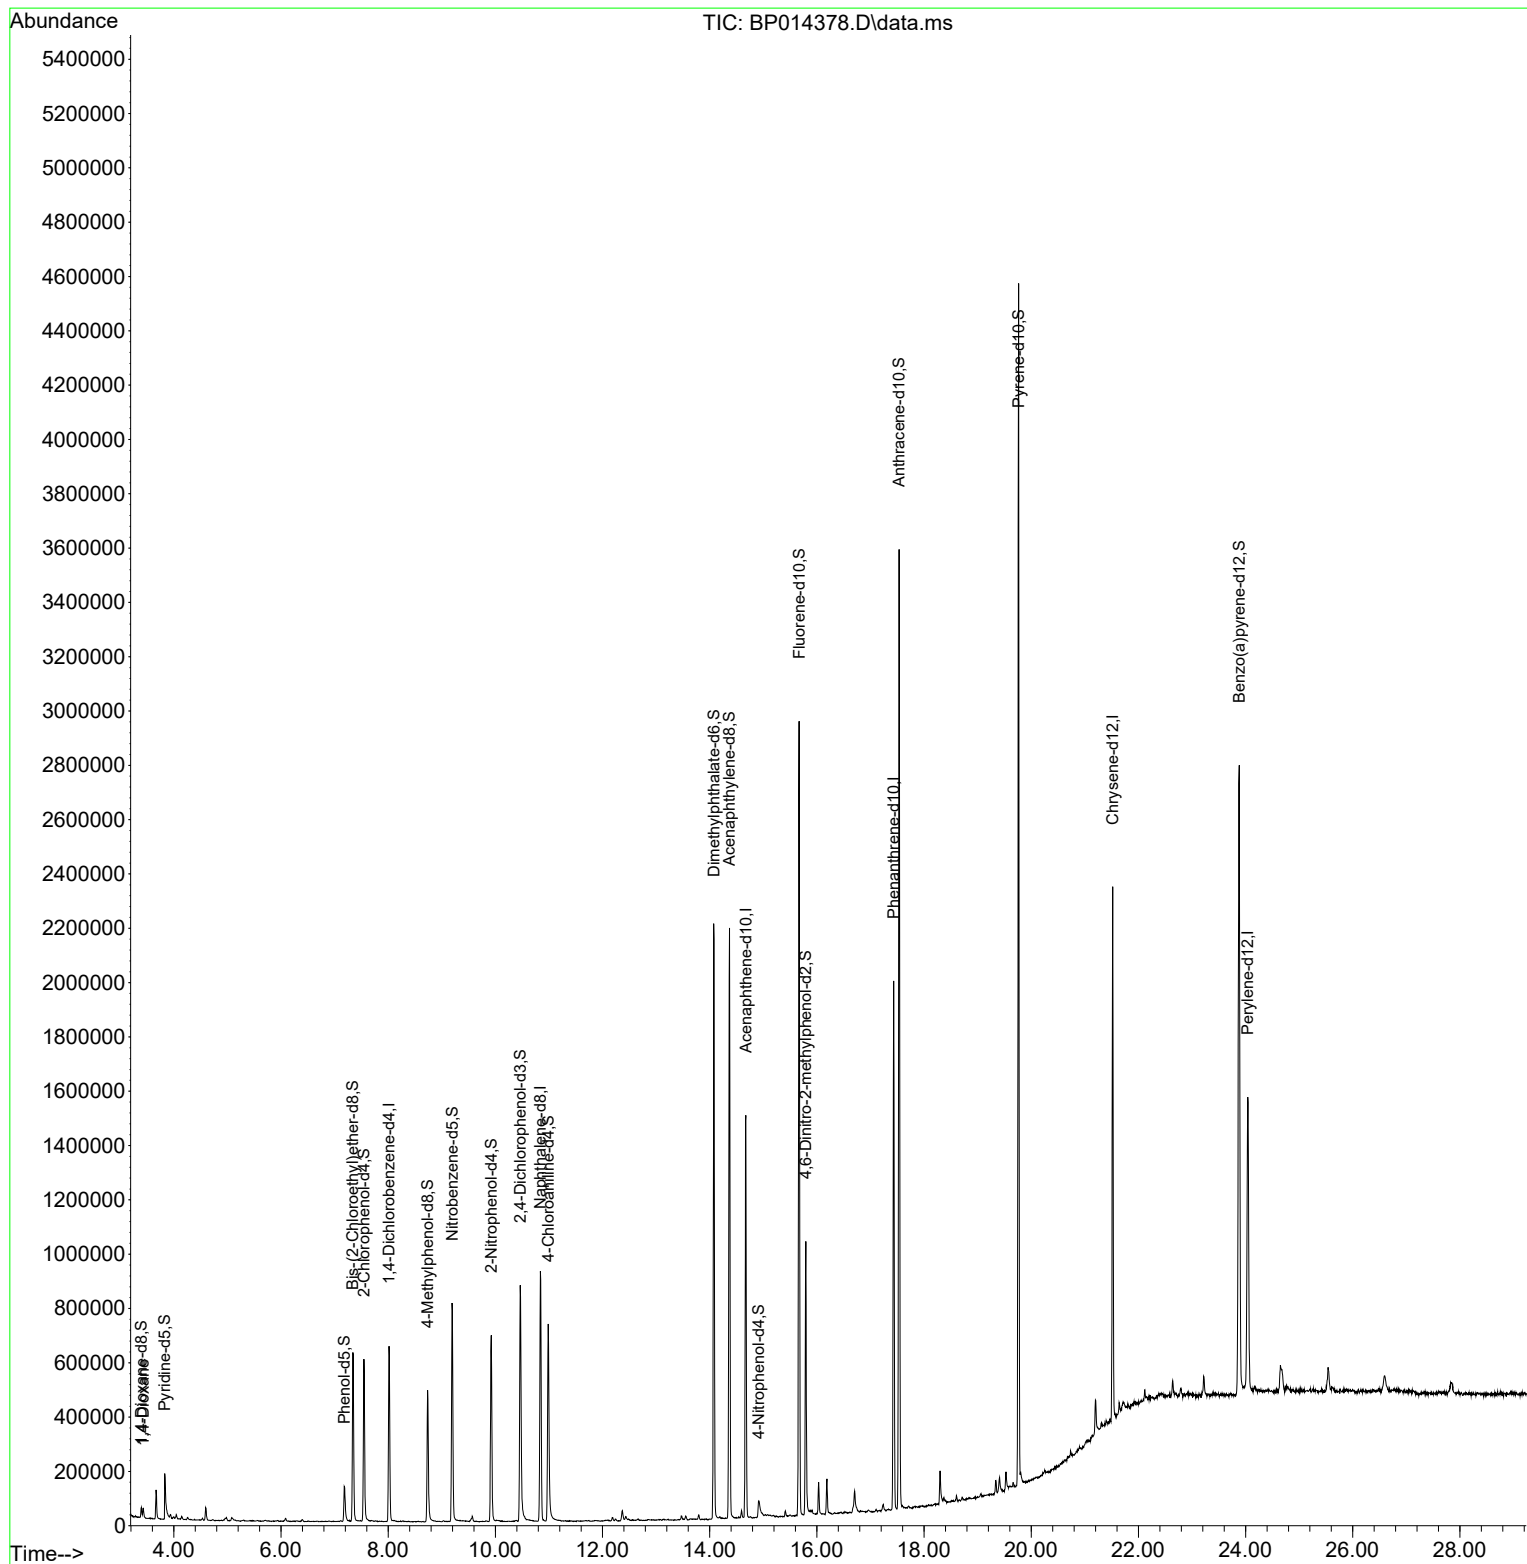

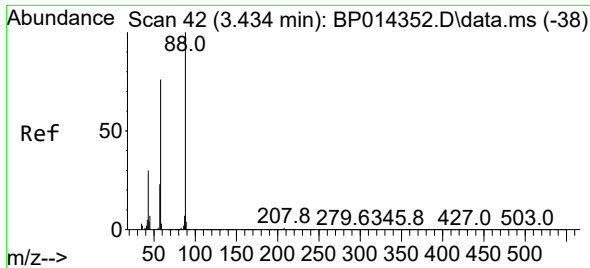

#2
 1,4-Dioxane
 Concen: 4.029 ng/uL
 RT: 3.428 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: BP014378.D
 Acq: 29 Mar 2023 23:48

Instrument :
 BNA_P
 ClientSampleId :
 CB956

Tgt Ion: 88 Resp: 18909
 Ion Ratio Lower Upper
 88 100
 43 33.5 24.4 36.6
 58 67.4 57.4 86.0

