




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014358.D
Acq On : 29 Mar 2023 12:01
Operator : CG/JU
Sample : 01982-11
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYGC0

Manual IntegrationsAPPROVED

Quant Time: Mar 30 01:01:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 30 00:56:20 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/30/2023
Supervised By :Jagrut Upadhyay 03/30/2023

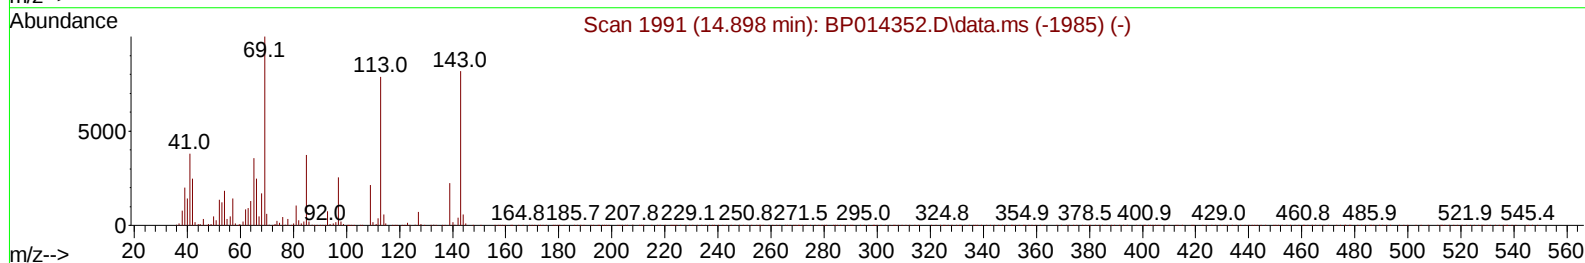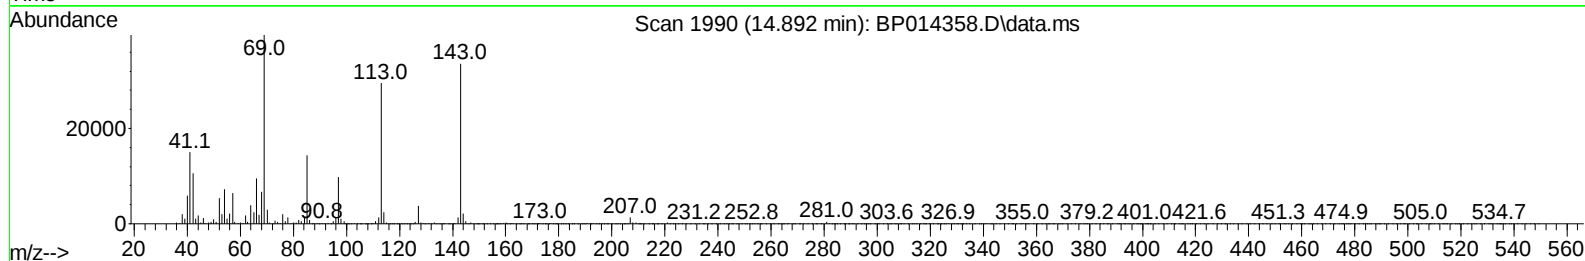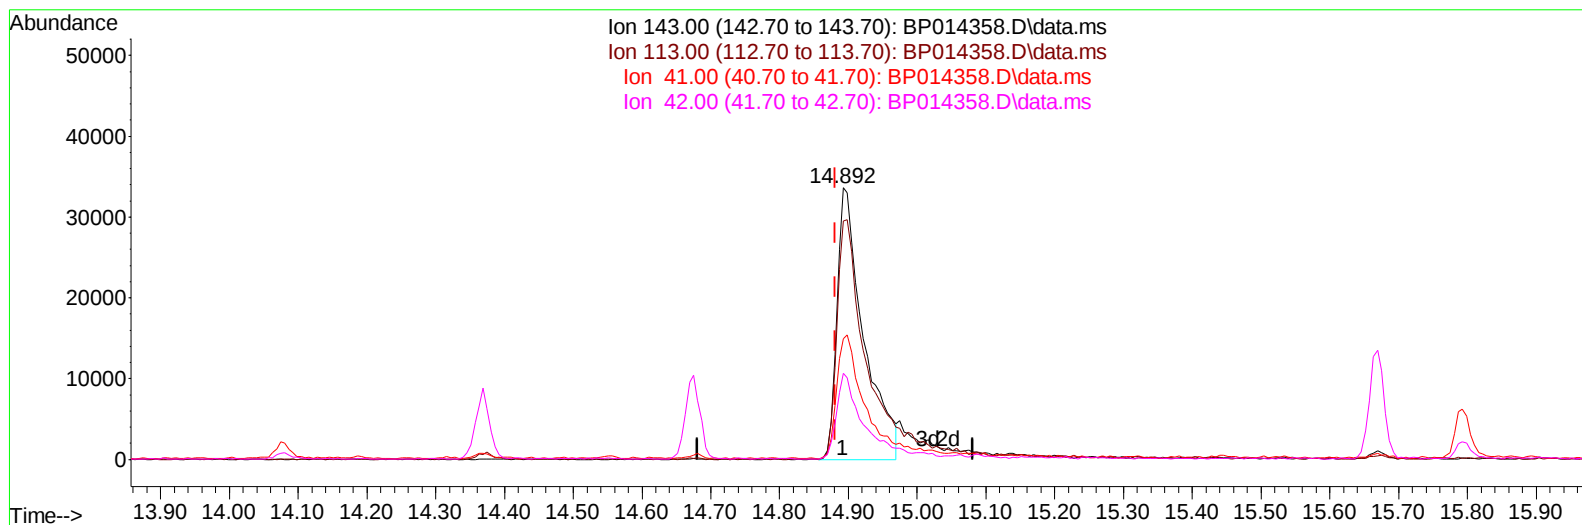

TIC: BP014358.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.892min (+ 0.012) 17.15 ng/u1

response 90005

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	87.72
41.00	44.20	44.57
42.00	31.50	31.65




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014358.D
Acq On : 29 Mar 2023 12:01
Operator : CG/JU
Sample : 01982-11
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYGC0

Manual IntegrationsAPPROVED

Quant Time: Mar 30 01:01:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 30 00:56:20 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/30/2023
Supervised By :Jagrut Upadhyay 03/30/2023

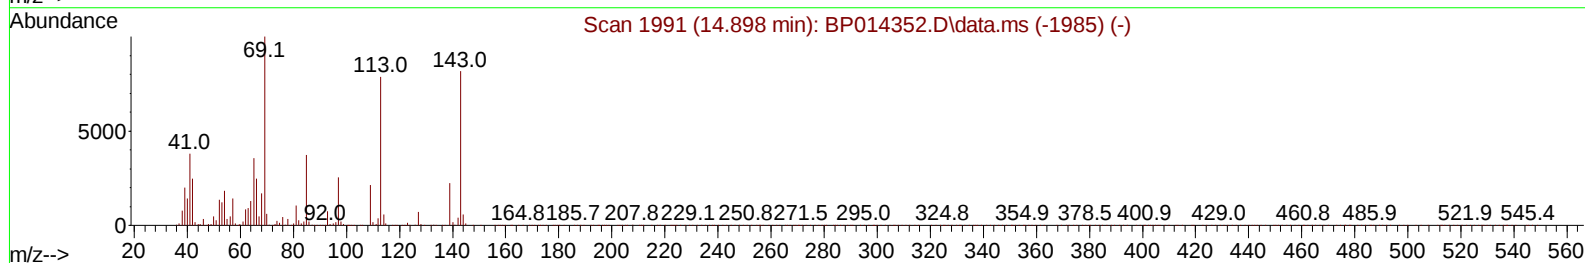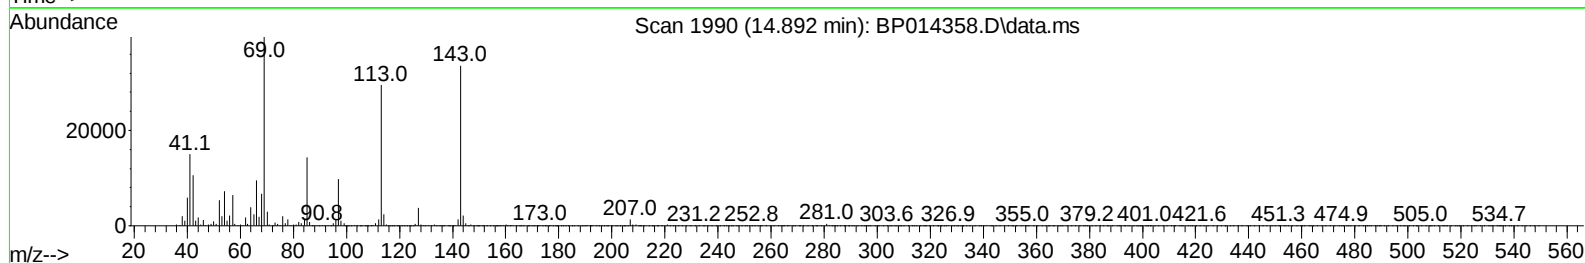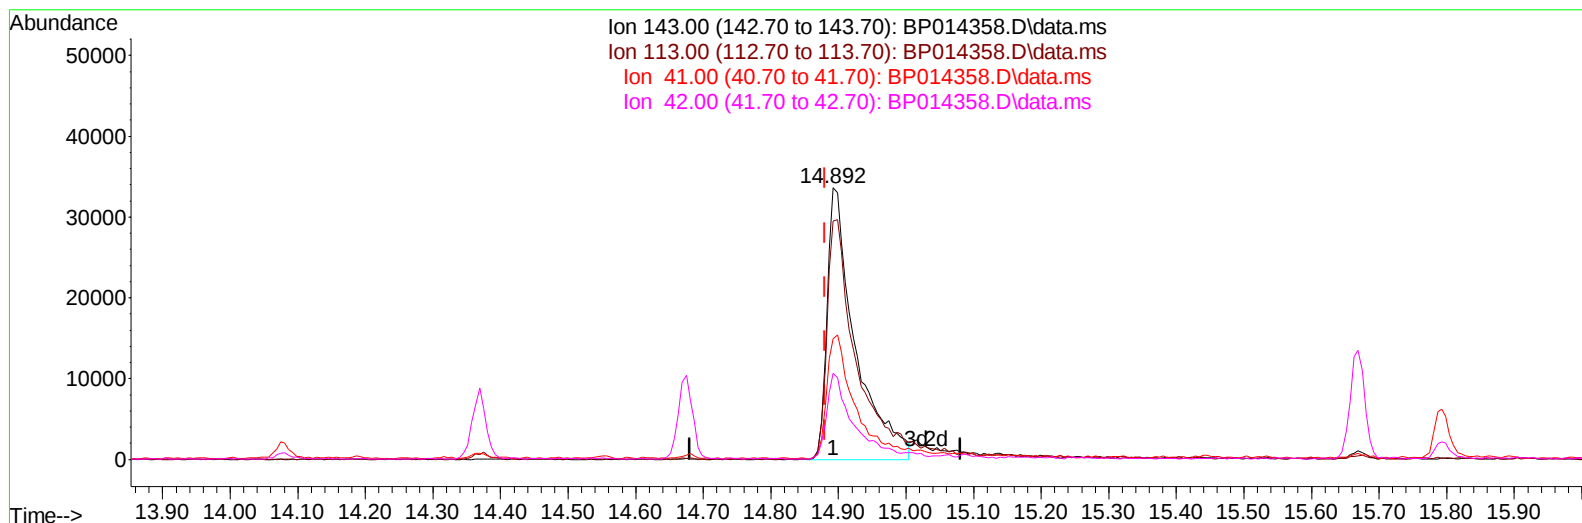

TIC: BP014358.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.892min (+ 0.012) 18.42 ng/ul m

response 96683

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	87.72
41.00	44.20	44.57
42.00	31.50	31.65

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
 Data File : BP014358.D
 Acq On : 29 Mar 2023 12:01
 Operator : CG/JU
 Sample : 01982-11
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EYGC0

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/30/2023
 Supervised By :Jagrut Upadhyay 03/30/2023

Quant Time: Mar 30 01:01:08 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 30 00:56:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.022	152	141476	20.000	ng/ul	0.00
20) Naphthalene-d8	10.846	136	631320	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.675	164	428460	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.434	188	1000666	20.000	ng/ul	0.00
79) Chrysene-d12	21.522	240	963471	20.000	ng/ul	0.00
88) Perylene-d12	24.045	264	921775	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	14153	3.879	ng/uL	0.00
4) Pyridine-d5	3.828	84	167332	17.898	ng/ul	0.00
7) Phenol-d5	7.181	99	242027	18.550	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.346	67	186271	22.251	ng/ul	0.00
11) 2-Chlorophenol-d4	7.552	132	216933	23.004	ng/ul	0.00
15) 4-Methylphenol-d8	8.734	113	210289	19.981	ng/ul	0.00
21) Nitrobenzene-d5	9.199	128	109251	21.436	ng/ul	0.00
24) 2-Nitrophenol-d4	9.922	143	126445	21.667	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.469	165	222874	20.970	ng/ul	0.00
31) 4-Chloroaniline-d4	10.993	131	289412	20.673	ng/ul	0.00
46) Dimethylphthalate-d6	14.081	166	831726	23.941	ng/ul	0.00
49) Acenaphthylene-d8	14.369	160	891356	23.123	ng/ul	0.00
54) 4-Nitrophenol-d4	14.892	143	96683m	18.422	ng/ul	0.01
60) Fluorene-d10	15.669	176	720620	24.874	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.792	200	116088	15.766	ng/ul	0.00
73) Anthracene-d10	17.534	188	1149606	23.739	ng/ul	0.00
81) Pyrene-d10	19.763	212	1395925	21.570	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.880	264	1188241	24.263	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014358.D
Acq On : 29 Mar 2023 12:01
Operator : CG/JU
Sample : 01982-11
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYGC0

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/30/2023
Supervised By :Jagrut Upadhyay 03/30/2023

Quant Time: Mar 30 01:01:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 30 00:56:20 2023
Response via : Initial Calibration

