




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014362.D
Acq On : 29 Mar 2023 14:15
Operator : CG/JU
Sample : 01982-18
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYGC7

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/30/2023
Supervised By :Jagrut Upadhyay 03/30/2023

Quant Time: Mar 30 01:01:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 30 00:56:20 2023
Response via : Initial Calibration

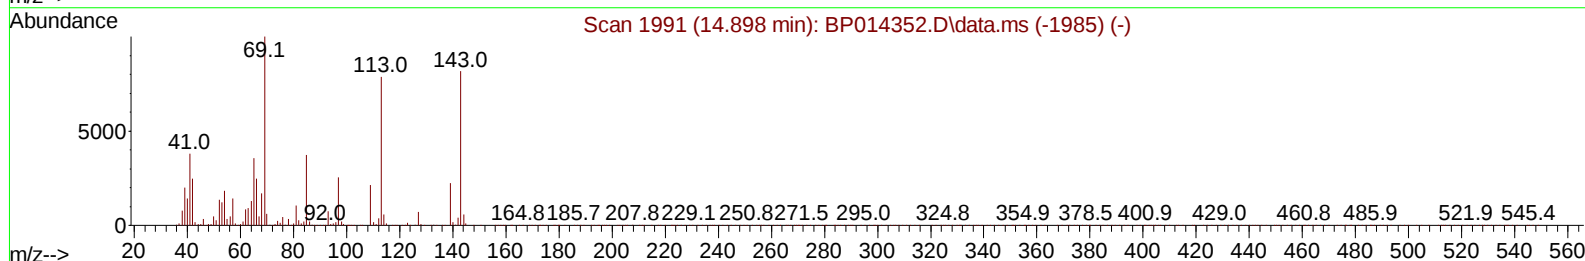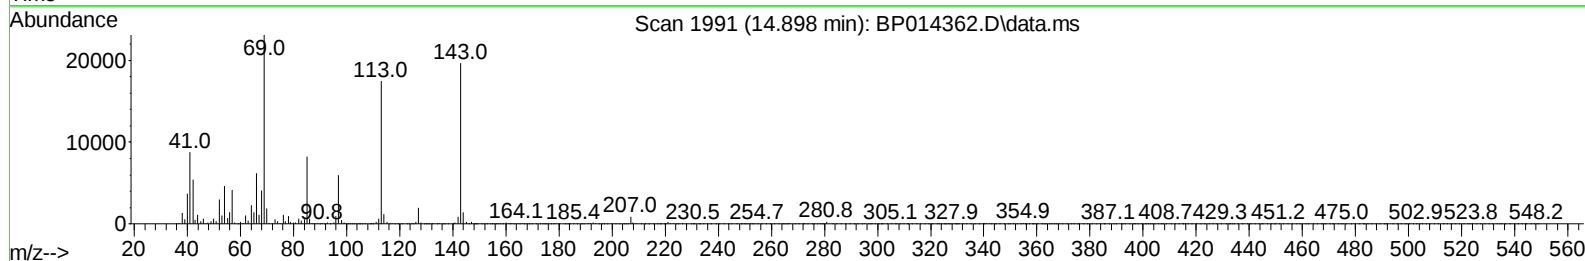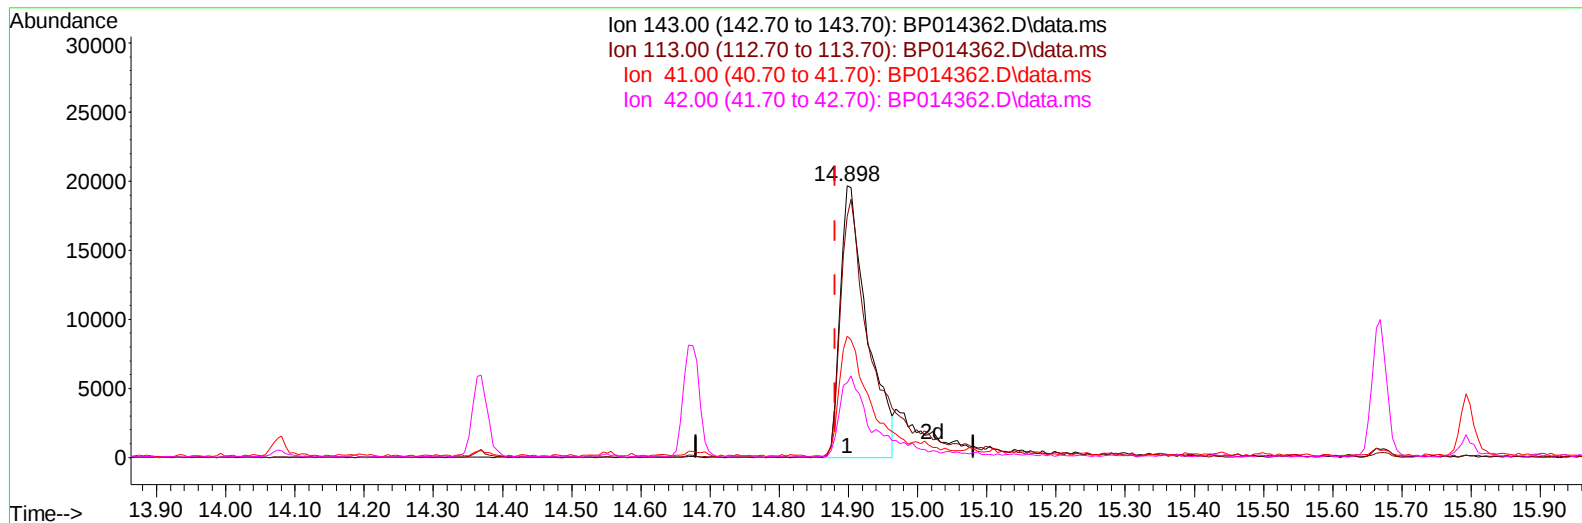

TIC: BP014362.D\data.ms

(54) 4-Nitrophenol-d4 (S)**14.898min (+ 0.018) 12.89 ng/u1****response 52955**

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	88.77
41.00	44.20	44.66
42.00	31.50	27.56




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014362.D
Acq On : 29 Mar 2023 14:15
Operator : CG/JU
Sample : 01982-18
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYGC7

Manual IntegrationsAPPROVED

Quant Time: Mar 30 01:01:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 30 00:56:20 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/30/2023
Supervised By :Jagrut Upadhyay 03/30/2023

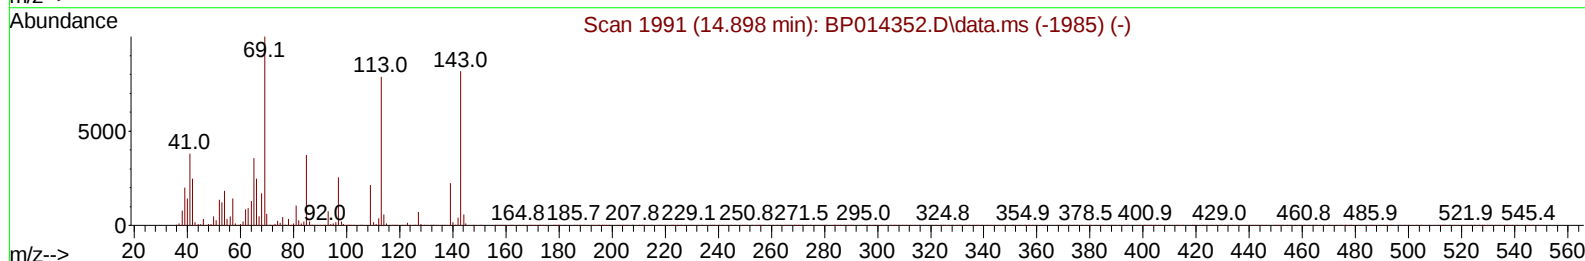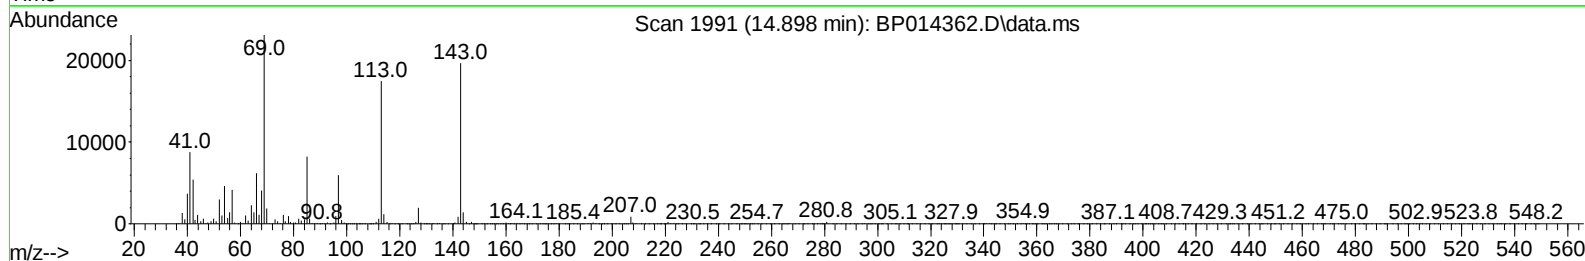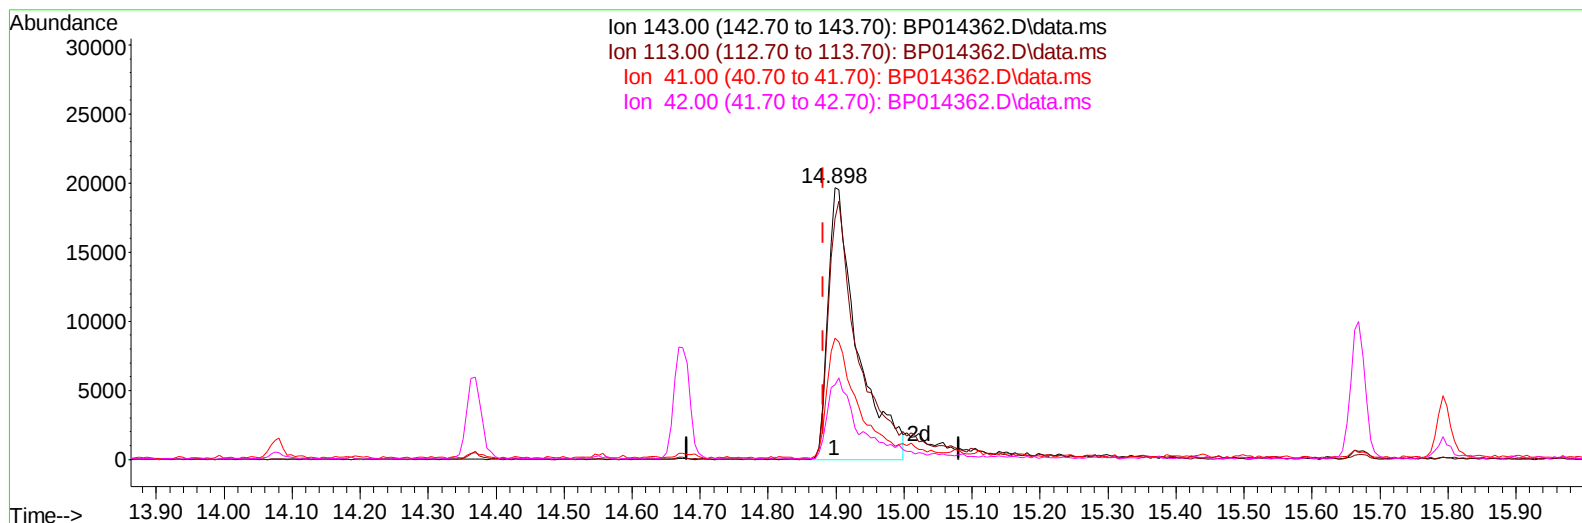

TIC: BP014362.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.898min (+ 0.018) 14.29 ng/ul m

response 58726

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	88.77
41.00	44.20	44.66
42.00	31.50	27.56

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
 Data File : BP014362.D
 Acq On : 29 Mar 2023 14:15
 Operator : CG/JU
 Sample : 01982-18
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EYGC7

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/30/2023
 Supervised By :Jagrut Upadhyay 03/30/2023

Quant Time: Mar 30 01:01:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 30 00:56:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.022	152	139014	20.000	ng/ul	0.00
20) Naphthalene-d8	10.846	136	606249	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.675	164	335396	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.433	188	932048	20.000	ng/ul	0.00
79) Chrysene-d12	21.521	240	904899	20.000	ng/ul	0.00
88) Perylene-d12	24.045	264	865421	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	14321	3.995	ng/uL	0.00
4) Pyridine-d5	3.828	84	160992	17.525	ng/ul	0.00
7) Phenol-d5	7.181	99	232683	18.149	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.346	67	161850	19.676	ng/ul	0.00
11) 2-Chlorophenol-d4	7.546	132	173562	18.731	ng/ul	0.00
15) 4-Methylphenol-d8	8.734	113	176523	17.069	ng/ul	0.00
21) Nitrobenzene-d5	9.199	128	89251	18.236	ng/ul	0.00
24) 2-Nitrophenol-d4	9.928	143	101623	18.134	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.469	165	174540	17.101	ng/ul	0.00
31) 4-Chloroaniline-d4	10.993	131	236363	17.582	ng/ul	0.00
46) Dimethylphthalate-d6	14.081	166	550317	20.236	ng/ul	0.00
49) Acenaphthylene-d8	14.369	160	588806	19.513	ng/ul	0.00
54) 4-Nitrophenol-d4	14.898	143	58726m	14.294	ng/ul	0.02
60) Fluorene-d10	15.669	176	480479	21.187	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.792	200	75962	11.076	ng/ul	0.00
73) Anthracene-d10	17.533	188	919626	20.388	ng/ul	0.00
81) Pyrene-d10	19.763	212	1120216	18.430	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.880	264	941728	20.482	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014362.D
Acq On : 29 Mar 2023 14:15
Operator : CG/JU
Sample : 01982-18
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYGC7

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/30/2023
Supervised By :Jagrut Upadhyay 03/30/2023

Quant Time: Mar 30 01:01:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 30 00:56:20 2023
Response via : Initial Calibration

