




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
 Data File : BP014371.D
 Acq On : 29 Mar 2023 19:53
 Operator : CG/JU
 Sample : 02067-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFZ73

Manual IntegrationsAPPROVED

Quant Time: Mar 30 01:04:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 30 00:56:20 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/30/2023
 Supervised By :Jagrut Upadhyay 03/30/2023

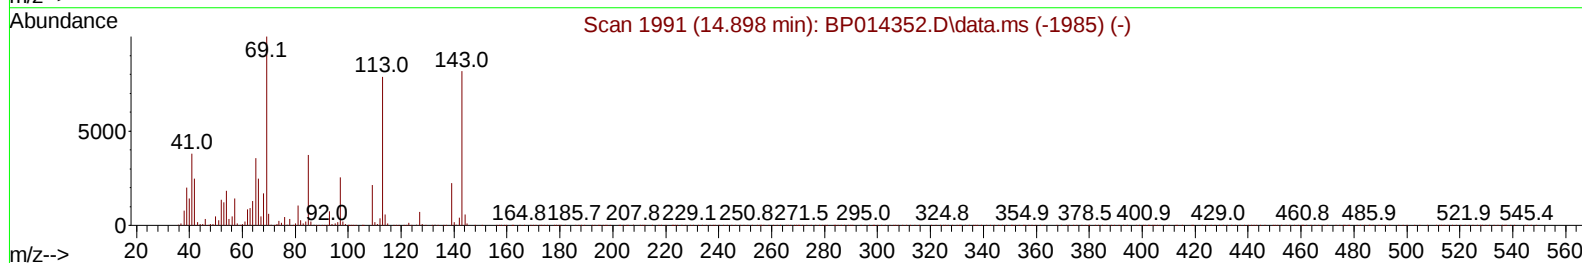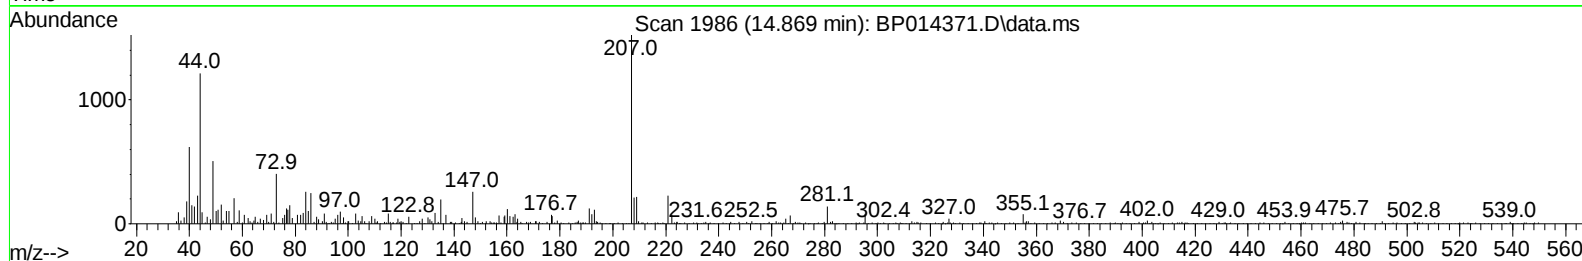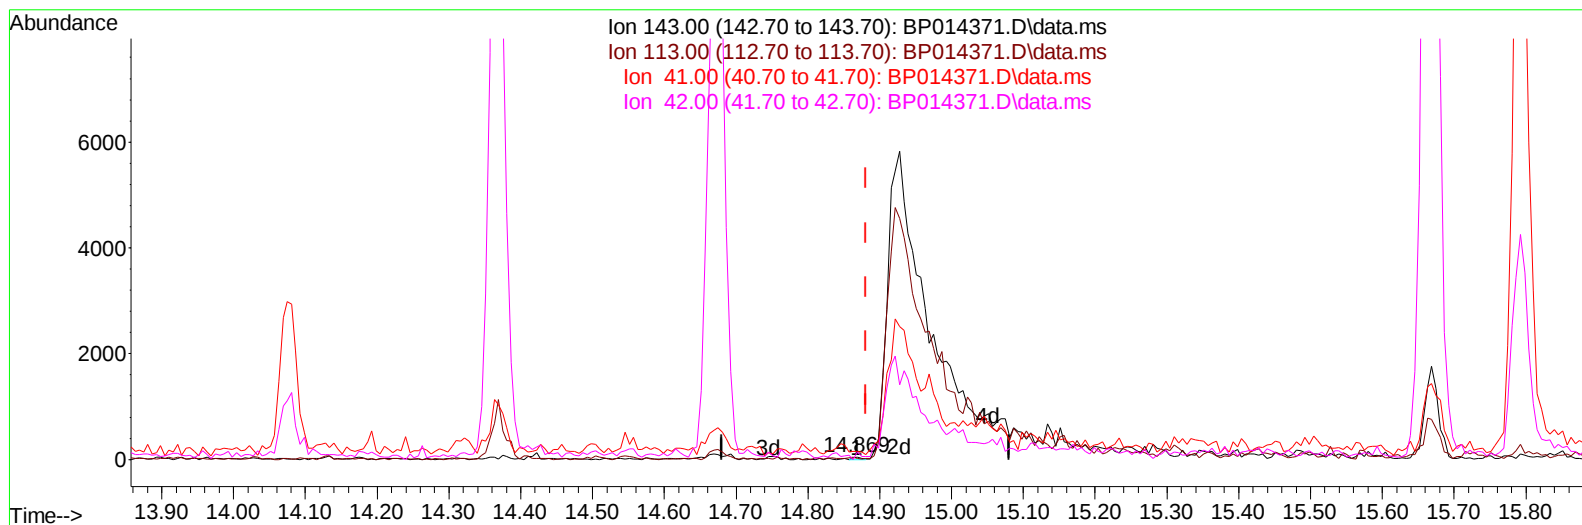

TIC: BP014371.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.869min (-0.012) 0.01 ng/u1

response 38

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	36.17#
41.00	44.20	319.15#
42.00	31.50	300.00#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014371.D
Acq On : 29 Mar 2023 19:53
Operator : CG/JU
Sample : 02067-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFZ73

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/30/2023
Supervised By :Jagrut Upadhyay 03/30/2023

Quant Time: Mar 30 01:04:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 30 00:56:20 2023
Response via : Initial Calibration

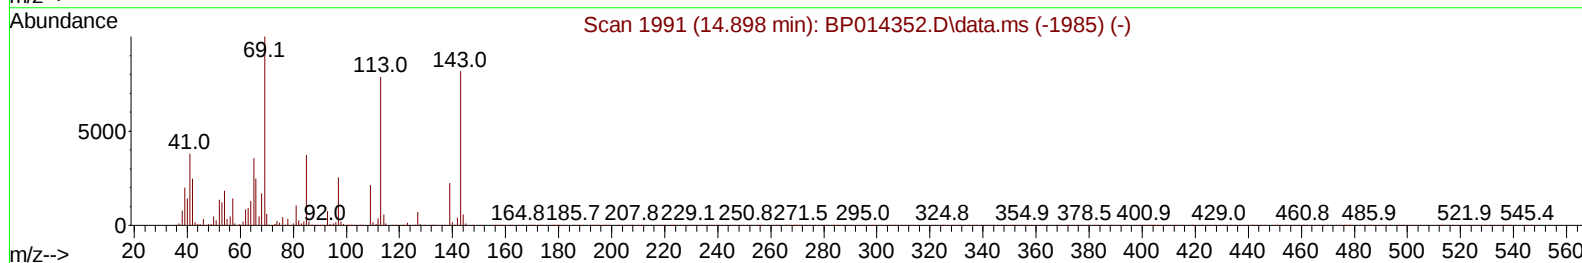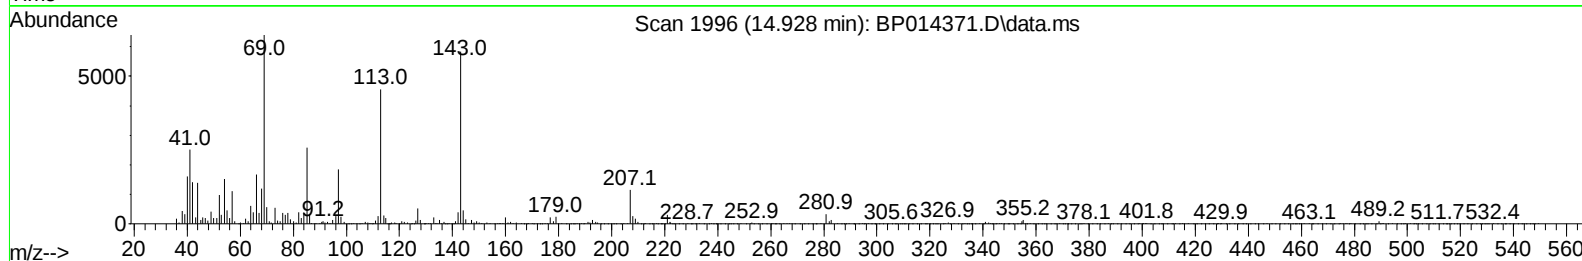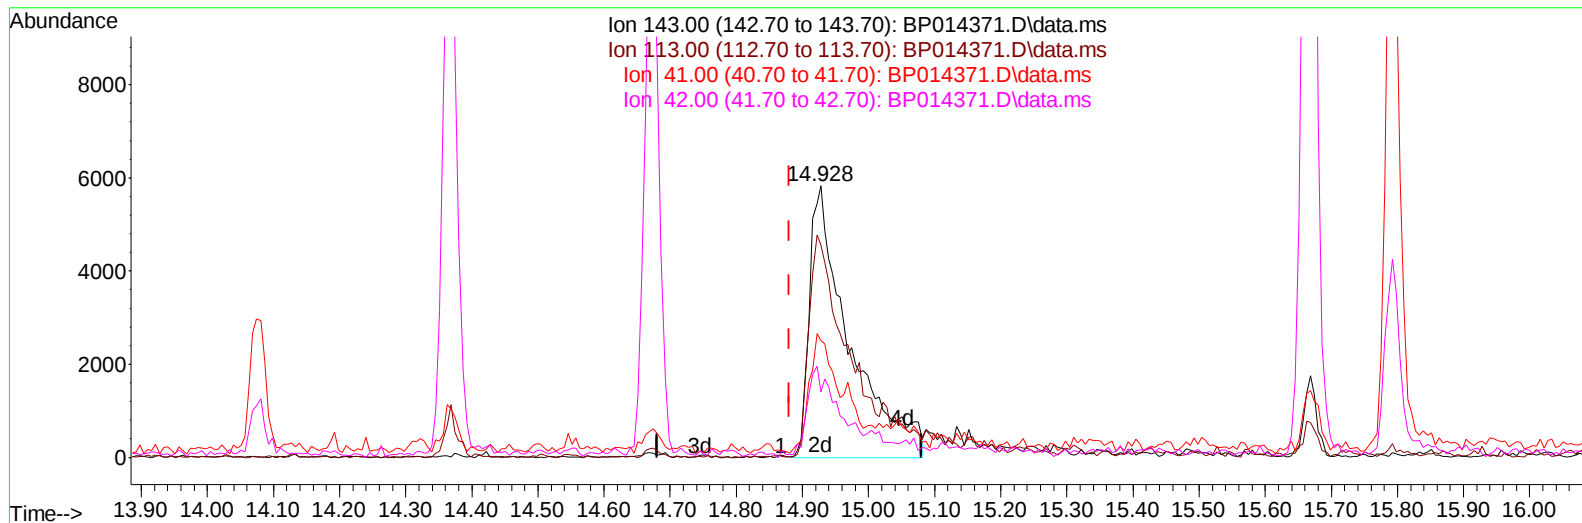

TIC: BP014371.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.928min (+ 0.047) 3.99 ng/ul m

response 24296

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	78.24
41.00	44.20	43.02
42.00	31.50	24.25#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
 Data File : BP014371.D
 Acq On : 29 Mar 2023 19:53
 Operator : CG/JU
 Sample : 02067-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFZ73

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/30/2023
 Supervised By :Jagrut Upadhyay 03/30/2023

Quant Time: Mar 30 01:04:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 30 00:56:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.022	152	172466	20.000	ng/ul	0.00
20) Naphthalene-d8	10.846	136	744893	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.675	164	497412	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.433	188	1098791	20.000	ng/ul	0.00
79) Chrysene-d12	21.521	240	803970	20.000	ng/ul	0.00
88) Perylene-d12	24.045	264	782375	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	17886	4.022	ng/uL	0.00
4) Pyridine-d5	3.834	84	82167	7.209	ng/ul	0.01
7) Phenol-d5	7.181	99	76562	4.814	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.346	67	305455	29.931	ng/ul	0.00
11) 2-Chlorophenol-d4	7.546	132	240934	20.958	ng/ul	0.00
15) 4-Methylphenol-d8	8.734	113	160274	12.492	ng/ul	0.00
21) Nitrobenzene-d5	9.199	128	175508	29.186	ng/ul	0.00
24) 2-Nitrophenol-d4	9.922	143	191303	27.782	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.463	165	312816	24.945	ng/ul	0.00
31) 4-Chloroaniline-d4	10.987	131	382331	23.146	ng/ul	0.00
46) Dimethylphthalate-d6	14.081	166	1360379	33.730	ng/ul	0.00
49) Acenaphthylene-d8	14.369	160	1367076	30.548	ng/ul	0.00
54) 4-Nitrophenol-d4	14.928	143	24296m	3.988	ng/ul	0.05
60) Fluorene-d10	15.669	176	1140808	33.919	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.792	200	226738	28.044	ng/ul	0.00
73) Anthracene-d10	17.533	188	1937680	36.439	ng/ul	0.00
81) Pyrene-d10	19.763	212	2085416	38.617	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.880	264	1559487	37.517	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014371.D
Acq On : 29 Mar 2023 19:53
Operator : CG/JU
Sample : 02067-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFZ73

Manual IntegrationsAPPROVED

Quant Time: Mar 30 01:04:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 30 00:56:20 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/30/2023
Supervised By :Jagrut Upadhyay 03/30/2023

