




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014373.D
Acq On : 29 Mar 2023 21:00
Operator : CG/JU
Sample : 02067-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFZ83

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/30/2023
Supervised By :Jagrut Upadhyay 03/30/2023

Quant Time: Mar 30 01:05:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 30 00:56:20 2023
Response via : Initial Calibration

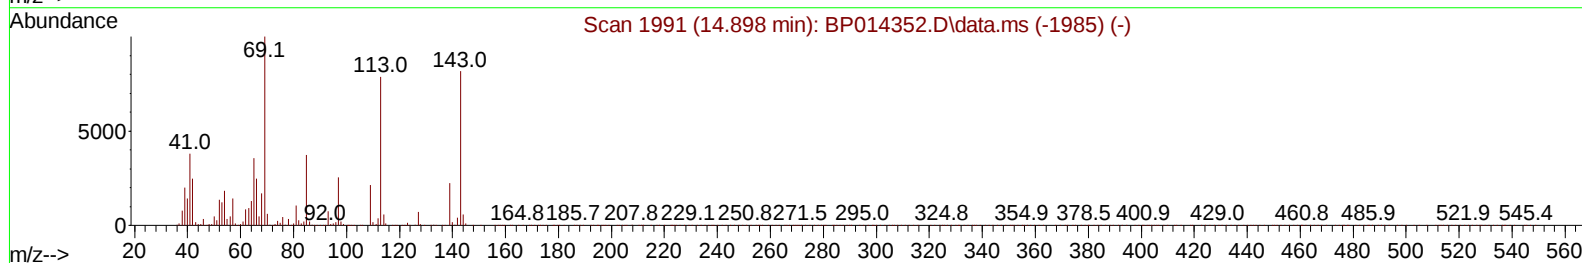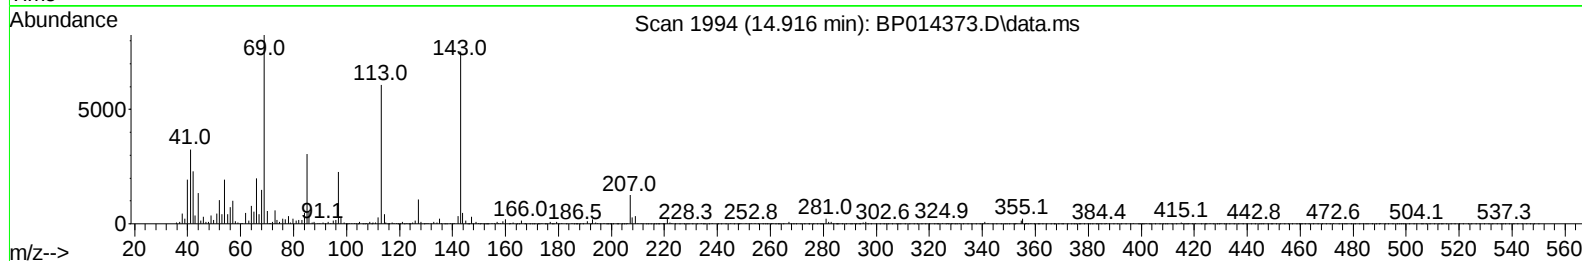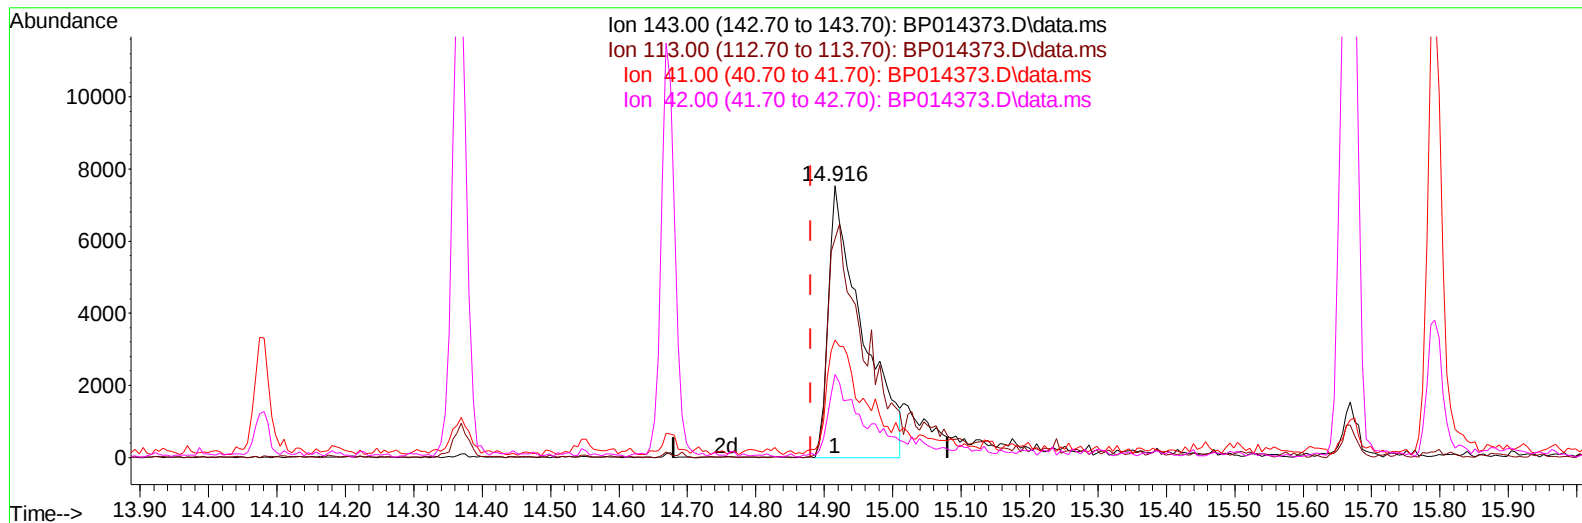

TIC: BP014373.D\data.ms

(54) 4-Nitrophenol-d4 (S)**14.916min (+ 0.036) 4.72 ng/u1****response 25663**

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	80.49
41.00	44.20	43.19
42.00	31.50	30.56




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014373.D
Acq On : 29 Mar 2023 21:00
Operator : CG/JU
Sample : 02067-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFZ83

Manual IntegrationsAPPROVED

Quant Time: Mar 30 01:05:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 30 00:56:20 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/30/2023
Supervised By :Jagrut Upadhyay 03/30/2023

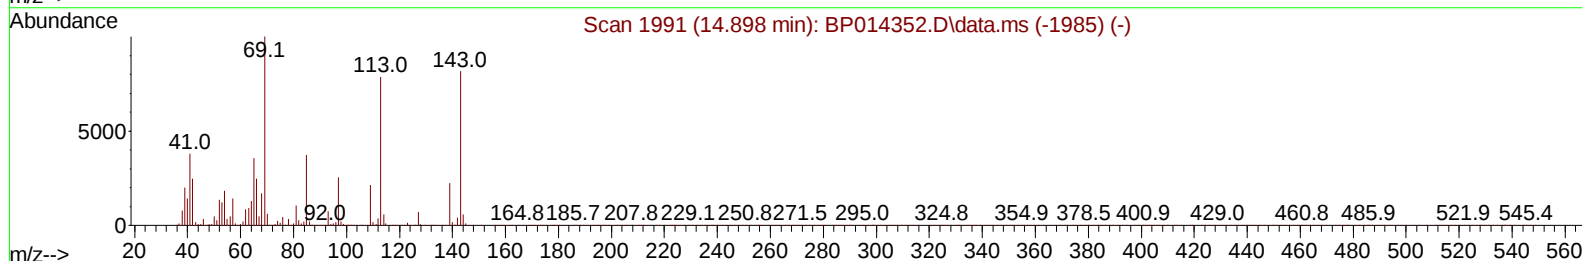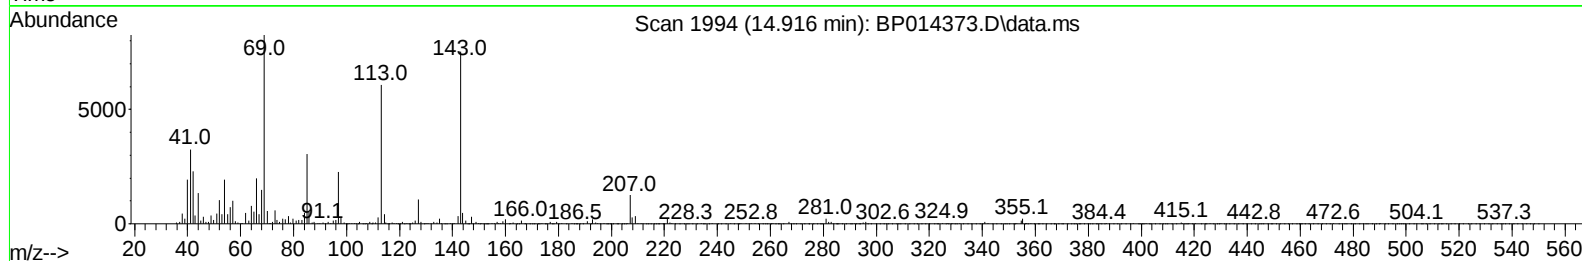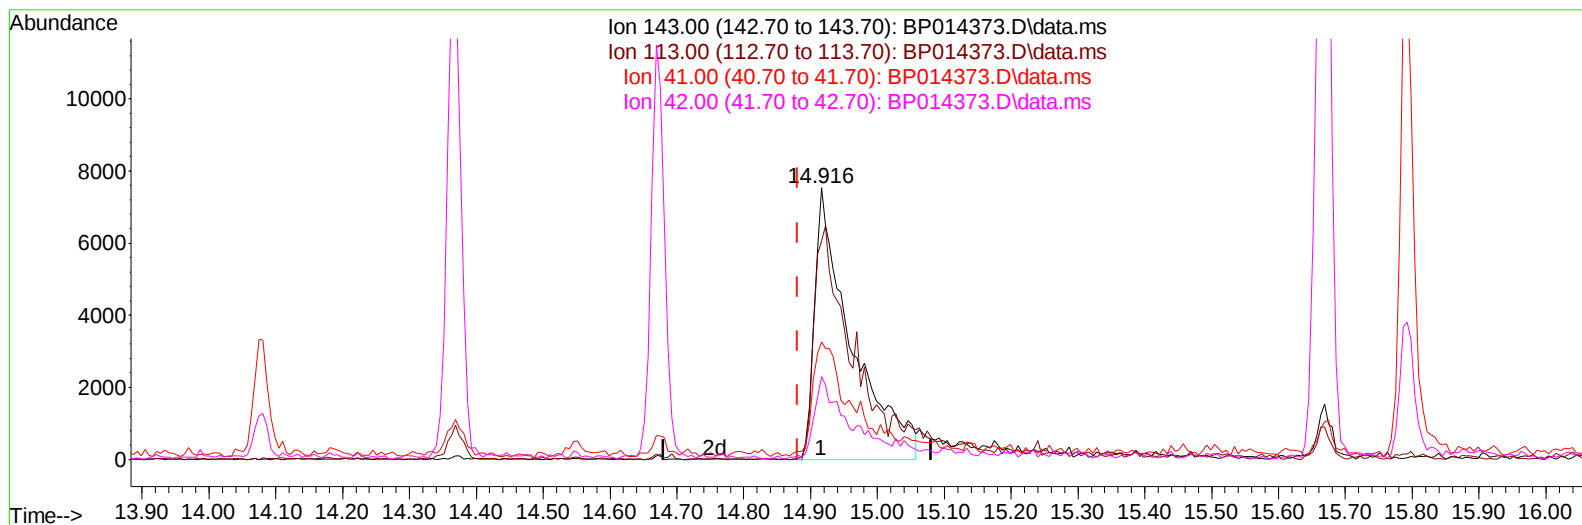

TIC: BP014373.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.916min (+ 0.036) 5.29 ng/ul m

response 28761

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	80.49
41.00	44.20	43.19
42.00	31.50	30.56

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
 Data File : BP014373.D
 Acq On : 29 Mar 2023 21:00
 Operator : CG/JU
 Sample : 02067-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFZ83

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/30/2023
 Supervised By :Jagrut Upadhyay 03/30/2023

Quant Time: Mar 30 01:05:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 30 00:56:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	154138	20.000	ng/ul	0.00
20) Naphthalene-d8	10.840	136	663764	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.675	164	443669	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.434	188	1007837	20.000	ng/ul	0.00
79) Chrysene-d12	21.522	240	921257	20.000	ng/ul	0.00
88) Perylene-d12	24.045	264	884639	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	18709	4.707	ng/uL	0.00
4) Pyridine-d5	3.828	84	107481	10.552	ng/ul	0.00
7) Phenol-d5	7.181	99	93392	6.570	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.340	67	318178	34.885	ng/ul	0.00
11) 2-Chlorophenol-d4	7.546	132	268789	26.161	ng/ul	0.00
15) 4-Methylphenol-d8	8.734	113	190886	16.647	ng/ul	0.00
21) Nitrobenzene-d5	9.193	128	184610	34.452	ng/ul	0.00
24) 2-Nitrophenol-d4	9.922	143	205324	33.463	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.463	165	332404	29.747	ng/ul	0.00
31) 4-Chloroaniline-d4	10.987	131	425428	28.903	ng/ul	0.00
46) Dimethylphthalate-d6	14.081	166	1376814	38.273	ng/ul	0.00
49) Acenaphthylene-d8	14.369	160	1395962	34.972	ng/ul	0.00
54) 4-Nitrophenol-d4	14.916	143	28761m	5.292	ng/ul	0.04
60) Fluorene-d10	15.669	176	1143716	38.125	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.793	200	223286	30.109	ng/ul	0.00
73) Anthracene-d10	17.534	188	1938901	39.752	ng/ul	0.00
81) Pyrene-d10	19.763	212	2296829	37.117	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.880	264	1913195	40.706	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014373.D
Acq On : 29 Mar 2023 21:00
Operator : CG/JU
Sample : 02067-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFZ83

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/30/2023
Supervised By :Jagrut Upadhyay 03/30/2023

Quant Time: Mar 30 01:05:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 30 00:56:20 2023
Response via : Initial Calibration

