




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
 Data File : BP014388.D
 Acq On : 30 Mar 2023 05:57
 Operator : CG/JU
 Sample : 02038-03
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EYF61

Manual IntegrationsAPPROVED

Quant Time: Mar 30 06:43:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 30 00:56:20 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/30/2023
 Supervised By :Jagrut Upadhyay 03/30/2023

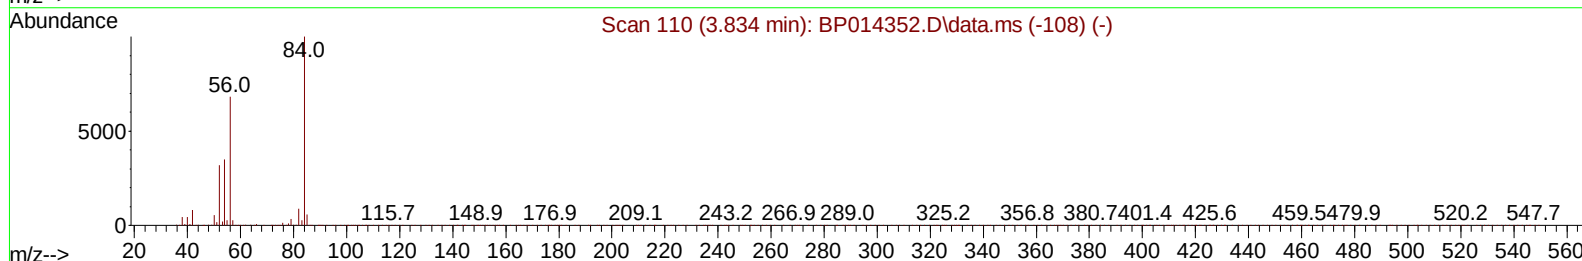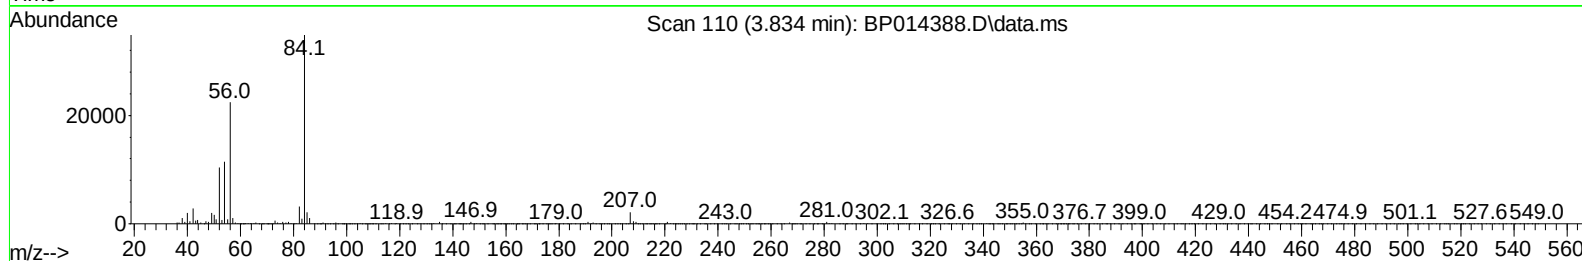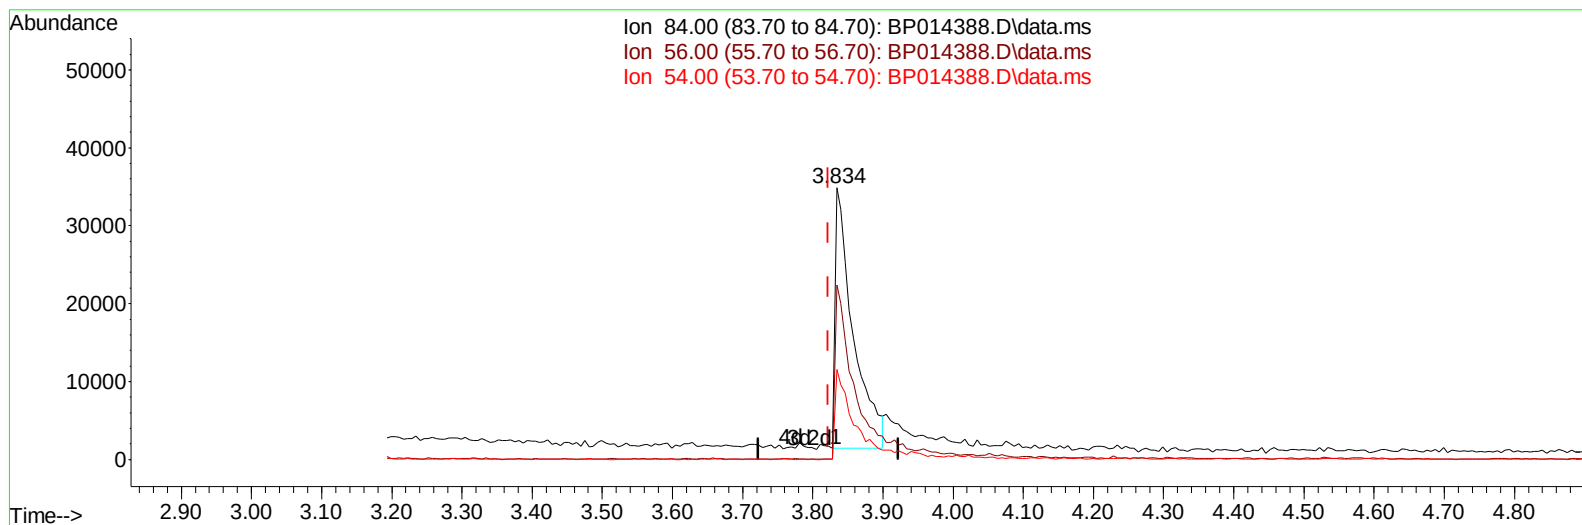

TIC: BP014388.D\data.ms

(4) Pyridine-d5 (S)

3.834min (+ 0.012) 6.00 ng/uL

response 59316

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.70	64.36
54.00	32.60	33.04
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014388.D
Acq On : 30 Mar 2023 05:57
Operator : CG/JU
Sample : 02038-03
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYF61

Manual IntegrationsAPPROVED

Quant Time: Mar 30 06:43:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 30 00:56:20 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/30/2023
Supervised By :Jagrut Upadhyay 03/30/2023

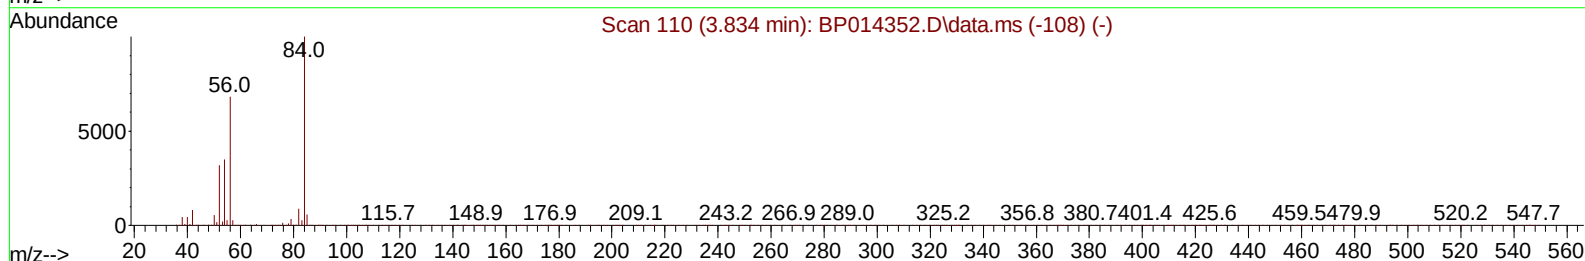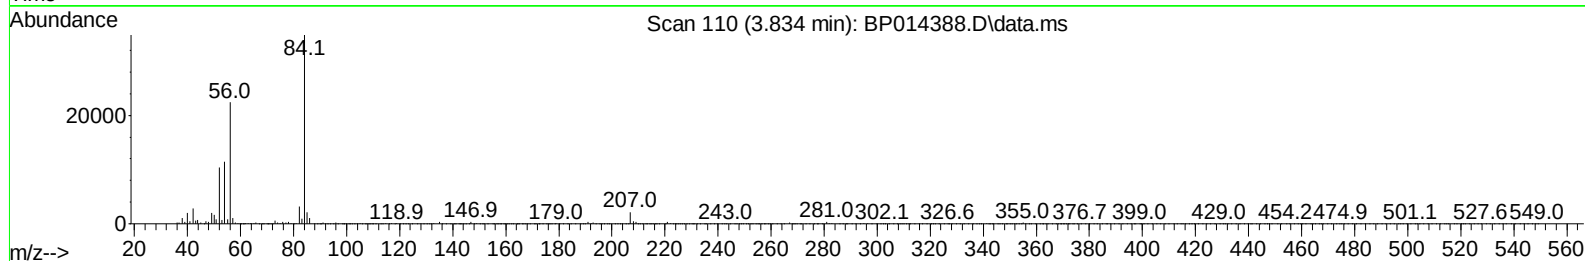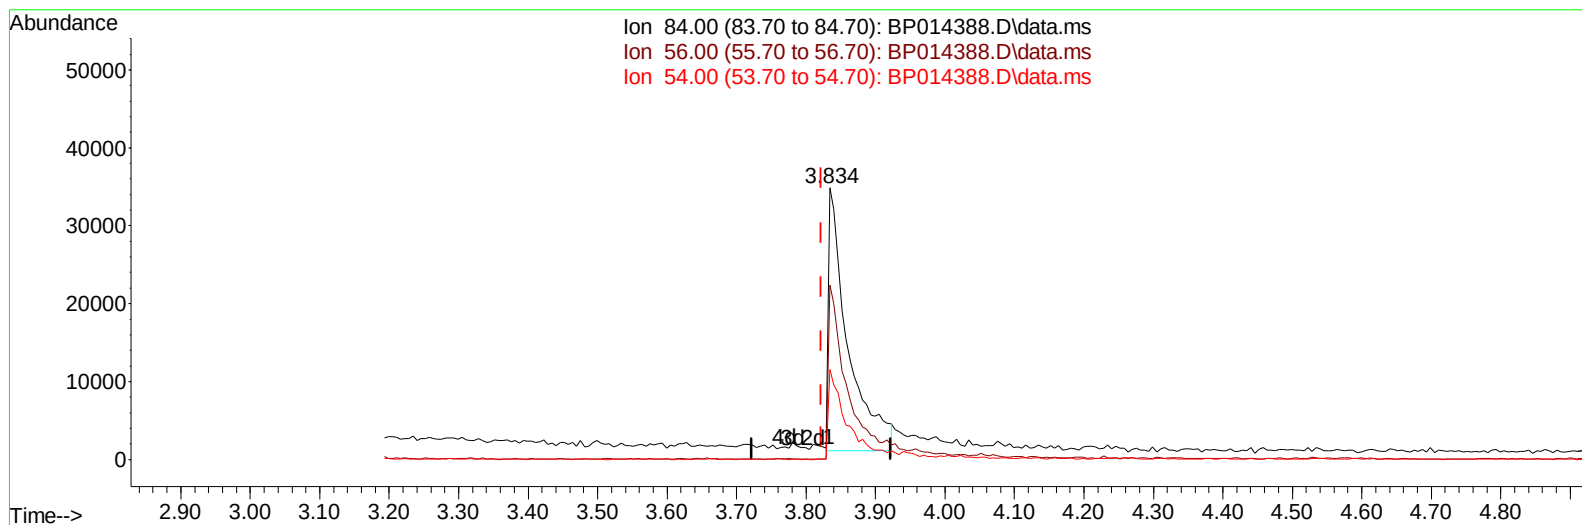

TIC: BP014388.D\data.ms

(4) Pyridine-d5 (S)

3.834min (+ 0.012) 6.70 ng/ul m

response 66145

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.70	64.36
54.00	32.60	33.04
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014388.D
Acq On : 30 Mar 2023 05:57
Operator : CG/JU
Sample : 02038-03
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYF61

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/30/2023
Supervised By :Jagrut Upadhyay 03/30/2023

Quant Time: Mar 30 06:43:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 30 00:56:20 2023
Response via : Initial Calibration

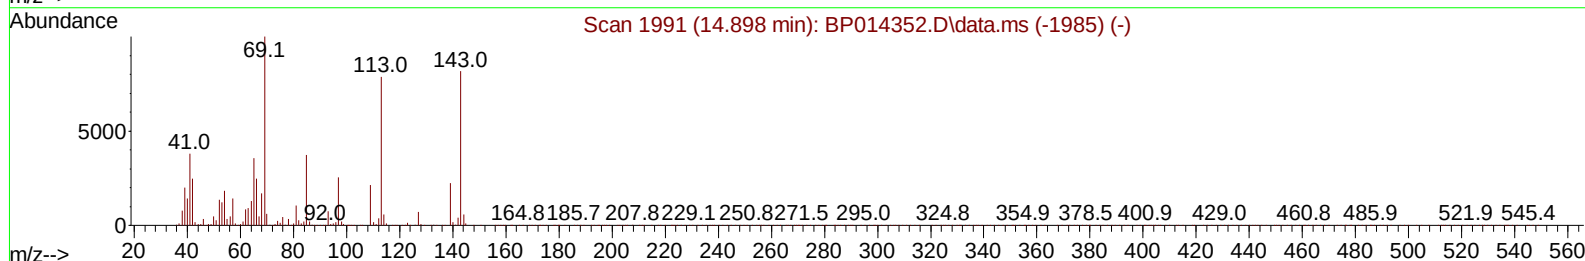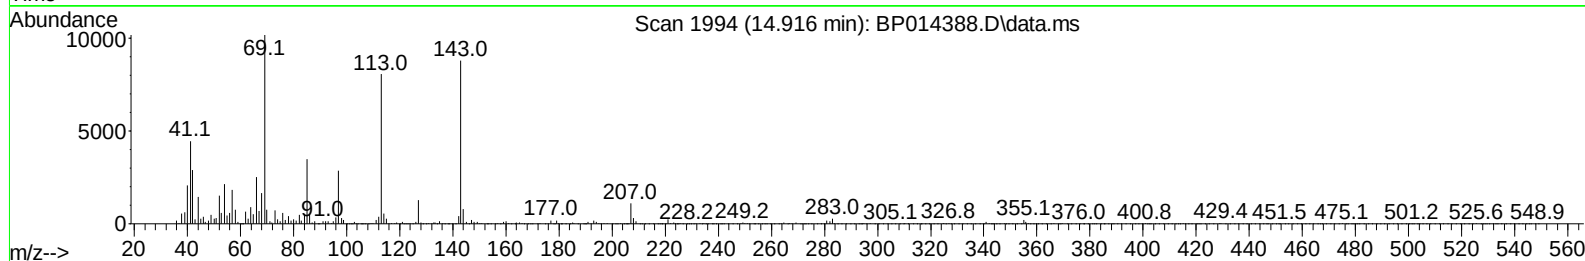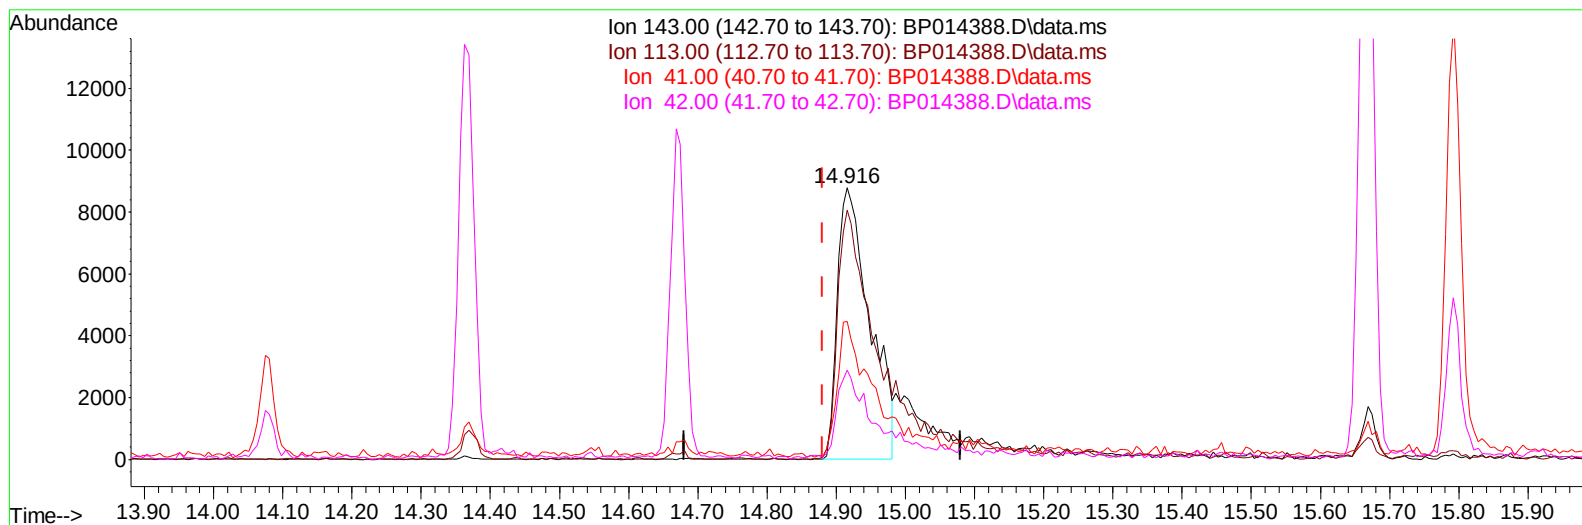

TIC: BP014388.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.916min (+ 0.035) 5.29 ng/ul

response 28410

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	91.77
41.00	44.20	50.77
42.00	31.50	32.87




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014388.D
Acq On : 30 Mar 2023 05:57
Operator : CG/JU
Sample : 02038-03
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYF61

Manual IntegrationsAPPROVED

Quant Time: Mar 30 06:43:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 30 00:56:20 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/30/2023
Supervised By :Jagrut Upadhyay 03/30/2023

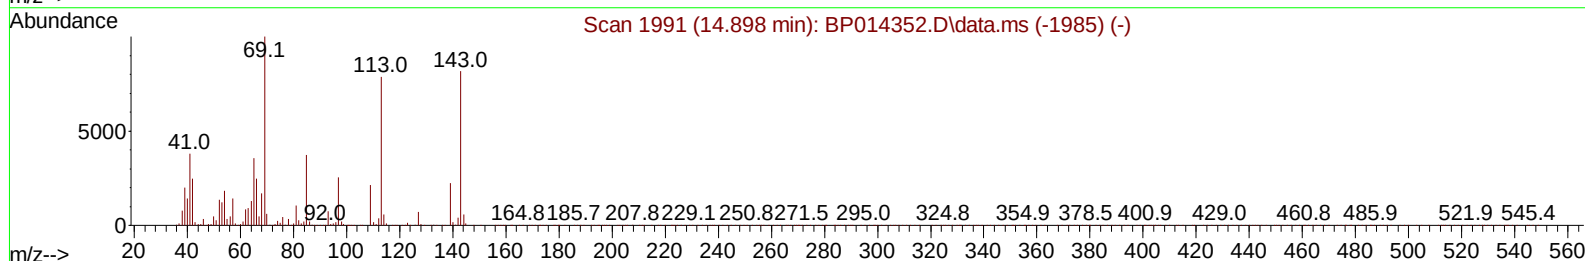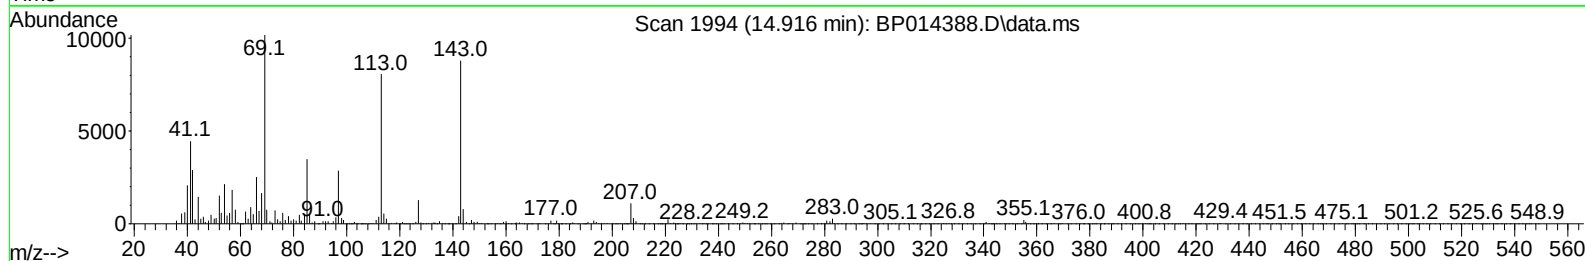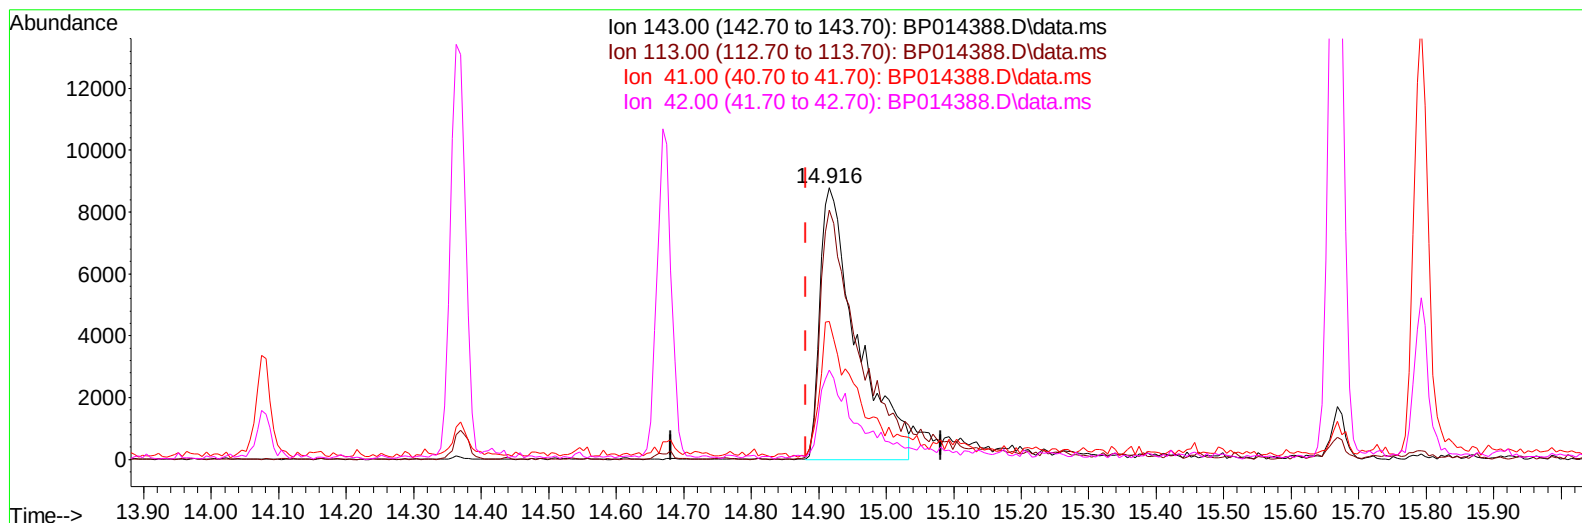

TIC: BP014388.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.916min (+ 0.035) 6.25 ng/ul m

response 33557

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	91.77
41.00	44.20	50.77
42.00	31.50	32.87

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
 Data File : BP014388.D
 Acq On : 30 Mar 2023 05:57
 Operator : CG/JU
 Sample : 02038-03
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EYF61

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/30/2023
 Supervised By :Jagrut Upadhyay 03/30/2023

Quant Time: Mar 30 06:43:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 30 00:56:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	149494	20.000	ng/ul	0.00
20) Naphthalene-d8	10.840	136	640335	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.675	164	438084	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.433	188	1043683	20.000	ng/ul	0.00
79) Chrysene-d12	21.522	240	981271	20.000	ng/ul	0.00
88) Perylene-d12	24.045	264	946255	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	18745	4.863	ng/uL	0.00
4) Pyridine-d5	3.834	84	66145m	6.696	ng/ul	0.01
7) Phenol-d5	7.181	99	103745	7.525	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.340	67	327323	37.003	ng/ul	0.00
11) 2-Chlorophenol-d4	7.546	132	280596	28.159	ng/ul	0.00
15) 4-Methylphenol-d8	8.734	113	207751	18.681	ng/ul	0.00
21) Nitrobenzene-d5	9.193	128	193912	37.512	ng/ul	0.00
24) 2-Nitrophenol-d4	9.922	143	214914	36.308	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.463	165	352761	32.723	ng/ul	0.00
31) 4-Chloroaniline-d4	10.987	131	401003	28.241	ng/ul	0.00
46) Dimethylphthalate-d6	14.081	166	1427359	40.184	ng/ul	0.00
49) Acenaphthylene-d8	14.369	160	1438138	36.488	ng/ul	0.00
54) 4-Nitrophenol-d4	14.916	143	33557m	6.253	ng/ul	0.04
60) Fluorene-d10	15.669	176	1174152	39.638	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.792	200	245416	31.957	ng/ul	0.00
73) Anthracene-d10	17.533	188	2058310	40.751	ng/ul	0.00
81) Pyrene-d10	19.763	212	2470622	37.484	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.880	264	2114035	42.050	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014388.D
Acq On : 30 Mar 2023 05:57
Operator : CG/JU
Sample : 02038-03
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYF61

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/30/2023
Supervised By :Jagrut Upadhyay 03/30/2023

Quant Time: Mar 30 06:43:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 30 00:56:20 2023
Response via : Initial Calibration

