

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
 Data File : BP014370.D
 Acq On : 29 Mar 2023 19:19
 Operator : CG/JU
 Sample : PB151680BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK680

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014370.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	42	rVB	51521	73764	1.38%	0.140%
2	3.823	106	108	133	rBV	533207	911541	17.03%	1.734%
3	4.146	160	163	169	rVB2	10323	13635	0.25%	0.026%
4	7.175	672	678	693	rBV	796812	1370096	25.60%	2.606%
5	7.346	700	707	720	rBV	647659	1043543	19.50%	1.985%
6	7.546	732	741	757	rBV	836165	1380728	25.79%	2.626%
7	8.016	810	821	837	rBV	582413	973734	18.19%	1.852%
8	8.734	936	943	964	rBV	1032354	1734476	32.40%	3.299%
9	9.193	1014	1021	1043	rBV	815952	1404505	26.24%	2.672%
10	9.922	1136	1145	1160	rBV	728581	1232358	23.02%	2.344%
11	10.463	1229	1237	1264	rBV	920533	1787021	33.38%	3.399%
12	10.846	1293	1302	1315	rBV	830593	1439527	26.89%	2.738%
13	10.987	1318	1326	1346	rBV	868678	1702325	31.80%	3.238%
14	12.393	1557	1565	1568	rBV4	8657	14562	0.27%	0.028%
15	12.446	1569	1574	1582	rVB3	11970	28471	0.53%	0.054%
16	13.551	1757	1762	1768	rBV6	8087	16255	0.30%	0.031%
17	14.081	1845	1852	1867	rBV	1965913	2864550	53.52%	5.449%
18	14.369	1893	1901	1915	rBV	2203438	3230711	60.36%	6.145%
19	14.675	1945	1953	1962	rBV	1407552	2088654	39.02%	3.973%
20	14.887	1982	1989	2014	rBV	456370	1251466	23.38%	2.380%
21	15.669	2115	2122	2137	rBV	2816264	4072949	76.09%	7.747%
22	15.792	2137	2143	2159	rVV	1057511	1545279	28.87%	2.939%
23	15.916	2159	2164	2168	rVB4	15589	27444	0.51%	0.052%
24	16.457	2253	2256	2266	rVB4	4457	9730	0.18%	0.019%
25	17.116	2364	2368	2371	rVB6	4363	6472	0.12%	0.012%
26	17.222	2383	2386	2392	rVB7	3783	6364	0.12%	0.012%
27	17.434	2415	2422	2432	rBV	1863655	2594320	48.47%	4.935%
28	17.534	2433	2439	2458	rVV	3128403	4544226	84.89%	8.644%
29	19.339	2742	2746	2752	rBV2	41252	59151	1.11%	0.113%
30	19.410	2755	2758	2766	rVB	34826	54527	1.02%	0.104%
31	19.663	2799	2801	2807	rBV6	10777	17041	0.32%	0.032%
32	19.763	2812	2818	2827	rBV	4065917	5352768	100.00%	10.182%
33	21.522	3112	3117	3126	rBV	1963926	2741488	51.22%	5.215%
34	23.880	3511	3518	3531	rVB2	2287193	4594072	85.83%	8.739%
35	24.045	3539	3546	3558	rVB	1066428	2384687	44.55%	4.536%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014370.D
Acq On : 29 Mar 2023 19:19
Operator : CG/JU
Sample : PB151680BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK680

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Title : SVOA CALIBRATION




Sum of corrected areas: 52572440

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014370.D
Acq On : 29 Mar 2023 19:19
Operator : CG/JU
Sample : PB151680BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK680

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

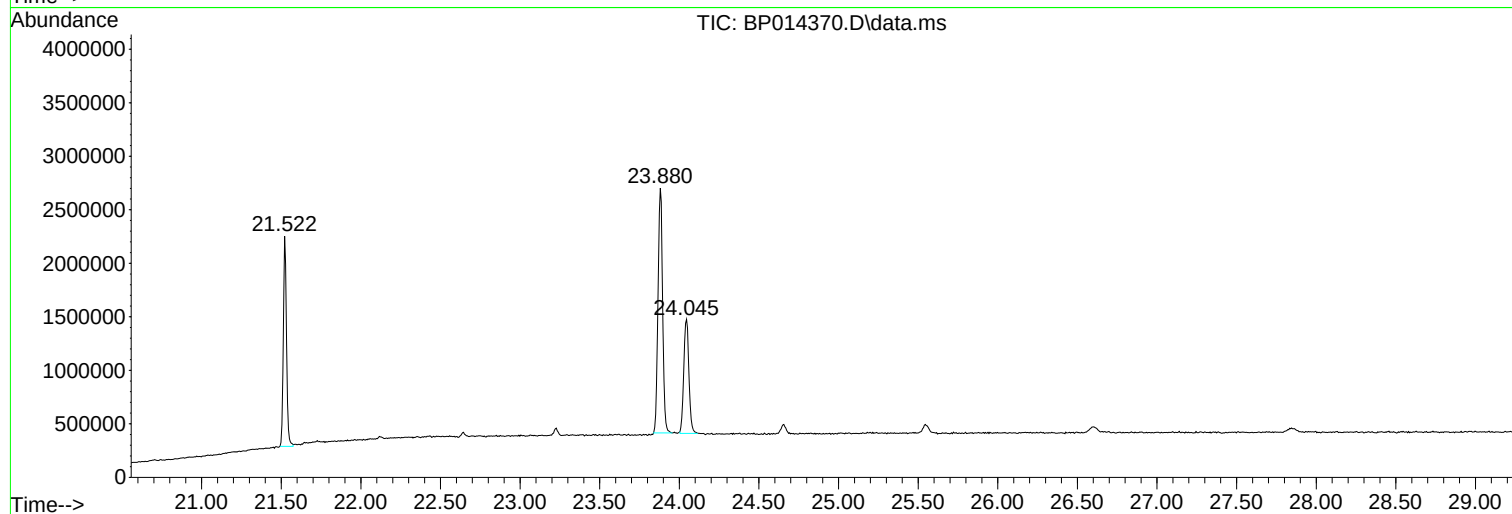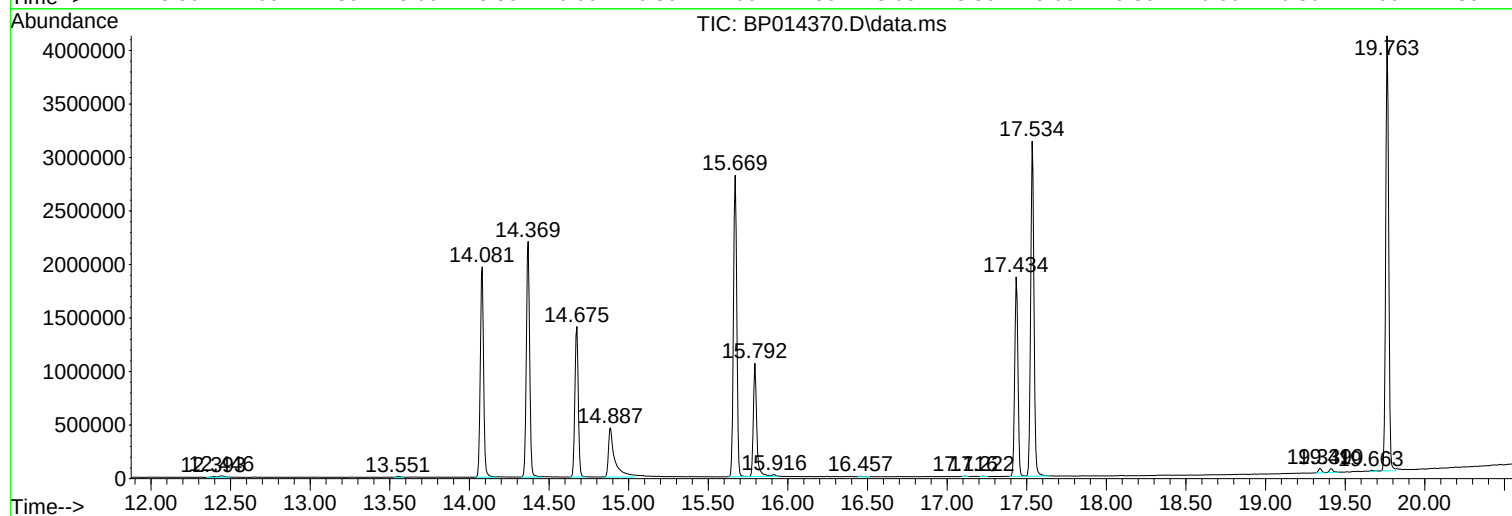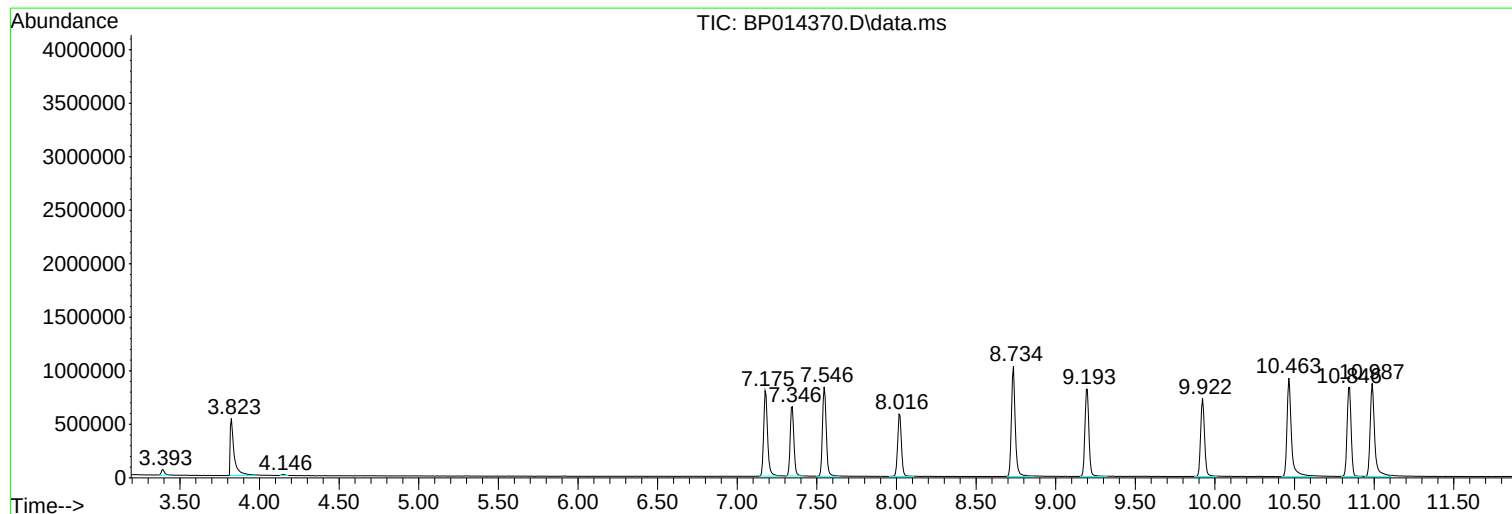

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014370.D
Acq On : 29 Mar 2023 19:19
Operator : CG/JU
Sample : PB151680BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK680

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014370.D
Acq On : 29 Mar 2023 19:19
Operator : CG/JU
Sample : PB151680BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK680

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc