

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
 Data File : BP014371.D
 Acq On : 29 Mar 2023 19:53
 Operator : CG/JU
 Sample : 02067-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFZ73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014371.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	40	rBV	35035	45832	0.84%	0.092%
2	3.834	108	110	126	rBV	128195	248266	4.57%	0.497%
3	4.046	141	146	152	rVB2	14214	23513	0.43%	0.047%
4	4.152	160	164	171	rVB	11658	19582	0.36%	0.039%
5	4.258	179	182	190	rVB7	9904	16819	0.31%	0.034%
6	5.081	319	322	326	rBV	11083	15829	0.29%	0.032%
7	5.299	354	359	366	rBV	31026	49556	0.91%	0.099%
8	6.399	540	546	552	rBV3	7521	13747	0.25%	0.028%
9	7.181	673	679	693	rBV	122923	231941	4.27%	0.464%
10	7.346	700	707	719	rBV	664620	1078050	19.86%	2.159%
11	7.546	734	741	760	rBV	568259	980174	18.06%	1.963%
12	7.905	797	802	813	rVB	61671	103696	1.91%	0.208%
13	8.016	814	821	837	rBV	663659	1186626	21.86%	2.376%
14	8.381	879	883	889	rVB4	9404	14815	0.27%	0.030%
15	8.734	935	943	956	rBV	421594	761451	14.03%	1.525%
16	9.193	1014	1021	1038	rBV	828173	1435092	26.44%	2.874%
17	9.375	1047	1052	1056	rVB8	3331	7345	0.14%	0.015%
18	9.575	1079	1086	1090	rBV2	11794	17388	0.32%	0.035%
19	9.922	1137	1145	1158	rBV	684554	1164333	21.45%	2.332%
20	10.463	1230	1237	1259	rBV	815748	1600912	29.49%	3.206%
21	10.704	1271	1278	1288	rVB	213661	347568	6.40%	0.696%
22	10.846	1294	1302	1315	rVB	964343	1658949	30.56%	3.322%
23	10.987	1318	1326	1350	rBV	689603	1374345	25.32%	2.752%
24	11.228	1360	1367	1376	rVB	55991	100376	1.85%	0.201%
25	12.245	1535	1540	1546	rVB7	6693	12814	0.24%	0.026%
26	12.375	1555	1562	1568	rBV	44030	87848	1.62%	0.176%
27	12.445	1568	1574	1582	rVB2	14333	34753	0.64%	0.070%
28	13.304	1716	1720	1728	rVB4	5390	10134	0.19%	0.020%
29	13.475	1743	1749	1753	rBV3	10384	17272	0.32%	0.035%
30	13.516	1753	1756	1760	rVV2	12684	20767	0.38%	0.042%
31	13.551	1760	1762	1770	rVB5	9117	16136	0.30%	0.032%
32	13.651	1772	1779	1782	rBV8	3554	6382	0.12%	0.013%
33	13.734	1786	1793	1795	rBV5	5726	9476	0.17%	0.019%
34	14.081	1844	1852	1864	rBV	2111390	3095599	57.03%	6.199%
35	14.192	1867	1871	1877	rVB9	6121	10559	0.19%	0.021%
36	14.310	1888	1891	1894	rBV4	4710	5701	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
 Data File : BP014371.D
 Acq On : 29 Mar 2023 19:53
 Operator : CG/JU
 Sample : 02067-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFZ73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	14.369	1894	1901	1915	rVV	2277905	3266794	60.18%	6.542%
38	14.675	1946	1953	1963	rBV	1565754	2309436	42.55%	4.625%
39	14.922	1989	1995	2013	rBV2	41216	176744	3.26%	0.354%
40	15.075	2019	2021	2026	rVB6	4477	5838	0.11%	0.012%
41	15.498	2089	2093	2098	rVB8	5201	6519	0.12%	0.013%
42	15.669	2115	2122	2135	rBV	3187254	4424309	81.51%	8.860%
43	15.792	2137	2143	2160	rVV	1069579	1601063	29.50%	3.206%
44	15.910	2160	2163	2167	rVV3	11666	15163	0.28%	0.030%
45	16.034	2179	2184	2194	rBV	66668	102732	1.89%	0.206%
46	17.104	2359	2366	2374	rBV	8864	21586	0.40%	0.043%
47	17.433	2416	2422	2432	rBV	1950778	2762324	50.89%	5.532%
48	17.533	2432	2439	2454	rVV	3619125	5127533	94.46%	10.268%
49	18.298	2565	2569	2578	rBV2	62363	113108	2.08%	0.227%
50	19.339	2742	2746	2752	rBV3	48028	70787	1.30%	0.142%
51	19.410	2754	2758	2763	rVV	42965	66690	1.23%	0.134%
52	19.533	2775	2779	2783	rBV4	38361	60533	1.12%	0.121%
53	19.763	2812	2818	2825	rBV	4148222	5428177	100.00%	10.870%
54	21.521	3112	3117	3125	rBV	1661463	2308590	42.53%	4.623%
55	23.880	3511	3518	3530	rVB2	1978879	4150355	76.46%	8.311%
56	24.045	3539	3546	3560	rVB2	964647	2094767	38.59%	4.195%




Sum of corrected areas: 49936694

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014371.D
Acq On : 29 Mar 2023 19:53
Operator : CG/JU
Sample : 02067-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFZ73

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

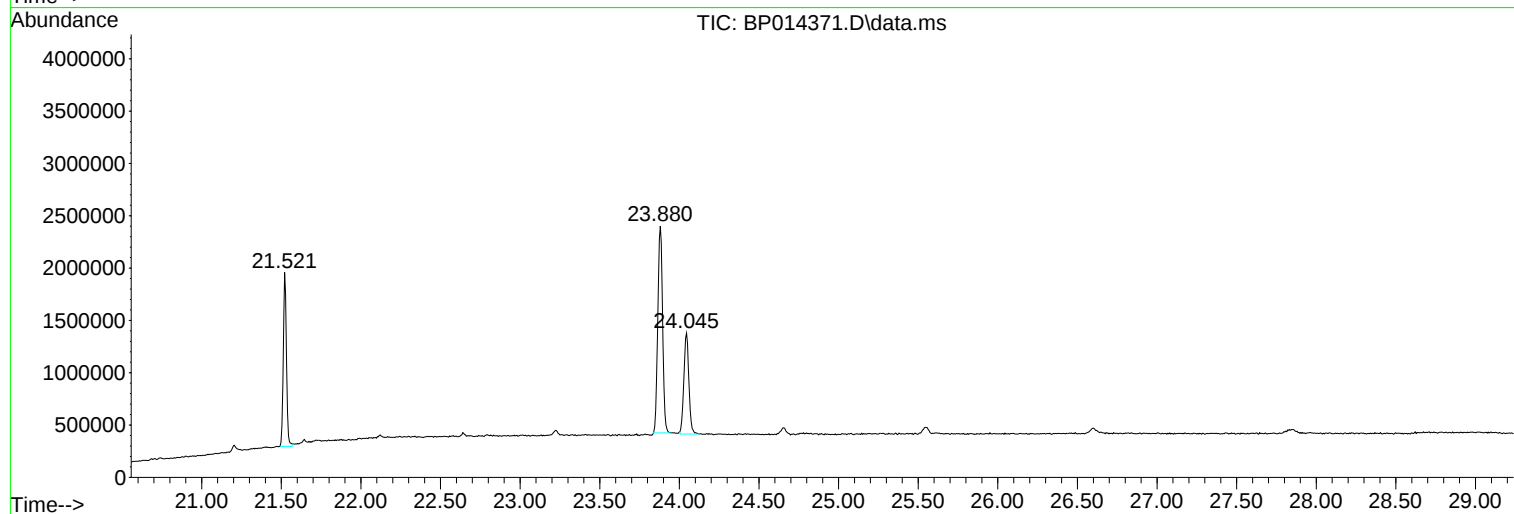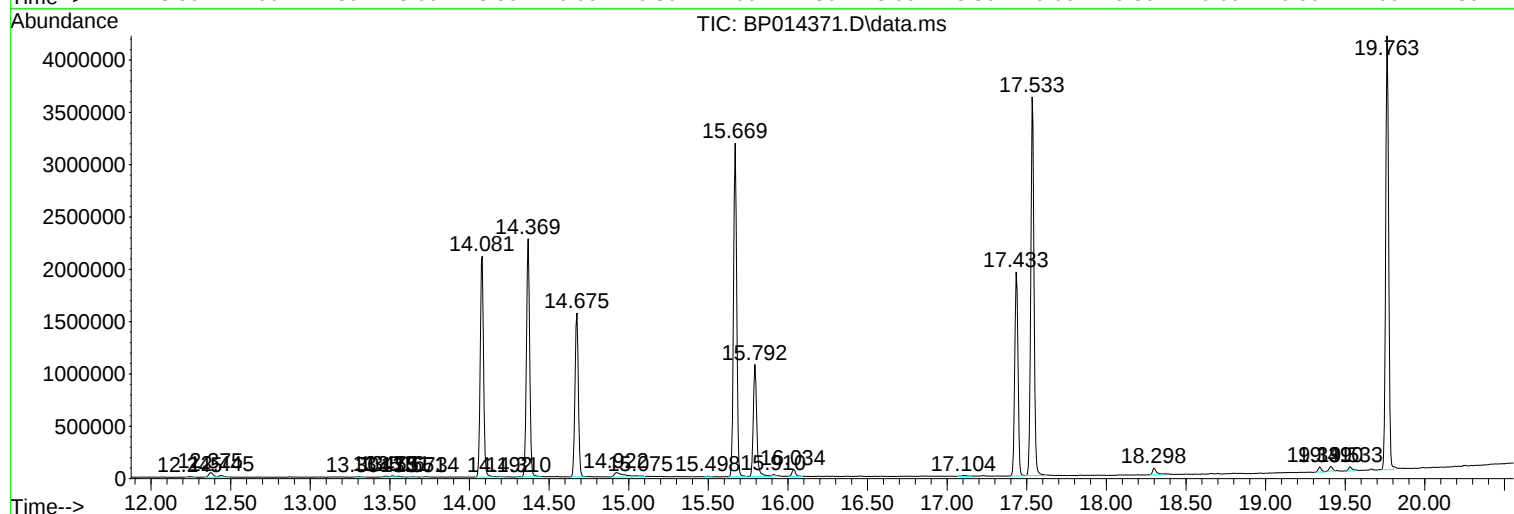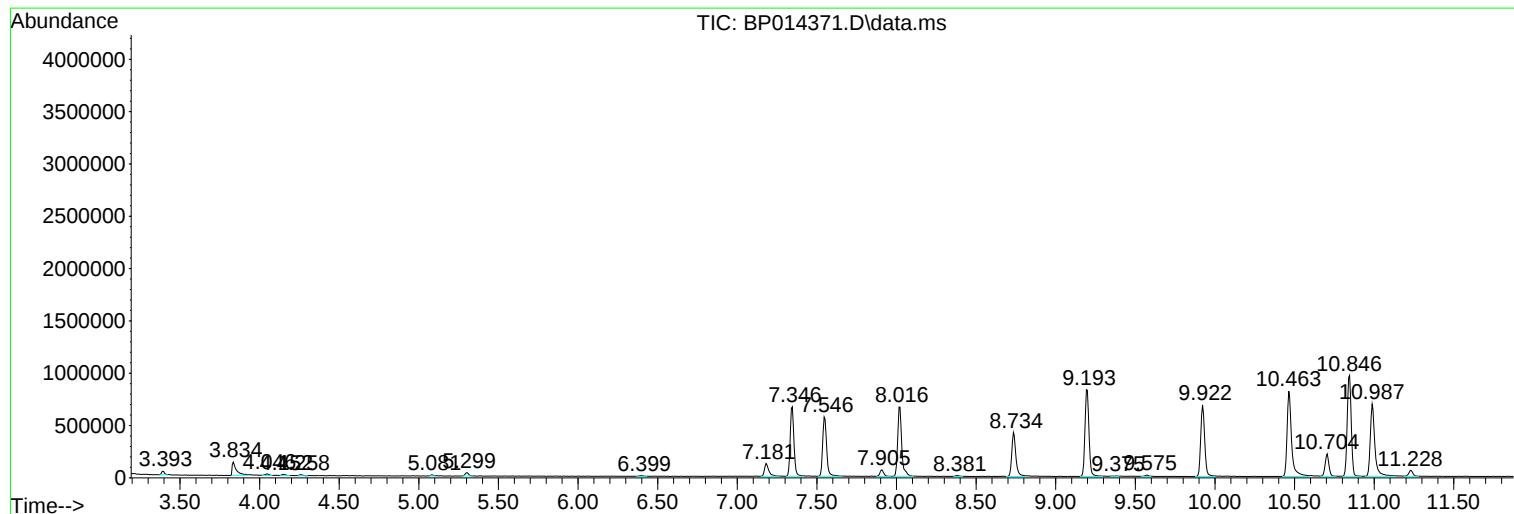

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014371.D
Acq On : 29 Mar 2023 19:53
Operator : CG/JU
Sample : 02067-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFZ73










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzene, 1,2,3-trichloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.704	4.19 ng/ul	347568	Naphthalene-d8	10.845

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1,2,3-trichloro-	180	C6H3Cl3	000087-61-6	98
2			Benzene, 1,3,5-trichloro-	180	C6H3Cl3	000108-70-3	97
3			Benzene, 1,3,5-trichloro-	180	C6H3Cl3	000108-70-3	95
4			Benzene, 1,2,3-trichloro-	180	C6H3Cl3	000087-61-6	95
5			Benzene, 1,2,4-trichloro-	180	C6H3Cl3	000120-82-1	95

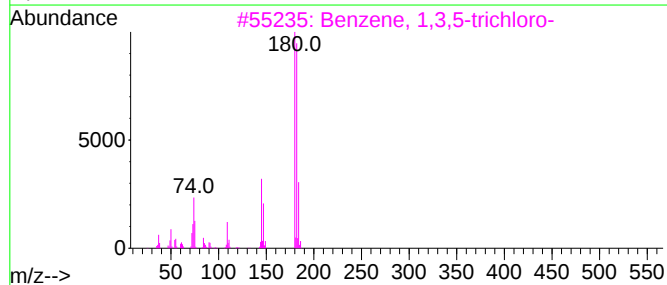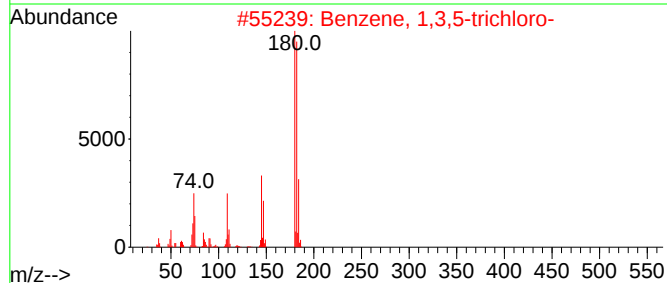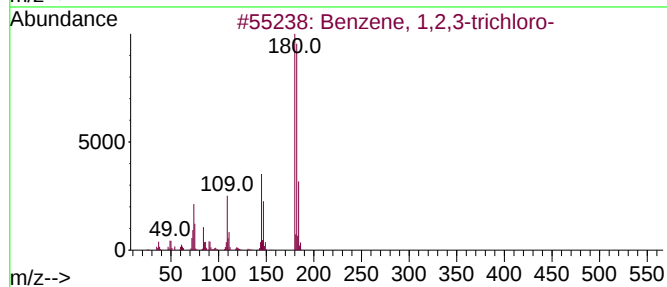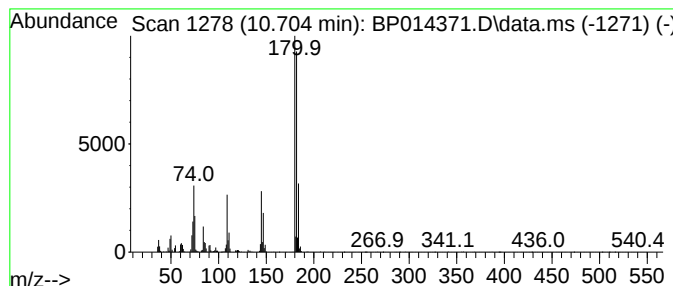

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014371.D
Acq On : 29 Mar 2023 19:53
Operator : CG/JU
Sample : 02067-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFZ73

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzene, 1,2,3-...	10.704	4.2	ng/u1	347568	2	10.845	1658950	20.0