

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
 Data File : BP014372.D
 Acq On : 29 Mar 2023 20:26
 Operator : CG/JU
 Sample : 02067-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFZ79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014372.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	42	rBV	43401	55250	0.92%	0.102%
2	3.840	109	111	121	rBV	71371	125319	2.09%	0.232%
3	4.046	142	146	152	rVB	18114	29504	0.49%	0.055%
4	4.152	160	164	168	rVB	9921	13832	0.23%	0.026%
5	4.258	177	182	188	rVB5	11947	17457	0.29%	0.032%
6	4.587	234	238	242	rBV6	3799	6646	0.11%	0.012%
7	5.081	317	322	326	rBV	16177	24539	0.41%	0.046%
8	5.299	351	359	368	rBV	139693	222495	3.70%	0.413%
9	5.693	421	426	429	rBV7	3895	6606	0.11%	0.012%
10	6.399	542	546	551	rVB3	10012	15147	0.25%	0.028%
11	7.117	663	668	673	rBV8	3573	6536	0.11%	0.012%
12	7.181	673	679	698	rBV	187530	354072	5.89%	0.657%
13	7.346	700	707	720	rBV	775940	1266058	21.07%	2.348%
14	7.546	733	741	758	rBV	758529	1259600	20.97%	2.336%
15	7.905	797	802	810	rBV	61174	101594	1.69%	0.188%
16	8.016	815	821	841	rBV	658065	1214924	20.22%	2.253%
17	8.381	877	883	889	rVB	4848	9931	0.17%	0.018%
18	8.734	936	943	957	rBV	603314	1060192	17.65%	1.966%
19	9.193	1012	1021	1043	rBV	997070	1702294	28.34%	3.157%
20	9.575	1081	1086	1092	rVB	14289	22167	0.37%	0.041%
21	9.922	1136	1145	1165	rBV	852854	1447347	24.09%	2.684%
22	10.463	1230	1237	1262	rBV	1028350	2006289	33.40%	3.720%
23	10.622	1262	1264	1270	rVV7	5728	9281	0.15%	0.017%
24	10.705	1270	1278	1284	rVV2	79255	136551	2.27%	0.253%
25	10.840	1293	1301	1313	rBV	947144	1615952	26.90%	2.997%
26	10.987	1319	1326	1347	rBV	402517	851220	14.17%	1.579%
27	12.246	1533	1540	1544	rBV9	6391	12487	0.21%	0.023%
28	12.375	1556	1562	1568	rBV2	33197	64614	1.08%	0.120%
29	12.440	1568	1573	1579	rVB2	15588	32016	0.53%	0.059%
30	13.299	1710	1719	1725	rBV	11535	24528	0.41%	0.045%
31	13.475	1743	1749	1753	rBV3	11384	17925	0.30%	0.033%
32	13.516	1753	1756	1759	rVV2	9637	13921	0.23%	0.026%
33	13.557	1759	1763	1768	rVB4	10146	18248	0.30%	0.034%
34	13.728	1787	1792	1798	rBV10	4731	9890	0.16%	0.018%
35	14.081	1841	1852	1865	rBV	2475071	3510053	58.43%	6.509%
36	14.187	1867	1870	1873	rVB5	5004	6873	0.11%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
 Data File : BP014372.D
 Acq On : 29 Mar 2023 20:26
 Operator : CG/JU
 Sample : 02067-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFZ79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	14.369	1894	1901	1918	rVV	2524217	3784892	63.00%	7.019%
38	14.675	1946	1953	1964	rBV	1521686	2260942	37.64%	4.193%
39	14.910	1986	1993	2013	rBV3	74417	281620	4.69%	0.522%
40	15.669	2115	2122	2132	rBV	3410828	4954328	82.47%	9.187%
41	15.793	2136	2143	2158	rBV	1247047	1857838	30.93%	3.445%
42	15.910	2160	2163	2167	rVB3	17123	22672	0.38%	0.042%
43	16.034	2179	2184	2196	rVB	59703	96042	1.60%	0.178%
44	16.369	2238	2241	2244	rBV5	5168	7057	0.12%	0.013%
45	17.110	2363	2367	2371	rVB5	6289	8202	0.14%	0.015%
46	17.234	2383	2388	2390	rVB6	4300	6997	0.12%	0.013%
47	17.434	2416	2422	2432	rBV	1889063	2641790	43.97%	4.899%
48	17.534	2432	2439	2454	rBV2	3693639	5353107	89.11%	9.927%
49	18.298	2565	2569	2578	rBV2	71737	129548	2.16%	0.240%
50	19.339	2742	2746	2750	rBV2	47356	62974	1.05%	0.117%
51	19.410	2754	2758	2765	rVB	46977	69902	1.16%	0.130%
52	19.528	2775	2778	2785	rBV4	44779	69192	1.15%	0.128%
53	19.763	2812	2818	2825	rBV	4633721	6007484	100.00%	11.140%
54	20.704	2975	2978	2982	rVB2	55243	54330	0.90%	0.101%
55	21.522	3112	3117	3126	rBV	1808621	2462517	40.99%	4.567%
56	23.880	3511	3518	3530	rVB2	2233644	4481562	74.60%	8.311%
57	24.045	3539	3546	3555	rVB2	944709	2021311	33.65%	3.748%




Sum of corrected areas: 53925665

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014372.D
Acq On : 29 Mar 2023 20:26
Operator : CG/JU
Sample : 02067-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFZ79

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

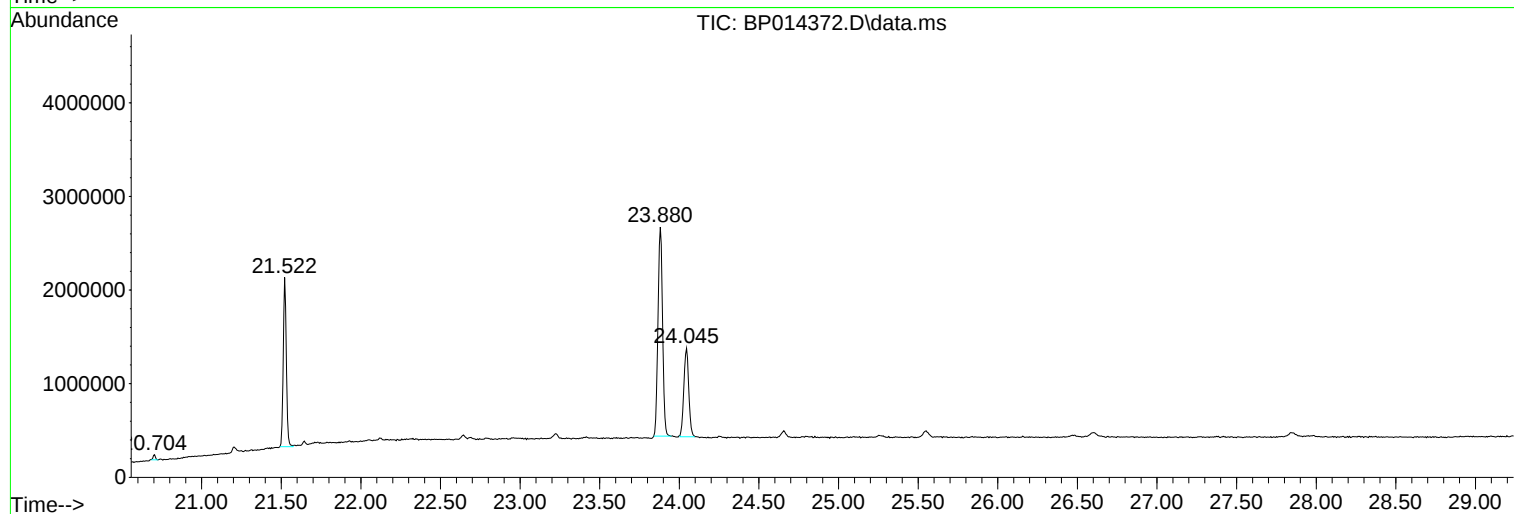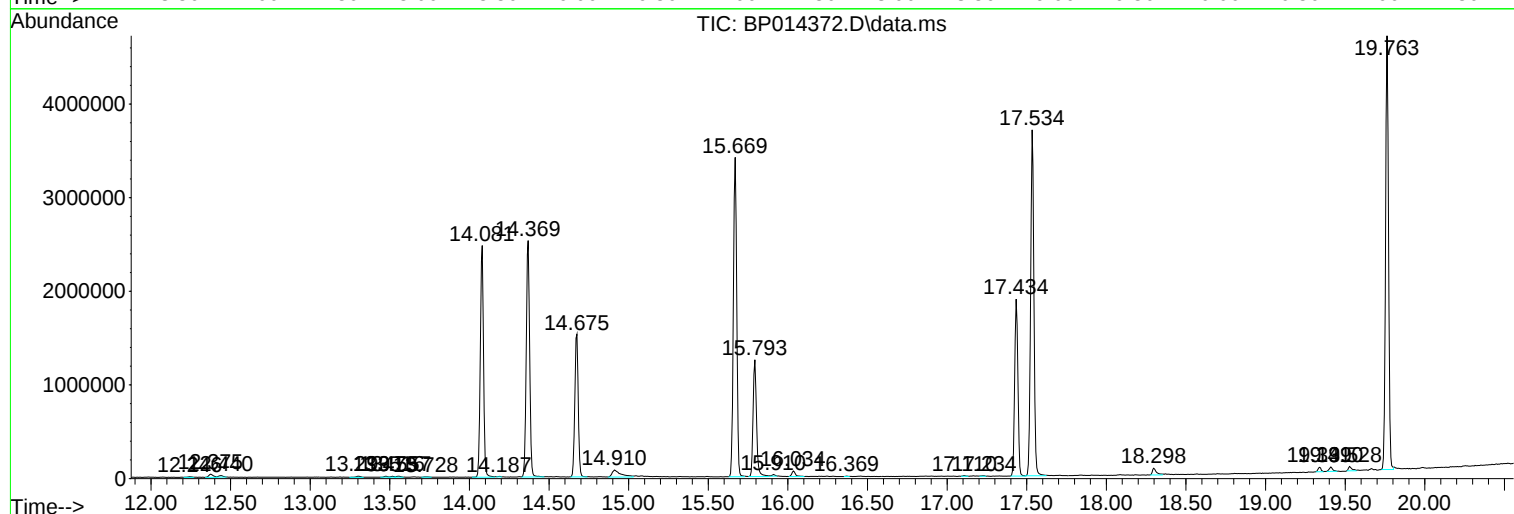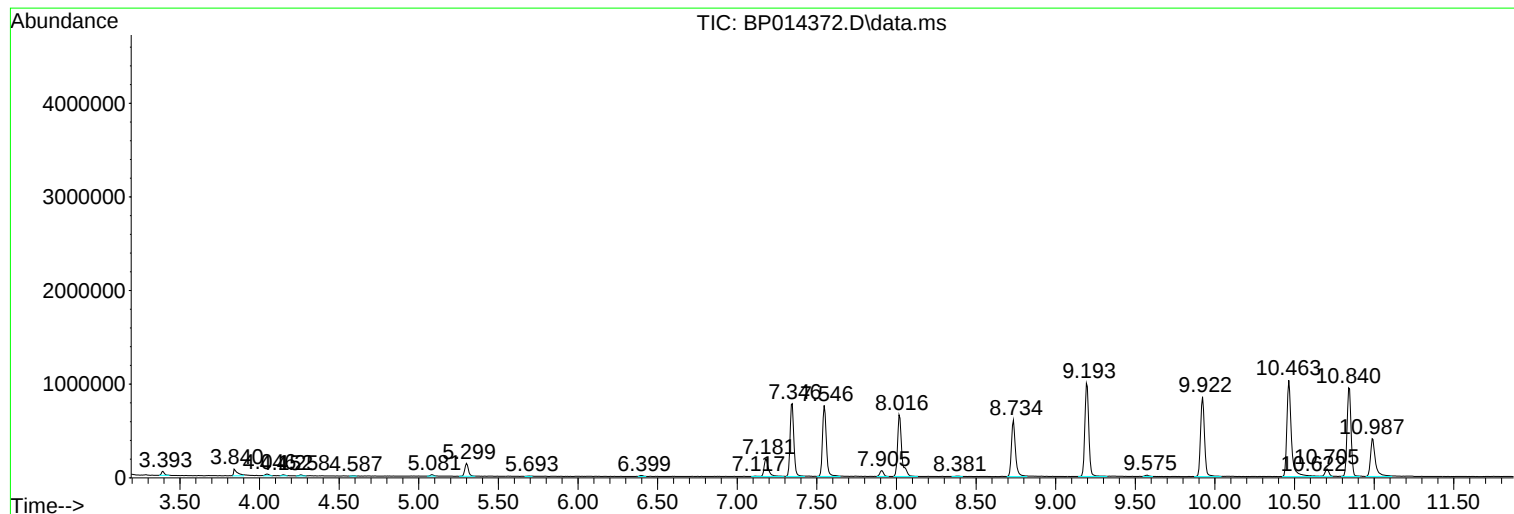

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014372.D
Acq On : 29 Mar 2023 20:26
Operator : CG/JU
Sample : 02067-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFZ79










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzene, chloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.299	3.66 ng/ul	222495	1,4-Dichlorobenzene-d4	8.016

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, chloro-	112	C6H5Cl	000108-90-7	96
2			Benzene, chloro-	112	C6H5Cl	000108-90-7	95
3			Benzene, chloro-	112	C6H5Cl	000108-90-7	94
4			Benzene, chloro-	112	C6H5Cl	000108-90-7	94
5			Benzene, chloro-	112	C6H5Cl	000108-90-7	94

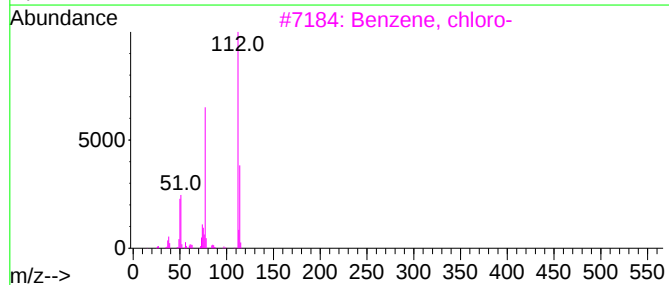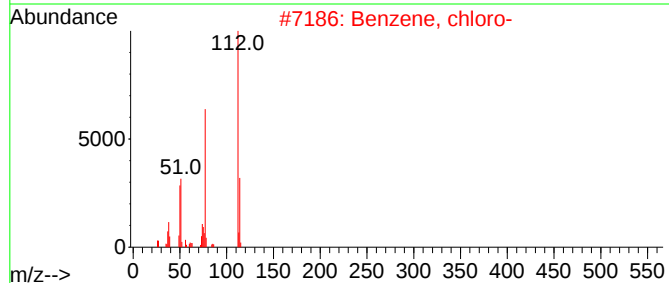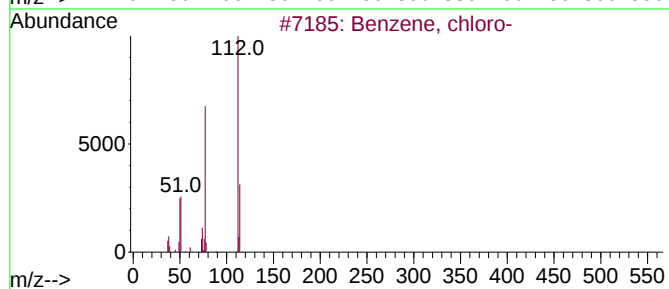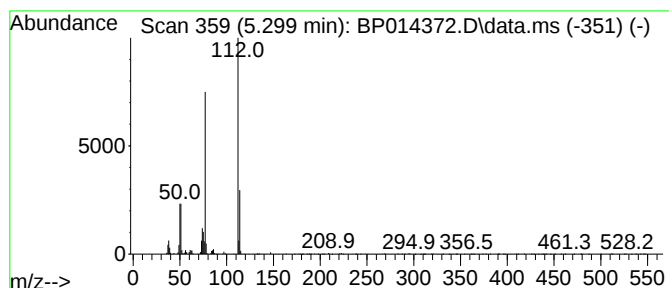

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014372.D
Acq On : 29 Mar 2023 20:26
Operator : CG/JU
Sample : 02067-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFZ79

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzene, chloro-	5.299	3.7	ng/u1	222495	1	8.016	1214920	20.0