

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
 Data File : BP014373.D
 Acq On : 29 Mar 2023 21:00
 Operator : CG/JU
 Sample : 02067-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFZ83

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014373.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	42	rVB	39047	55476	0.93%	0.107%
2	3.828	106	109	126	rBV	181727	338695	5.70%	0.653%
3	4.046	142	146	153	rVB	18124	27193	0.46%	0.052%
4	4.152	159	164	169	rBV	9580	14468	0.24%	0.028%
5	4.258	178	182	186	rBV6	10884	16005	0.27%	0.031%
6	5.081	317	322	333	rVB	14756	25084	0.42%	0.048%
7	6.399	539	546	551	rBV4	9240	16528	0.28%	0.032%
8	7.181	673	679	694	rBV	152041	288013	4.85%	0.555%
9	7.340	700	706	719	rBV	675037	1112514	18.73%	2.145%
10	7.546	733	741	759	rBV	636540	1080123	18.18%	2.082%
11	8.016	813	821	830	rBV	590804	984112	16.57%	1.897%
12	8.734	937	943	962	rBV	502346	899070	15.14%	1.733%
13	9.193	1013	1021	1038	rBV	865673	1498765	25.23%	2.889%
14	9.322	1038	1043	1050	rBV	4967	14221	0.24%	0.027%
15	9.575	1079	1086	1092	rVB	19630	34212	0.58%	0.066%
16	9.922	1137	1145	1161	rBV	738923	1259894	21.21%	2.429%
17	10.463	1230	1237	1266	rBV	889494	1723975	29.02%	3.323%
18	10.840	1294	1301	1315	rVB	852543	1469980	24.75%	2.834%
19	10.987	1318	1326	1357	rBV	801164	1587148	26.72%	3.060%
20	12.252	1536	1541	1547	rVB5	6931	13715	0.23%	0.026%
21	12.387	1558	1564	1567	rBV7	3992	7883	0.13%	0.015%
22	12.440	1567	1573	1582	rVB4	13688	33135	0.56%	0.064%
23	13.051	1670	1677	1685	rVB4	2756	6068	0.10%	0.012%
24	13.134	1687	1691	1696	rBV7	3977	6677	0.11%	0.013%
25	13.475	1744	1749	1753	rBV4	18146	27426	0.46%	0.053%
26	13.516	1753	1756	1761	rVB	17089	23701	0.40%	0.046%
27	14.081	1843	1852	1864	rBV	2140600	3144032	52.93%	6.061%
28	14.187	1867	1870	1878	rVB10	7026	13610	0.23%	0.026%
29	14.369	1894	1901	1917	rBV	2344290	3357271	56.52%	6.472%
30	14.546	1929	1931	1935	rVB4	4978	5993	0.10%	0.012%
31	14.675	1944	1953	1964	rBV	1396563	2052373	34.55%	3.956%
32	14.916	1988	1994	2011	rBV3	52527	198378	3.34%	0.382%
33	15.498	2086	2093	2096	rBV9	4010	7593	0.13%	0.015%
34	15.669	2115	2122	2136	rBV	3181459	4439361	74.74%	8.558%
35	15.793	2137	2143	2159	rVV	1081242	1581717	26.63%	3.049%
36	15.910	2159	2163	2170	rVB4	16748	31007	0.52%	0.060%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
 Data File : BP014373.D
 Acq On : 29 Mar 2023 21:00
 Operator : CG/JU
 Sample : 02067-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFZ83

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	16.034	2177	2184	2196	rVB	92189	144243	2.43%	0.278%
38	16.369	2238	2241	2246	rBV7	4645	7738	0.13%	0.015%
39	16.457	2251	2256	2261	rBV9	3777	7186	0.12%	0.014%
40	17.104	2364	2366	2373	rVB8	5060	8495	0.14%	0.016%
41	17.434	2415	2422	2432	rBV	1828173	2540459	42.77%	4.897%
42	17.534	2432	2439	2454	rVV	3593852	5134237	86.44%	9.898%
43	17.634	2454	2456	2464	rVB9	10954	19729	0.33%	0.038%
44	17.839	2488	2491	2498	rVB9	3990	6968	0.12%	0.013%
45	18.081	2529	2532	2535	rBV4	6196	8679	0.15%	0.017%
46	18.298	2565	2569	2578	rBV2	88023	156326	2.63%	0.301%
47	19.339	2742	2746	2753	rBV3	52500	70005	1.18%	0.135%
48	19.410	2754	2758	2767	rVV	49475	84920	1.43%	0.164%
49	19.528	2775	2778	2786	rBV2	48638	91845	1.55%	0.177%
50	19.763	2812	2818	2825	rBV	4591799	5939900	100.00%	11.451%
51	21.198	3058	3062	3071	rBV4	119746	269221	4.53%	0.519%
52	21.522	3112	3117	3127	rBV	1936323	2588681	43.58%	4.990%
53	23.880	3511	3518	3530	rVB2	2532204	5096414	85.80%	9.825%
54	24.045	3539	3546	3555	rVB	1116692	2303501	38.78%	4.441%




Sum of corrected areas: 51873963

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014373.D
Acq On : 29 Mar 2023 21:00
Operator : CG/JU
Sample : 02067-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFZ83

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

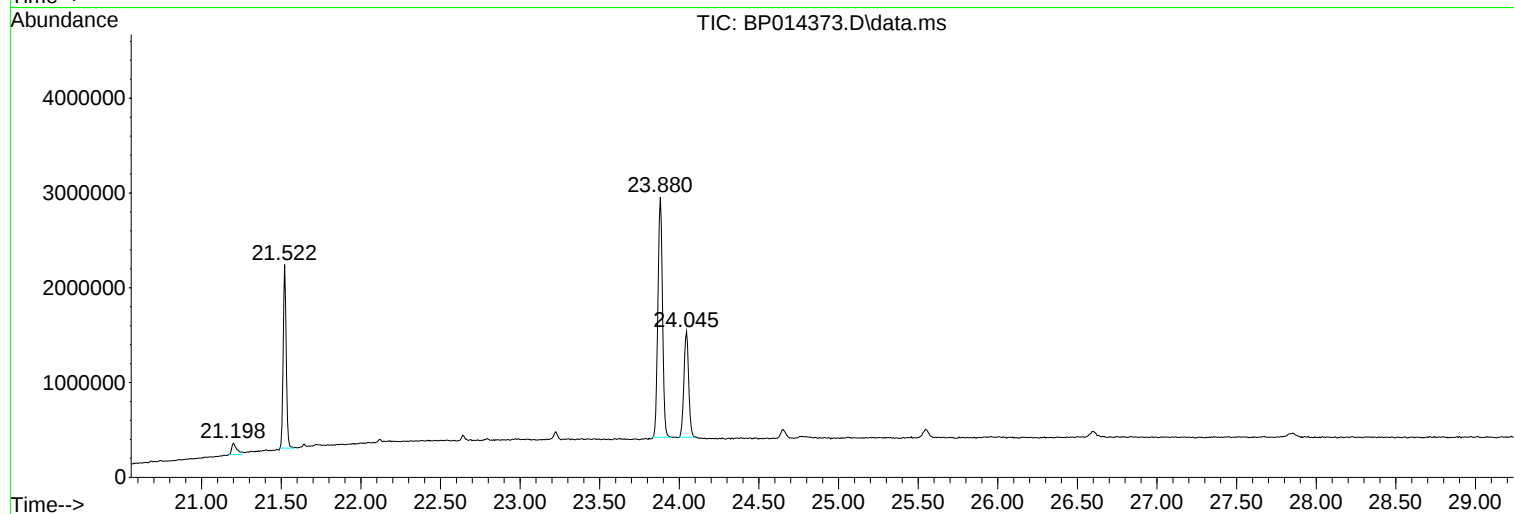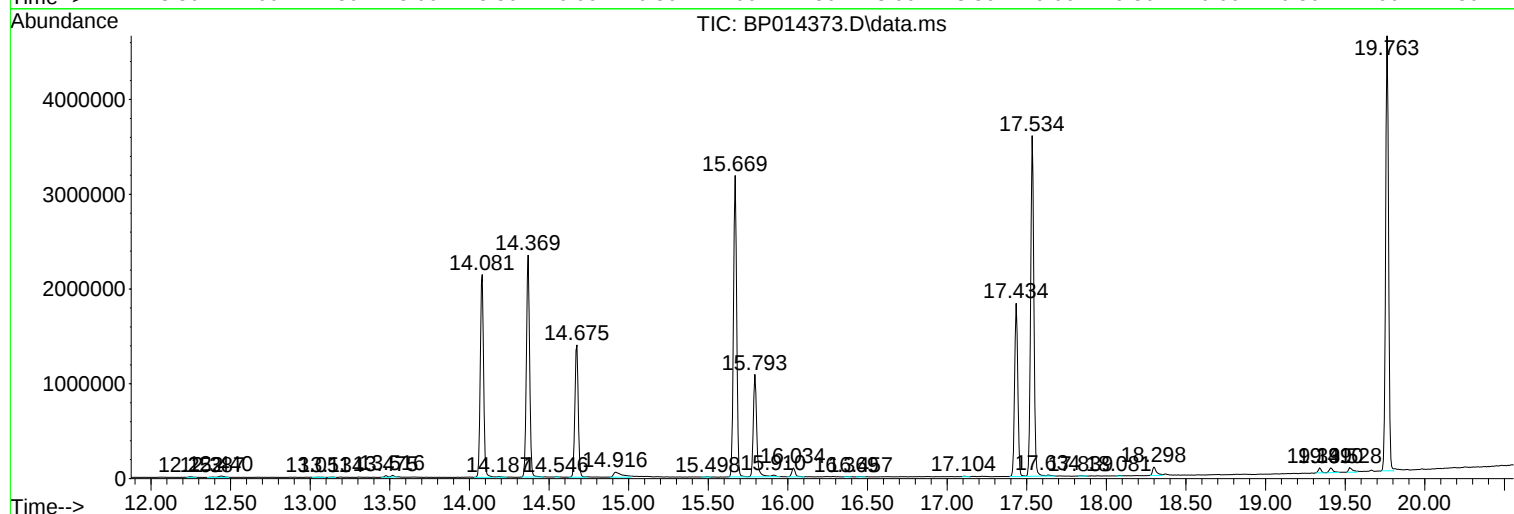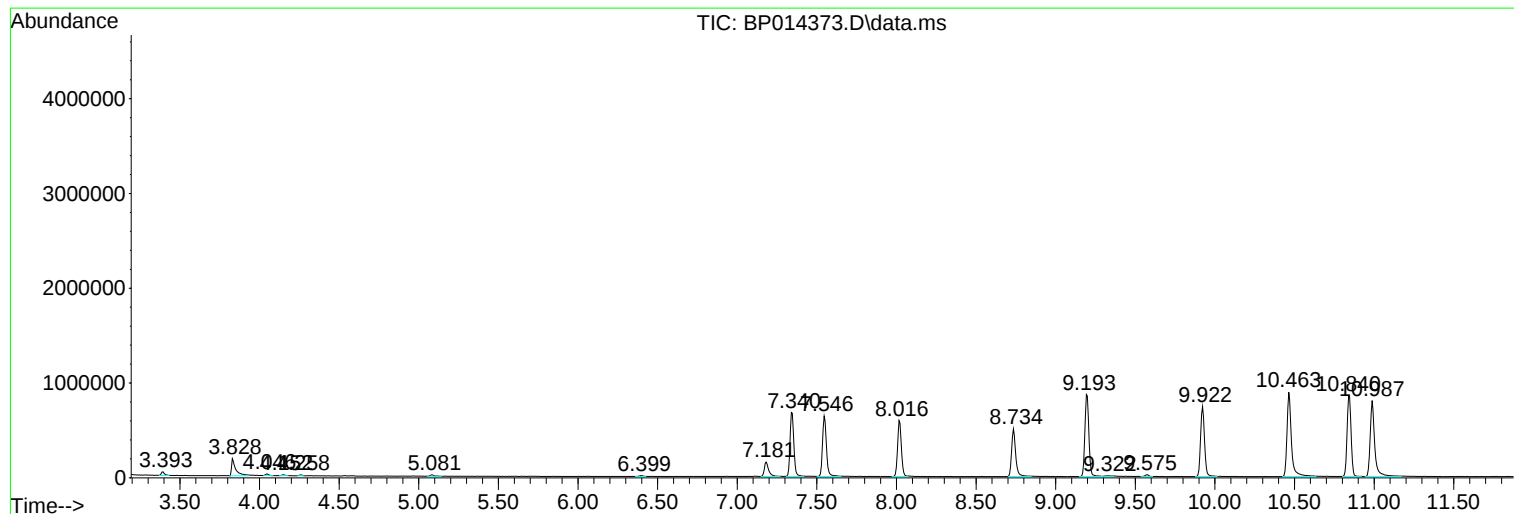

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014373.D
Acq On : 29 Mar 2023 21:00
Operator : CG/JU
Sample : 02067-03
Misc :
ALS Vial : 23 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
BFZ83

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
21.198	2.08 ng/ul	269221	Chrysene-d12		21.522	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	1-Tetracosene		336	C24H48	010192-32-2	96
2	Cyclotetracosane		336	C24H48	000297-03-0	95
3	5-Octadecene, (E)-		252	C18H36	007206-21-5	94
4	1-Hexacosene		364	C26H52	018835-33-1	93
5	Carbonic acid, octadecyl 2,2,2-t...		444	C21H39Cl3O3	1000314-56-3	90

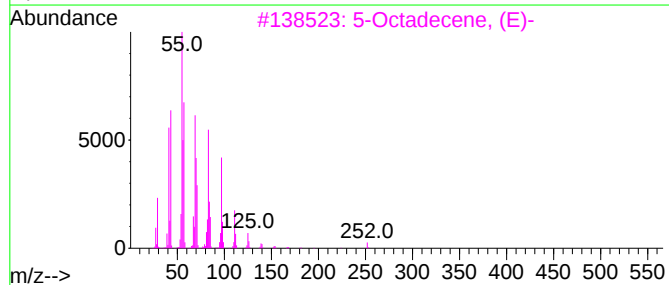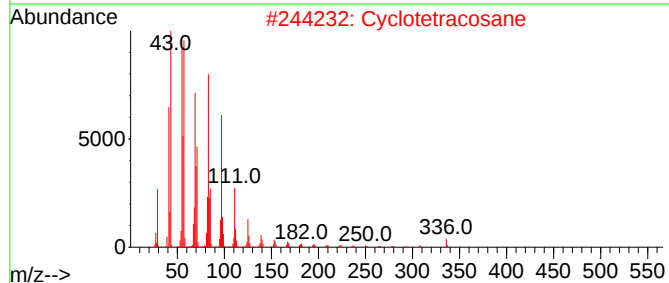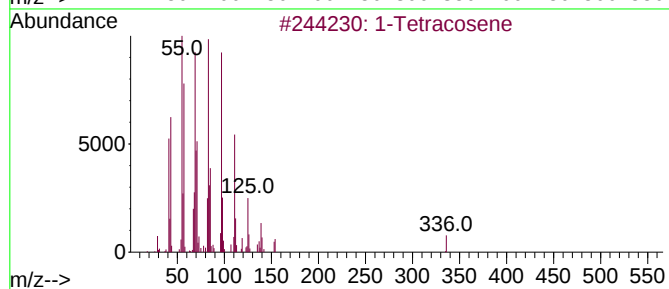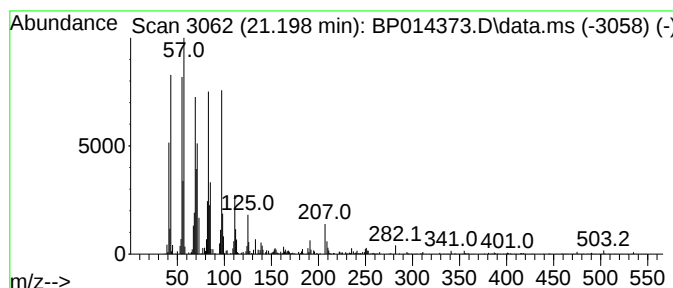

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014373.D
Acq On : 29 Mar 2023 21:00
Operator : CG/JU
Sample : 02067-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFZ83

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.198	2.1	ng/u1	269221	5	21.522	2588680	20.0