

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
 Data File : BP014384.D
 Acq On : 30 Mar 2023 03:43
 Operator : CG/JU
 Sample : PB151679BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK679

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014384.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	43	rVB	40850	60080	1.30%	0.128%
2	3.822	106	108	137	rBV	483916	1021702	22.07%	2.174%
3	4.146	159	163	168	rBV3	9777	18607	0.40%	0.040%
4	7.175	672	678	694	rBV	655136	1171423	25.30%	2.493%
5	7.340	699	706	718	rBV	543630	881392	19.04%	1.876%
6	7.546	734	741	754	rBV	695738	1128717	24.38%	2.402%
7	8.016	814	821	831	rBV	559206	917781	19.82%	1.953%
8	8.734	936	943	959	rBV	849970	1476918	31.90%	3.143%
9	9.193	1014	1021	1037	rBV	677922	1179441	25.47%	2.510%
10	9.922	1138	1145	1159	rBV	610773	1039024	22.44%	2.211%
11	10.463	1229	1237	1255	rBV	737088	1474780	31.85%	3.139%
12	10.840	1294	1301	1312	rBV	790788	1355301	29.27%	2.884%
13	10.987	1319	1326	1345	rBV	738016	1460481	31.54%	3.108%
14	12.445	1569	1574	1578	rBV4	9026	16718	0.36%	0.036%
15	13.557	1759	1763	1769	rVB8	3093	6410	0.14%	0.014%
16	13.645	1775	1778	1782	rBV6	2838	4819	0.10%	0.010%
17	14.081	1844	1852	1870	rBV	1619985	2446999	52.85%	5.208%
18	14.369	1894	1901	1917	rBV	1831594	2776074	59.96%	5.908%
19	14.675	1945	1953	1963	rBV	1410274	2123190	45.86%	4.518%
20	14.886	1983	1989	2012	rBV	397864	1123578	24.27%	2.391%
21	15.669	2114	2122	2135	rBV	2467963	3599116	77.73%	7.659%
22	15.792	2137	2143	2159	rVV	868026	1289481	27.85%	2.744%
23	15.910	2160	2163	2168	rVB5	12527	19919	0.43%	0.042%
24	16.451	2252	2255	2263	rVB9	3284	6782	0.15%	0.014%
25	17.110	2363	2367	2371	rVB6	5366	8282	0.18%	0.018%
26	17.433	2415	2422	2432	rBV	1814726	2487374	53.72%	5.293%
27	17.533	2432	2439	2457	rVV	2784709	3841783	82.97%	8.176%
28	18.098	2530	2535	2536	rBV5	3261	5469	0.12%	0.012%
29	19.339	2742	2746	2752	rBV2	37700	51710	1.12%	0.110%
30	19.410	2754	2758	2765	rVV	29660	52419	1.13%	0.112%
31	19.763	2812	2818	2826	rBV	3477720	4630187	100.00%	9.854%
32	21.521	3112	3117	3127	rBV	1859295	2684607	57.98%	5.713%
33	23.880	3511	3518	3530	rVB2	2084520	4155846	89.76%	8.844%
34	24.045	3539	3546	3558	rVB2	1134755	2473421	53.42%	5.264%

Sum of corrected areas: 46989831




Instrument :
BNA_P
ClientSampleId :
SBLK679

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014384.D
Acq On : 30 Mar 2023 03:43
Operator : CG/JU
Sample : PB151679BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK679

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

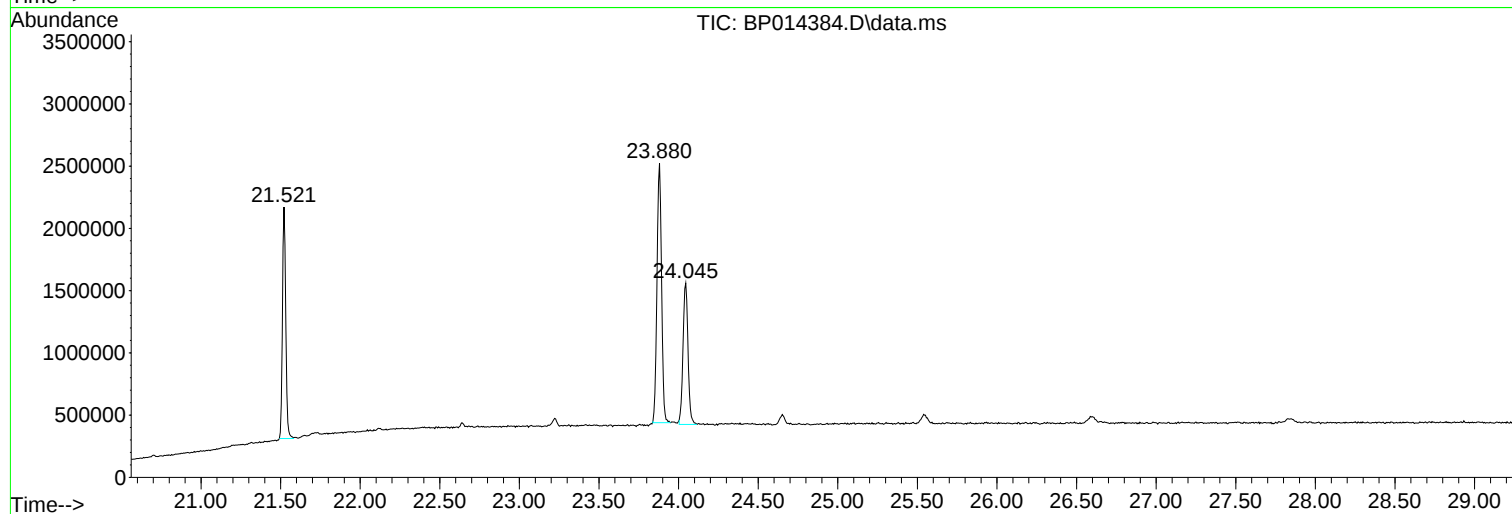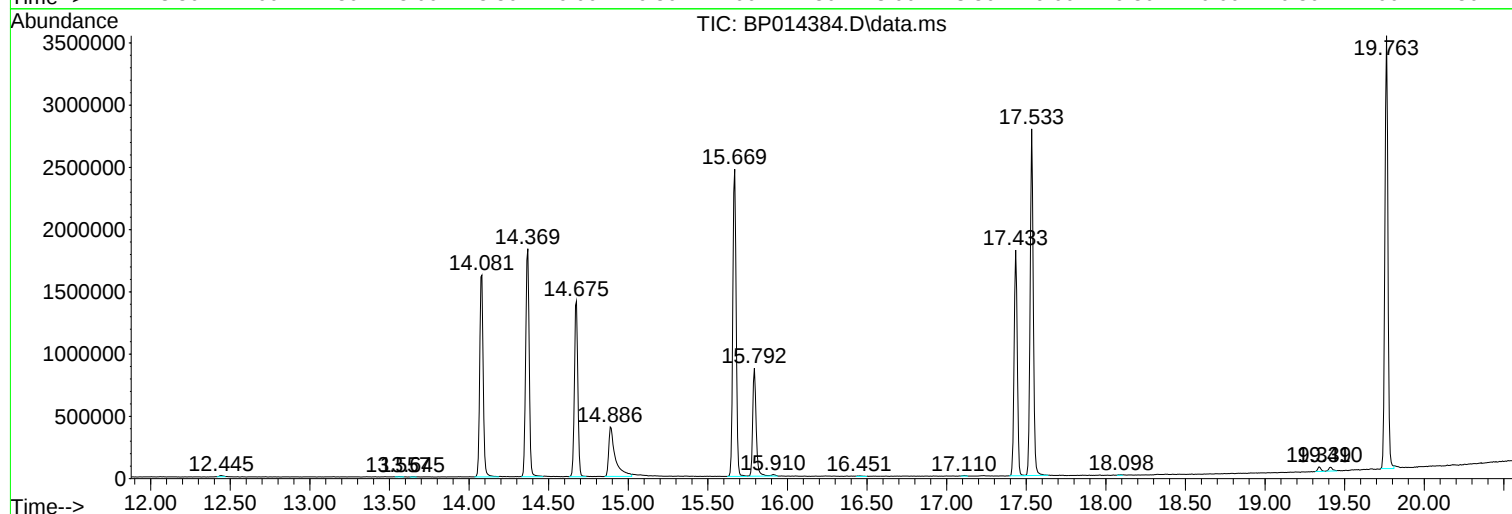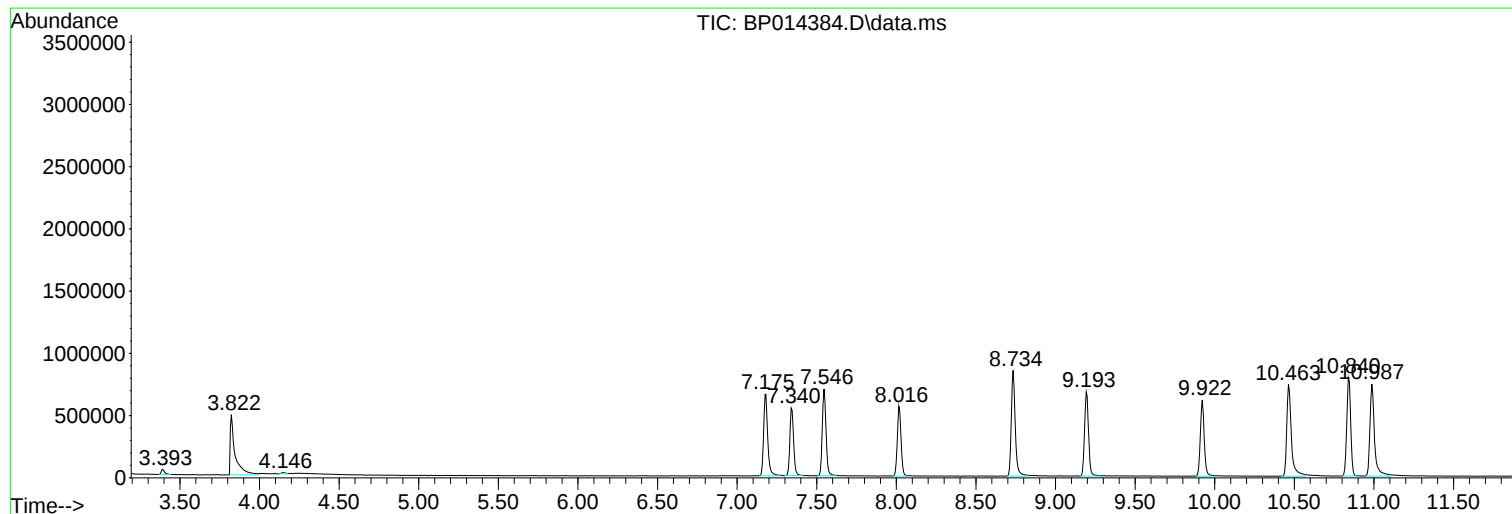

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014384.D
Acq On : 30 Mar 2023 03:43
Operator : CG/JU
Sample : PB151679BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK679

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014384.D
Acq On : 30 Mar 2023 03:43
Operator : CG/JU
Sample : PB151679BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK679

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc