

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
 Data File : BP014385.D
 Acq On : 30 Mar 2023 04:16
 Operator : CG/JU
 Sample : PB151682BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK682

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014385.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	44	rVB	50552	72703	1.36%	0.137%
2	3.822	105	108	133	rBV	565711	985896	18.38%	1.864%
3	4.146	160	163	168	rVB2	12522	18026	0.34%	0.034%
4	7.175	671	678	694	rBV	856226	1458447	27.19%	2.758%
5	7.340	700	706	720	rVB	673120	1089864	20.32%	2.061%
6	7.546	733	741	755	rBV	878370	1444300	26.93%	2.731%
7	8.016	812	821	834	rBV	598536	983858	18.35%	1.861%
8	8.734	935	943	955	rBV	1078832	1839456	34.30%	3.479%
9	9.193	1013	1021	1036	rBV	864945	1472851	27.46%	2.785%
10	9.922	1136	1145	1157	rBV	751952	1311146	24.45%	2.479%
11	10.463	1228	1237	1263	rBV	981208	1905157	35.52%	3.603%
12	10.840	1292	1301	1314	rBV	873179	1450836	27.05%	2.744%
13	10.987	1318	1326	1345	rBV	875072	1726306	32.19%	3.265%
14	12.381	1557	1563	1570	rBV2	28152	62653	1.17%	0.118%
15	12.440	1570	1573	1582	rVB3	15539	30588	0.57%	0.058%
16	13.557	1756	1763	1771	rBV9	8053	16013	0.30%	0.030%
17	14.075	1844	1851	1868	rBV	1901707	2852231	53.18%	5.394%
18	14.369	1894	1901	1919	rBV	2214813	3291675	61.38%	6.225%
19	14.675	1944	1953	1963	rBV	1329441	2029204	37.84%	3.837%
20	14.886	1982	1989	2013	rBV	474062	1237289	23.07%	2.340%
21	15.669	2115	2122	2132	rBV	2794503	4044706	75.42%	7.649%
22	15.792	2137	2143	2159	rBV	1000765	1503132	28.03%	2.843%
23	15.910	2159	2163	2169	rVB4	15369	27962	0.52%	0.053%
24	17.110	2364	2367	2371	rBV6	5309	7026	0.13%	0.013%
25	17.222	2384	2386	2392	rVB4	4379	5702	0.11%	0.011%
26	17.433	2416	2422	2430	rBV	1868312	2619440	48.84%	4.954%
27	17.533	2433	2439	2457	rVV	3263072	4659996	86.89%	8.812%
28	19.339	2743	2746	2752	rVB2	41653	53391	1.00%	0.101%
29	19.410	2755	2758	2768	rVB	38408	61292	1.14%	0.116%
30	19.763	2812	2818	2831	rBV	4001032	5362991	100.00%	10.142%
31	21.521	3112	3117	3126	rBV	1881426	2606092	48.59%	4.928%
32	23.880	3510	3518	3528	rBV2	2118137	4374960	81.58%	8.273%
33	24.045	3539	3546	3558	rVB2	1028746	2274919	42.42%	4.302%




Sum of corrected areas: 52880108

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014385.D
Acq On : 30 Mar 2023 04:16
Operator : CG/JU
Sample : PB151682BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK682

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

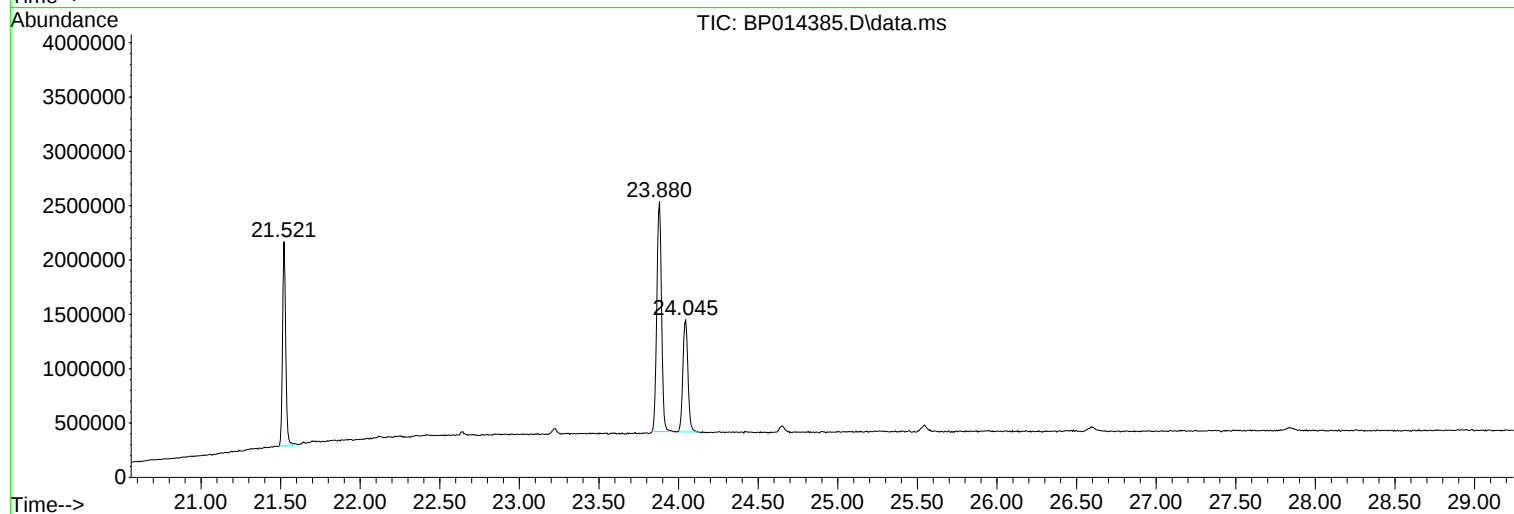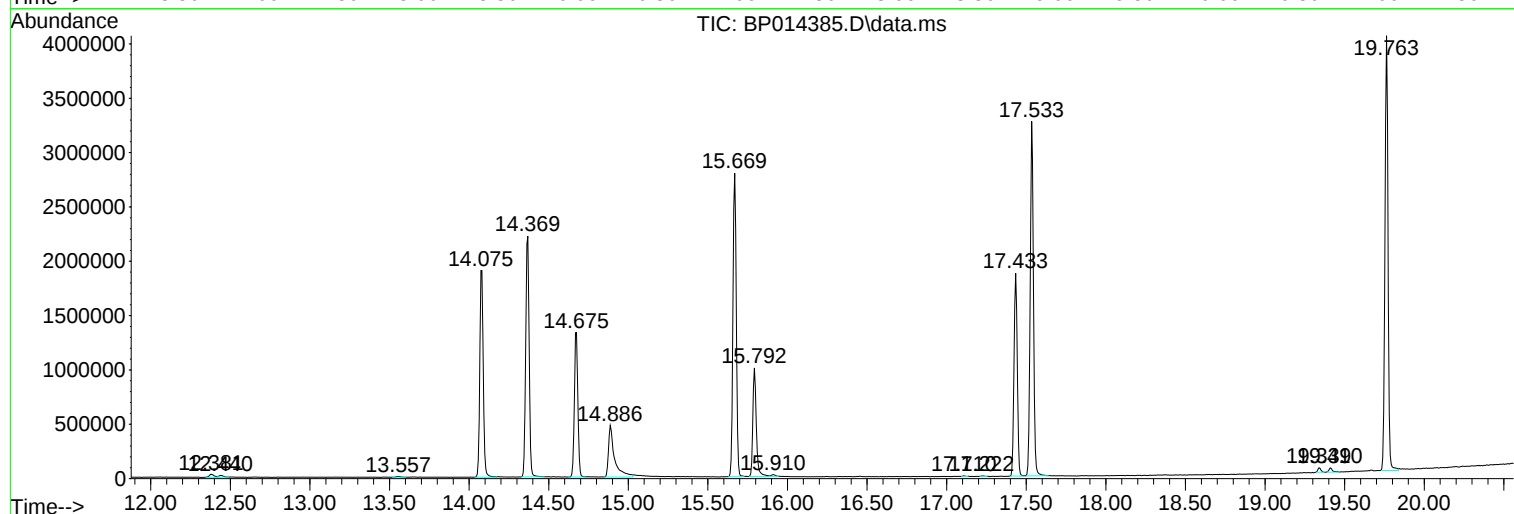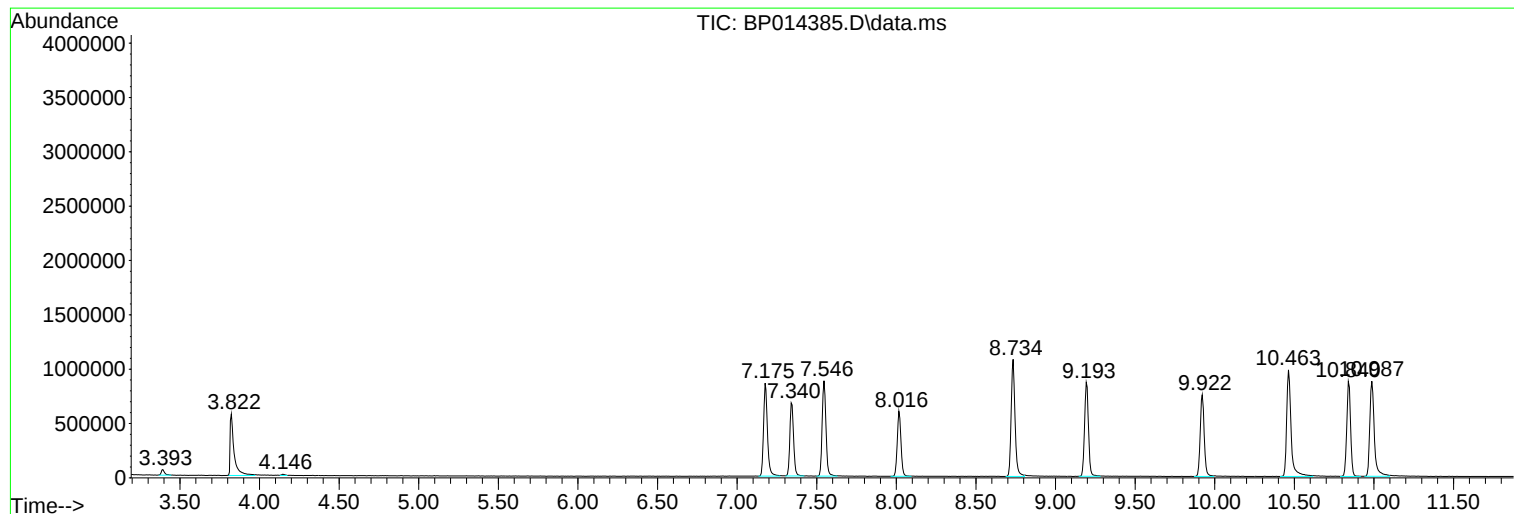

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014385.D
Acq On : 30 Mar 2023 04:16
Operator : CG/JU
Sample : PB151682BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK682

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014385.D
Acq On : 30 Mar 2023 04:16
Operator : CG/JU
Sample : PB151682BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK682

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc