

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
 Data File : BP014388.D
 Acq On : 30 Mar 2023 05:57
 Operator : CG/JU
 Sample : 02038-03
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EYF61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014388.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	45	rVB	36682	57369	0.89%	0.106%
2	3.834	108	110	128	rBV	96173	192563	3.00%	0.357%
3	4.046	142	146	153	rVB2	16112	26060	0.41%	0.048%
4	4.152	159	164	170	rVB4	11224	19853	0.31%	0.037%
5	4.258	178	182	187	rVB5	9412	14059	0.22%	0.026%
6	5.081	317	322	330	rBV	13412	23782	0.37%	0.044%
7	6.393	542	545	551	rVB4	9326	13594	0.21%	0.025%
8	7.111	659	667	671	rBV7	6618	12571	0.20%	0.023%
9	7.181	673	679	692	rVV	165401	309038	4.82%	0.573%
10	7.340	700	706	720	rBV	711873	1141492	17.79%	2.116%
11	7.546	734	741	758	rBV	678021	1129794	17.61%	2.094%
12	8.016	813	821	831	rBV	588561	966812	15.07%	1.792%
13	8.734	937	943	959	rBV	542006	957833	14.93%	1.775%
14	9.193	1014	1021	1041	rBV	909749	1557129	24.27%	2.886%
15	9.569	1076	1085	1092	rBV2	19864	35271	0.55%	0.065%
16	9.922	1137	1145	1165	rBV	750406	1306940	20.37%	2.422%
17	10.463	1229	1237	1262	rBV	919948	1800175	28.06%	3.337%
18	10.840	1294	1301	1316	rBV	858614	1421732	22.16%	2.635%
19	10.987	1318	1326	1340	rBV	739835	1479279	23.06%	2.742%
20	12.069	1506	1510	1516	rVB2	13867	19957	0.31%	0.037%
21	12.381	1557	1563	1569	rBV4	11072	25324	0.39%	0.047%
22	12.440	1569	1573	1582	rVB	16237	31595	0.49%	0.059%
23	13.304	1716	1720	1725	rVB6	3883	6526	0.10%	0.012%
24	13.475	1745	1749	1754	rBV8	4699	7415	0.12%	0.014%
25	13.545	1758	1761	1767	rBV8	4549	7980	0.12%	0.015%
26	13.640	1771	1777	1783	rVB8	3823	7936	0.12%	0.015%
27	14.081	1842	1852	1866	rBV	2193913	3260574	50.83%	6.044%
28	14.369	1890	1901	1916	rBV	2242227	3463250	53.99%	6.419%
29	14.675	1944	1953	1963	rBV	1320522	2016950	31.44%	3.738%
30	14.916	1988	1994	2011	rBV3	68333	257166	4.01%	0.477%
31	15.087	2018	2023	2026	rBV6	3807	6876	0.11%	0.013%
32	15.492	2088	2092	2098	rVB7	3743	6858	0.11%	0.013%
33	15.669	2115	2122	2129	rBV	3153375	4547468	70.89%	8.429%
34	15.722	2129	2131	2137	rVV4	23452	36735	0.57%	0.068%
35	15.792	2137	2143	2155	rVV	1228323	1756540	27.38%	3.256%
36	15.910	2159	2163	2168	rVB4	15828	27690	0.43%	0.051%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
 Data File : BP014388.D
 Acq On : 30 Mar 2023 05:57
 Operator : CG/JU
 Sample : 02038-03
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EYF61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	16.034	2179	2184	2192	rBV	47975	70964	1.11%	0.132%
38	16.245	2211	2220	2223	rBV	5804	13001	0.20%	0.024%
39	17.222	2383	2386	2392	rVB7	5409	8811	0.14%	0.016%
40	17.433	2415	2422	2432	rBV	1888724	2630230	41.00%	4.875%
41	17.533	2432	2439	2453	rVV	3800343	5434131	84.71%	10.072%
42	18.298	2564	2569	2577	rBV2	120878	210330	3.28%	0.390%
43	19.339	2742	2746	2752	rBV3	54691	75560	1.18%	0.140%
44	19.410	2753	2758	2771	rBV	52192	116991	1.82%	0.217%
45	19.527	2774	2778	2786	rBV3	69280	125920	1.96%	0.233%
46	19.669	2798	2802	2804	rBV5	17124	21084	0.33%	0.039%
47	19.763	2812	2818	2831	rBV	4951138	6414733	100.00%	11.890%
48	21.522	3112	3117	3126	rBV	2010060	2781013	43.35%	5.155%
49	23.880	3511	3518	3530	rVB2	2806373	5637927	87.89%	10.450%
50	24.045	3539	3546	3555	rVB2	1147149	2458438	38.32%	4.557%




Sum of corrected areas: 53951319

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014388.D
Acq On : 30 Mar 2023 05:57
Operator : CG/JU
Sample : 02038-03
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYF61

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

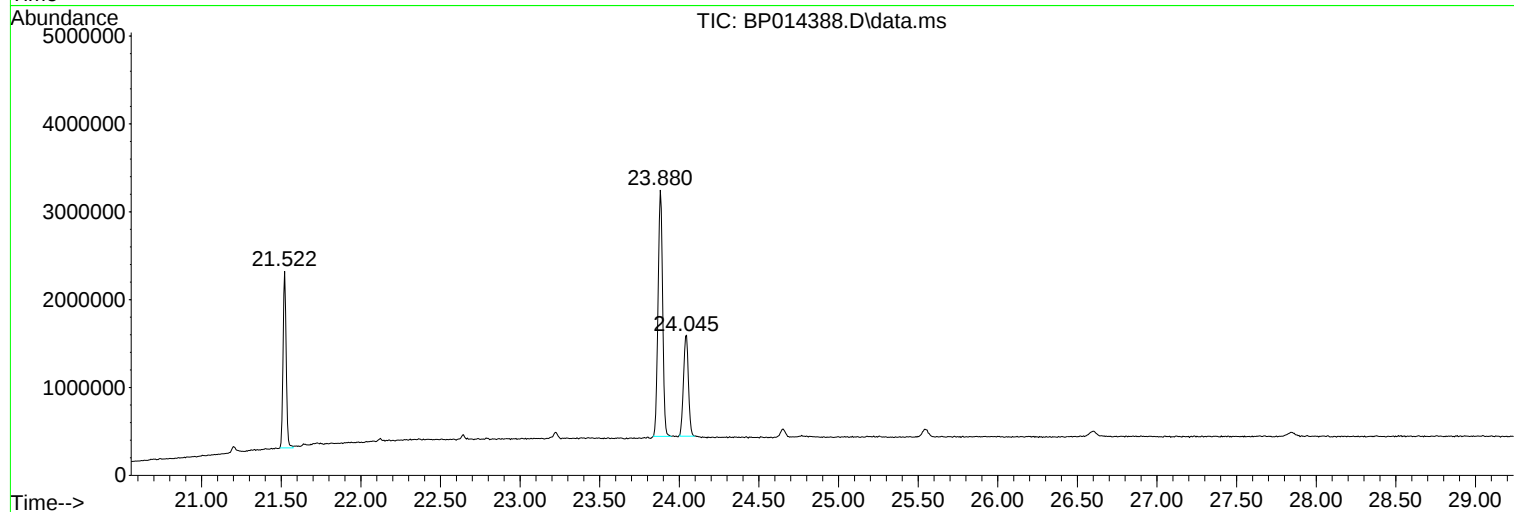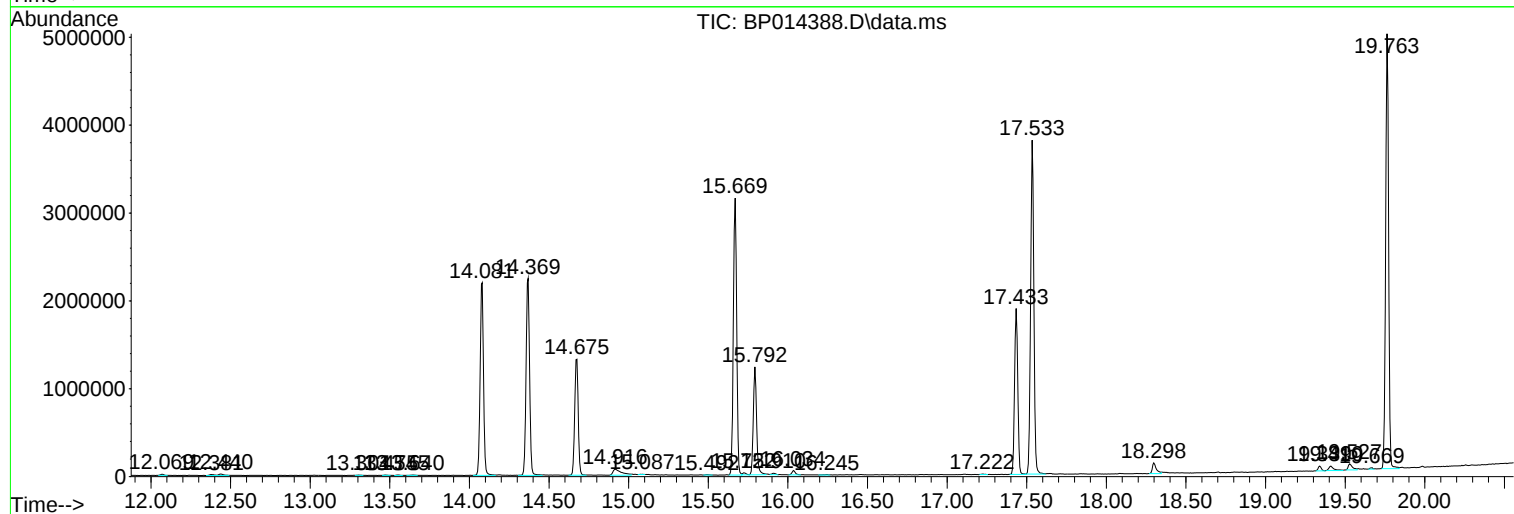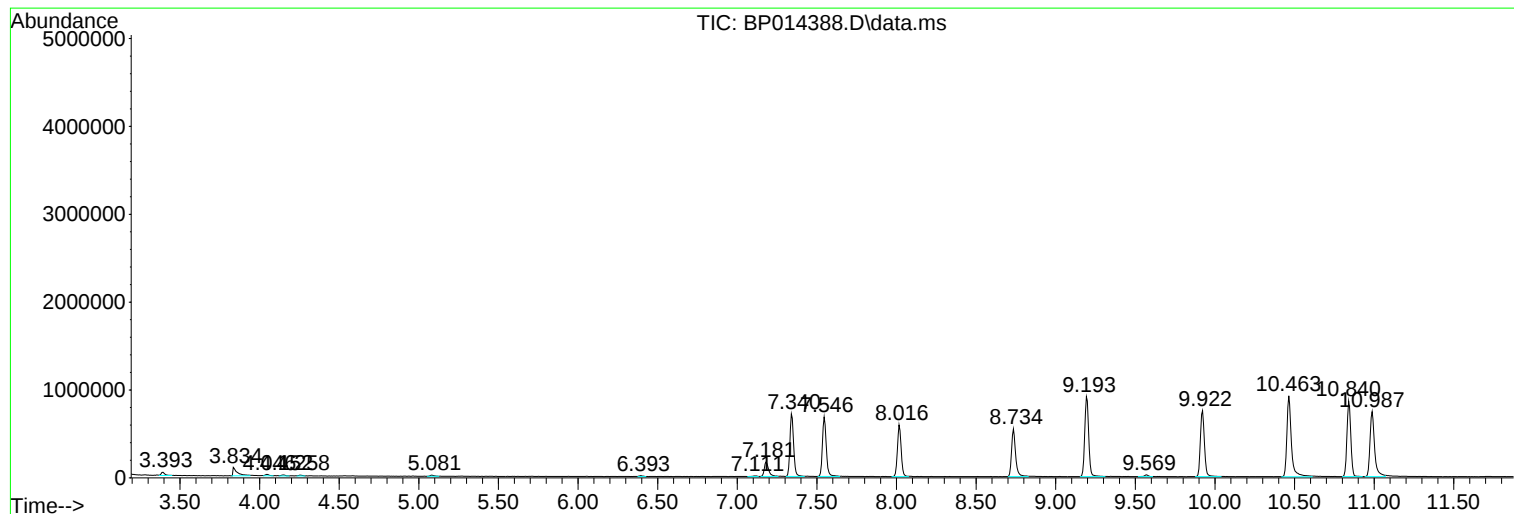

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014388.D
Acq On : 30 Mar 2023 05:57
Operator : CG/JU
Sample : 02038-03
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYF61

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032923\
Data File : BP014388.D
Acq On : 30 Mar 2023 05:57
Operator : CG/JU
Sample : 02038-03
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYF61

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc