

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033122\
 Data File : BP009636.D
 Acq On : 31 Mar 2022 13:19
 Operator : CG/JU
 Sample : N2155-04RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 22L076-DRE

Quant Time: Mar 31 14:43:15 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 31 04:36:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.740	152	256818	20.000	ng	0.00
21) Naphthalene-d8	10.534	136	1039666	20.000	ng	0.00
39) Acenaphthene-d10	14.386	164	695539	20.000	ng	0.00
64) Phenanthrene-d10	17.157	188	1063480	20.000	ng	0.00
76) Chrysene-d12	21.274	240	1034199	20.000	ng	0.00
86) Perylene-d12	23.662	264	1153756	20.000	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.352	112	207132	14.082	ng	0.00
7) Phenol-d6	6.934	99	1073045	53.942	ng	0.00
23) Nitrobenzene-d5	8.899	82	1636437	83.643	ng	0.00
42) 2,4,6-Tribromophenol	15.898	330	64453	5.616	ng	0.00
45) 2-Fluorobiphenyl	13.010	172	3747933	74.701	ng	0.00
79) Terphenyl-d14	19.739	244	4357608	75.628	ng	0.00
Target Compounds						Qvalue
9) Benzaldehyde	6.893	77	5073	Below Cal	#	80
15) Benzyl Alcohol	7.987	79	127606	8.046	ng	98
17) 2-Methylphenol	7.993	107	70504	5.127	ng	# 19
31) Naphthalene	10.581	128	374281	6.989	ng	99
33) 4-Chloroaniline	10.581	127	47573	2.177	ng	# 31
37) 2-Methylnaphthalene	12.198	142	215840	5.744	ng	99
38) 1-Methylnaphthalene	12.422	142	129738	3.544	ng	97
41) Hexachlorocyclopentadiene	12.557	237	29	7.291	ng	77
52) Acenaphthene	14.451	154	148444	3.940	ng	98
54) 2,4-Dinitrophenol	14.522	184	97	4.546	ng	# 1
55) Dibenzofuran	14.792	168	156659	2.475	ng	# 95
58) Fluorene	15.445	166	148485	2.983	ng	# 97
71) Phenanthrene	17.198	178	1530310	26.881	ng	99
72) Anthracene	17.292	178	382619	6.807	ng	99
73) Carbazole	17.569	167	163323	2.971	ng	98
74) Di-n-butylphthalate	18.127	149	159104	2.470	ng	98
75) Fluoranthene	19.186	202	1830930	26.566	ng	98
78) Pyrene	19.539	202	1575530	23.119	ng	99
81) Benzo(a)anthracene	21.263	228	831068	12.231	ng	99
83) Chrysene	21.316	228	724151	11.255	ng	97
84) Bis(2-ethylhexyl)phtha...	21.192	149	156419	3.874	ng	# 98
87) Indeno(1,2,3-cd)pyrene	26.151	276	507575	5.799	ng	# 91
88) Benzo(b)fluoranthene	22.939	252	1230354	17.863	ng	93
89) Benzo(k)fluoranthene	22.939	252	1230354	18.245	ng	93
90) Benzo(a)pyrene	23.557	252	668102	11.337	ng	97
92) Benzo(g,h,i)perylene	26.915	276	530669	7.394	ng	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033122\
Data File : BP009636.D
Acq On : 31 Mar 2022 13:19
Operator : CG/JU
Sample : N2155-04RE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
22L076-DRE

Quant Time: Mar 31 14:43:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 31 04:36:51 2022
Response via : Initial Calibration









#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.740 min Scan# 80
Delta R.T. -0.000 min
Lab File: BP009636.D
Acq: 31 Mar 2022 13:19




Instrument :
BNA_P
ClientSampleId :
22L076-DRE


Tgt Ion:152 Resp: 256818
Ion Ratio Lower Upper
152 100
150 156.3 124.5 186.7
115 59.7 48.2 72.4



#5
2-Fluorophenol
Concen: 14.082 ng
RT: 5.352 min Scan# 402
Delta R.T. 0.006 min
Lab File: BP009636.D
Acq: 31 Mar 2022 13:19

Tgt Ion:112 Resp: 207132
Ion Ratio Lower Upper
112 100
64 54.9 45.0 67.4
63 28.8 23.0 34.6







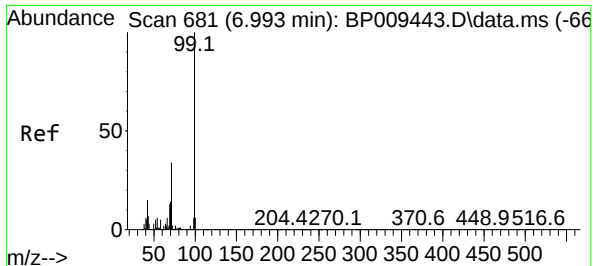

#7
Phenol-d6
Concen: 53.942 ng
RT: 6.934 min Scan# 61
Delta R.T. -0.000 min
Lab File: BP009636.D
Acq: 31 Mar 2022 13:19




Instrument :
BNA_P
ClientSampleId :
22L076-DRE


Tgt Ion: 99 Resp: 1073045
Ion Ratio Lower Upper
99 100
42 15.5 12.8 19.2
71 32.9 26.3 39.5



#15
Benzyl Alcohol
Concen: 8.046 ng
RT: 7.987 min Scan# 850
Delta R.T. -0.000 min
Lab File: BP009636.D
Acq: 31 Mar 2022 13:19

Tgt Ion: 79 Resp: 127606
Ion Ratio Lower Upper
79 100
108 76.3 62.5 93.7
77 63.3 51.7 77.5









#17
2-Methylphenol
Concen: 5.127 ng
RT: 7.993 min Scan# 81
Delta R.T. -0.206 min
Lab File: BP009636.D
Acq: 31 Mar 2022 13:19




Instrument :
BNA_P
ClientSampleId :
22L076-DRE


Tgt Ion:107 Resp: 70504
Ion Ratio Lower Upper
107 100
108 141.6 90.2 135.2#
77 112.0 36.3 54.5#
79 171.3 35.4 53.0#



#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.534 min Scan# 1283
Delta R.T. -0.000 min
Lab File: BP009636.D
Acq: 31 Mar 2022 13:19

Tgt Ion:136 Resp: 1039666
Ion Ratio Lower Upper
136 100
137 10.6 8.6 12.8
54 6.5 5.8 8.8
68 6.2 5.2 7.8









#23
Nitrobenzene-d5
Concen: 83.643 ng
RT: 8.899 min Scan# 1005
Delta R.T. -0.000 min
Lab File: BP009636.D
Acq: 31 Mar 2022 13:19




Instrument :
BNA_P
ClientSampleId :
22L076-DRE


Tgt Ion: 82 Resp: 1636437
Ion Ratio Lower Upper
82 100
128 43.8 34.2 51.4
54 41.4 34.7 52.1



#31
Naphthalene
Concen: 6.989 ng
RT: 10.581 min Scan# 1291
Delta R.T. -0.000 min
Lab File: BP009636.D
Acq: 31 Mar 2022 13:19

Tgt Ion: 128 Resp: 374281
Ion Ratio Lower Upper
128 100
129 11.1 8.6 13.0
127 12.8 10.5 15.7









#33
4-Chloroaniline
Concen: 2.177 ng
RT: 10.581 min Scan# 11
Delta R.T. -0.118 min
Lab File: BP009636.D
Acq: 31 Mar 2022 13:19




Instrument :
BNA_P
ClientSampleId :
22L076-DRE


Tgt Ion:	127	Resp:	47573
Ion	Ratio	Lower	Upper
127	100		
129	87.0	25.5	38.3#
65	0.0	24.3	36.5#
92	1.7	15.8	23.8#



#37
2-Methylnaphthalene
Concen: 5.744 ng
RT: 12.198 min Scan# 1566
Delta R.T. -0.006 min
Lab File: BP009636.D
Acq: 31 Mar 2022 13:19

Tgt Ion:	142	Resp:	215840
Ion	Ratio	Lower	Upper
142	100		
141	88.1	70.2	105.4
115	35.1	27.4	41.2









#38
1-Methylnaphthalene
Concen: 3.544 ng
RT: 12.422 min Scan# 1
Delta R.T. -0.000 min
Lab File: BP009636.D
Acq: 31 Mar 2022 13:19




Instrument :
BNA_P
ClientSampleId :
22L076-DRE


Tgt Ion:142 Resp: 129738
Ion Ratio Lower Upper
142 100
141 88.9 73.5 110.3
116 4.0 3.3 4.9



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.386 min Scan# 1938
Delta R.T. -0.006 min
Lab File: BP009636.D
Acq: 31 Mar 2022 13:19

Tgt Ion:164 Resp: 695539
Ion Ratio Lower Upper
164 100
162 99.5 79.1 118.7
160 43.8 34.9 52.3









#41
Hexachlorocyclopentadiene
Concen: 7.291 ng
RT: 12.557 min Scan# 1
Delta R.T. -0.000 min
Lab File: BP009636.D
Acq: 31 Mar 2022 13:19




Instrument :
BNA_P
ClientSampleId :
22L076-DRE


Tgt Ion:	237	Resp:	29
Ion	Ratio	Lower	Upper
237	100		
235	45.9	42.6	82.6
272	0.0	0.0	32.8



#42
2,4,6-Tribromophenol
Concen: 5.616 ng
RT: 15.898 min Scan# 2195
Delta R.T. 0.006 min
Lab File: BP009636.D
Acq: 31 Mar 2022 13:19

Tgt Ion:	330	Resp:	64453
Ion	Ratio	Lower	Upper
330	100		
332	94.5	77.0	115.6
141	28.3	27.6	41.4









#45
2-Fluorobiphenyl
Concen: 74.701 ng
RT: 13.010 min Scan# 1713
Delta R.T. -0.000 min
Lab File: BP009636.D
Acq: 31 Mar 2022 13:19




Instrument :
BNA_P
ClientSampleId :
22L076-DRE


Tgt Ion:172 Resp: 3747933
Ion Ratio Lower Upper
172 100
171 35.3 28.0 42.0
170 23.5 18.6 27.8



#52
Acenaphthene
Concen: 3.940 ng
RT: 14.451 min Scan# 1949
Delta R.T. -0.006 min
Lab File: BP009636.D
Acq: 31 Mar 2022 13:19

Tgt Ion:154 Resp: 148444
Ion Ratio Lower Upper
154 100
153 109.8 90.2 135.4
152 54.1 42.7 64.1









#54
2,4-Dinitrophenol
Concen: 4.546 ng
RT: 14.522 min Scan# 1961
Delta R.T. -0.006 min
Lab File: BP009636.D
Acq: 31 Mar 2022 13:19




Instrument :
BNA_P
ClientSampleId :
22L076-DRE


Tgt Ion:184 Resp: 97
Ion Ratio Lower Upper
184 100
63 297.2 46.3 69.5#
154 926.2 45.8 68.6#



#55
Dibenzofuran
Concen: 2.475 ng
RT: 14.792 min Scan# 2007
Delta R.T. -0.000 min
Lab File: BP009636.D
Acq: 31 Mar 2022 13:19

Tgt Ion:168 Resp: 156659
Ion Ratio Lower Upper
168 100
139 38.3 29.1 43.7
169 17.4 10.6 16.0#





#58

Fluorene

Concen: 2.983 ng

RT: 15.445 min Scan# 21

Delta R.T. -0.000 min

Lab File: BP009636.D

Acq: 31 Mar 2022 13:19

Instrument :

BNA_P

ClientSampleId :

22L076-DRE





Tgt Ion:166 Resp: 148485

Ion Ratio Lower Upper

166 100

165 96.3 79.2 118.8

167 16.3 10.7 16.1#



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.157 min Scan# 2409

Delta R.T. -0.000 min

Lab File: BP009636.D

Acq: 31 Mar 2022 13:19




Tgt Ion:188 Resp: 1063480


Ion Ratio Lower Upper

188 100

94 8.4 7.9 11.9

80 9.2 8.8 13.2









#71
Phenanthrene
Concen: 26.881 ng
RT: 17.198 min Scan# 2425
Delta R.T. -0.000 min
Lab File: BP009636.D
Acq: 31 Mar 2022 13:19




Instrument :
BNA_P
ClientSampleId :
22L076-DRE


Tgt Ion:178 Resp: 1530310
Ion Ratio Lower Upper
178 100
176 18.9 15.4 23.2
179 15.2 12.3 18.5



#72
Anthracene
Concen: 6.807 ng
RT: 17.292 min Scan# 2432
Delta R.T. -0.000 min
Lab File: BP009636.D
Acq: 31 Mar 2022 13:19

Tgt Ion:178 Resp: 382619
Ion Ratio Lower Upper
178 100
176 18.1 14.8 22.2
179 16.0 12.2 18.4









#73
 Carbazole
 Concen: 2.971 ng
 RT: 17.569 min Scan# 2487
 Delta R.T. -0.000 min
 Lab File: BP009636.D
 Acq: 31 Mar 2022 13:19




Instrument :
 BNA_P
 ClientSampleId :
 22L076-DRE


Tgt Ion:167	Resp: 163323		
Ion Ratio	Lower	Upper	
167	100		
166	22.7	17.2	25.8
139	13.3	10.3	15.5



#74
 Di-n-butylphthalate
 Concen: 2.470 ng
 RT: 18.127 min Scan# 2574
 Delta R.T. -0.000 min
 Lab File: BP009636.D
 Acq: 31 Mar 2022 13:19

Tgt Ion:149	Resp: 159104		
Ion Ratio	Lower	Upper	
149 100			
150 9.7	7.3	10.9	
104 4.3	4.2	6.2	





#75

Fluoranthene

Concen: 26.566 ng

RT: 19.186 min Scan# 21

Delta R.T. 0.006 min

Lab File: BP009636.D

Acq: 31 Mar 2022 13:19

Instrument :

BNA_P

ClientSampleId :

22L076-DRE





Tgt Ion:202 Resp: 1830930

Ion Ratio Lower Upper

202 100

101 9.5 0.0 31.5

203 17.8 0.0 37.8



#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.274 min Scan# 3109

Delta R.T. -0.000 min

Lab File: BP009636.D

Acq: 31 Mar 2022 13:19




Tgt Ion:240 Resp: 1034199


Ion Ratio Lower Upper

240 100

120 9.4 9.0 13.4

236 26.0 20.6 30.8





#78

Pyrene

Concen: 23.119 ng

RT: 19.539 min Scan# 2814

Delta R.T. -0.000 min

Lab File: BP009636.D

Acq: 31 Mar 2022 13:19

Instrument :

BNA_P

ClientSampleId :

22L076-DRE





Tgt Ion:202 Resp: 1575530

Ion Ratio Lower Upper

202 100

200 20.6 16.8 25.2

203 18.1 14.2 21.4



#79

Terphenyl-d14

Concen: 75.628 ng

RT: 19.739 min Scan# 2848

Delta R.T. -0.000 min

Lab File: BP009636.D

Acq: 31 Mar 2022 13:19




Tgt Ion:244 Resp: 4357608


Ion Ratio Lower Upper

244 100

212 6.5 5.8 8.6

122 8.7 8.3 12.5





#81

Benzo(a)anthracene

Concen: 12.231 ng

RT: 21.263 min Scan# 3110

Delta R.T. -0.000 min

Lab File: BP009636.D

Acq: 31 Mar 2022 13:19

Instrument :

BNA_P

ClientSampleId :

22L076-DRE





Tgt Ion:228 Resp: 831068

Ion Ratio Lower Upper

228 100

226 27.6 22.0 33.0

229 21.2 16.1 24.1



#83

Chrysene

Concen: 11.255 ng

RT: 21.316 min Scan# 3116

Delta R.T. 0.006 min

Lab File: BP009636.D

Acq: 31 Mar 2022 13:19




Tgt Ion:228 Resp: 724151


Ion Ratio Lower Upper

228 100

226 30.3 24.2 36.2

229 23.2 16.1 24.1









#84
Bis(2-ethylhexyl)phthalate
Concen: 3.874 ng
RT: 21.192 min Scan# 3095
Delta R.T. -0.000 min
Lab File: BP009636.D
Acq: 31 Mar 2022 13:19




Instrument :
BNA_P
ClientSampleId :
22L076-DRE


Tgt Ion:149 Resp: 156419
Ion Ratio Lower Upper
149 100
167 28.6 22.6 33.8
279 6.7 3.8 5.6#



#86
Perylene-d12
Concen: 20.000 ng
RT: 23.662 min Scan# 3515
Delta R.T. 0.012 min
Lab File: BP009636.D
Acq: 31 Mar 2022 13:19

Tgt Ion:264 Resp: 1153756
Ion Ratio Lower Upper
264 100
260 23.7 19.4 29.0
265 22.9 17.2 25.8





#87

Indeno(1,2,3-cd)pyrene

Concen: 5.799 ng

RT: 26.151 min Scan# 3392

Delta R.T. 0.012 min

Lab File: BP009636.D

Acq: 31 Mar 2022 13:19

Instrument :

BNA_P

ClientSampleId :

22L076-DRE





Tgt Ion:276 Resp: 507575

Ion Ratio Lower Upper

276 100

138 17.9 20.5 30.7#

277 24.1 20.4 30.6



#88

Benzo(b)fluoranthene

Concen: 17.863 ng

RT: 22.939 min Scan# 3392

Delta R.T. 0.012 min

Lab File: BP009636.D

Acq: 31 Mar 2022 13:19




Tgt Ion:252 Resp: 1230354


Ion Ratio Lower Upper

252 100

253 25.7 17.8 26.8

125 12.1 8.1 12.1









#89
Benzo(k)fluoranthene
Concen: 18.245 ng
RT: 22.939 min Scan# 31
Delta R.T. -0.041 min
Lab File: BP009636.D
Acq: 31 Mar 2022 13:19




Instrument :
BNA_P
ClientSampleId :
22L076-DRE


Tgt Ion:252 Resp: 1230354
Ion Ratio Lower Upper
252 100
253 25.7 17.5 26.3
125 12.1 8.3 12.5



#90
Benzo(a)pyrene
Concen: 11.337 ng
RT: 23.557 min Scan# 3497
Delta R.T. 0.006 min
Lab File: BP009636.D
Acq: 31 Mar 2022 13:19

Tgt Ion:252 Resp: 668102
Ion Ratio Lower Upper
252 100
253 24.2 17.8 26.6
125 12.4 9.3 13.9





#92

Benzo(g,h,i)perylene

Concen: 7.394 ng

RT: 26.915 min Scan# 40

Delta R.T. 0.018 min

Lab File: BP009636.D


Acq: 31 Mar 2022 13:19

Instrument :

BNA_P

ClientSampleId :

22L076-DRE



Tgt Ion:276 Resp: 530669

Ion Ratio Lower Upper

276 100

277 27.1 19.2 28.8

138 20.6 18.0 27.0

