
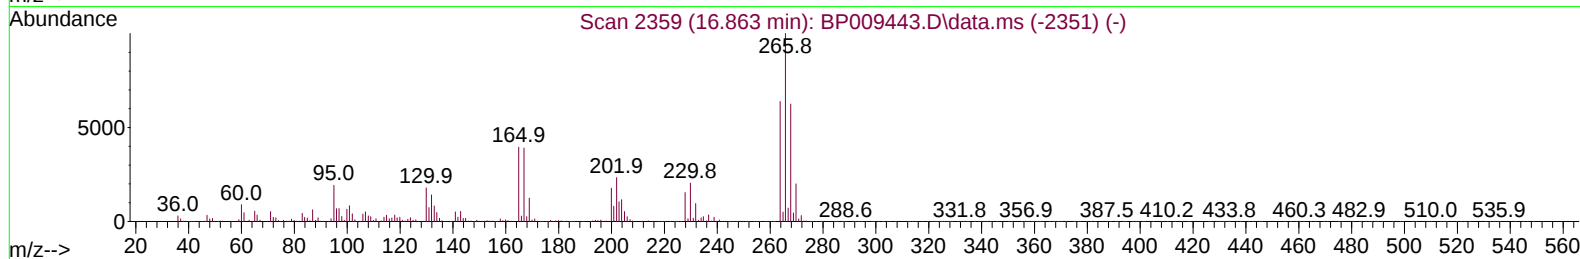
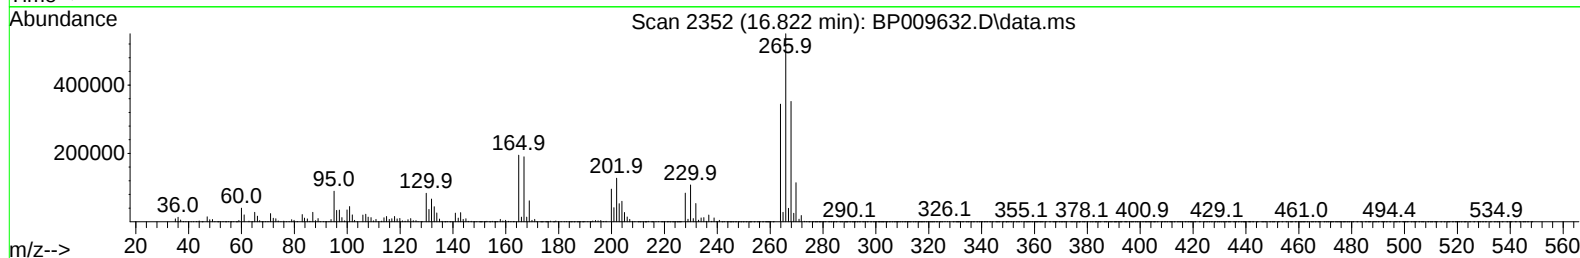


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033122\
Data File : BP009632.D
Acq On : 31 Mar 2022 10:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 31 14:23:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 31 04:36:51 2022
Response via : Initial Calibration

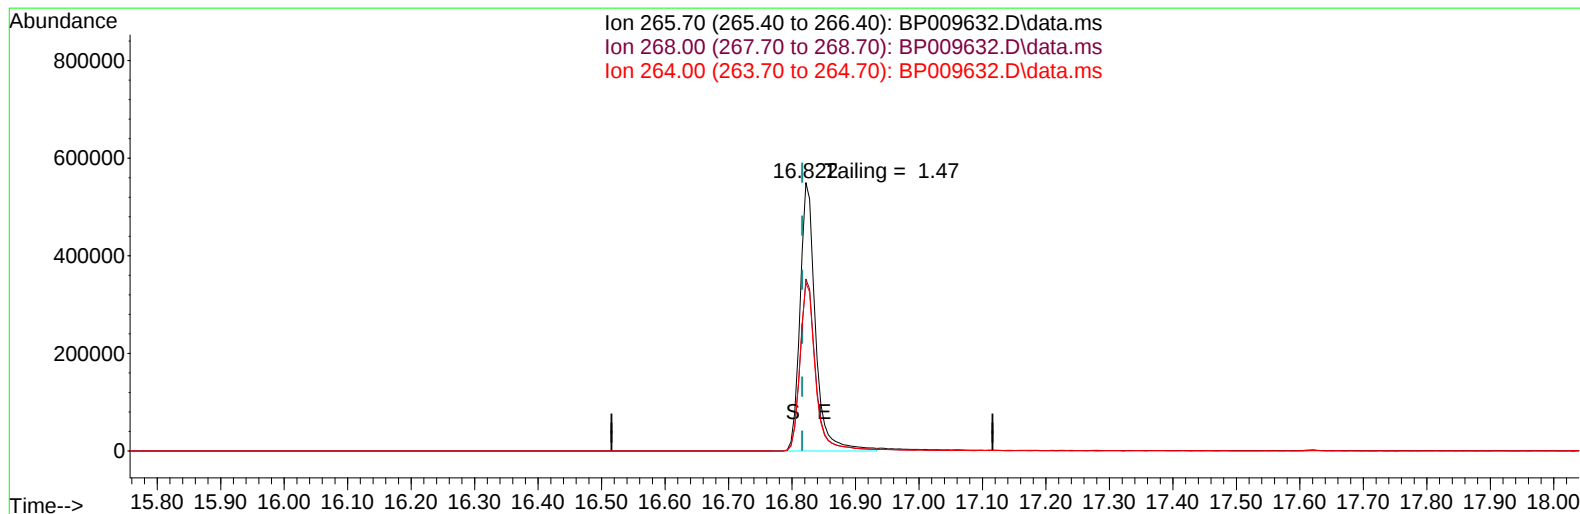

TIC: BP009632.D\data.ms

(70) Pentachlorophenol (C)




16.822min (+ 0.006) 138379.53 ng

response 958412

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.04
264.00	63.60	62.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033122\
Data File : BP009632.D
Acq On : 31 Mar 2022 10:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 31 14:23:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 31 04:36:51 2022
Response via : Initial Calibration

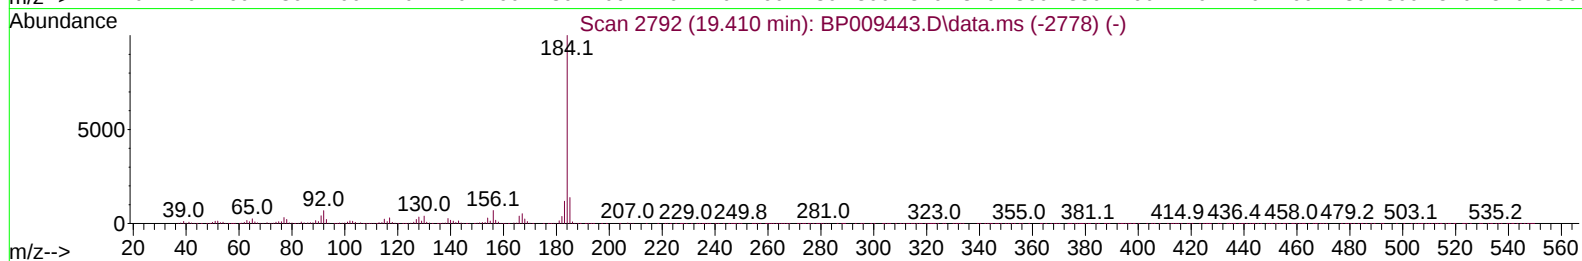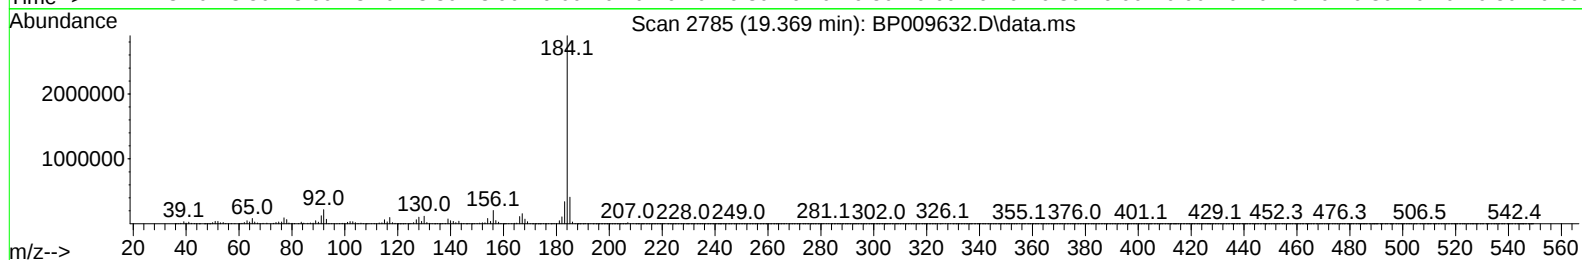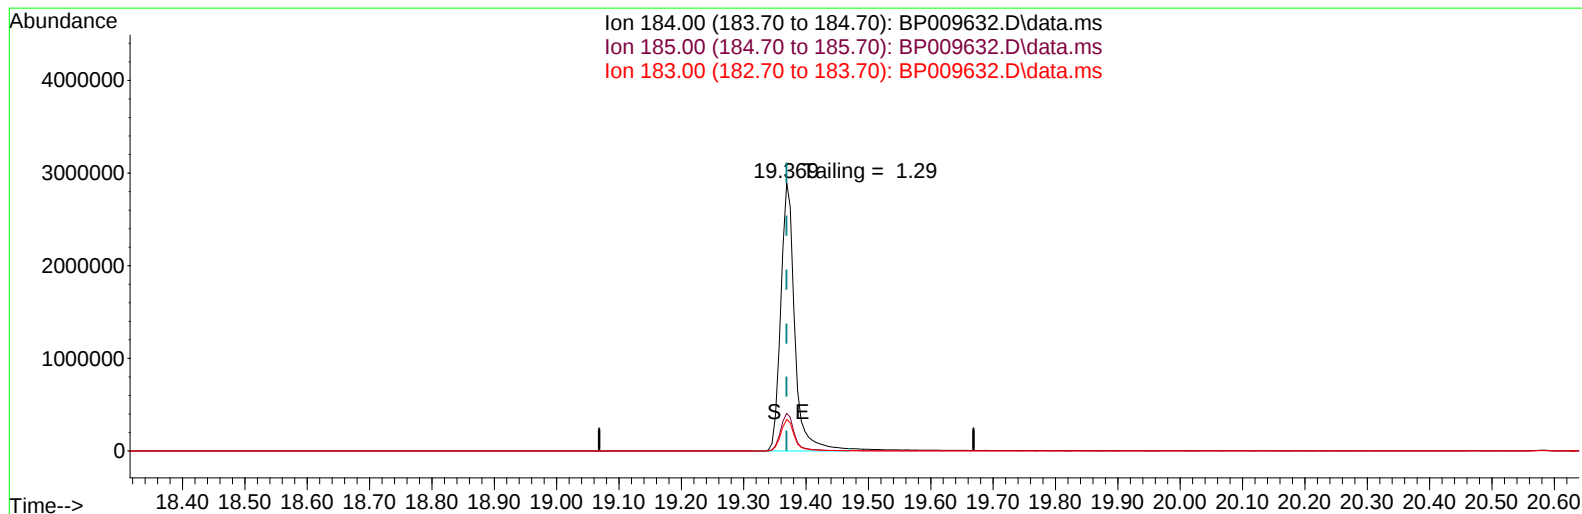

TIC: BP009632.D\data.ms

(77) Benzidine**19.369min (+ 0.000) 40593.78 ng****response 4630763**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.10
183.00	11.70	11.75
0.00	0.00	0.00