

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033122\
 Data File : BP009639.D
 Acq On : 31 Mar 2022 15:01
 Operator : CG/JU
 Sample : N2195-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 TP-2-1-5FT

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009639.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.346	395	401	421	rBV	2608321	4620274	45.09%	8.488%
2	6.934	663	671	695	rBV	2487978	4776118	46.61%	8.774%
3	7.740	801	808	817	rBV	834558	1481239	14.46%	2.721%
4	8.899	998	1005	1016	rBV	1644056	3165008	30.89%	5.814%
5	10.534	1276	1283	1299	rBV	1087949	2141403	20.90%	3.934%
6	13.010	1696	1704	1721	rBV	4965964	7798549	76.11%	14.326%
7	14.392	1931	1939	1946	rBV	1379979	2214830	21.61%	4.069%
8	15.892	2188	2194	2214	rBV	2931701	4783504	46.68%	8.788%
9	17.157	2403	2409	2414	rBV	1609041	2526470	24.66%	4.641%
10	17.198	2414	2416	2423	rVB	276079	383108	3.74%	0.704%
11	18.069	2561	2564	2574	rVB3	195945	356138	3.48%	0.654%
12	19.186	2749	2754	2760	rBV	982667	1426324	13.92%	2.620%
13	19.539	2810	2814	2824	rVB	951199	1380713	13.47%	2.536%
14	19.739	2843	2848	2854	rBV	7945963	10247026	100.00%	18.824%
15	21.274	3104	3109	3114	rBV2	2548656	4117264	40.18%	7.564%
16	23.662	3510	3515	3522	rVB2	1528964	3016891	29.44%	5.542%




Sum of corrected areas: 54434859

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033122\
Data File : BP009639.D
Acq On : 31 Mar 2022 15:01
Operator : CG/JU
Sample : N2195-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TP-2-1-5FT

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

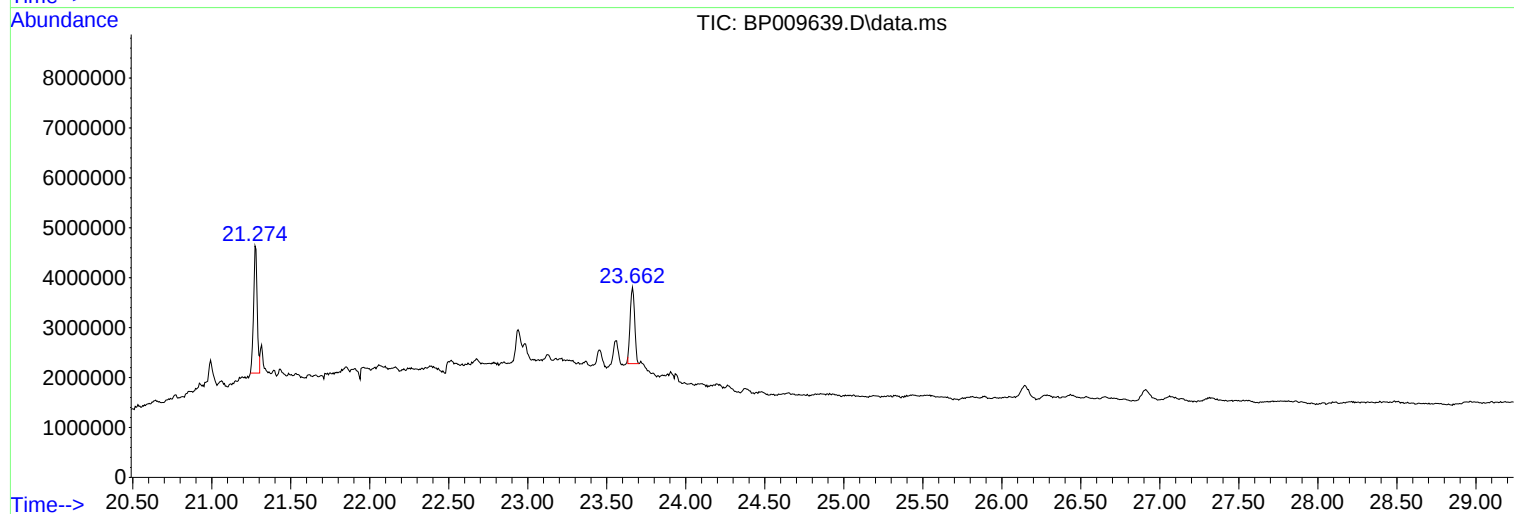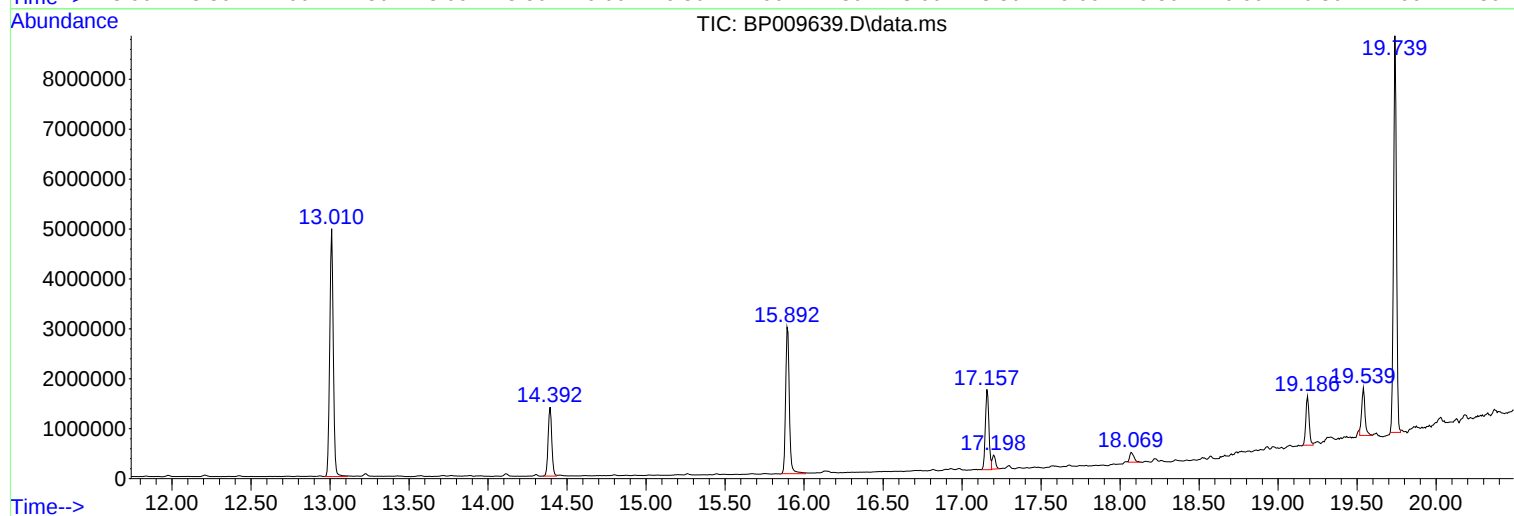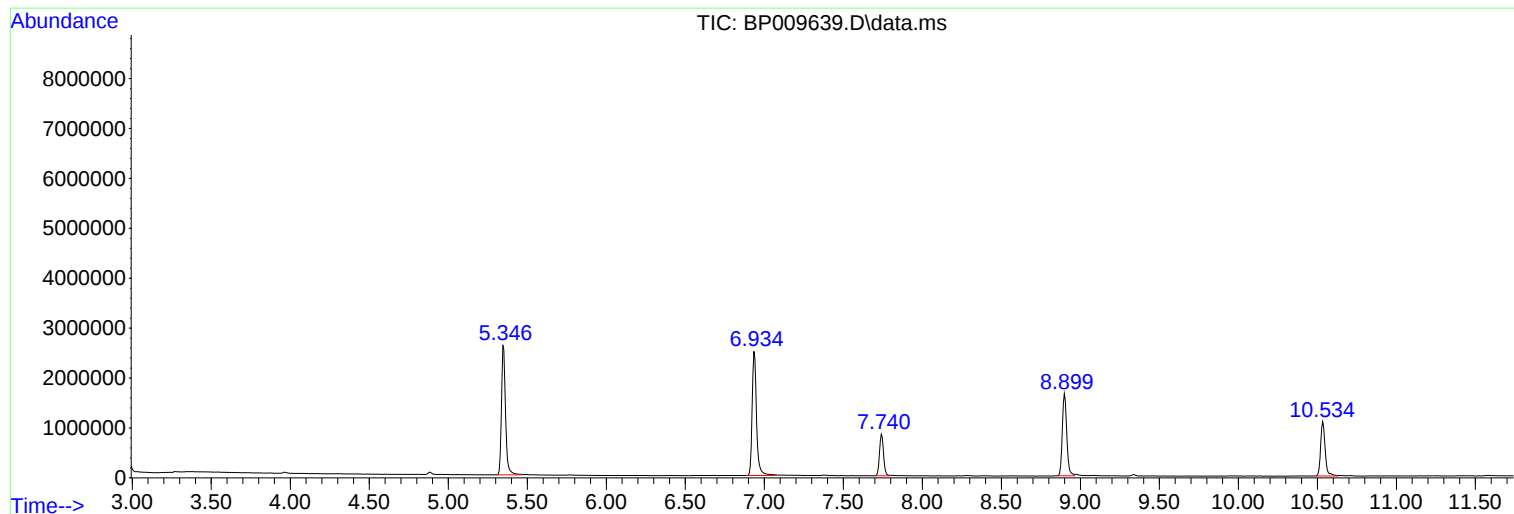

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033122\
Data File : BP009639.D
Acq On : 31 Mar 2022 15:01
Operator : CG/JU
Sample : N2195-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TP-2-1-5FT










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 n-Hexadecanoic acid Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
18.069	2.82 ng	356138	Phenanthrene-d10	17.157

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			n-Hexadecanoic acid	256	C16H32O2	000057-10-3	98
2			Tetradecanoic acid	228	C14H28O2	000544-63-8	97
3			n-Decanoic acid	172	C10H20O2	000334-48-5	91
4			Tridecanoic acid	214	C13H26O2	000638-53-9	90
5			Pentadecanoic acid	242	C15H30O2	001002-84-2	90

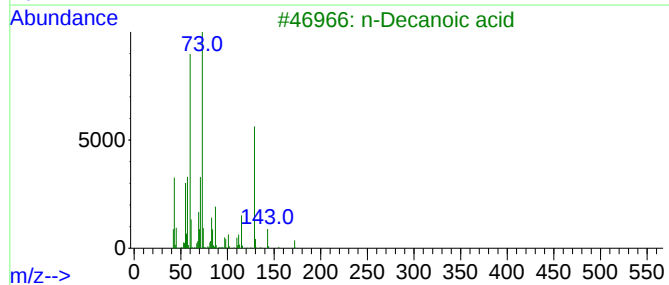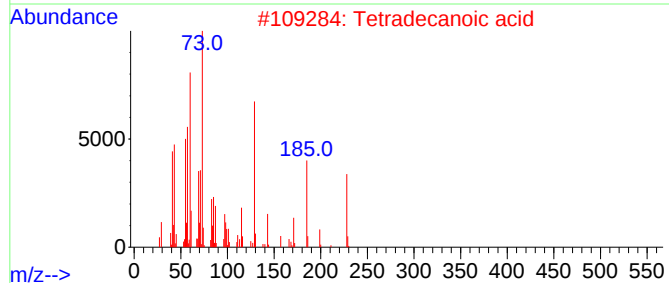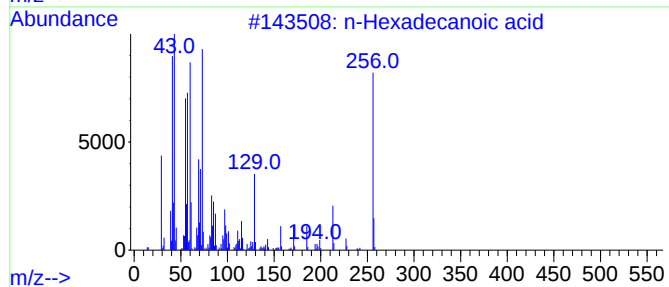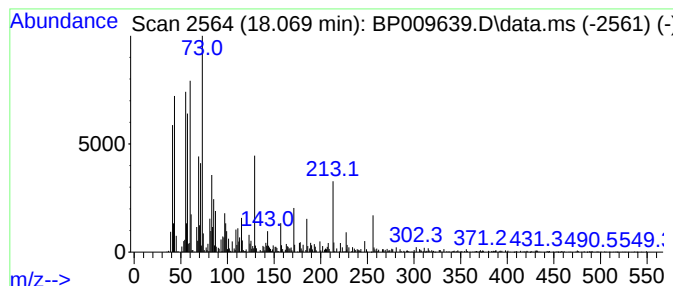

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033122\
Data File : BP009639.D
Acq On : 31 Mar 2022 15:01
Operator : CG/JU
Sample : N2195-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TP-2-1-5FT

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
n-Hexadecanoic ...	18.069	2.8	ng	356138	4	17.157	2526470	20.0