
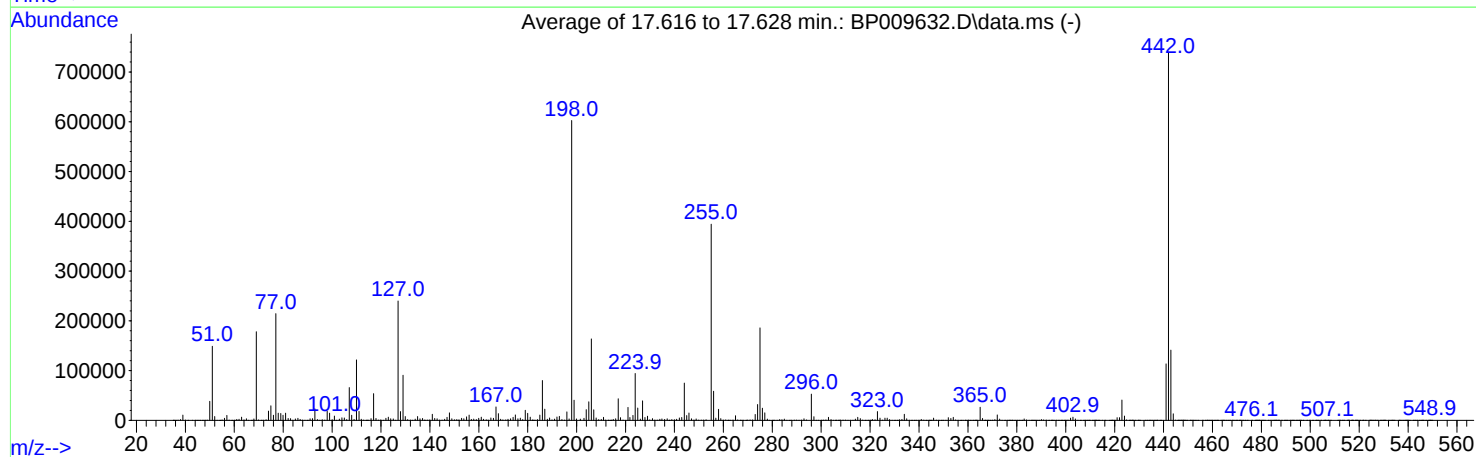


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033122\
 Data File : BP009632.D
 Acq On : 31 Mar 2022 10:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 31 04:36:51 2022

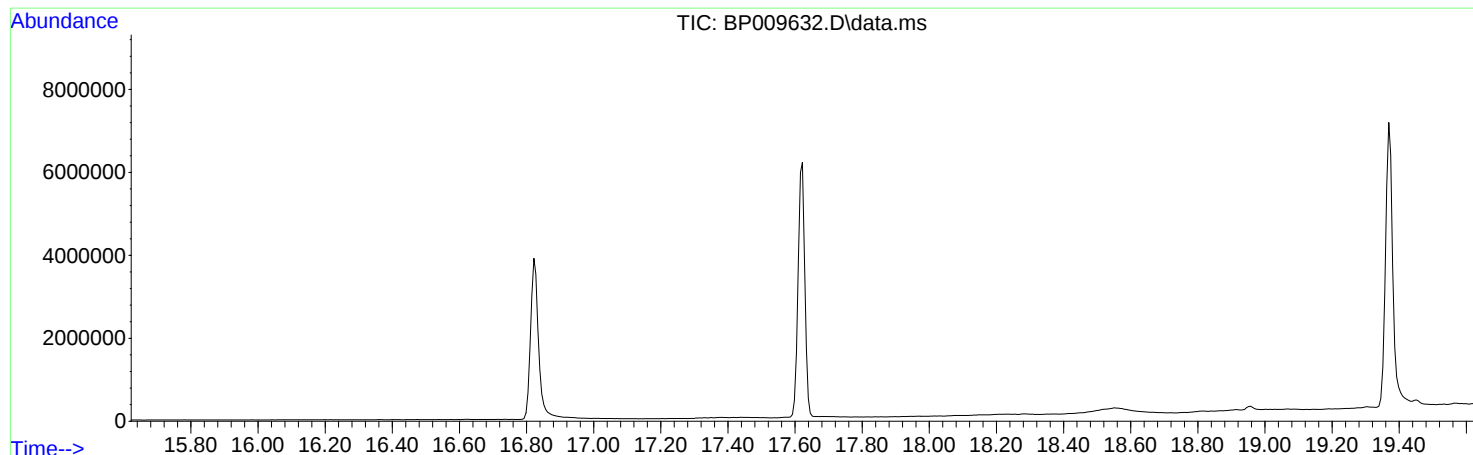




AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.7	148889	PASS
68	69	0.00	2	1.6	2923	PASS
69	198	0.00	100	29.5	177989	PASS
70	69	0.00	2	0.5	914	PASS
127	198	10	80	39.8	239757	PASS
197	198	0.00	2	0.5	3071	PASS
198	198	100	100	100.0	602512	PASS
199	198	5	9	6.7	40551	PASS
275	198	10	60	30.8	185775	PASS
365	198	1	100	4.4	26457	PASS
441	198	0.01	100	18.8	113499	PASS
442	442	100	100	100.0	739099	PASS
443	442	15	24	19.1	141285	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033122\
Data File : BP009632.D
Acq On : 31 Mar 2022 10:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 31 14:23:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 31 04:36:51 2022
Response via : Initial Calibration

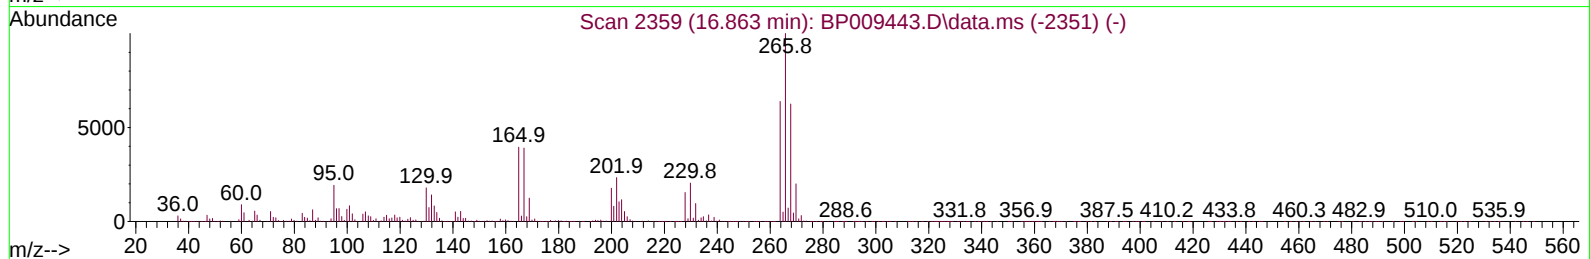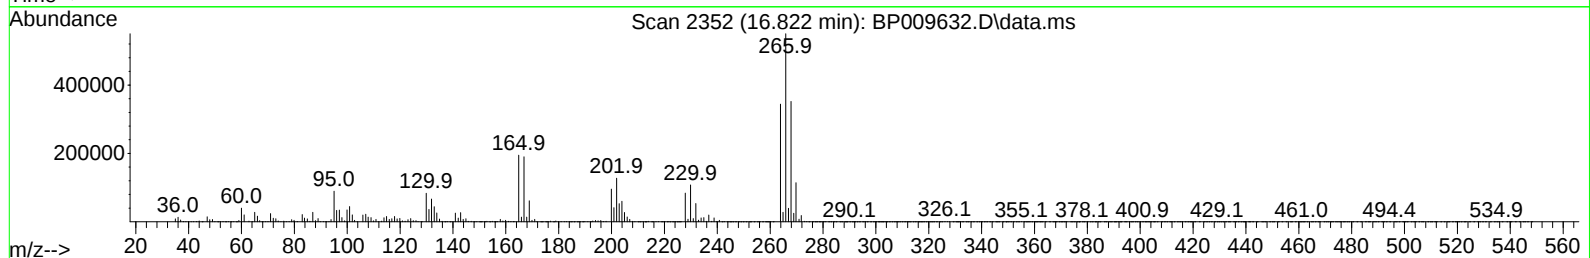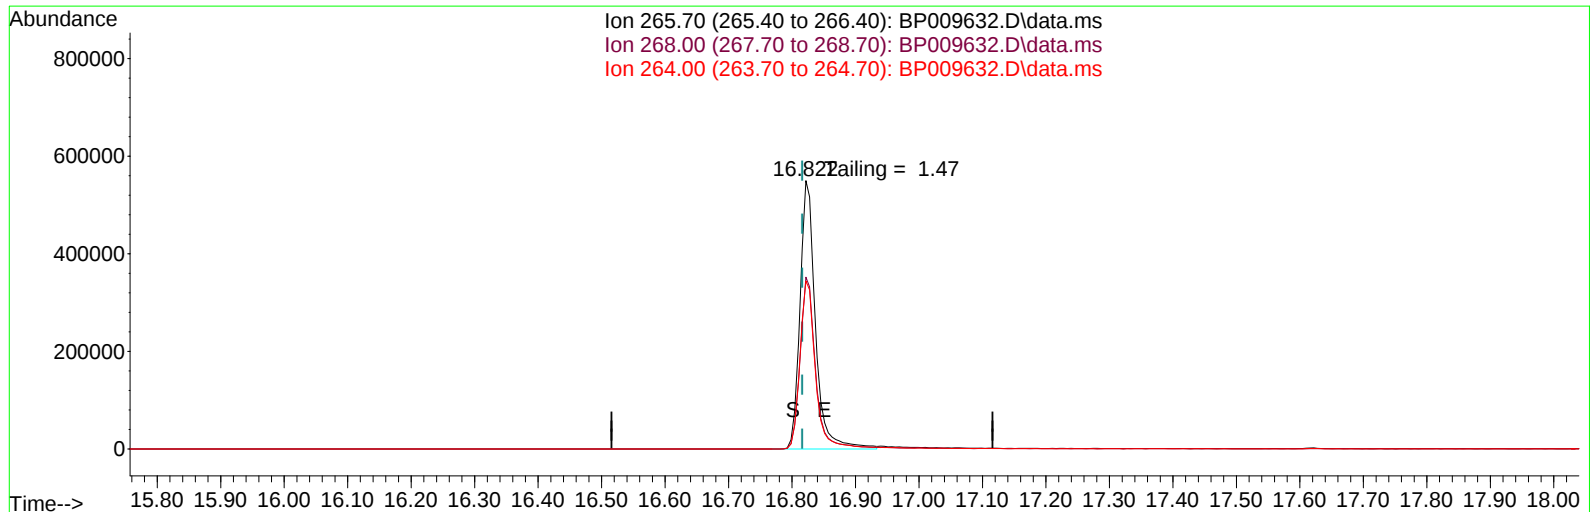

TIC: BP009632.D\data.ms

(70) Pentachlorophenol (C)

16.822min (+ 0.006) 138379.53 ng




response 958412

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.04
264.00	63.60	62.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033122\
Data File : BP009632.D
Acq On : 31 Mar 2022 10:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 31 14:23:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 31 04:36:51 2022
Response via : Initial Calibration

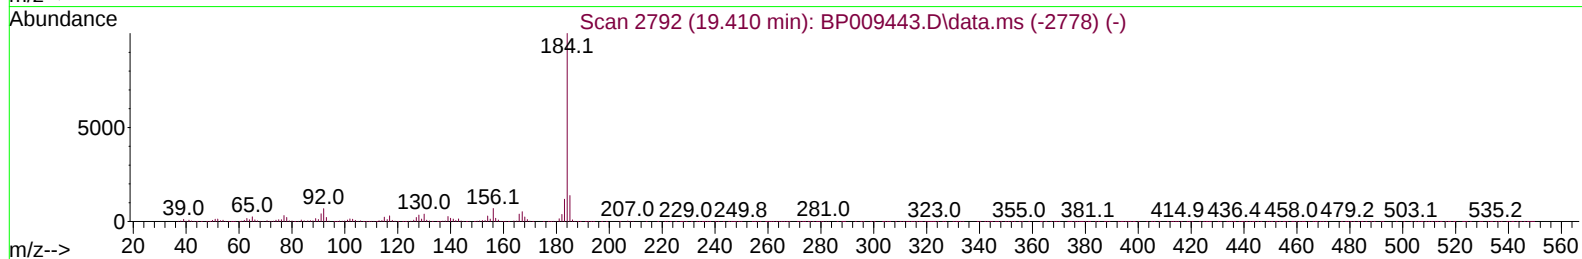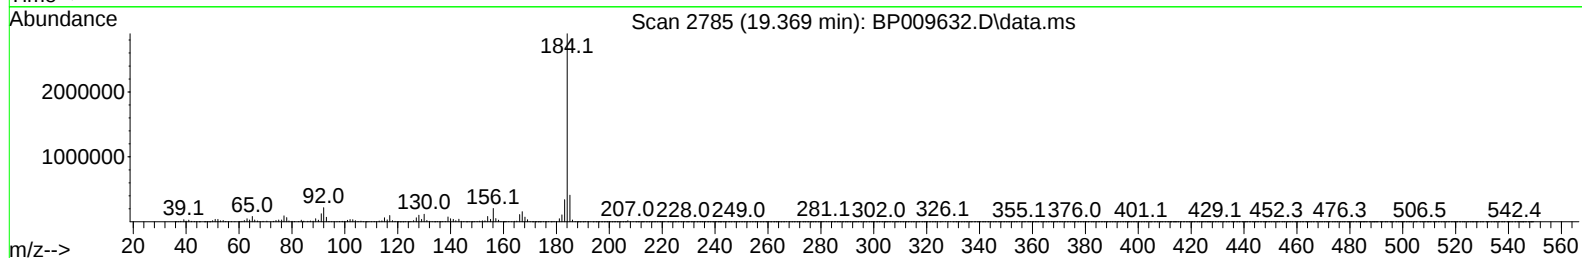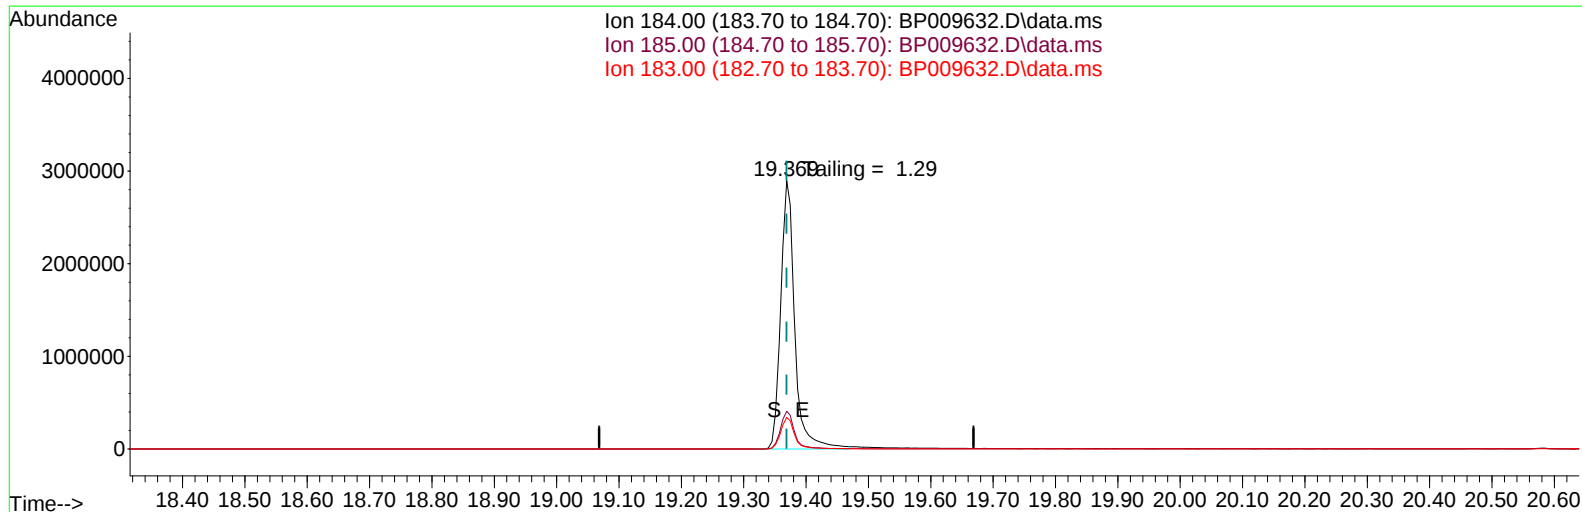

TIC: BP009632.D\data.ms

(77) Benzidine

19.369min (+ 0.000) 40593.78 ng

response 4630763

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.10
183.00	11.70	11.75
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/31/2022	BNA_P	<u>BP009632.D</u>
Compound Name	Response	Retention Time
DDT	2251510	20.58
DDD	61246	20.15
DDE	5440	19.65
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
66686	2318196	2.88

Instrument :
BNA_P
ClientSampleId :
DFTPP