
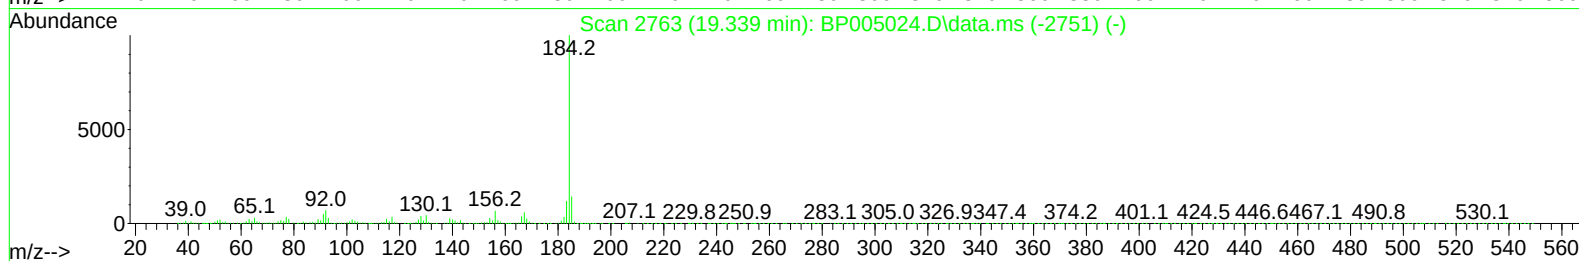
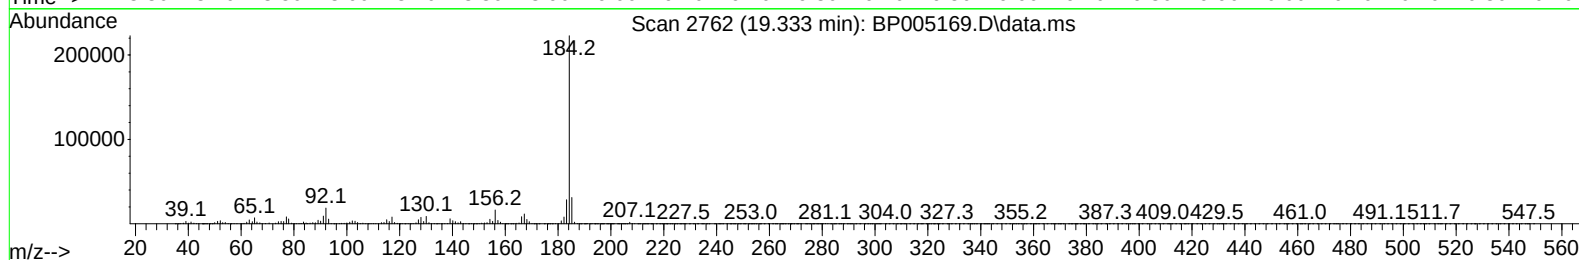


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040521\
 Data File : BP005169.D
 Acq On : 05 Apr 2021 09:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 11:07:15 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 01 12:23:57 2021
 Response via : Initial Calibration

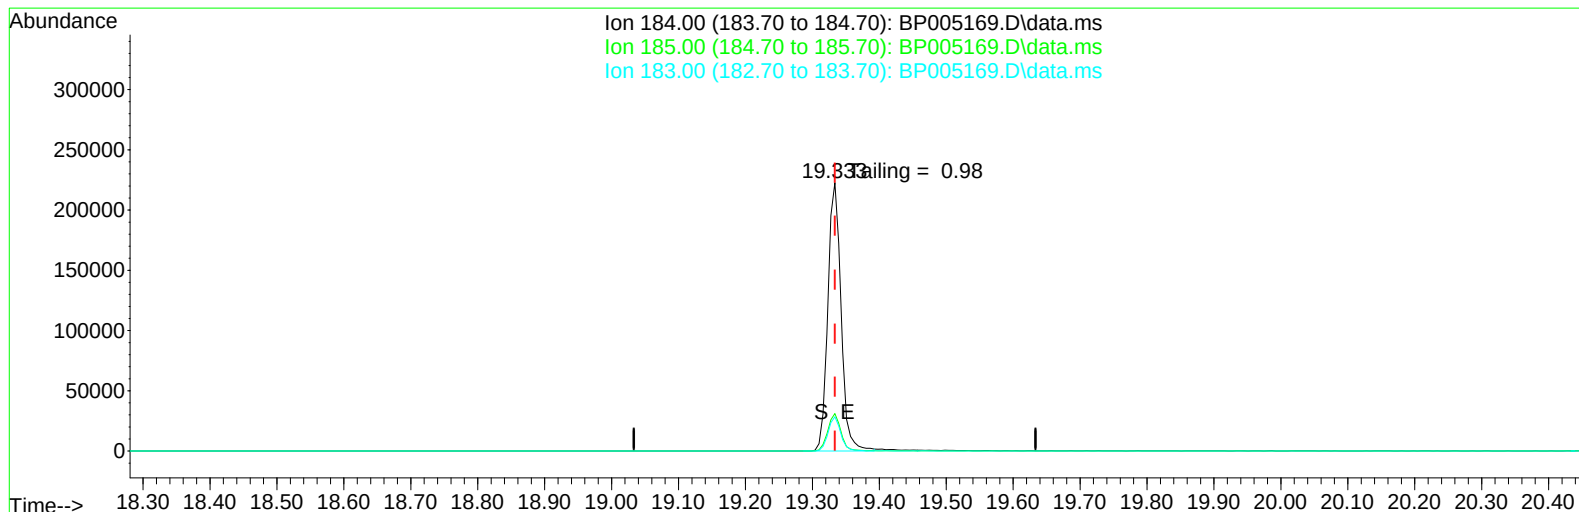




TIC: BP005169.D\data.ms

(77) Benzidine**19.333min (-0.000) 31230.17 ng****response 309024**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.98
183.00	12.00	12.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040521\
 Data File : BP005169.D
 Acq On : 05 Apr 2021 09:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 11:07:15 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 01 12:23:57 2021
 Response via : Initial Calibration

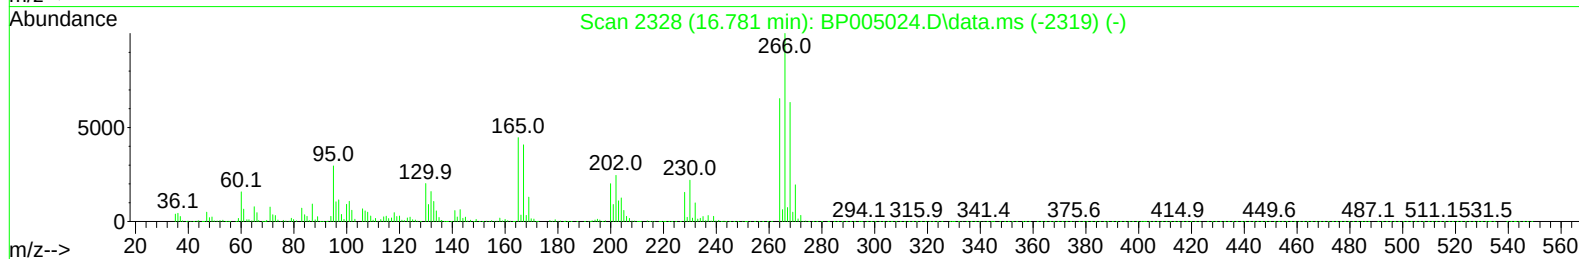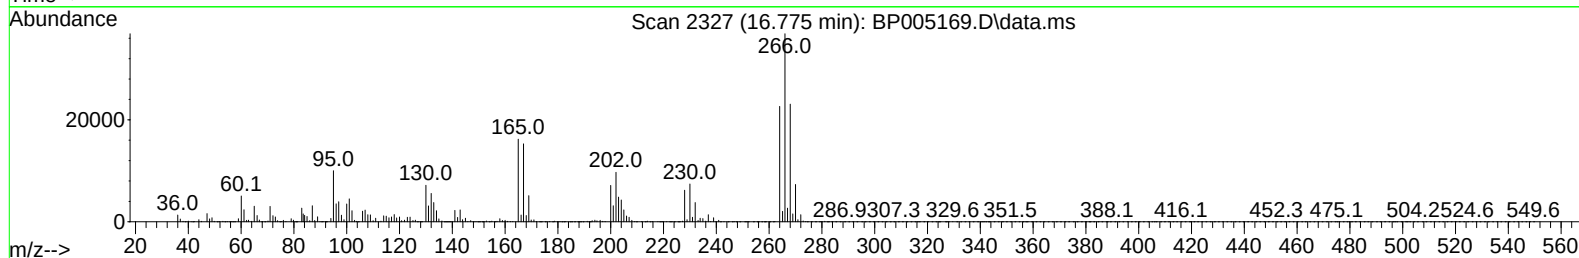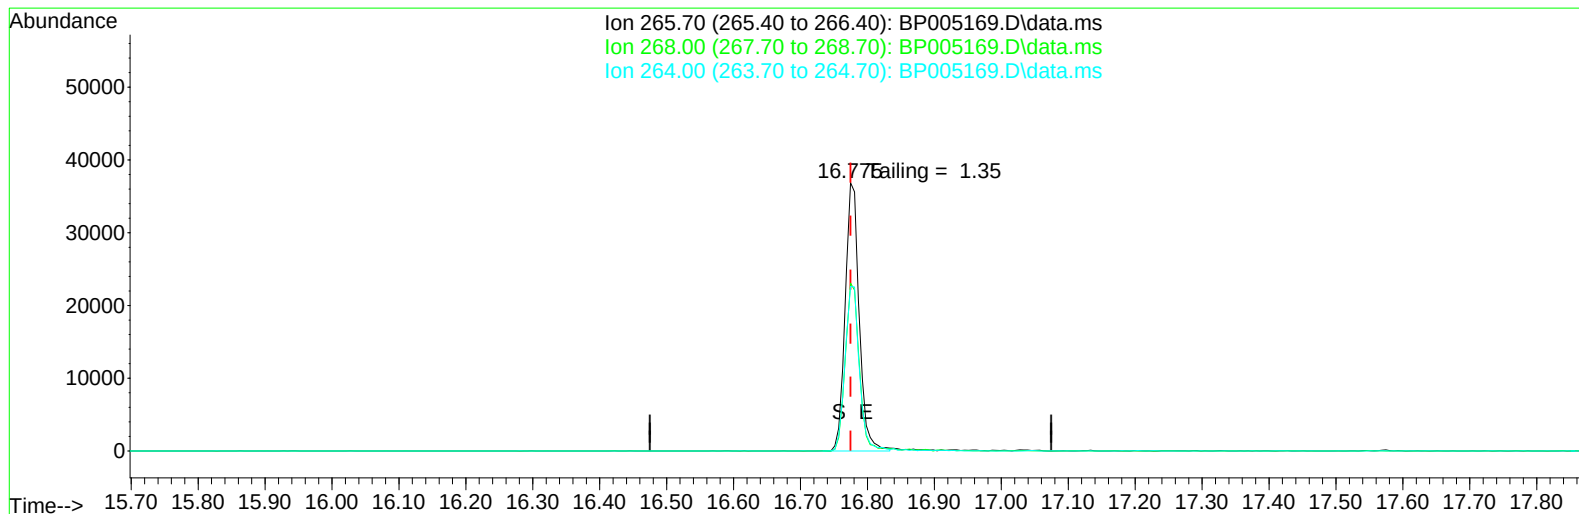

TIC: BP005169.D\data.ms

(70) Pentachlorophenol (C)

16.775min (-0.000) 202846.52 ng

response 54097

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	62.54
264.00	63.30	61.34
0.00	0.00	0.00