

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040521\
 Data File : BP005189.D
 Acq On : 05 Apr 2021 21:03
 Operator : CG/JU
 Sample : M1911-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 TP-6S-(0-4)

Manual Integrations
 APPROVED

mohammad
 4/6/2021 3:23:14 PM

Quant Time: Apr 06 00:34:00 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 01 12:23:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.705	152	28771	20.00	ng	0.00
21) Naphthalene-d8	10.493	136	103998	20.00	ng	# 0.00
39) Acenaphthene-d10	14.357	164	56416	20.00	ng	0.00
64) Phenanthrene-d10	17.122	188	116867	20.00	ng	# 0.00
76) Chrysene-d12	21.227	240	129016	20.00	ng	# 0.00
86) Perylene-d12	23.539	264	130756	20.00	ng	0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.299	112	281171	150.40	ng	0.00
7) Phenol-d6	6.887	99	352348	131.57	ng	0.00
23) Nitrobenzene-d5	8.863	82	228432	94.25	ng	0.00
42) 2,4,6-Tribromophenol	15.863	330	101248	137.74	ng	0.00
45) 2-Fluorobiphenyl	12.975	172	392519	94.12	ng	0.00
79) Terphenyl-d14	19.698	244	546362	77.09	ng	0.00
Target Compounds						Qvalue
10) Phenol	6.910	94	5600	2.04	ng	69
50) Dimethylphthalate	13.816	163	12295	2.83	ng	# 93
71) Phenanthrene	17.163	178	49094	7.25	ng	98
72) Anthracene	17.251	178	13686	2.07	ng	96
75) Fluoranthene	19.145	202	104230	13.08	ng	94
78) Pyrene	19.498	202	100779	11.37	ng	# 95
81) Benzo(a)anthracene	21.216	228	57545	6.57	ng	# 82
83) Chrysene	21.263	228	59046	6.86	ng	# 80
87) Indeno(1,2,3-cd)pyrene	25.909	276	42377	4.32	ng	# 91
88) Benzo(b)fluoranthene	22.839	252	75612m	8.14	ng	
89) Benzo(k)fluoranthene	22.874	252	29486m	3.31	ng	
90) Benzo(a)pyrene	23.445	252	57594	6.92	ng	# 76
92) Benzo(g,h,i)perylene	26.633	276	39673	4.85	ng	# 82

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040521\
Data File : BP005189.D
Acq On : 05 Apr 2021 21:03
Operator : CG/JU
Sample : M1911-01
Misc :
ALS Vial : 21 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampled :
TP-6S-(0-4)

Manual Integrations
APPROVED

mohammad
4/6/2021 3:23:14 PM

Quant Time: Apr 06 00:34:00 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 01 12:23:57 2021
Response via : Initial Calibration

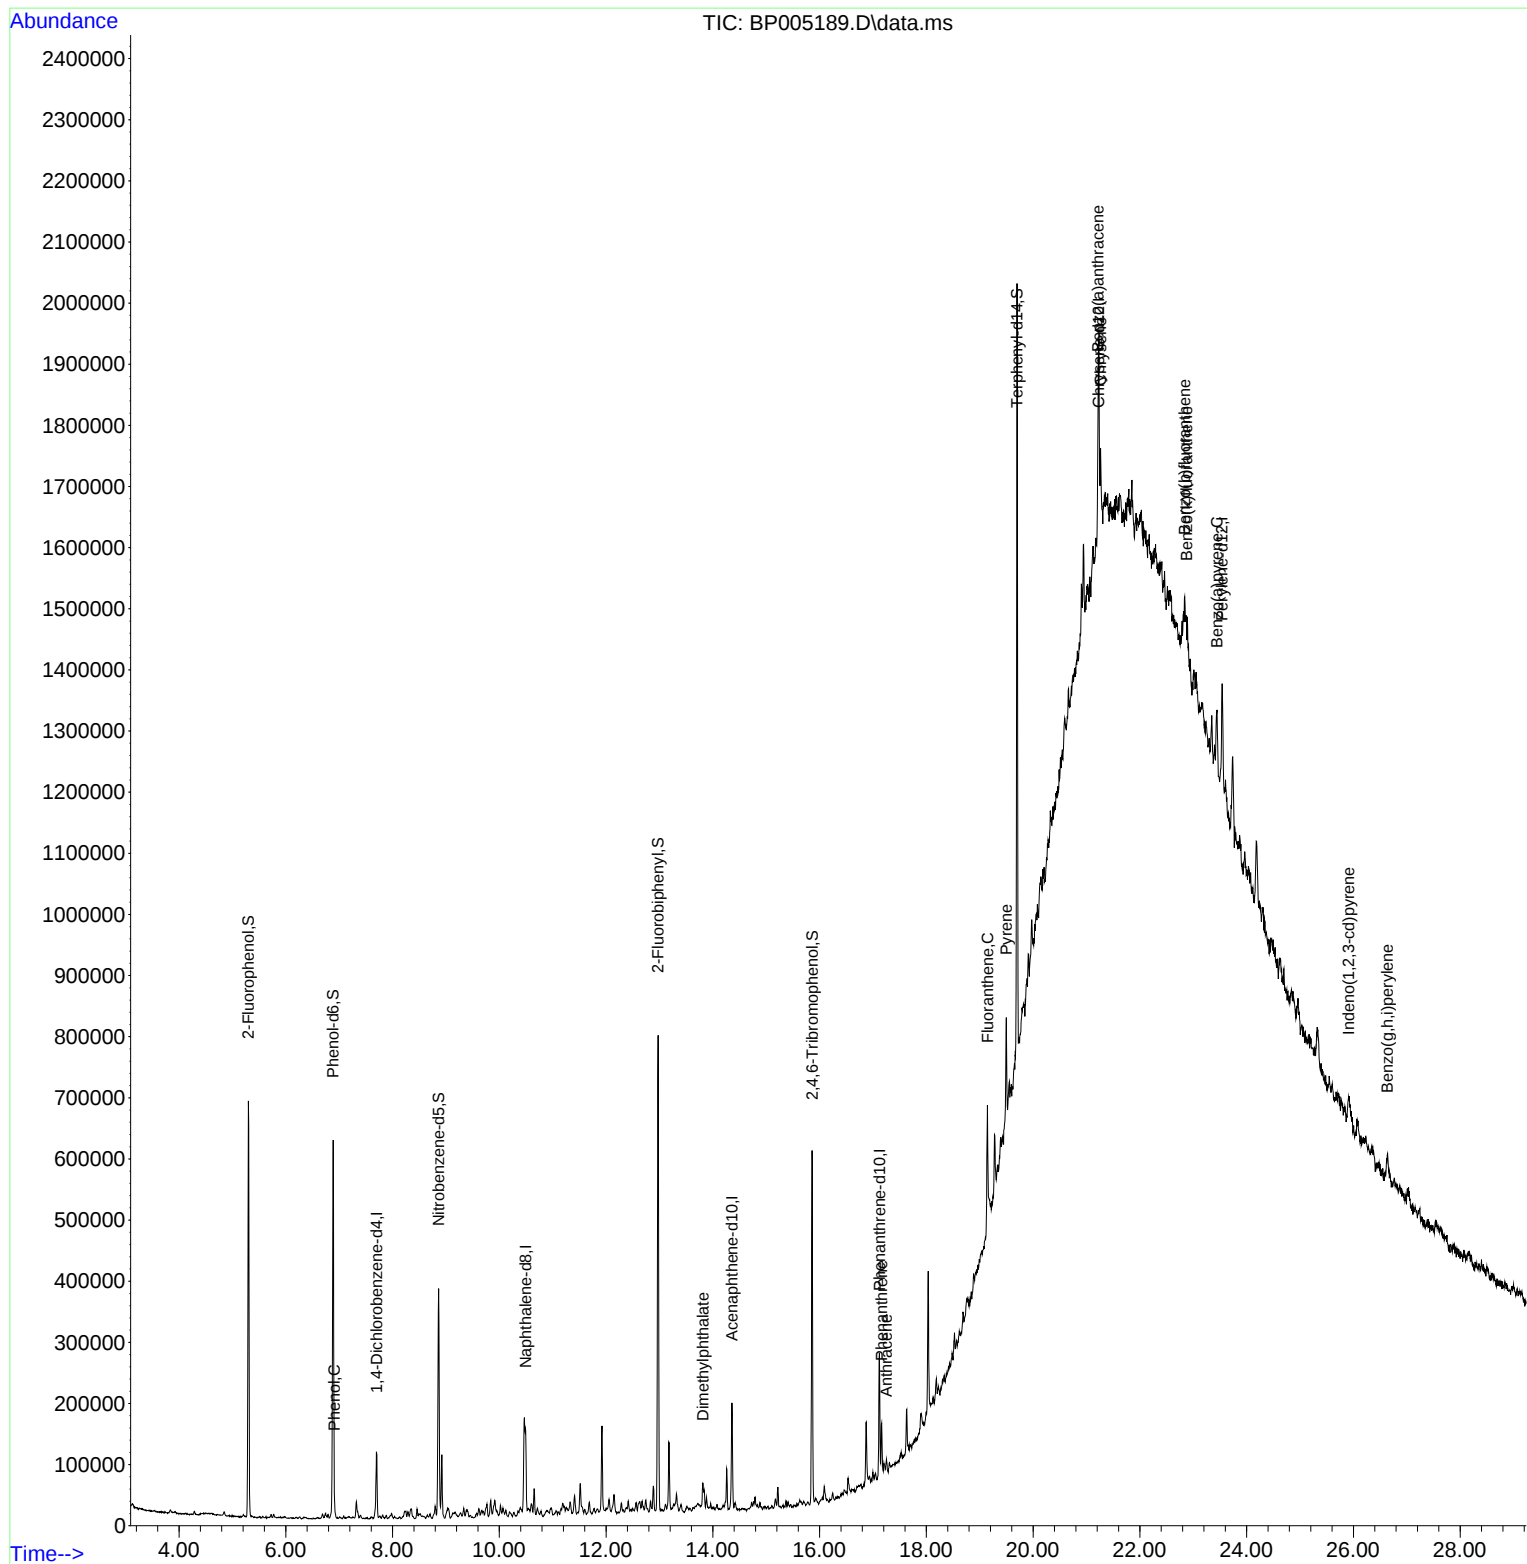

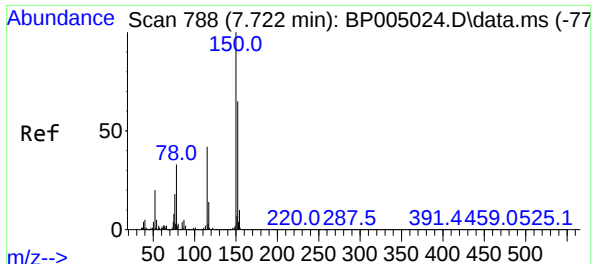





#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.705 min Scan# 785
Delta R.T. -0.000 min
Lab File: BP005189.D
Acq: 05 Apr 2021 21:03

Tgt Ion	Ratio	Lower	Upper
152	100		
150	143.7	123.8	185.6
115	64.3	43.8	65.6

Instrument :
BNA_P
ClientSampleId :
TP-6S-(0-4)




Manual Integrations
APPROVED


mohammad
4/6/2021 3:23:14 PM

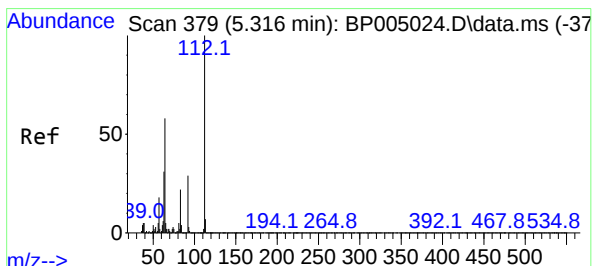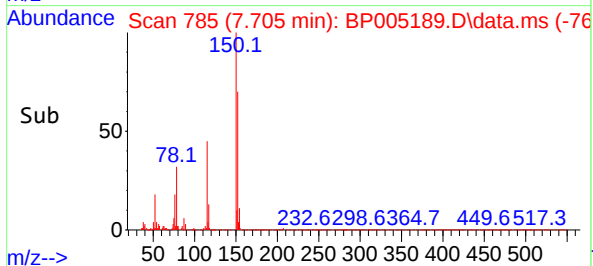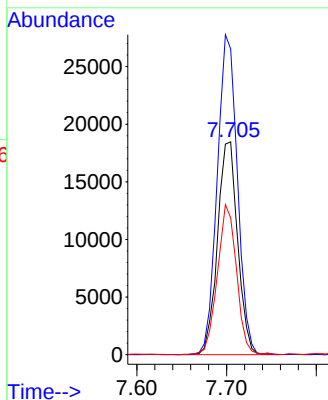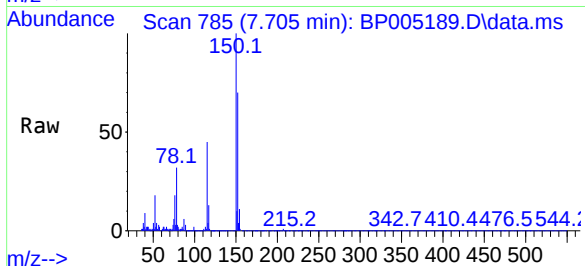

#5
2-Fluorophenol
Concen: 150.40 ng
RT: 5.299 min Scan# 376
Delta R.T. -0.006 min
Lab File: BP005189.D
Acq: 05 Apr 2021 21:03


Tgt Ion	Ratio	Lower	Upper
112	100		
64	57.6	32.8	49.2#
63	30.6	17.0	25.4#

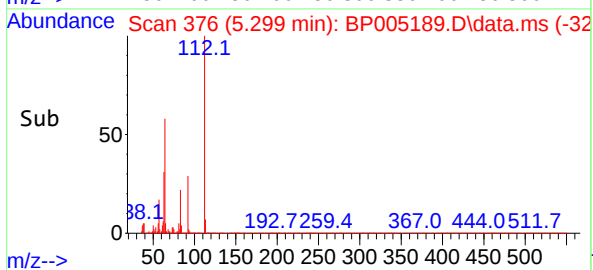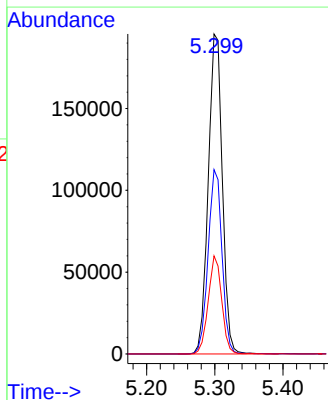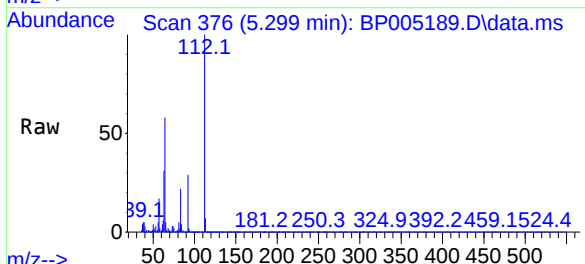

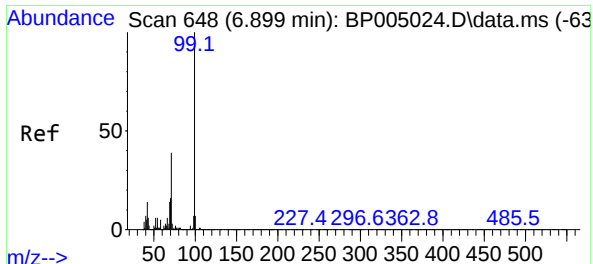

#7
Phenol-d6
Concen: 131.57 ng
RT: 6.887 min Scan# 646
Delta R.T. -0.000 min
Lab File: BP005189.D
Acq: 05 Apr 2021 21:03




Instrument :
BNA_P
ClientSampleId :
TP-6S-(0-4)

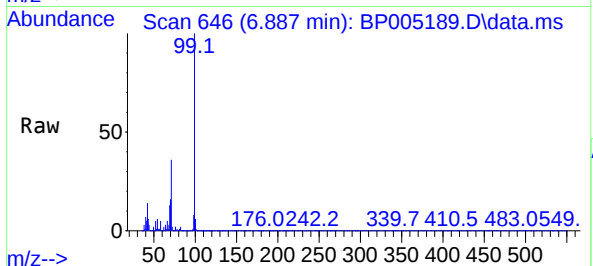

Tgt Ion: 99 Resp: 352348
Ion Ratio Lower Upper
99 100
42 13.7 8.6 13.0#
71 36.3 23.4 35.2#




Manual Integrations
APPROVED


mohammad
4/6/2021 3:23:14 PM

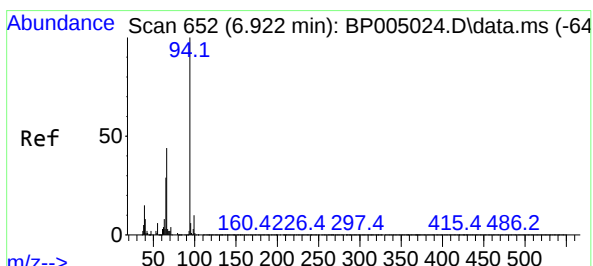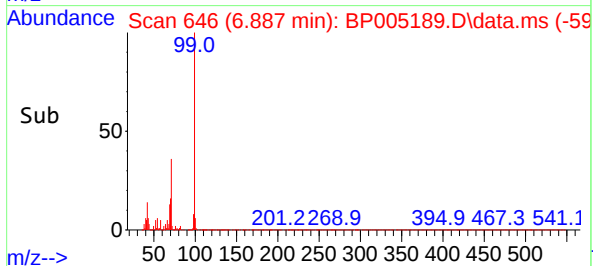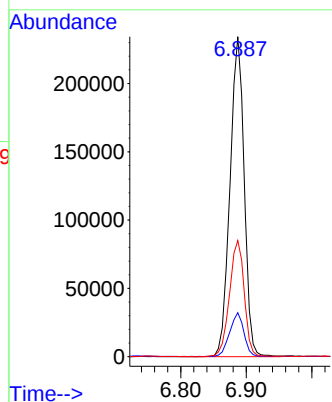

#10
Phenol
Concen: 2.04 ng
RT: 6.910 min Scan# 650
Delta R.T. -0.006 min
Lab File: BP005189.D
Acq: 05 Apr 2021 21:03

Tgt Ion: 94 Resp: 5600
Ion Ratio Lower Upper
94 100
65 38.4 2.3 42.3
66 46.4 10.9 50.9

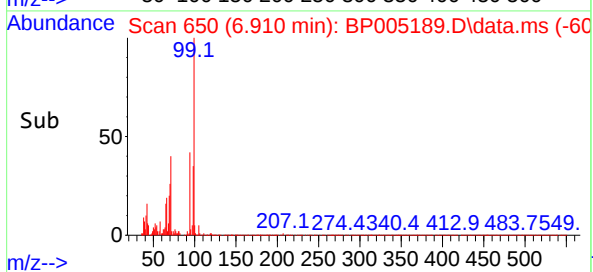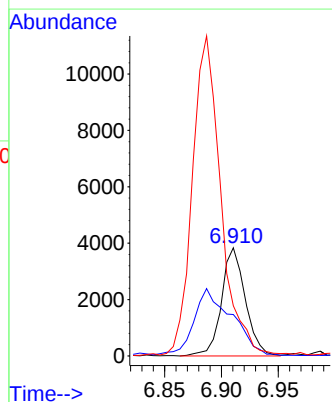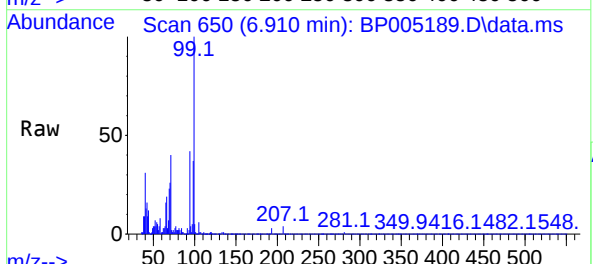







#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.493 min Scan# 1259
Delta R.T. -0.006 min
Lab File: BP005189.D
Acq: 05 Apr 2021 21:03

Tgt Ion:	136	Resp:	103998
Ion Ratio	Lower	Upper	
136	100		
137	11.3	8.6	13.0
54	7.0	3.6	5.4#
68	6.6	3.3	4.9#

Instrument :
BNA_P
ClientSampleId :
TP-6S-(0-4)




Manual Integrations
APPROVED


mohammad
4/6/2021 3:23:14 PM

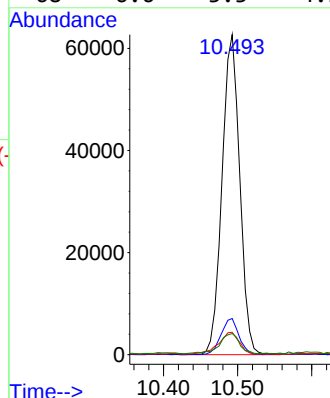

#23
Nitrobenzene-d5
Concen: 94.25 ng
RT: 8.863 min Scan# 982
Delta R.T. -0.006 min
Lab File: BP005189.D
Acq: 05 Apr 2021 21:03

Tgt Ion:	82	Resp:	228432
Ion Ratio	Lower	Upper	
82	100		
128	39.3	45.6	68.4#
54	39.1	30.1	45.1

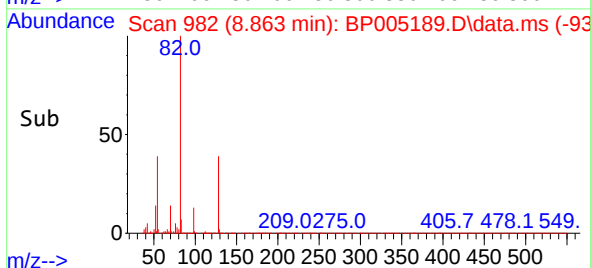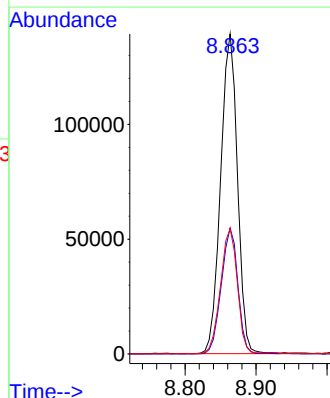







#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.357 min Scan# 1916
Delta R.T. -0.006 min
Lab File: BP005189.D
Acq: 05 Apr 2021 21:03

Tgt Ion:	164	Resp:	56416
Ion Ratio	Lower	Upper	
164	100		
162	106.7	79.4	119.2
160	45.5	36.1	54.1

Instrument :
BNA_P
ClientSampleId :
TP-6S-(0-4)




Manual Integrations
APPROVED


mohammad
4/6/2021 3:23:14 PM

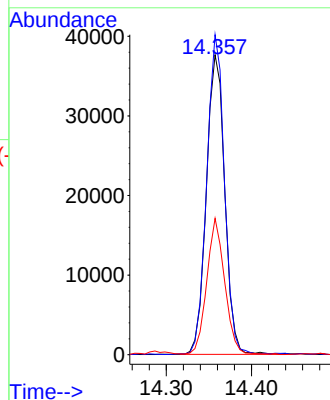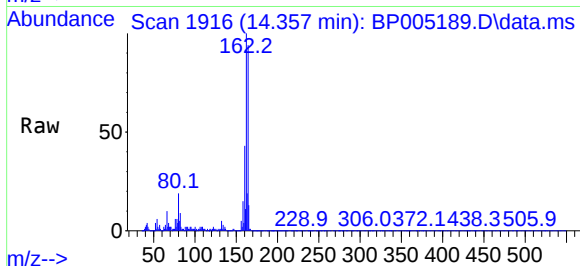

#42
2,4,6-Tribromophenol
Concen: 137.74 ng
RT: 15.863 min Scan# 2172
Delta R.T. -0.000 min
Lab File: BP005189.D
Acq: 05 Apr 2021 21:03


Tgt Ion:	330	Resp:	101248
Ion Ratio	Lower	Upper	
330	100		
332	95.2	77.1	115.7
141	34.6	23.4	35.2

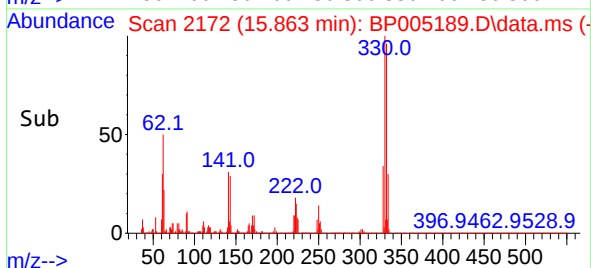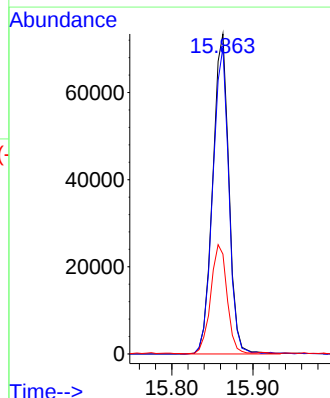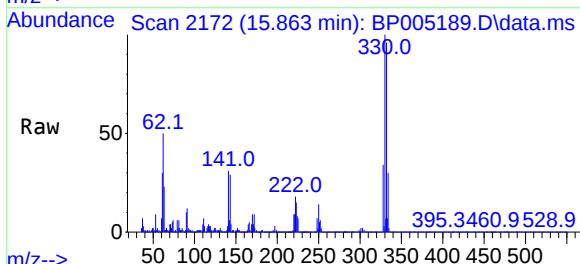



#45
2-Fluorobiphenyl
Concen: 94.12 ng
RT: 12.975 min Scan# 1681
Delta R.T. -0.006 min
Lab File: BP005189.D
Acq: 05 Apr 2021 21:03




Instrument :
BNA_P
ClientSampleId :
TP-6S-(0-4)

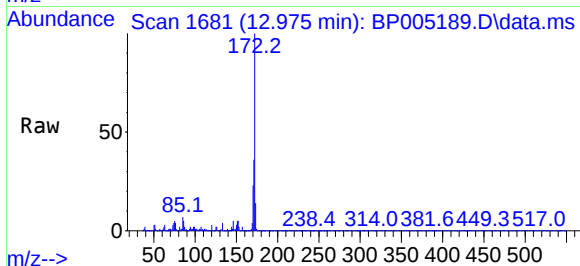


Tgt Ion:172 Resp: 392519
Ion Ratio Lower Upper
172 100
171 36.2 28.5 42.7
170 23.1 19.2 28.8

Manual Integrations
APPROVED



mohammad
4/6/2021 3:23:14 PM

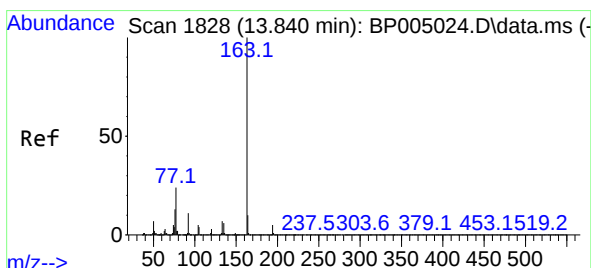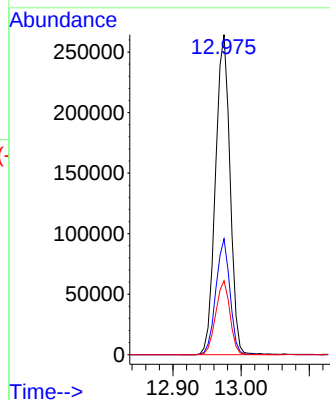


#50
Dimethylphthalate
Concen: 2.83 ng
RT: 13.816 min Scan# 1824
Delta R.T. -0.012 min
Lab File: BP005189.D
Acq: 05 Apr 2021 21:03

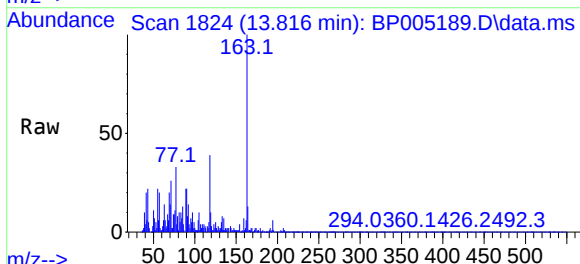

Tgt Ion:163 Resp: 12295
Ion Ratio Lower Upper
163 100
194 6.0 3.3 4.9#
164 13.1 8.2 12.2#

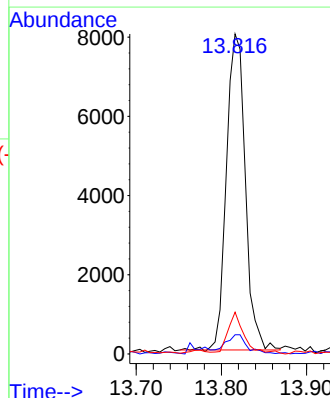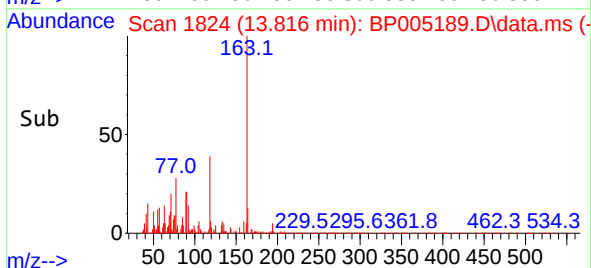







#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.122 min Scan# 2386
Delta R.T. -0.006 min
Lab File: BP005189.D
Acq: 05 Apr 2021 21:03

Tgt Ion:188 Resp: 116867
Ion Ratio Lower Upper
188 100
94 10.2 6.2 9.2#
80 11.3 6.2 9.2#

Instrument :
BNA_P
ClientSampleId :
TP-6S-(0-4)




Manual Integrations
APPROVED


mohammad
4/6/2021 3:23:14 PM

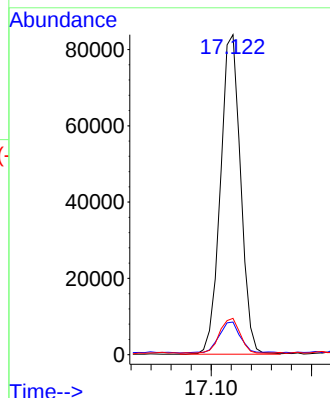

#71
Phenanthrene
Concen: 7.25 ng
RT: 17.163 min Scan# 2393
Delta R.T. -0.006 min
Lab File: BP005189.D
Acq: 05 Apr 2021 21:03

Tgt Ion:178 Resp: 49094
Ion Ratio Lower Upper
178 100
176 19.0 15.3 22.9
179 14.1 12.5 18.7

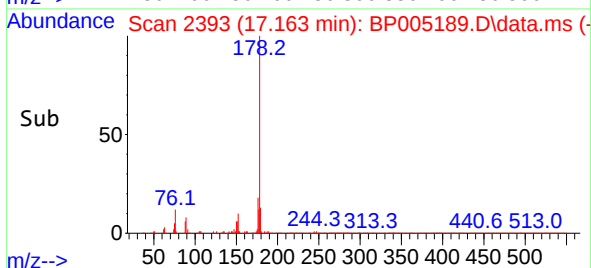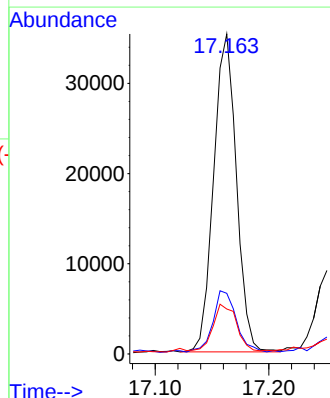







#72
 Anthracene
 Concen: 2.07 ng
 RT: 17.251 min Scan# 2408
 Delta R.T. -0.006 min
 Lab File: BP005189.D
 Acq: 05 Apr 2021 21:03

Tgt Ion:	178	Resp:	13686
Ion Ratio	Lower	Upper	
178	100		
176	20.2	15.0	22.4
179	17.8	12.5	18.7

Instrument :
 BNA_P
 ClientSampleId :
 TP-6S-(0-4)




Manual Integrations
 APPROVED


mohammad
 4/6/2021 3:23:14 PM

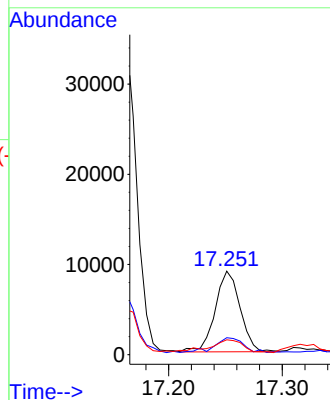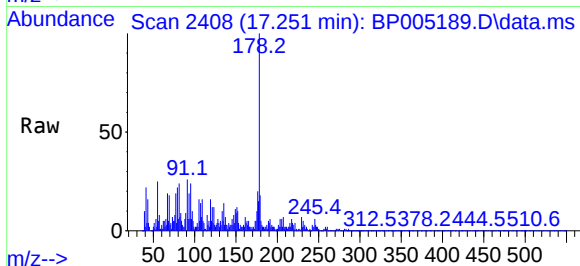


#75
 Fluoranthene
 Concen: 13.08 ng
 RT: 19.145 min Scan# 2730
 Delta R.T. -0.000 min
 Lab File: BP005189.D
 Acq: 05 Apr 2021 21:03

Tgt Ion:	202	Resp:	104230
Ion Ratio	Lower	Upper	
202	100		
101	9.6	0.0	29.4
203	21.8	0.0	37.8

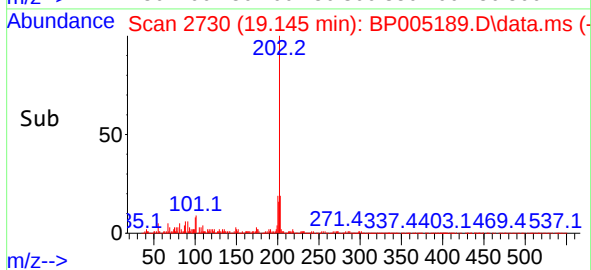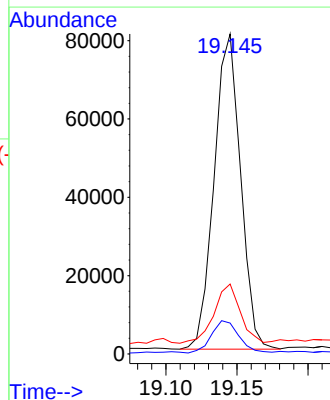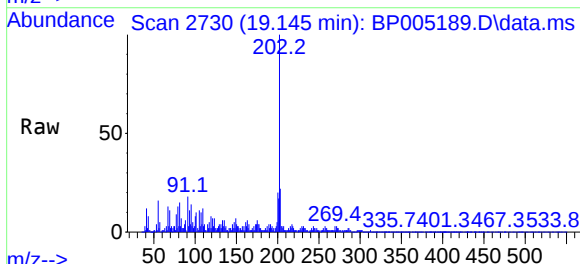


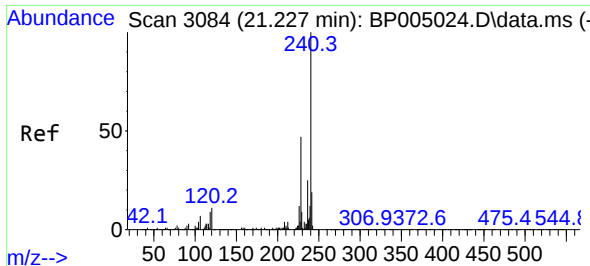

#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.227 min Scan# 3084
Delta R.T. -0.000 min
Lab File: BP005189.D
Acq: 05 Apr 2021 21:03

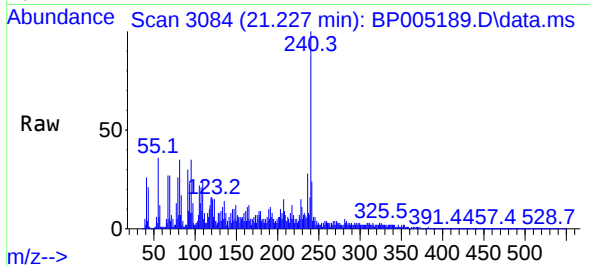



Tgt Ion:240 Resp: 129016
Ion Ratio Lower Upper
240 100
120 15.6 7.8 11.6#
236 27.6 20.8 31.2

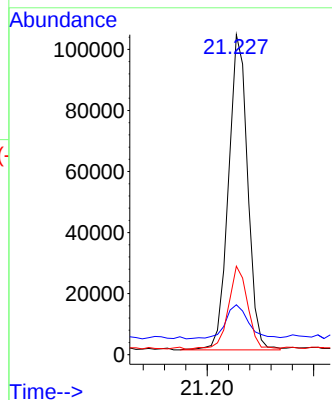


Instrument :
BNA_P
ClientSampleId :
TP-6S-(0-4)

Manual Integrations
APPROVED



mohammad
4/6/2021 3:23:14 PM

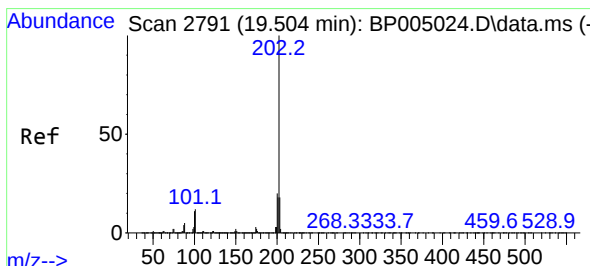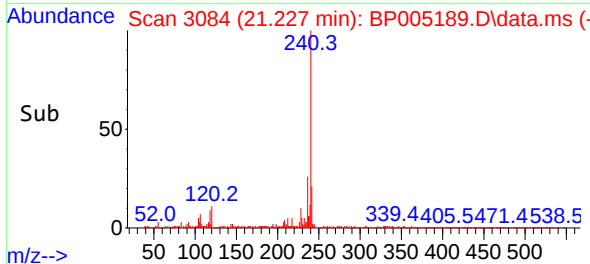


#78
Pyrene
Concen: 11.37 ng
RT: 19.498 min Scan# 2790
Delta R.T. -0.000 min
Lab File: BP005189.D
Acq: 05 Apr 2021 21:03

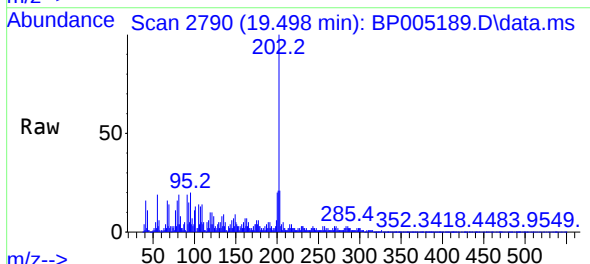


Tgt Ion:202 Resp: 100779
Ion Ratio Lower Upper
202 100
200 20.5 17.1 25.7
203 21.4 14.2 21.2#

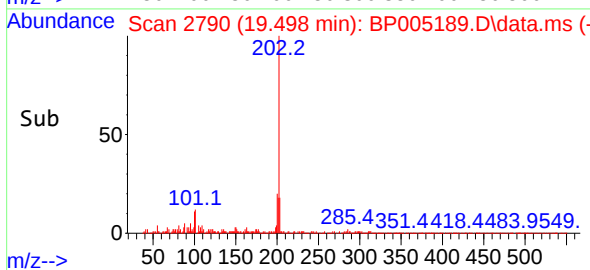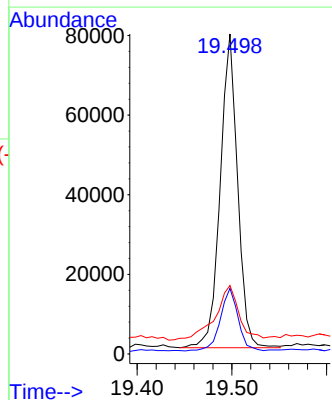



#79
 Terphenyl-d14
 Concen: 77.09 ng
 RT: 19.698 min Scan# 2824
 Delta R.T. -0.000 min
 Lab File: BP005189.D
 Acq: 05 Apr 2021 21:03




Instrument :
 BNA_P
 ClientSampleId :
 TP-6S-(0-4)



Tgt Ion:244 Resp: 546362
 Ion Ratio Lower Upper
 244 100
 212 6.6 5.8 8.6
 122 11.3 7.8 11.8




Manual Integrations
 APPROVED


mohammad
 4/6/2021 3:23:14 PM

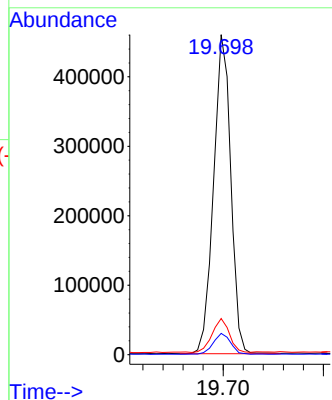


#81
 Benzo(a)anthracene
 Concen: 6.57 ng
 RT: 21.216 min Scan# 3082
 Delta R.T. 0.006 min
 Lab File: BP005189.D
 Acq: 05 Apr 2021 21:03

Tgt Ion:228 Resp: 57545
 Ion Ratio Lower Upper
 228 100
 226 30.4 22.1 33.1
 229 36.1 15.9 23.9#

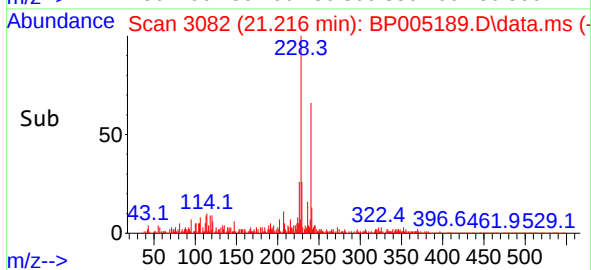
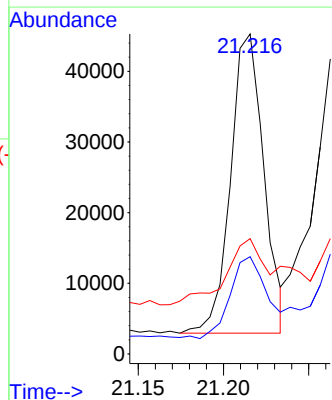






#83
Chrysene
Concen: 6.86 ng
RT: 21.263 min Scan# 3090
Delta R.T. -0.000 min
Lab File: BP005189.D
Acq: 05 Apr 2021 21:03





Tgt Ion: 228 Resp: 59046
Ion Ratio Lower Upper
228 100
226 33.8 24.4 36.6
229 39.1 15.8 23.6#

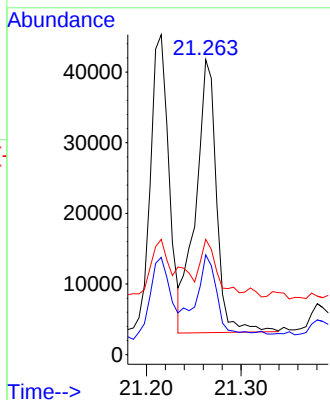

#86
Perylene-d12
Concen: 20.00 ng
RT: 23.539 min Scan# 3477
Delta R.T. 0.029 min
Lab File: BP005189.D
Acq: 05 Apr 2021 21:03




Tgt Ion: 264 Resp: 130756
Ion Ratio Lower Upper
264 100
260 24.5 18.8 28.2
265 25.9 17.4 26.2

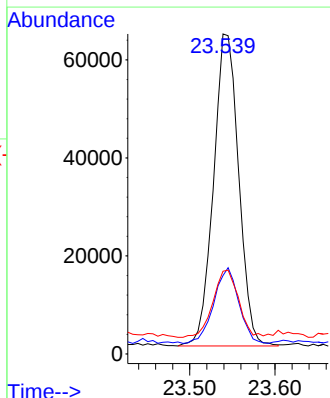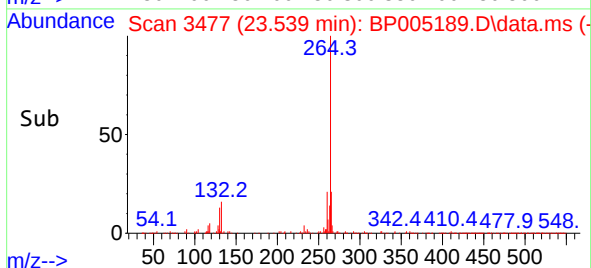

Instrument :
BNA_P
ClientSampleId :
TP-6S-(0-4)

Manual Integrations
APPROVED

mohammad
4/6/2021 3:23:14 PM







#87
Indeno(1,2,3-cd)pyrene
Concen: 4.32 ng
RT: 25.909 min Scan# 3880
Delta R.T. 0.047 min
Lab File: BP005189.D
Acq: 05 Apr 2021 21:03

Tgt Ion: 276 Resp: 42377
Ion Ratio Lower Upper
276 100
138 16.4 18.7 28.1#
277 23.0 20.4 30.6

Instrument :
BNA_P
ClientSampled :
TP-6S-(0-4)




Manual Integrations
APPROVED


mohammad
4/6/2021 3:23:14 PM

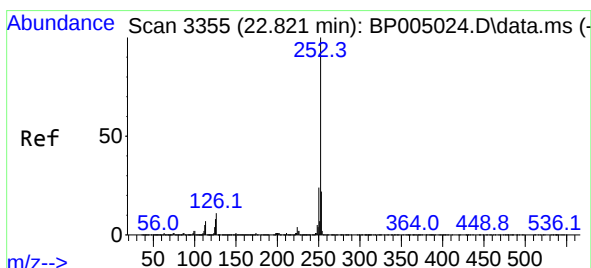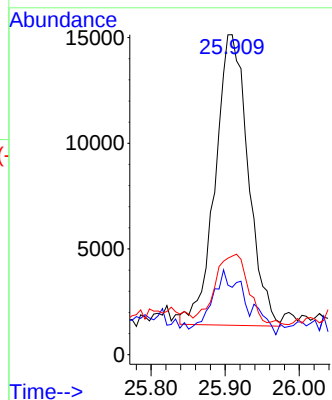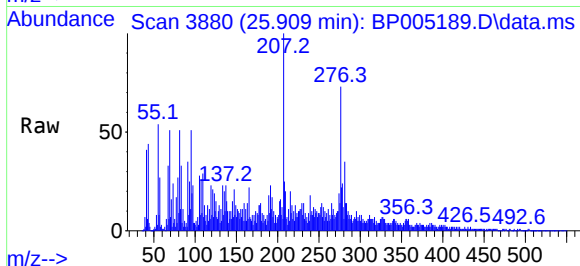

#88
Benzo(b)fluoranthene
Concen: 8.14 ng m
RT: 22.839 min Scan# 3358
Delta R.T. 0.023 min
Lab File: BP005189.D
Acq: 05 Apr 2021 21:03


Tgt Ion: 252 Resp: 75612
Ion Ratio Lower Upper
252 100
253 30.7 17.6 26.4#
125 19.0 7.3 10.9#

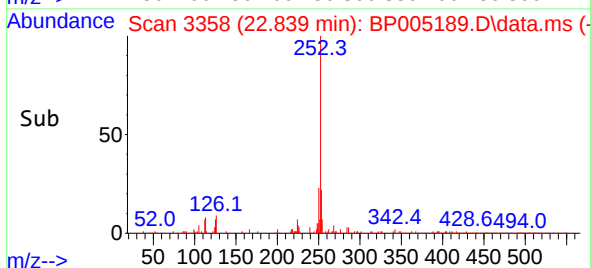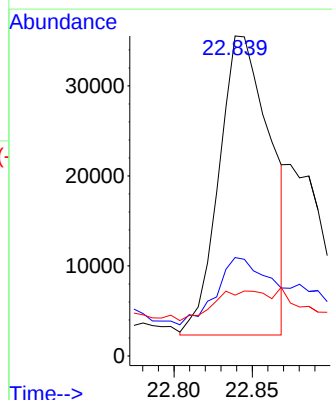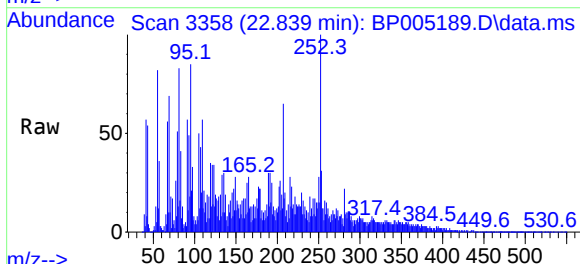



#89
Benzo(k)fluoranthene
Concen: 3.31 ng m
RT: 22.874 min Scan# 3364
Delta R.T. 0.012 min
Lab File: BP005189.D
Acq: 05 Apr 2021 21:03




Instrument :
BNA_P
ClientSampleId :
TP-6S-(0-4)

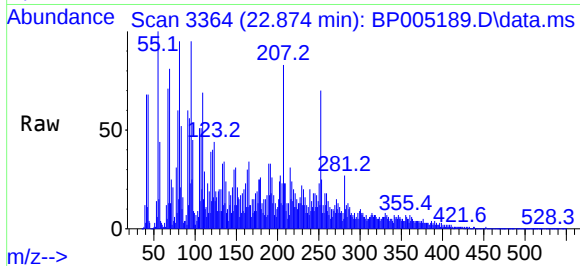

Tgt Ion:252 Resp: 29486
Ion Ratio Lower Upper
252 100
253 35.3 17.8 26.8#
125 27.7 7.4 11.2#




Manual Integrations
APPROVED


mohammad
4/6/2021 3:23:14 PM

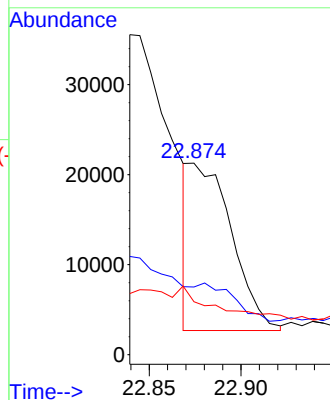

#90
Benzo(a)pyrene
Concen: 6.92 ng
RT: 23.445 min Scan# 3461
Delta R.T. 0.035 min
Lab File: BP005189.D
Acq: 05 Apr 2021 21:03


Tgt Ion:252 Resp: 57594
Ion Ratio Lower Upper
252 100
253 32.4 17.4 26.0#
125 20.6 8.2 12.4#

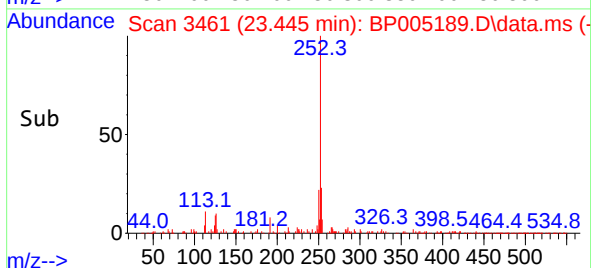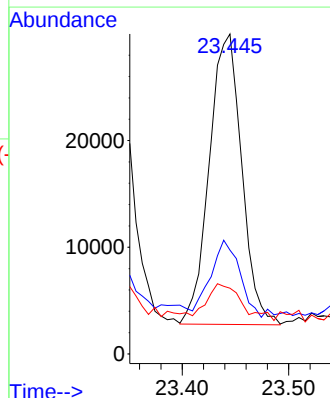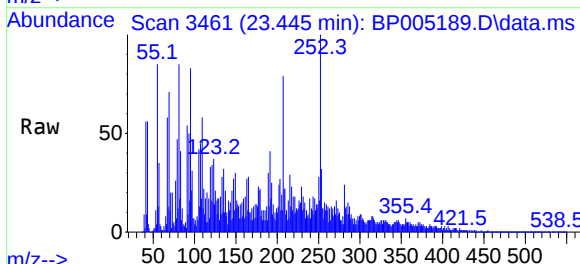



#92
Benzo(g,h,i)perylene
Concen: 4.85 ng
RT: 26.633 min Scan# 4003
Delta R.T. 0.053 min
Lab File: BP005189.D
Acq: 05 Apr 2021 21:03

Instrument :
BNA_P
ClientSampleId :
TP-6S-(0-4)



Tgt Ion	Ratio	Lower	Upper
276	100		
277	32.9	19.0	28.6#
138	28.7	16.6	24.8#

Manual Integrations
APPROVED

mohammad
4/6/2021 3:23:14 PM

