
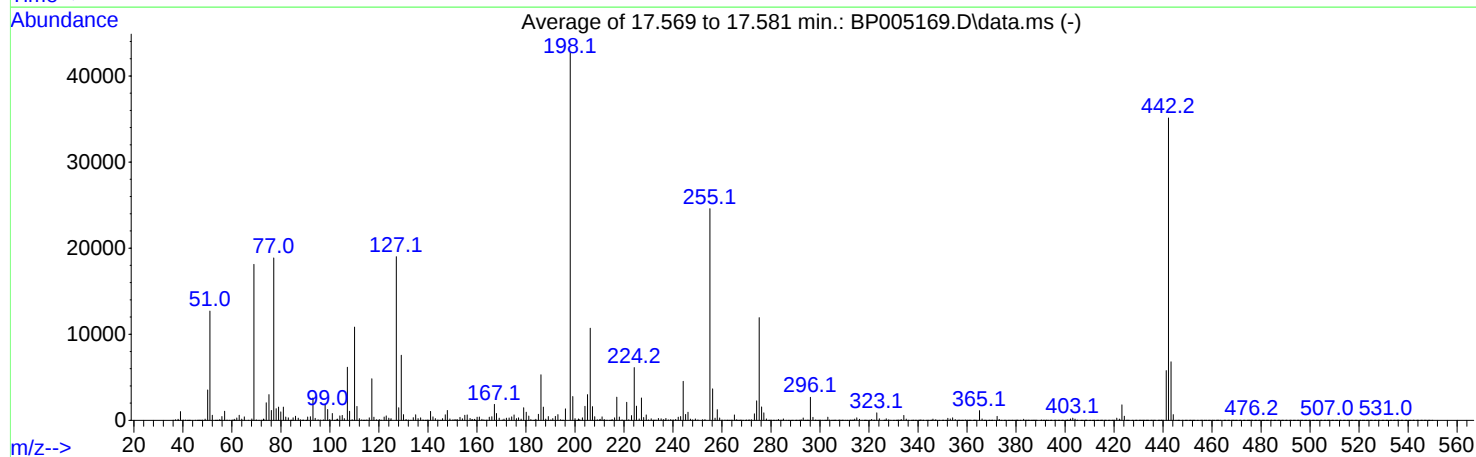


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040521\
 Data File : BP005169.D
 Acq On : 05 Apr 2021 09:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 06 12:33:08 2021

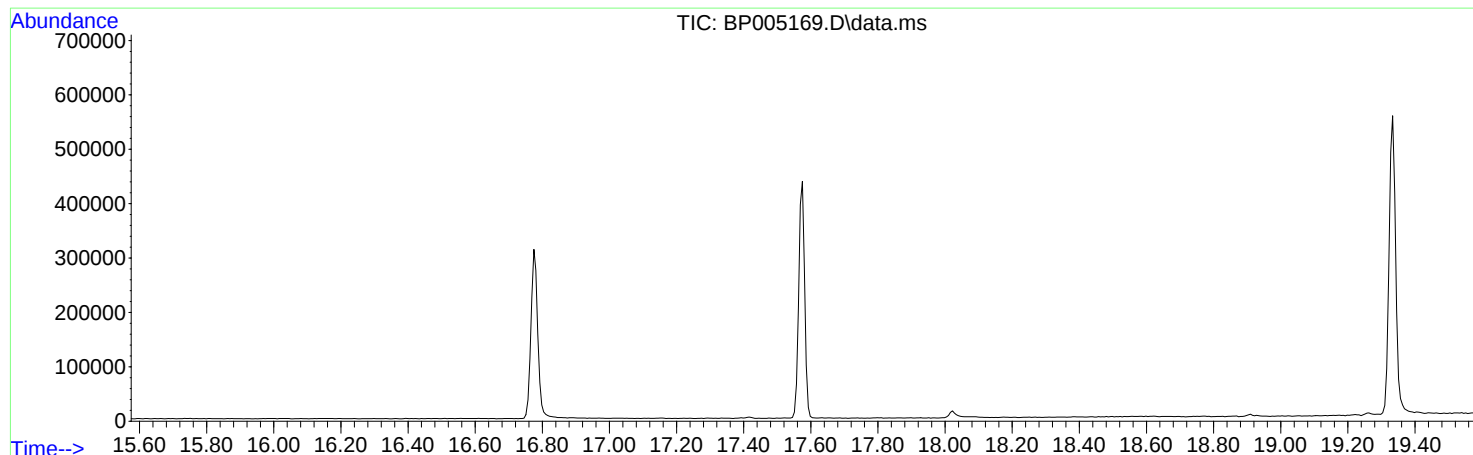




AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.7	12694	PASS
68	69	0.00	2	0.9	165	PASS
69	198	0.00	100	42.4	18127	PASS
70	69	0.00	2	0.3	60	PASS
127	198	10	80	44.5	19015	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	42724	PASS
199	198	5	9	6.5	2779	PASS
275	198	10	60	27.9	11926	PASS
365	198	1	100	2.7	1143	PASS
441	198	0.01	100	13.5	5785	PASS
442	442	100	100	100.0	35115	PASS
443	442	15	24	19.4	6805	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040521\
 Data File : BP005169.D
 Acq On : 05 Apr 2021 09:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Apr 05 11:07:15 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 01 12:23:57 2021
 Response via : Initial Calibration

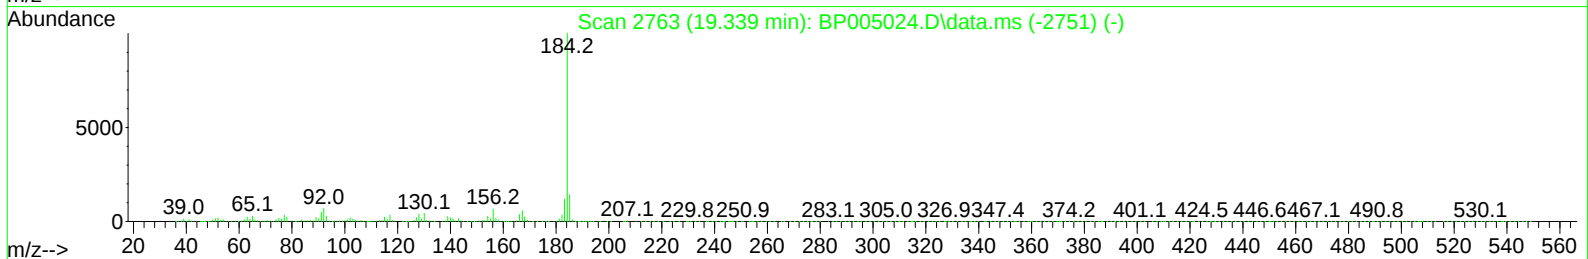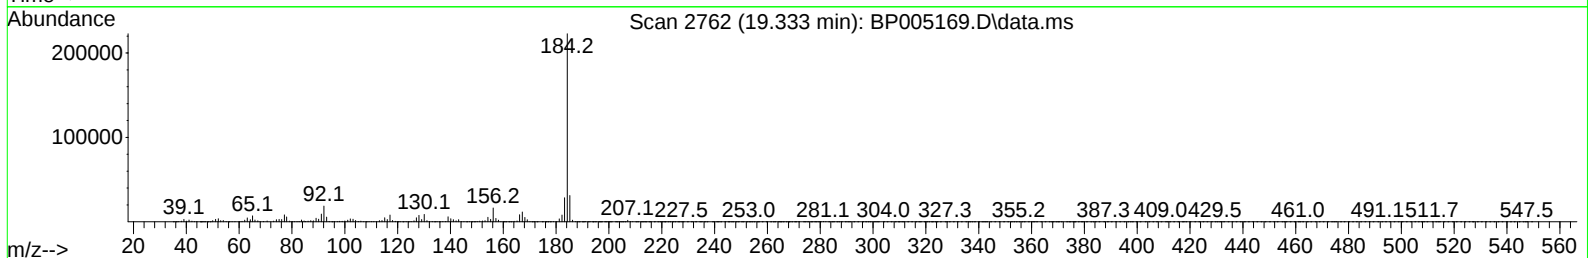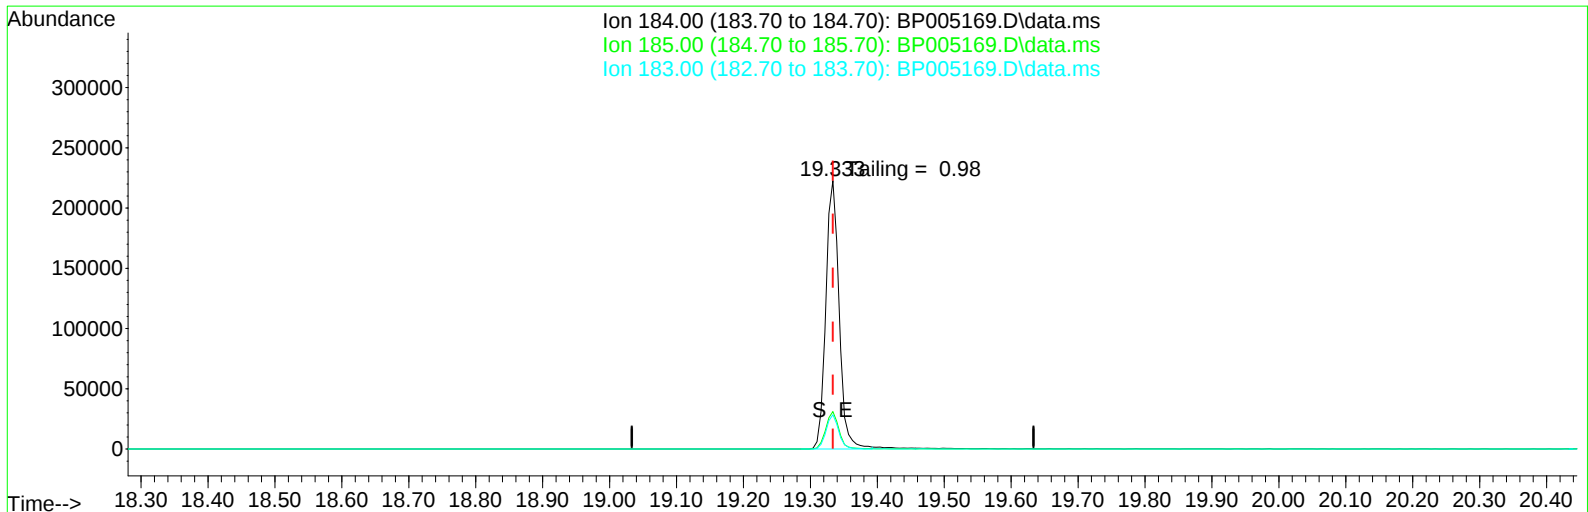

TIC: BP005169.D\data.ms

(77) Benzidine

19.333min (-0.000) 31230.17 ng




response 309024

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.98
183.00	12.00	12.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040521\
 Data File : BP005169.D
 Acq On : 05 Apr 2021 09:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Apr 05 11:07:15 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 01 12:23:57 2021
 Response via : Initial Calibration

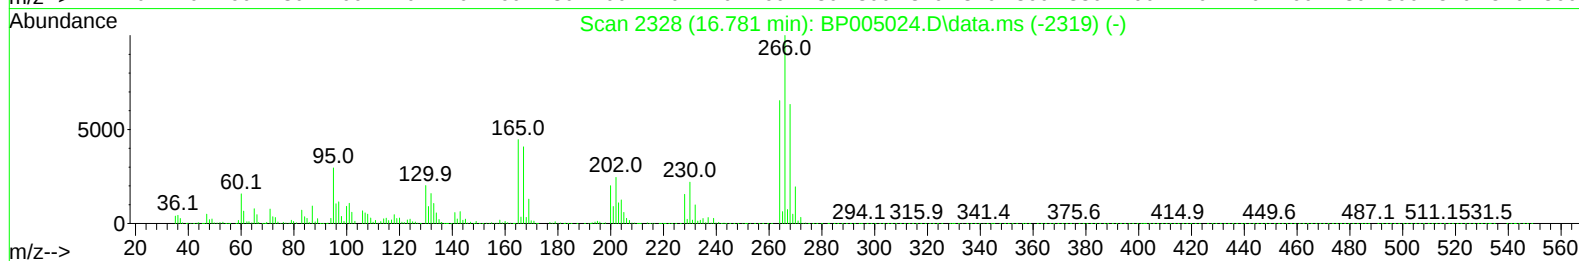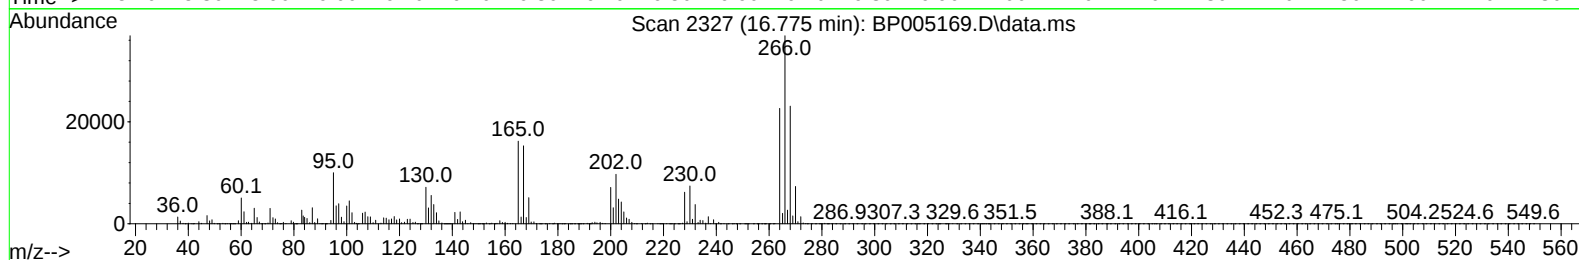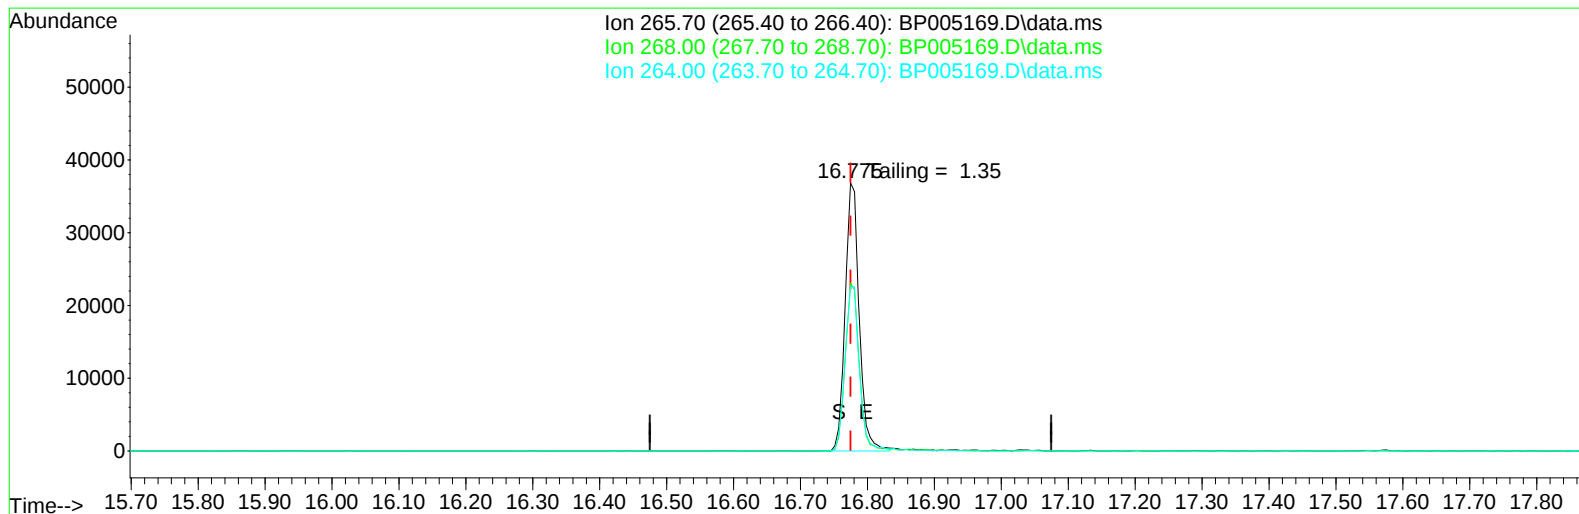

TIC: BP005169.D\data.ms

(70) Pentachlorophenol (C)

16.775min (-0.000) 202846.52 ng

response 54097

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	62.54
264.00	63.30	61.34
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/5/2021	BNA_P	BP005169.D
Compound Name	Response	Retention Time
DDT	154894	20.533
DDD	9936	20.104
DDE	648	19.604
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10584	165478	6.40