

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040722\
 Data File : BP009701.D
 Acq On : 07 Apr 2022 16:22
 Operator : CG/JU
 Sample : SSTD02018
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020618

Quant Time: Apr 07 18:16:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 07 18:14:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.981	152	121585	20.000	ng/ul	0.00
20) Naphthalene-d8	10.793	136	547420	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.610	164	395860	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.363	188	876017	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.445	240	925502	20.000	ng/ul	0.00
88) Perylene-d12	23.921	264	873970	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	21348	7.057	ng/uL	0.00
4) Pyridine-d5	3.811	84	148544	19.680	ng/ul	0.00
7) Phenol-d5	7.128	99	204591	20.772	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.304	67	127322	21.540	ng/ul	0.00
11) 2-Chlorophenol-d4	7.504	132	161137	20.926	ng/ul	0.00
15) 4-Methylphenol-d8	8.681	113	173313	23.020	ng/ul	0.00
21) Nitrobenzene-d5	9.140	128	79195	24.807	ng/ul	0.00
24) 2-Nitrophenol-d4	9.863	143	85527	28.265	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.404	165	179671	22.285	ng/ul	0.00
31) 4-Chloroaniline-d4	10.916	131	247379	21.699	ng/ul	0.00
46) Dimethylphthalate-d6	14.022	166	615792	22.196	ng/ul	0.00
49) Acenaphthylene-d8	14.304	160	737782	20.127	ng/ul	0.00
54) 4-Nitrophenol-d4	14.786	143	108244	24.637	ng/ul	0.00
60) Fluorene-d10	15.604	176	515759	21.366	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.710	200	93580	26.318	ng/ul	0.00
73) Anthracene-d10	17.463	188	842348	20.460	ng/ul	0.00
81) Pyrene-d10	19.686	212	1011477	19.882	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.762	264	904066	20.452	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.428	88	21182	7.003	ng/uL#	20
5) Pyridine	3.828	79	153717	19.193	ng/ul#	38
6) Benzaldehyde	7.110	77	144190	24.883	ng/ul	96
8) Phenol	7.157	94	207186	20.896	ng/ul#	87
10) Bis(2-Chloroethyl)ether	7.399	93	167349	21.146	ng/ul#	77
12) 2-Chlorophenol	7.540	128	159455	20.462	ng/ul	95
13) 2-Methylphenol	8.416	108	163674	22.127	ng/ul	97
14) 2,2'-oxybis(1-Chloropr...	8.510	45	248978	26.163	ng/ul#	84
16) Acetophenone	8.804	105	282151	24.530	ng/ul#	80
17) N-Nitroso-di-n-propyla...	8.793	70	144446	25.204	ng/ul#	72
18) 4-Methylphenol	8.746	108	177027	22.767	ng/ul	93
19) Hexachloroethane	9.069	117	69386	21.807	ng/ul	83
22) Nitrobenzene	9.181	77	202918	24.407	ng/ul#	85
23) Isophorone	9.716	82	416810	22.676	ng/ul	97
25) 2-Nitrophenol	9.898	139	94488	26.688	ng/ul#	80
26) 2,4-Dimethylphenol	9.957	107	218585	22.870	ng/ul#	80
27) Bis(2-Chloroethoxy)met...	10.193	93	244529	21.758	ng/ul#	98
29) 2,4-Dichlorophenol	10.434	162	174541	21.988	ng/ul#	85
30) Naphthalene	10.840	128	556292	20.001	ng/ul	97
32) 4-Chloroaniline	10.940	127	245754	21.783	ng/ul	98
33) Hexachlorobutadiene	11.140	225	125049	21.738	ng/ul	94
34) Caprolactam	11.704	113	32428	14.156	ng/ul#	9
35) 4-Chloro-3-methylphenol	12.057	107	211470	26.313	ng/ul#	72
36) 2-Methylnaphthalene	12.445	142	408872	21.937	ng/ul	93

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040722\
 Data File : BP009701.D
 Acq On : 07 Apr 2022 16:22
 Operator : CG/JU
 Sample : SSTD02018
 Misc :
 ALS Vial : 4 Sample Multiplier: 1


Instrument :
 BNA_P
 ClientSampleId :
 SSTD020618


Quant Time: Apr 07 18:16:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 07 18:14:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.663	142	414033	22.217	ng/ul#	96
39) 1,2,4,5-Tetrachloroben...	12.810	216	239793	19.047	ng/ul#	92
40) Hexachlorocyclopentadiene	12.798	237	159436	20.164	ng/ul	98
41) 2,4,6-Trichlorophenol	13.045	196	155445	21.322	ng/ul#	84
42) 2,4,5-Trichlorophenol	13.110	196	165703	21.484	ng/ul#	90
43) 1,1'-Biphenyl	13.451	154	570528	18.883	ng/ul	93
44) 2-Chloronaphthalene	13.486	162	438824	19.097	ng/ul	94
45) 2-Nitroaniline	13.681	65	132109	32.707	ng/ul#	80
47) Dimethylphthalate	14.069	163	590029	21.974	ng/ul#	92
48) 2,6-Dinitrotoluene	14.175	165	110422	30.095	ng/ul	99
50) Acenaphthylene	14.334	152	724876	19.946	ng/ul	95
51) 3-Nitroaniline	14.504	138	115160	24.859	ng/ul#	83
52) Acenaphthene	14.675	153	469898	19.895	ng/ul	97
53) 2,4-Dinitrophenol	14.704	184	56373	25.132	ng/ul#	78
55) 4-Nitrophenol	14.804	109	99149	28.557	ng/ul#	54
56) Dibenzofuran	15.010	168	693157	20.747	ng/ul	98
57) 2,4-Dinitrotoluene	14.963	165	166197	31.524	ng/ul#	83
58) 2,3,4,6-Tetrachlorophenol	15.233	232	152760	25.330	ng/ul#	85
59) Diethylphthalate	15.433	149	615715	23.695	ng/ul#	92
61) Fluorene	15.663	166	569577	21.748	ng/ul	91
62) 4-Chlorophenyl-phenyle...	15.657	204	300752	22.631	ng/ul	96
63) 4-Nitroaniline	15.663	138	125769	28.009	ng/ul#	78
66) 4,6-Dinitro-2-methylph...	15.728	198	94699	25.332	ng/ul#	91
67) N-Nitrosodiphenylamine	15.863	169	502709	19.611	ng/ul	95
68) 4-Bromophenyl-phenylether	16.551	248	188633	20.642	ng/ul	97
69) Hexachlorobenzene	16.669	284	216992	20.681	ng/ul#	90
70) Atrazine	16.822	200	205091	22.440	ng/ul#	90
71) Pentachlorophenol	17.010	266	141163	22.790	ng/ul#	79
72) Phenanthrene	17.404	178	935258	20.025	ng/ul	98
74) Anthracene	17.498	178	953784	20.457	ng/ul	98
75) 1,2,3,4-Tetrachloroben...	13.416	216	254935	17.269	ng/ul#	84
76) Pentachlorobenzene	14.933	250	246769	18.767	ng/ul	90
77) Carbazole	17.757	167	845785	20.381	ng/ul#	96
78) Di-n-butylphthalate	18.322	149	1071224	23.284	ng/ul#	93
80) Fluoranthene	19.363	202	1155869	19.718	ng/ul	96
82) Pyrene	19.716	202	1181909	19.722	ng/ul#	94
83) Butylbenzylphthalate	20.592	149	486054	25.121	ng/ul#	81
84) 3,3'-Dichlorobenzidine	21.357	252	410275	21.036	ng/ul#	95
85) Benzo(a)anthracene	21.427	228	1162644	19.873	ng/ul	94
86) Bis(2-ethylhexyl)phtha...	21.363	149	727729	23.660	ng/ul#	82
87) Chrysene	21.486	228	1123058	19.809	ng/ul	99
89) Di-n-octyl phthalate	22.321	149	1198246	25.327	ng/ul	100
90) Benzo(b)fluoranthene	23.168	252	1164738	21.146	ng/ul	98
91) Benzo(k)fluoranthene	23.215	252	1058940	21.211	ng/ul#	97
93) Benzo(a)pyrene	23.815	252	1072673	20.322	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.515	276	1092575	17.482	ng/ul#	97
95) Dibenzo(a,h)anthracene	26.533	278	941546	17.846	ng/ul#	96
96) Benzo(g,h,i)perylene	27.309	276	891651	16.660	ng/ul#	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Apr 07 18:16:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 07 18:14:16 2022
Response via : Initial Calibration




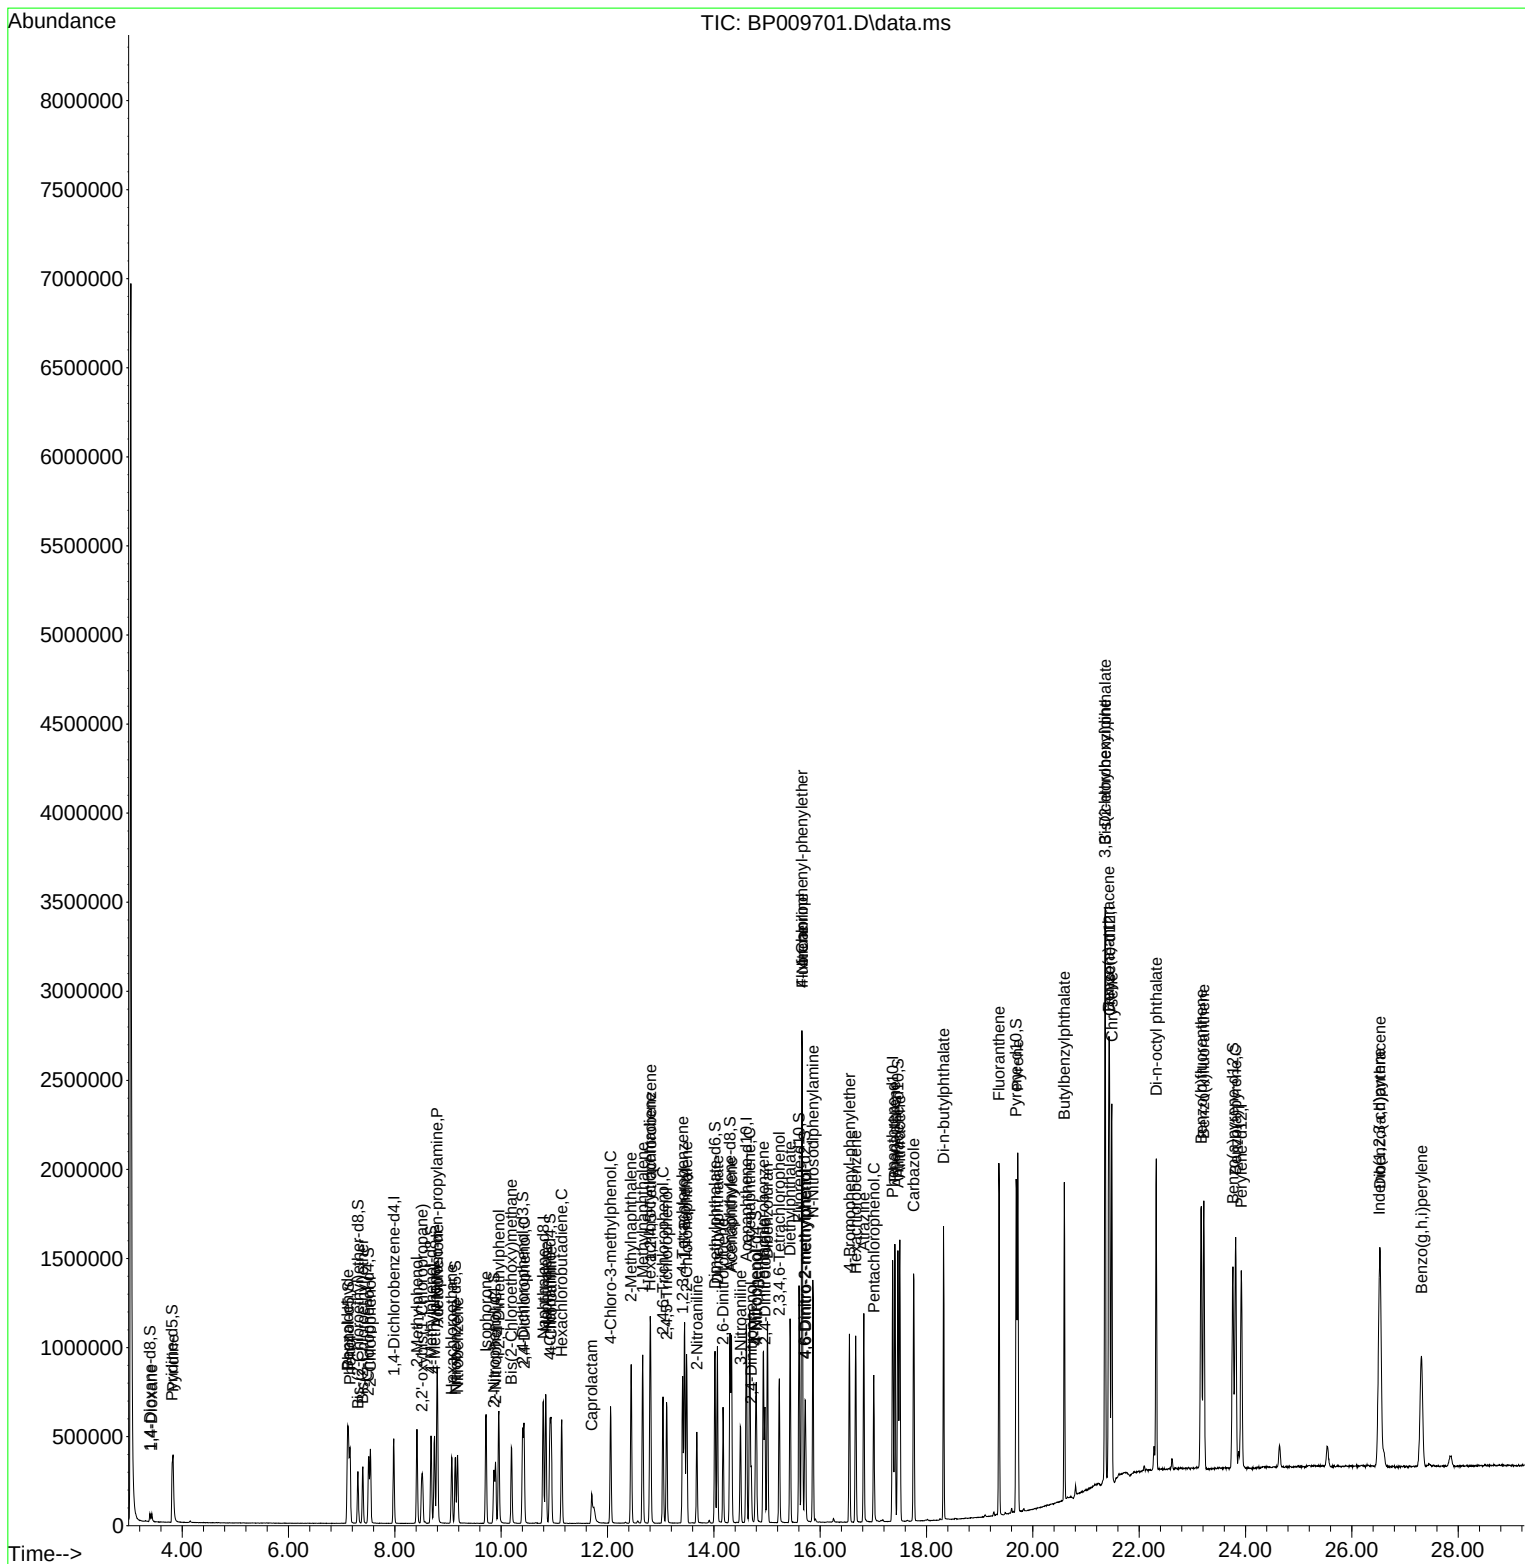




#2
 1,4-Dioxane
 Concen: 7.003 ng/uL
 RT: 3.428 min Scan# 71
 Delta R.T. 0.000 min
 Lab File: BP009701.D
 Acq: 07 Apr 2022 16:22




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020618


Tgt Ion: 88 Resp: 21182
 Ion Ratio Lower Upper
 88 100
 43 33.2 6.8 10.2#
 58 84.1 28.4 42.6#

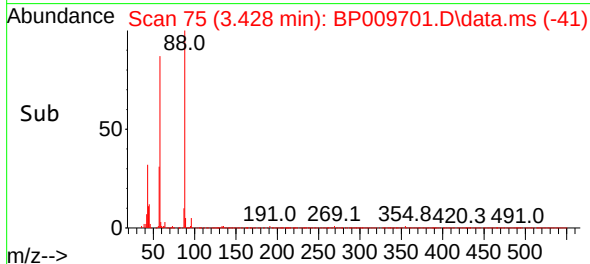

#5
 Pyridine
 Concen: 19.193 ng/uL
 RT: 3.828 min Scan# 143
 Delta R.T. 0.000 min
 Lab File: BP009701.D
 Acq: 07 Apr 2022 16:22

Tgt Ion: 79 Resp: 153717
 Ion Ratio Lower Upper
 79 100
 52 93.6 35.5 53.3#
 51 43.9 20.2 30.4#


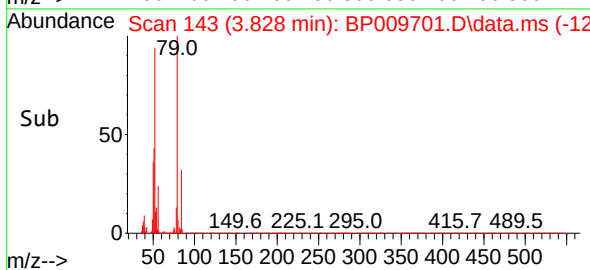




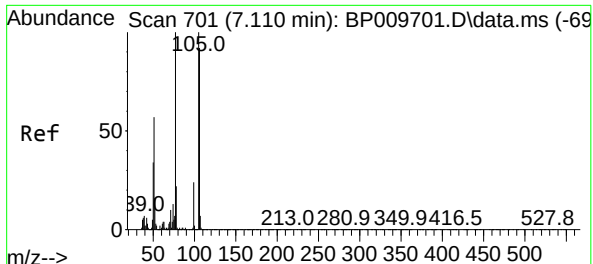

#6
Benzaldehyde
Concen: 24.883 ng/ul
RT: 7.110 min Scan# 701
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22




Instrument :
BNA_P
ClientSampleId :
SSTD020618


Tgt Ion: 77 Resp: 144190
Ion Ratio Lower Upper
77 100
105 100.0 77.0 115.4
106 91.8 77.0 115.4

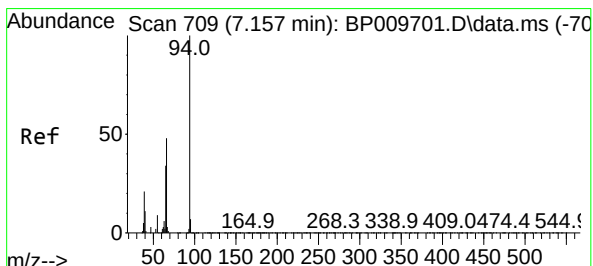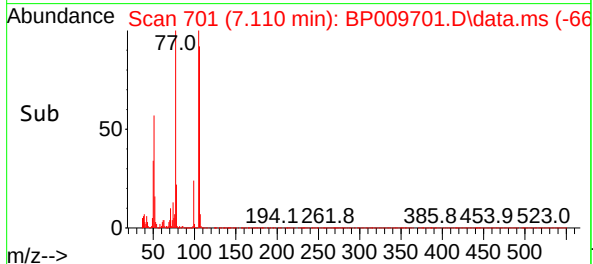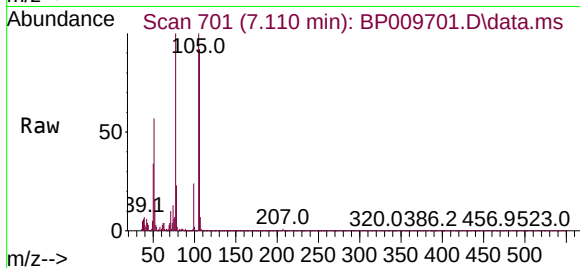

#8
Phenol
Concen: 20.896 ng/ul
RT: 7.157 min Scan# 709
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22

Tgt Ion: 94 Resp: 207186
Ion Ratio Lower Upper
94 100
65 33.9 19.0 28.6
66 49.1 34.6 51.8


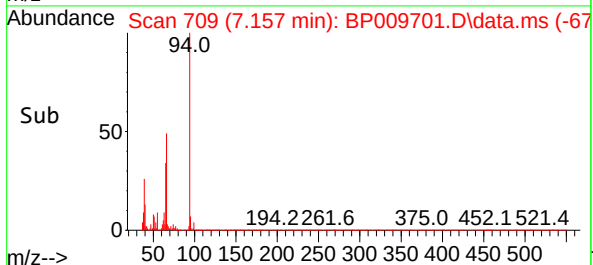
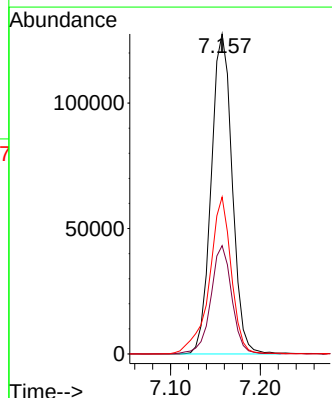
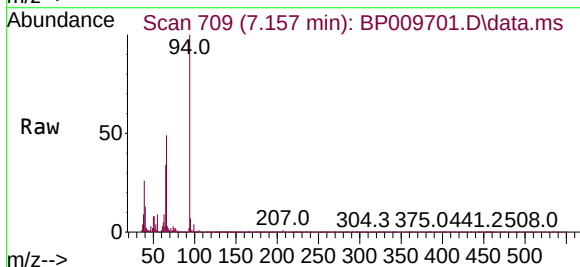




#10
Bis(2-Chloroethyl)ether
Concen: 21.146 ng/ul
RT: 7.399 min Scan# 750
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22




Instrument :
BNA_P
ClientSampleId :
SSTD020618


Tgt Ion: 93 Resp: 167349
Ion Ratio Lower Upper
93 100
63 82.8 45.0 67.4#
95 33.0 26.3 39.5



#12
2-Chlorophenol
Concen: 20.462 ng/ul
RT: 7.540 min Scan# 774
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22

Tgt Ion: 128 Resp: 159455
Ion Ratio Lower Upper
128 100
64 53.5 45.3 67.9
130 32.3 29.0 43.6









#13
2-Methylphenol
Concen: 22.127 ng/ul
RT: 8.416 min Scan# 91
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22




Instrument :
BNA_P
ClientSampleId :
SSTD020618


Tgt Ion:108 Resp: 163674
Ion Ratio Lower Upper
108 100
107 91.2 70.8 106.2



#14
2,2'-oxybis(1-Chloropropane)
Concen: 26.163 ng/ul
RT: 8.510 min Scan# 939
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22

Tgt Ion: 45 Resp: 248978
Ion Ratio Lower Upper
45 100
77 14.1 17.1 25.7#
79 9.8 13.2 19.8#









#16
 Acetophenone
 Concen: 24.530 ng/ul
 RT: 8.804 min Scan# 989
 Delta R.T. 0.000 min
 Lab File: BP009701.D
 Acq: 07 Apr 2022 16:22




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020618


Tgt Ion:105 Resp: 282151
 Ion Ratio Lower Upper
 105 100
 77 80.7 53.4 80.2#
 51 30.5 13.8 20.8#



#17
 N-Nitroso-di-n-propylamine
 Concen: 25.204 ng/ul
 RT: 8.793 min Scan# 987
 Delta R.T. 0.000 min
 Lab File: BP009701.D
 Acq: 07 Apr 2022 16:22

Tgt Ion: 70 Resp: 144446
 Ion Ratio Lower Upper
 70 100
 42 64.5 31.8 47.8#
 101 11.6 15.6 23.4#
 130 21.7 13.7 20.5#









#18
4-Methylphenol
Concen: 22.767 ng/ul
RT: 8.746 min Scan# 91
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22




Instrument :
BNA_P
ClientSampleId :
SSTD020618


Tgt Ion:108 Resp: 177027
Ion Ratio Lower Upper
108 100
107 111.9 83.6 125.4



#19
Hexachloroethane
Concen: 21.807 ng/ul
RT: 9.069 min Scan# 1034
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22

Tgt Ion:117 Resp: 69386
Ion Ratio Lower Upper
117 100
201 106.9 106.5 159.7
199 67.7 59.0 88.6









#22
Nitrobenzene
Concen: 24.407 ng/ul
RT: 9.181 min Scan# 1053
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22




Instrument :
BNA_P
ClientSampleId :
SSTD020618


Tgt Ion: 77 Resp: 202918
Ion Ratio Lower Upper
77 100
123 43.4 42.3 63.5
65 15.6 5.8 8.8#



#23
Isophorone
Concen: 22.676 ng/ul
RT: 9.716 min Scan# 1144
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22

Tgt Ion: 82 Resp: 416810
Ion Ratio Lower Upper
82 100
95 8.3 7.8 11.8
138 17.3 12.9 19.3









#25
2-Nitrophenol
Concen: 26.688 ng/ul
RT: 9.898 min Scan# 1175
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22




Instrument :
BNA_P
ClientSampleId :
SSTD020618


Tgt Ion:139 Resp: 94488
Ion Ratio Lower Upper
139 100
65 56.2 49.4 74.2
109 31.8 44.7 67.1#



#26
2,4-Dimethylphenol
Concen: 22.870 ng/ul
RT: 9.957 min Scan# 1185
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22

Tgt Ion:107 Resp: 218585
Ion Ratio Lower Upper
107 100
121 46.4 34.1 51.1
122 80.4 46.3 69.5#









#27
 Bis(2-Chloroethoxy)methane
 Concen: 21.758 ng/ul
 RT: 10.193 min Scan# 1225
 Delta R.T. 0.000 min
 Lab File: BP009701.D
 Acq: 07 Apr 2022 16:22




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020618


Tgt Ion: 93 Resp: 244529
 Ion Ratio Lower Upper
 93 100
 95 32.8 26.2 39.4
 123 11.8 6.2 9.4#



#29
 2,4-Dichlorophenol
 Concen: 21.988 ng/ul
 RT: 10.434 min Scan# 1266
 Delta R.T. 0.000 min
 Lab File: BP009701.D
 Acq: 07 Apr 2022 16:22

Tgt Ion: 162 Resp: 174541
 Ion Ratio Lower Upper
 162 100
 164 64.7 37.0 55.6#
 98 38.5 31.0 46.6









#30
Naphthalene
Concen: 20.001 ng/ul
RT: 10.840 min Scan# 1335
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22




Instrument :
BNA_P
ClientSampleId :
SSTD020618


Tgt Ion:128 Resp: 556292
Ion Ratio Lower Upper
128 100
129 10.9 8.6 13.0
127 13.0 12.2 18.4



#32
4-Chloroaniline
Concen: 21.783 ng/ul
RT: 10.940 min Scan# 1352
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22

Tgt Ion:127 Resp: 245754
Ion Ratio Lower Upper
127 100
129 32.1 24.6 37.0









#33
Hexachlorobutadiene
Concen: 21.738 ng/ul
RT: 11.140 min Scan# 11
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22




Instrument :
BNA_P
ClientSampleId :
SSTD020618


Tgt Ion:225 Resp: 125049
Ion Ratio Lower Upper
225 100
223 61.1 53.4 80.0
227 63.6 53.8 80.8



#34
Caprolactam
Concen: 14.156 ng/ul
RT: 11.704 min Scan# 1482
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22

Tgt Ion:113 Resp: 32428
Ion Ratio Lower Upper
113 100
55 182.6 58.2 87.2#
56 138.8 68.6 103.0#









#35
4-Chloro-3-methylphenol
Concen: 26.313 ng/ul
RT: 12.057 min Scan# 1542
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22




Instrument :
BNA_P
ClientSampleId :
SSTD020618


Tgt Ion:107 Resp: 211470
Ion Ratio Lower Upper
107 100
144 24.5 15.8 23.8#
142 72.4 38.9 58.3#

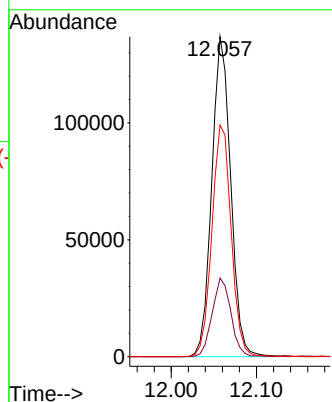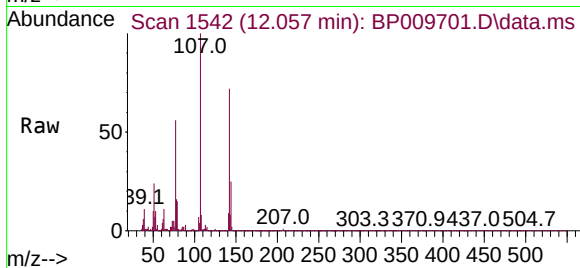

#36
2-Methylnaphthalene
Concen: 21.937 ng/ul
RT: 12.445 min Scan# 1608
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22

Tgt Ion:142 Resp: 408872
Ion Ratio Lower Upper
142 100
141 86.5 64.3 96.5









#37
1-Methylnaphthalene
Concen: 22.217 ng/ul
RT: 12.663 min Scan# 1645
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22




Instrument :
BNA_P
ClientSampleId :
SSTD020618


Tgt Ion:142 Resp: 414033
Ion Ratio Lower Upper
142 100
141 90.7 69.8 104.8
116 3.9 5.6 8.4#

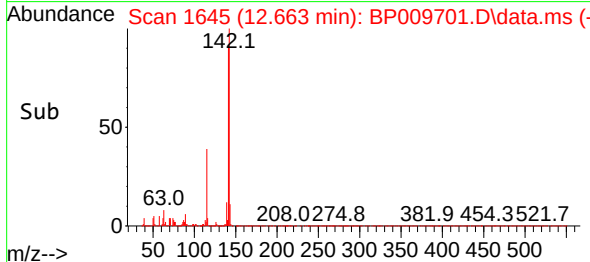

#39
1,2,4,5-Tetrachlorobenzene
Concen: 19.047 ng/ul
RT: 12.810 min Scan# 1670
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22

Tgt Ion:216 Resp: 239793
Ion Ratio Lower Upper
216 100
214 79.2 58.2 87.2
179 22.0 14.2 21.2#
108 16.8 15.3 22.9


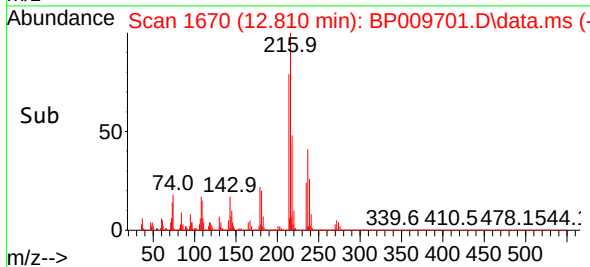
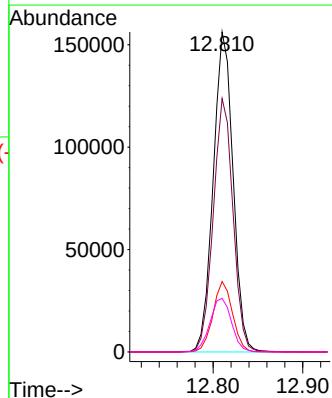
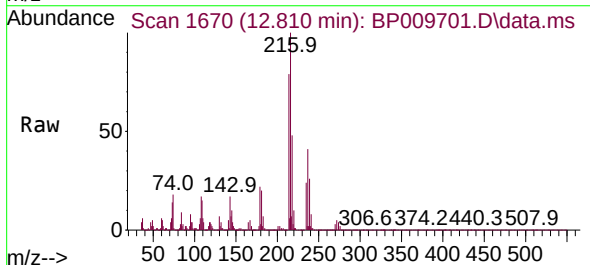




#40
Hexachlorocyclopentadiene
Concen: 20.164 ng/ul
RT: 12.798 min Scan# 1668
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22




Instrument :
BNA_P
ClientSampleId :
SSTD020618


Tgt Ion:237 Resp: 159436
Ion Ratio Lower Upper
237 100
235 65.2 53.2 79.8
272 12.7 10.8 16.2



#41
2,4,6-Trichlorophenol
Concen: 21.322 ng/ul
RT: 13.045 min Scan# 1710
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22

Tgt Ion:196 Resp: 155445
Ion Ratio Lower Upper
196 100
198 94.2 64.1 96.1
200 32.0 19.9 29.9#





#42

2,4,5-Trichlorophenol

Concen: 21.484 ng/ul

RT: 13.110 min Scan# 1721

Delta R.T. 0.000 min

Lab File: BP009701.D

Acq: 07 Apr 2022 16:22

Instrument :

BNA_P

ClientSampleId :

SSTD020618





Tgt Ion:196 Resp: 165703

Ion Ratio Lower Upper

196 100

198 92.8 68.6 103.0

200 32.0 32.8 49.2#



#43

1,1'-Biphenyl

Concen: 18.883 ng/ul

RT: 13.451 min Scan# 1779

Delta R.T. 0.000 min

Lab File: BP009701.D

Acq: 07 Apr 2022 16:22




Tgt Ion:154 Resp: 570528


Ion Ratio Lower Upper

154 100

153 40.7 28.6 43.0

76 11.3 8.5 12.7



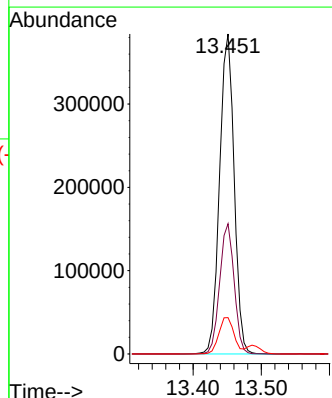





#44
2-Chloronaphthalene
Concen: 19.097 ng/ul
RT: 13.486 min Scan# 1785
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22




Instrument :
BNA_P
ClientSampleId :
SSTD020618


Tgt Ion:162 Resp: 438824
Ion Ratio Lower Upper
162 100
164 32.3 27.5 41.3
127 41.5 37.1 55.7



#45
2-Nitroaniline
Concen: 32.707 ng/ul
RT: 13.681 min Scan# 1818
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22

Tgt Ion: 65 Resp: 132109
Ion Ratio Lower Upper
65 100
92 63.6 77.9 116.9#
138 96.0 81.5 122.3









#47
Dimethylphthalate
Concen: 21.974 ng/ul
RT: 14.069 min Scan# 1884
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22




Instrument :
BNA_P
ClientSampleId :
SSTD020618


Tgt Ion:163 Resp: 590029
Ion Ratio Lower Upper
163 100
194 4.5 4.1 6.1
164 10.2 11.3 16.9#



#48
2,6-Dinitrotoluene
Concen: 30.095 ng/ul
RT: 14.175 min Scan# 1902
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22

Tgt Ion:165 Resp: 110422
Ion Ratio Lower Upper
165 100
89 64.0 51.7 77.5
121 23.5 18.3 27.5









#50
Acenaphthylene
Concen: 19.946 ng/ul
RT: 14.334 min Scan# 1929
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22




Instrument :
BNA_P
ClientSampleId :
SSTD020618


Tgt Ion:152 Resp: 724876
Ion Ratio Lower Upper
152 100
151 19.3 18.3 27.5
153 13.0 11.0 16.6



#51
3-Nitroaniline
Concen: 24.859 ng/ul
RT: 14.504 min Scan# 1958
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22

Tgt Ion:138 Resp: 115160
Ion Ratio Lower Upper
138 100
108 14.6 15.8 23.8#
92 123.8 117.1 175.7









#52
Acenaphthene
Concen: 19.895 ng/ul
RT: 14.675 min Scan# 1987
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22




Instrument :
BNA_P
ClientSampleId :
SSTD020618


Tgt Ion:153 Resp: 469898
Ion Ratio Lower Upper
153 100
152 45.9 34.3 51.5
154 89.4 70.0 105.0



#53
2,4-Dinitrophenol
Concen: 25.132 ng/ul
RT: 14.704 min Scan# 1992
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22

Tgt Ion:184 Resp: 56373
Ion Ratio Lower Upper
184 100
63 72.8 34.6 52.0#
154 78.0 57.7 86.5


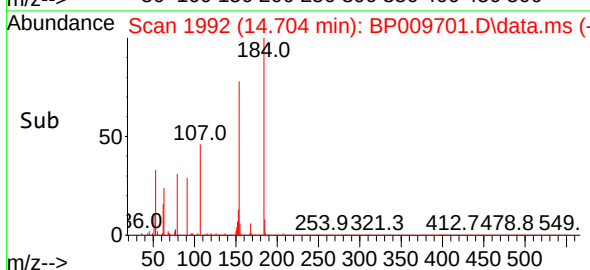






#55
4-Nitrophenol
Concen: 28.557 ng/ul
RT: 14.804 min Scan# 2009
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22




Instrument :
BNA_P
ClientSampleId :
SSTD020618


Tgt Ion:109 Resp: 99149
Ion Ratio Lower Upper
109 100
139 113.4 61.4 92.2#
65 126.4 65.3 97.9#



#56
Dibenzofuran
Concen: 20.747 ng/ul
RT: 15.010 min Scan# 2044
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22

Tgt Ion:168 Resp: 693157
Ion Ratio Lower Upper
168 100
139 38.7 30.1 45.1









#57
2,4-Dinitrotoluene
Concen: 31.524 ng/ul
RT: 14.963 min Scan# 2036
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22




Instrument :
BNA_P
ClientSampleId :
SSTD020618


Tgt Ion:165 Resp: 166197
Ion Ratio Lower Upper
165 100
63 47.8 29.5 44.3#
182 3.0 2.8 4.2

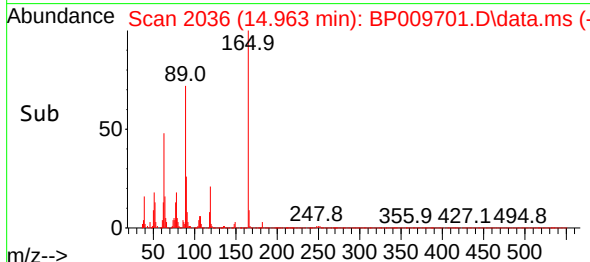

#58
2,3,4,6-Tetrachlorophenol
Concen: 25.330 ng/ul
RT: 15.233 min Scan# 2082
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22

Tgt Ion:232 Resp: 152760
Ion Ratio Lower Upper
232 100
131 45.0 25.4 38.2#
130 2.3 4.2 6.2#
166 30.1 28.1 42.1



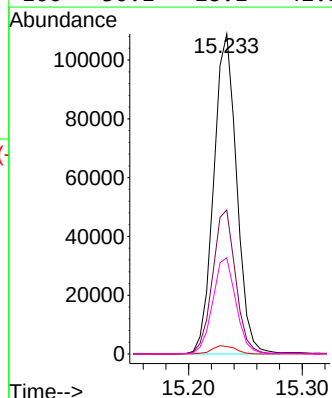
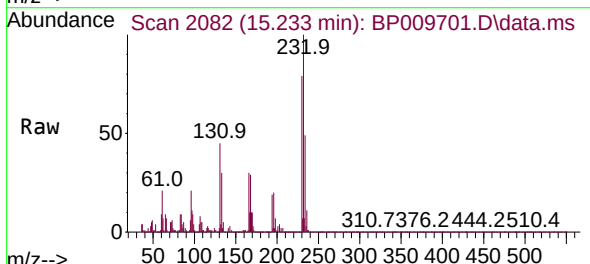




#59
Diethylphthalate
Concen: 23.695 ng/ul
RT: 15.433 min Scan# 2116
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22




Instrument :
BNA_P
ClientSampleId :
SSTD020618


Tgt Ion:149 Resp: 615715
Ion Ratio Lower Upper
149 100
177 21.6 22.0 33.0#
150 12.5 10.2 15.2



#61
Fluorene
Concen: 21.748 ng/ul
RT: 15.663 min Scan# 2155
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22

Tgt Ion:166 Resp: 569577
Ion Ratio Lower Upper
166 100
165 96.6 70.3 105.5
167 12.9 9.5 14.3









#62
4-Chlorophenyl-phenylether
Concen: 22.631 ng/ul
RT: 15.657 min Scan# 2154
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22




Instrument :
BNA_P
ClientSampleId :
SSTD020618


Tgt Ion:204 Resp: 300752
Ion Ratio Lower Upper
204 100
206 32.8 27.6 41.4
141 61.4 46.6 69.8



#63
4-Nitroaniline
Concen: 28.009 ng/ul
RT: 15.663 min Scan# 2155
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22

Tgt Ion:138 Resp: 125769
Ion Ratio Lower Upper
138 100
92 53.1 41.6 62.4
108 87.3 97.6 146.4#









#66
4,6-Dinitro-2-methylphenol
Concen: 25.332 ng/ul
RT: 15.728 min Scan# 2166
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22




Instrument :
BNA_P
ClientSampleId :
SSTD020618


Tgt Ion:198 Resp: 94699
Ion Ratio Lower Upper
198 100
182 4.3 6.0 9.0#
77 26.4 17.7 26.5

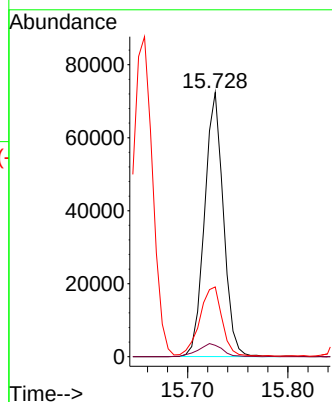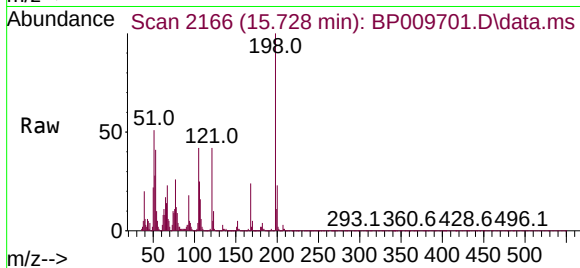

#67
N-Nitrosodiphenylamine
Concen: 19.611 ng/ul
RT: 15.863 min Scan# 2189
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22

Tgt Ion:169 Resp: 502709
Ion Ratio Lower Upper
169 100
168 65.2 48.3 72.5
167 35.4 29.6 44.4



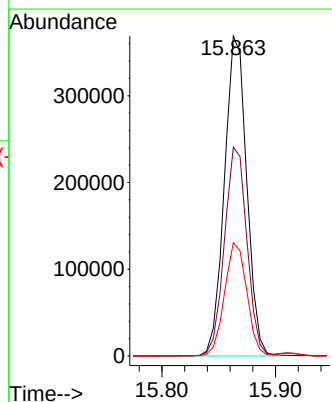





#68
4-Bromophenyl-phenylether
Concen: 20.642 ng/ul
RT: 16.551 min Scan# 2306
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22




Instrument :
BNA_P
ClientSampleId :
SSTD020618


Tgt Ion:248 Resp: 188633
Ion Ratio Lower Upper
248 100
250 100.4 79.4 119.0
141 79.4 67.2 100.8

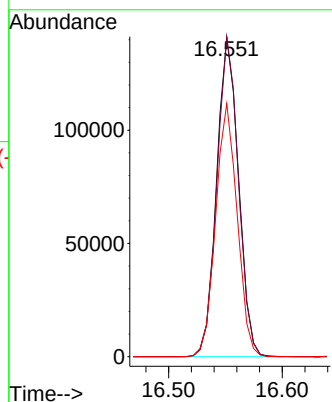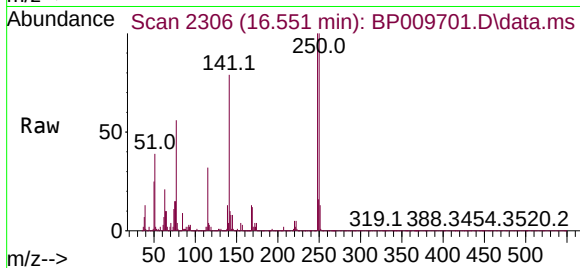

#69
Hexachlorobenzene
Concen: 20.681 ng/ul
RT: 16.669 min Scan# 2326
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22

Tgt Ion:284 Resp: 216992
Ion Ratio Lower Upper
284 100
142 34.2 19.2 28.8#
249 33.3 27.4 41.2





#70

Atrazine

Concen: 22.440 ng/ul

RT: 16.822 min Scan# 21

Delta R.T. 0.000 min

Lab File: BP009701.D

Acq: 07 Apr 2022 16:22

Instrument :

BNA_P

ClientSampleId :

SSTD020618





Tgt Ion:200 Resp: 205091

Ion Ratio Lower Upper

200 100

173 26.0 19.2 28.8

215 49.1 32.2 48.4#

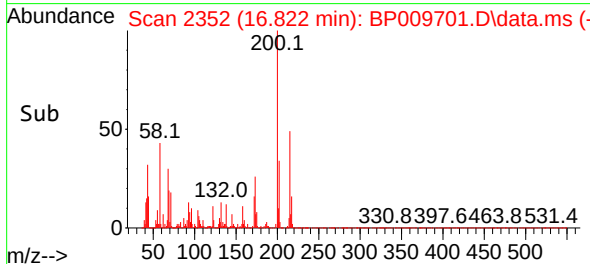

#71

Pentachlorophenol

Concen: 22.790 ng/ul

RT: 17.010 min Scan# 2384

Delta R.T. 0.000 min

Lab File: BP009701.D

Acq: 07 Apr 2022 16:22




Tgt Ion:266 Resp: 141163


Ion Ratio Lower Upper

266 100

264 58.6 57.3 85.9

268 59.7 65.7 98.5#



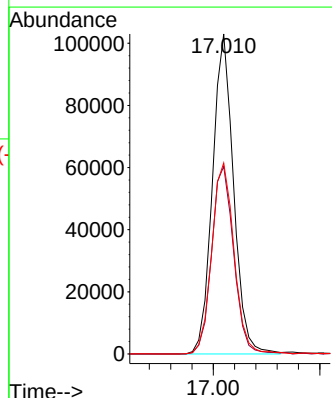
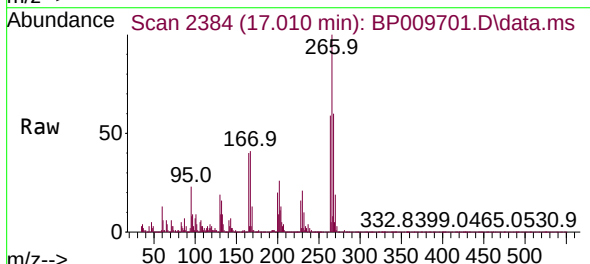




#72
Phenanthrene
Concen: 20.025 ng/ul
RT: 17.404 min Scan# 2451
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22




Instrument :
BNA_P
ClientSampleId :
SSTD020618


Tgt Ion:178 Resp: 935258
Ion Ratio Lower Upper
178 100
179 15.6 11.7 17.5
176 18.7 14.5 21.7



#74
Anthracene
Concen: 20.457 ng/ul
RT: 17.498 min Scan# 2467
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22

Tgt Ion:178 Resp: 953784
Ion Ratio Lower Upper
178 100
179 15.2 12.3 18.5
176 18.2 13.4 20.2









#75
1,2,3,4-Tetrachlorobenzene
Concen: 17.269 ng/uL
RT: 13.416 min Scan# 1773
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22




Instrument :
BNA_P
ClientSampleId :
SSTD020618


Tgt Ion:216 Resp: 254935
Ion Ratio Lower Upper
216 100
214 79.8 50.4 75.6#
218 49.1 35.2 52.8

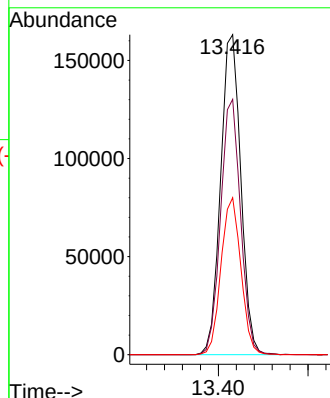

#76
Pentachlorobenzene
Concen: 18.767 ng/uL
RT: 14.933 min Scan# 2031
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22

Tgt Ion:250 Resp: 246769
Ion Ratio Lower Upper
250 100
248 62.3 43.5 65.3
252 64.4 46.5 69.7



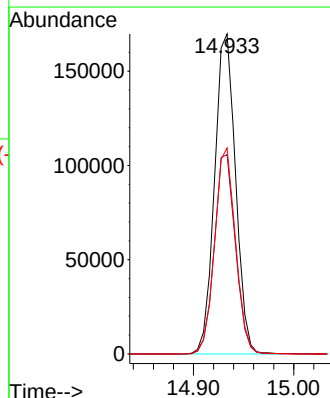





#77
 Carbazole
 Concen: 20.381 ng/ul
 RT: 17.757 min Scan# 2511
 Delta R.T. 0.000 min
 Lab File: BP009701.D
 Acq: 07 Apr 2022 16:22




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020618


Tgt Ion:167 Resp: 845785
 Ion Ratio Lower Upper
 167 100
 166 21.1 15.8 23.8
 139 12.9 8.3 12.5#



#78
 Di-n-butylphthalate
 Concen: 23.284 ng/ul
 RT: 18.322 min Scan# 2607
 Delta R.T. 0.000 min
 Lab File: BP009701.D
 Acq: 07 Apr 2022 16:22

Tgt Ion:149 Resp: 1071224
 Ion Ratio Lower Upper
 149 100
 150 9.0 9.6 14.4#
 104 5.6 6.2 9.4#









#80
Fluoranthene
Concen: 19.718 ng/ul
RT: 19.363 min Scan# 211
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22




Instrument :
BNA_P
ClientSampleId :
SSTD020618


Tgt Ion:202 Resp: 1155869
Ion Ratio Lower Upper
202 100
101 9.6 9.6 14.4
100 7.7 6.3 9.5



#82
Pyrene
Concen: 19.722 ng/ul
RT: 19.716 min Scan# 2844
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22

Tgt Ion:202 Resp: 1181909
Ion Ratio Lower Upper
202 100
101 11.2 10.6 15.8
100 9.2 9.8 14.6#





#83

Butylbenzylphthalate

Concen: 25.121 ng/ul

RT: 20.592 min Scan# 2993

Delta R.T. 0.000 min

Lab File: BP009701.D

Acq: 07 Apr 2022 16:22

Instrument :

BNA_P

ClientSampleId :

SSTD020618





Tgt Ion:149 Resp: 486054

Ion Ratio Lower Upper

149 100

91 72.9 71.1 106.7

206 22.0 28.8 43.2#



#84

3,3'-Dichlorobenzidine

Concen: 21.036 ng/ul

RT: 21.357 min Scan# 3123

Delta R.T. 0.000 min

Lab File: BP009701.D

Acq: 07 Apr 2022 16:22




Tgt Ion:252 Resp: 410275


Ion Ratio Lower Upper

252 100

254 65.6 49.8 74.6

126 8.9 4.3 6.5#


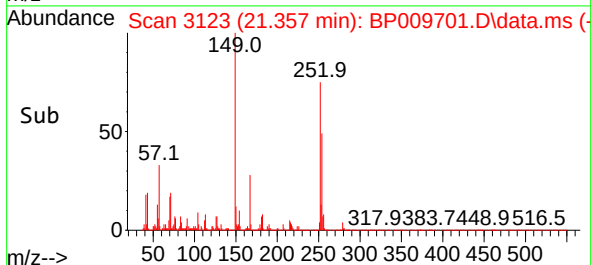
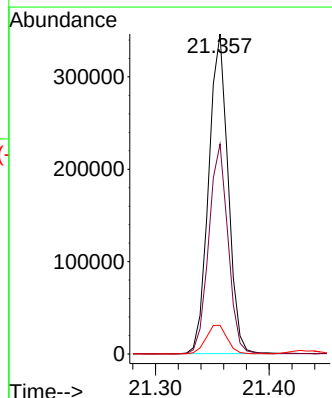
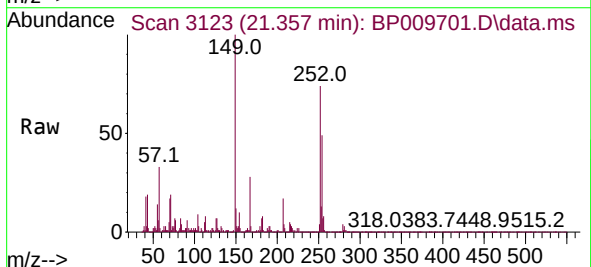




#85
Benzo(a)anthracene
Concen: 19.873 ng/ul
RT: 21.427 min Scan# 3135
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22




Instrument :
BNA_P
ClientSampleId :
SSTD020618


Tgt Ion:228 Resp: 1162644
Ion Ratio Lower Upper
228 100
229 19.9 18.2 27.2
226 25.5 22.8 34.2

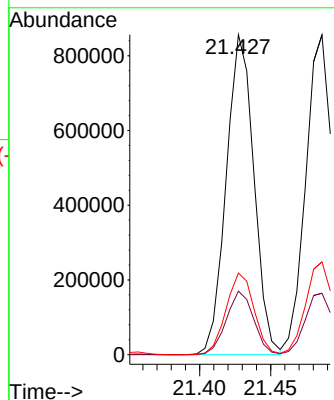

#86
Bis(2-ethylhexyl)phthalate
Concen: 23.660 ng/ul
RT: 21.363 min Scan# 3124
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22

Tgt Ion:149 Resp: 727729
Ion Ratio Lower Upper
149 100
167 28.4 32.8 49.2#
279 4.8 5.6 8.4#

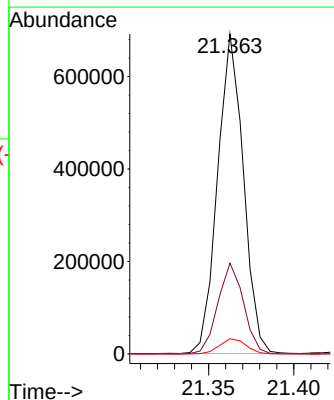



#87

Chrysene

Concen: 19.809 ng/ul

RT: 21.486 min Scan# 3145

Delta R.T. 0.000 min

Lab File: BP009701.D

Acq: 07 Apr 2022 16:22

Instrument :

BNA_P

ClientSampleId :

SSTD020618





Tgt Ion:228 Resp: 1123058

Ion Ratio Lower Upper

228 100

226 29.0 22.7 34.1

229 19.2 15.2 22.8

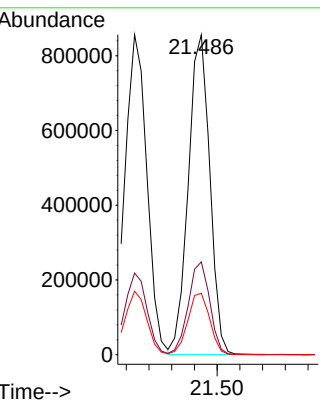

#89

Di-n-octyl phthalate

Concen: 25.327 ng/ul




RT: 22.321 min Scan# 3287


Delta R.T. 0.000 min

Lab File: BP009701.D

Acq: 07 Apr 2022 16:22

Tgt Ion:149 Resp: 1198246

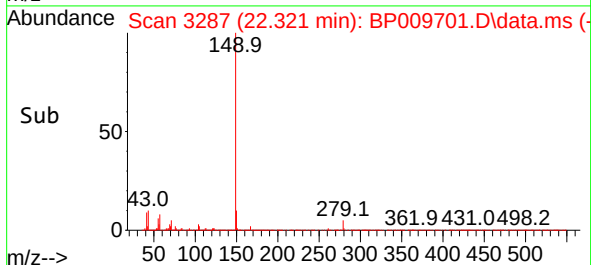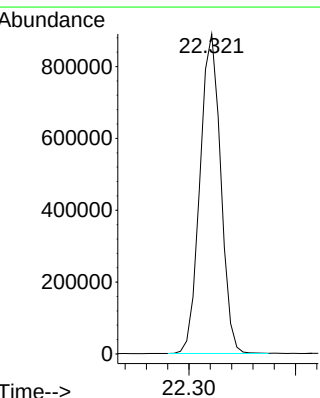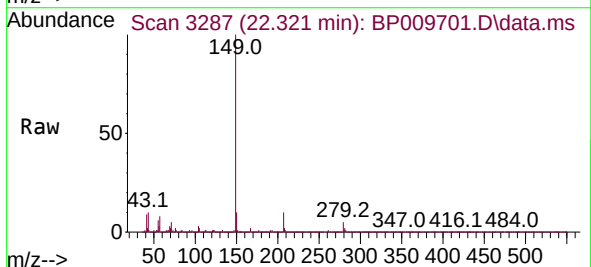



#90

Benzo(b)fluoranthene

Concen: 21.146 ng/ul

RT: 23.168 min Scan# 3431

Delta R.T. 0.000 min

Lab File: BP009701.D

Acq: 07 Apr 2022 16:22

Instrument :

BNA_P

ClientSampleId :

SSTD020618





Tgt Ion:252 Resp: 1164738

Ion Ratio Lower Upper

252 100

253 21.3 17.4 26.0

125 8.0 7.3 10.9

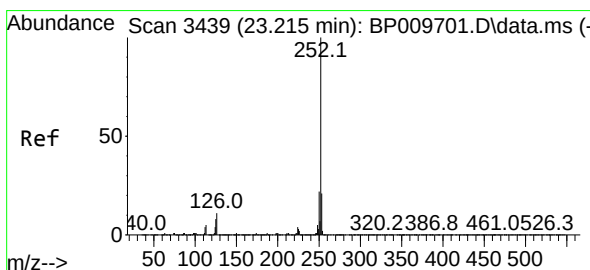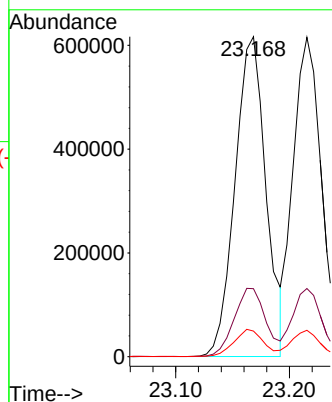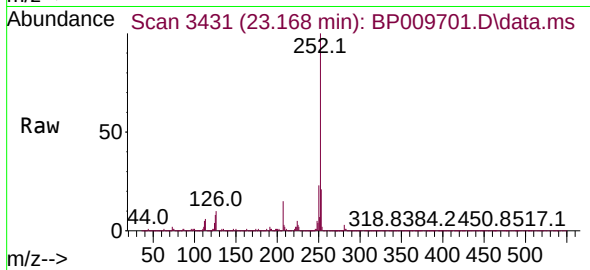

#91

Benzo(k)fluoranthene

Concen: 21.211 ng/ul

RT: 23.215 min Scan# 3439

Delta R.T. 0.000 min

Lab File: BP009701.D

Acq: 07 Apr 2022 16:22




Tgt Ion:252 Resp: 1058940


Ion Ratio Lower Upper

252 100

253 21.3 17.9 26.9

125 8.2 5.1 7.7#


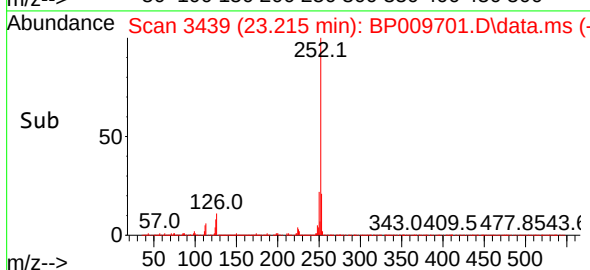

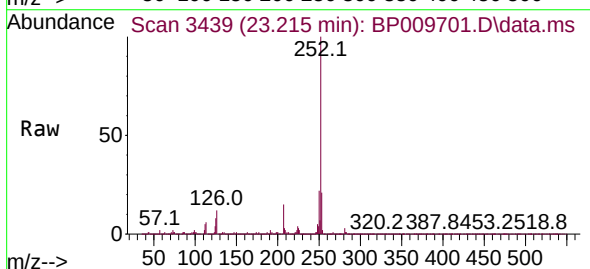




#93
Benzo(a)pyrene
Concen: 20.322 ng/ul
RT: 23.815 min Scan# 3541
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22




Instrument :
BNA_P
ClientSampleId :
SSTD020618


Tgt Ion:252 Resp: 1072673
Ion Ratio Lower Upper
252 100
253 22.1 17.5 26.3
125 8.9 6.4 9.6



#94
Indeno(1,2,3-cd)pyrene
Concen: 17.482 ng/ul
RT: 26.515 min Scan# 4000
Delta R.T. 0.000 min
Lab File: BP009701.D
Acq: 07 Apr 2022 16:22

Tgt Ion:276 Resp: 1092575
Ion Ratio Lower Upper
276 100
138 18.6 12.3 18.5#
277 24.1 19.3 28.9









#95
 Dibenzo(a,h)anthracene
 Concen: 17.846 ng/ul
 RT: 26.533 min Scan# 4003
 Delta R.T. 0.000 min
 Lab File: BP009701.D
 Acq: 07 Apr 2022 16:22

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020618

Tgt Ion:278 Resp: 941546
 Ion Ratio Lower Upper
 278 100
 139 13.2 6.6 10.0#
 279 23.5 18.4 27.6

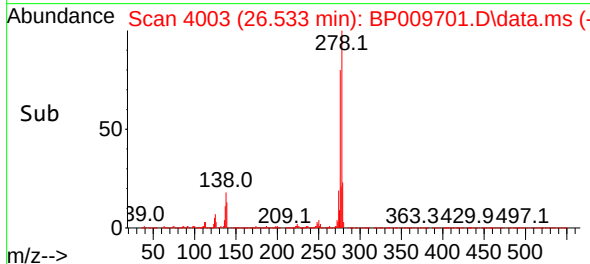

#96
 Benzo(g,h,i)perylene
 Concen: 16.660 ng/ul
 RT: 27.309 min Scan# 4135
 Delta R.T. 0.000 min
 Lab File: BP009701.D
 Acq: 07 Apr 2022 16:22

Tgt Ion:276 Resp: 891651
 Ion Ratio Lower Upper
 276 100
 138 17.7 11.6 17.4#
 277 23.6 15.9 23.9

