

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040722\
 Data File : BP009705.D
 Acq On : 07 Apr 2022 19:13
 Operator : CG/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SICV622

Quant Time: Apr 08 03:26:45 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 07 19:16:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.987	152	199656	20.000	ng/ul	0.00
20) Naphthalene-d8	10.799	136	919096	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.622	164	691099	20.000	ng/ul	0.01
64) Phenanthrene-d10	17.375	188	1578333	20.000	ng/ul	# 0.01
79) Chrysene-d12	21.457	240	1684037	20.000	ng/ul	# 0.01
88) Perylene-d12	23.945	264	1594884	20.000	ng/ul	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	31533	7.049	ng/uL	0.00
4) Pyridine-d5	3.811	84	225093	18.249	ng/ul	0.00
7) Phenol-d5	7.134	99	296551	16.918	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.311	67	206742	19.812	ng/ul	0.00
11) 2-Chlorophenol-d4	7.516	132	235357	17.800	ng/ul	0.01
15) 4-Methylphenol-d8	8.693	113	262696	17.953	ng/ul	0.01
21) Nitrobenzene-d5	9.146	128	125304	18.906	ng/ul	0.00
24) 2-Nitrophenol-d4	9.869	143	137820	18.967	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.410	165	265056	17.432	ng/ul	0.00
31) 4-Chloroaniline-d4	10.928	131	377070	17.411	ng/ul	0.01
46) Dimethylphthalate-d6	14.034	166	962960	17.738	ng/ul	0.01
49) Acenaphthylene-d8	14.316	160	1088953	16.932	ng/ul	0.01
54) 4-Nitrophenol-d4	14.804	143	183123	18.600	ng/ul	0.02
60) Fluorene-d10	15.616	176	784868	17.186	ng/ul	0.01
65) 4,6-Dinitro-2-methylph...	15.728	200	172448	18.443	ng/ul	0.02
73) Anthracene-d10	17.475	188	1306077	17.283	ng/ul	0.01
81) Pyrene-d10	19.698	212	1583069	17.212	ng/ul	0.01
92) Benzo(a)pyrene-d12	23.780	264	1441586	17.357	ng/ul	0.02
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.434	88	33254	7.292	ng/uL#	23
5) Pyridine	3.834	79	210377	16.347	ng/ul#	50
6) Benzaldehyde	7.117	77	212109	19.731	ng/ul	97
8) Phenol	7.164	94	302689	17.252	ng/ul#	92
10) Bis(2-Chloroethyl)ether	7.405	93	239887	17.552	ng/ul#	78
12) 2-Chlorophenol	7.546	128	234543	17.595	ng/ul	93
13) 2-Methylphenol	8.422	108	235497	17.212	ng/ul	99
14) 2,2'-oxybis(1-Chloropr...	8.516	45	355295	17.587	ng/ul#	83
16) Acetophenone	8.811	105	414178	17.965	ng/ul#	82
17) N-Nitroso-di-n-propyla...	8.799	70	222916	18.650	ng/ul#	72
18) 4-Methylphenol	8.758	108	262206	17.697	ng/ul	95
19) Hexachloroethane	9.081	117	97458	17.316	ng/ul	85
22) Nitrobenzene	9.187	77	306128	17.994	ng/ul#	85
23) Isophorone	9.722	82	638988	18.228	ng/ul	96
25) 2-Nitrophenol	9.905	139	145856	18.820	ng/ul#	84
26) 2,4-Dimethylphenol	9.963	107	319026	17.346	ng/ul#	79
27) Bis(2-Chloroethoxy)met...	10.205	93	356540	17.323	ng/ul#	97
29) 2,4-Dichlorophenol	10.440	162	257840	17.491	ng/ul#	83
30) Naphthalene	10.846	128	816896	17.282	ng/ul	97
32) 4-Chloroaniline	10.952	127	373381	17.422	ng/ul	97
33) Hexachlorobutadiene	11.146	225	180317	16.984	ng/ul	93
34) Caprolactam	11.722	113	53833	11.042	ng/ul#	12
35) 4-Chloro-3-methylphenol	12.069	107	325465	18.221	ng/ul#	70
36) 2-Methylnaphthalene	12.451	142	613786	17.774	ng/ul	89

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040722\
 Data File : BP009705.D
 Acq On : 07 Apr 2022 19:13
 Operator : CG/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 8 Sample Multiplier: 1


Instrument :
 BNA_P
 ClientSampleId :
 SICV622


Quant Time: Apr 08 03:26:45 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 07 19:16:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.669	142	593420	17.019	ng/ul#	94
39) 1,2,4,5-Tetrachloroben...	12.822	216	352004	16.648	ng/ul	94
40) Hexachlorocyclopentadiene	12.810	237	246169	16.777	ng/ul	96
41) 2,4,6-Trichlorophenol	13.051	196	235529	17.443	ng/ul#	82
42) 2,4,5-Trichlorophenol	13.122	196	256032	17.545	ng/ul#	85
43) 1,1'-Biphenyl	13.457	154	849002	16.837	ng/ul	93
44) 2-Chloronaphthalene	13.499	162	652980	16.846	ng/ul	94
45) 2-Nitroaniline	13.693	65	223117	19.642	ng/ul#	82
47) Dimethylphthalate	14.081	163	921943	17.645	ng/ul#	92
48) 2,6-Dinitrotoluene	14.187	165	201130	20.928	ng/ul	94
50) Acenaphthylene	14.346	152	1124797	17.722	ng/ul	95
51) 3-Nitroaniline	14.516	138	206330	20.651	ng/ul#	82
52) Acenaphthene	14.687	153	713847	17.178	ng/ul	97
53) 2,4-Dinitrophenol	14.716	184	110164	18.964	ng/ul#	83
55) 4-Nitrophenol	14.816	109	162578	17.939	ng/ul#	52
56) Dibenzofuran	15.022	168	1051448	17.191	ng/ul	98
57) 2,4-Dinitrotoluene	14.975	165	278312	19.721	ng/ul#	87
58) 2,3,4,6-Tetrachlorophenol	15.245	232	246450	18.523	ng/ul#	88
59) Diethylphthalate	15.445	149	956865	17.696	ng/ul	93
61) Fluorene	15.669	166	863735	17.145	ng/ul	92
62) 4-Chlorophenyl-phenyle...	15.669	204	457773	17.090	ng/ul	99
63) 4-Nitroaniline	15.681	138	222208	22.205	ng/ul#	79
66) 4,6-Dinitro-2-methylph...	15.740	198	170161	18.309	ng/ul#	90
67) N-Nitrosodiphenylamine	15.875	169	783093	17.332	ng/ul	95
68) 4-Bromophenyl-phenylether	16.563	248	290943	17.029	ng/ul	94
69) Hexachlorobenzene	16.681	284	329090	16.752	ng/ul#	91
70) Atrazine	16.834	200	303412	16.270	ng/ul#	88
71) Pentachlorophenol	17.022	266	223295	16.792	ng/ul	86
72) Phenanthrene	17.416	178	1442027	17.116	ng/ul	98
74) Anthracene	17.510	178	1462112	17.117	ng/ul	98
75) 1,2,3,4-Tetrachloroben...	13.422	216	376440	16.497	ng/ul#	86
76) Pentachlorobenzene	14.945	250	375590	16.886	ng/ul	92
77) Carbazole	17.769	167	1353260	17.531	ng/ul#	95
78) Di-n-butylphthalate	18.334	149	1716930	18.088	ng/ul#	92
80) Fluoranthene	19.375	202	1794946	16.955	ng/ul#	96
82) Pyrene	19.728	202	1830639	17.055	ng/ul#	94
83) Butylbenzylphthalate	20.604	149	803001	18.237	ng/ul#	79
84) 3,3'-Dichlorobenzidine	21.369	252	727035	20.260	ng/ul#	97
85) Benzo(a)anthracene	21.439	228	1884937	17.656	ng/ul	95
86) Bis(2-ethylhexyl)phtha...	21.375	149	1195674	18.053	ng/ul#	82
87) Chrysene	21.498	228	1733458	16.829	ng/ul	98
89) Di-n-octyl phthalate	22.333	149	1960353	17.543	ng/ul	100
90) Benzo(b)fluoranthene	23.180	252	1833308	17.301	ng/ul	99
91) Benzo(k)fluoranthene	23.233	252	1717883	17.766	ng/ul#	98
93) Benzo(a)pyrene	23.833	252	1696480	17.272	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.551	276	1675195	16.310	ng/ul#	96
95) Dibenzo(a,h)anthracene	26.568	278	1480006	16.617	ng/ul#	96
96) Benzo(g,h,i)perylene	27.345	276	1399927	16.530	ng/ul#	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Apr 08 03:26:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 07 19:16:52 2022
Response via : Initial Calibration









#2
 1,4-Dioxane
 Concen: 7.292 ng/uL
 RT: 3.434 min Scan# 70
 Delta R.T. 0.006 min
 Lab File: BP009705.D
 Acq: 07 Apr 2022 19:13




Instrument :
 BNA_P
 ClientSampleId :
 SICV622


Tgt Ion: 88 Resp: 33254
 Ion Ratio Lower Upper
 88 100
 43 33.9 6.8 10.2#
 58 81.3 28.4 42.6#

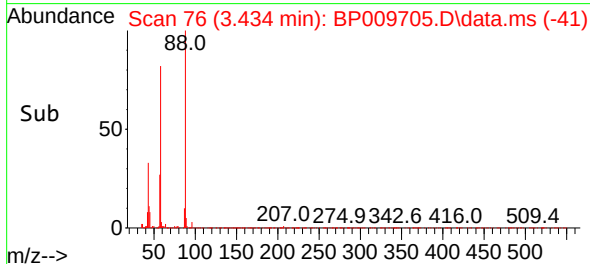

#5
 Pyridine
 Concen: 16.347 ng/uL
 RT: 3.834 min Scan# 144
 Delta R.T. 0.006 min
 Lab File: BP009705.D
 Acq: 07 Apr 2022 19:13

Tgt Ion: 79 Resp: 210377
 Ion Ratio Lower Upper
 79 100
 52 84.5 35.5 53.3#
 51 40.3 20.2 30.4#


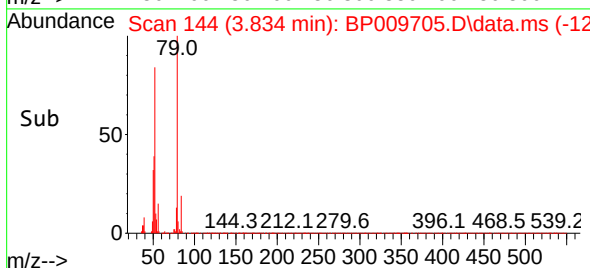
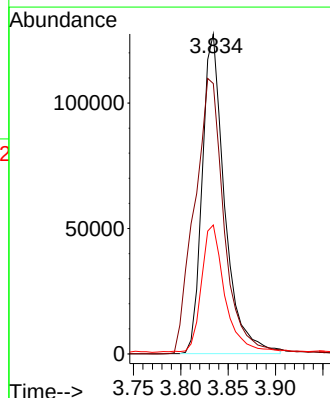



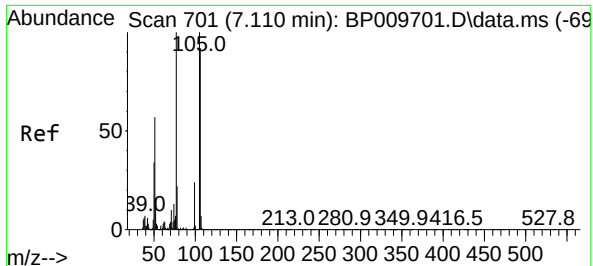

#6
Benzaldehyde
Concen: 19.731 ng/ul
RT: 7.117 min Scan# 701
Delta R.T. 0.006 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13




Instrument :
BNA_P
ClientSampleId :
SICV622


Tgt Ion: 77 Resp: 212109
Ion Ratio Lower Upper
77 100
105 96.2 77.0 115.4
106 91.2 77.0 115.4

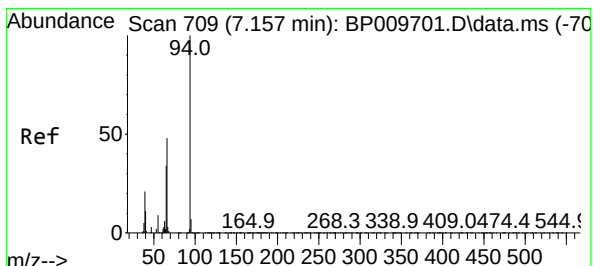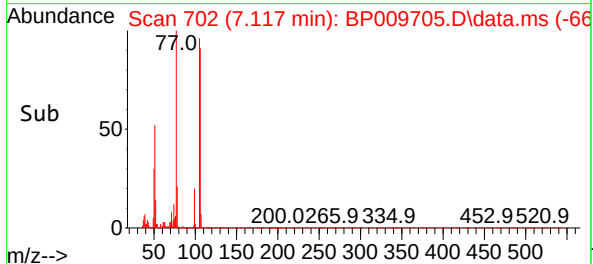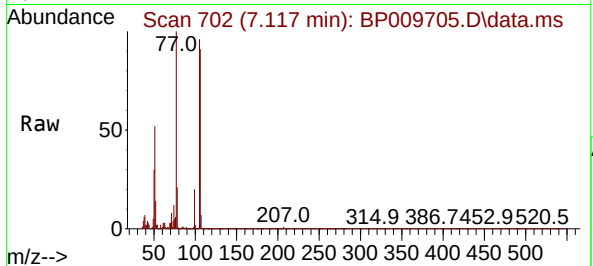

#8
Phenol
Concen: 17.252 ng/ul
RT: 7.164 min Scan# 710
Delta R.T. 0.006 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13

Tgt Ion: 94 Resp: 302689
Ion Ratio Lower Upper
94 100
65 32.3 19.0 28.6#
66 44.9 34.6 51.8


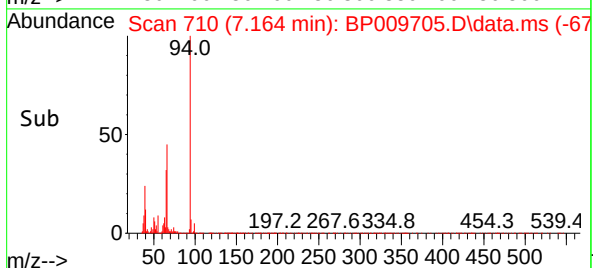
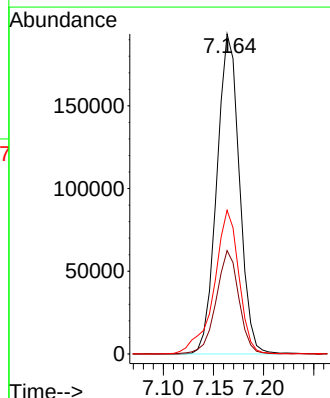
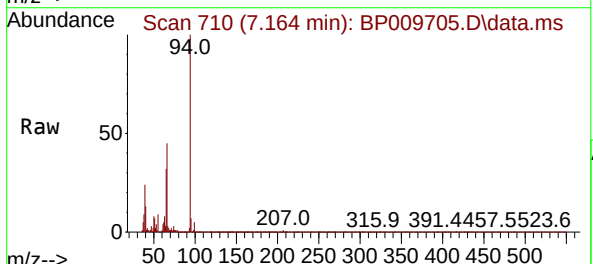




#10
Bis(2-Chloroethyl)ether
Concen: 17.552 ng/ul
RT: 7.405 min Scan# 750
Delta R.T. 0.006 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13




Instrument :
BNA_P
ClientSampleId :
SICV622


Tgt Ion: 93 Resp: 239887
Ion Ratio Lower Upper
93 100
63 81.6 45.0 67.4#
95 33.4 26.3 39.5



#12
2-Chlorophenol
Concen: 17.595 ng/ul
RT: 7.546 min Scan# 775
Delta R.T. 0.006 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13

Tgt Ion:128 Resp: 234543
Ion Ratio Lower Upper
128 100
64 51.8 45.3 67.9
130 31.0 29.0 43.6









#13
2-Methylphenol
Concen: 17.212 ng/ul
RT: 8.422 min Scan# 91
Delta R.T. 0.006 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13




Instrument :
BNA_P
ClientSampleId :
SICV622


Tgt Ion:108 Resp: 235497
Ion Ratio Lower Upper
108 100
107 89.7 70.8 106.2



#14
2,2'-oxybis(1-Chloropropane)
Concen: 17.587 ng/ul
RT: 8.516 min Scan# 940
Delta R.T. 0.006 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13

Tgt Ion: 45 Resp: 355295
Ion Ratio Lower Upper
45 100
77 13.2 17.1 25.7#
79 9.8 13.2 19.8#









#16
Acetophenone
Concen: 17.965 ng/ul
RT: 8.811 min Scan# 990
Delta R.T. 0.006 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13




Instrument :
BNA_P
ClientSampleId :
SICV622


Tgt Ion:105 Resp: 414178
Ion Ratio Lower Upper
105 100
77 78.8 53.4 80.2
51 30.5 13.8 20.8#



#17
N-Nitroso-di-n-propylamine
Concen: 18.650 ng/ul
RT: 8.799 min Scan# 988
Delta R.T. 0.006 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13

Tgt Ion: 70 Resp: 222916
Ion Ratio Lower Upper
70 100
42 63.5 31.8 47.8#
101 9.6 15.6 23.4#
130 21.5 13.7 20.5#


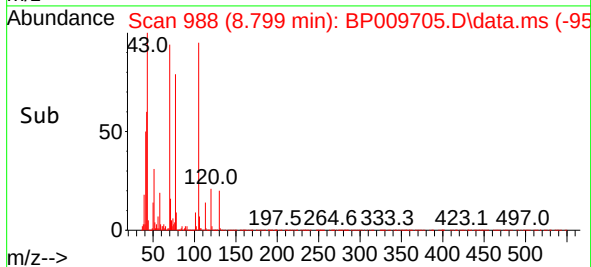

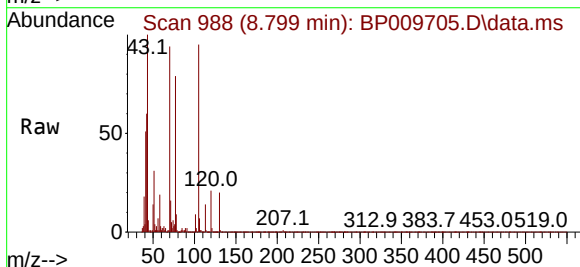




#18
4-Methylphenol
Concen: 17.697 ng/ul
RT: 8.758 min Scan# 91
Delta R.T. 0.012 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13




Instrument :
BNA_P
ClientSampleId :
SICV622


Tgt Ion:108 Resp: 262206
Ion Ratio Lower Upper
108 100
107 109.1 83.6 125.4

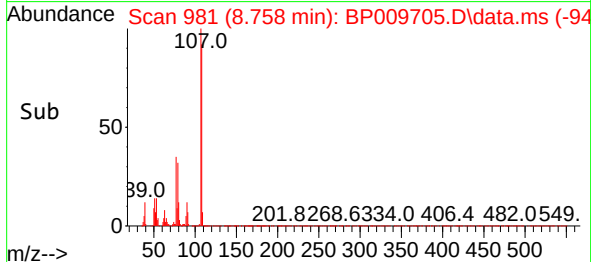

#19
Hexachloroethane
Concen: 17.316 ng/ul
RT: 9.081 min Scan# 1036
Delta R.T. 0.012 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13

Tgt Ion:117 Resp: 97458
Ion Ratio Lower Upper
117 100
201 113.1 106.5 159.7
199 64.1 59.0 88.6


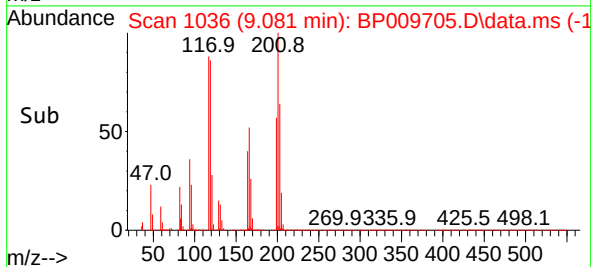

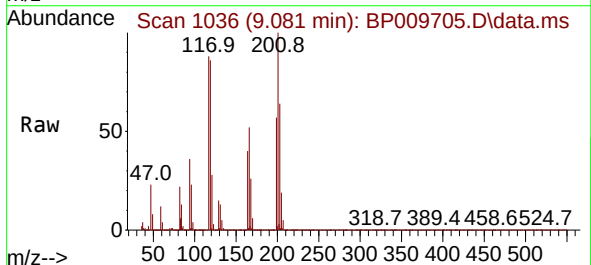




#22
 Nitrobenzene
 Concen: 17.994 ng/ul
 RT: 9.187 min Scan# 1053
 Delta R.T. 0.006 min
 Lab File: BP009705.D
 Acq: 07 Apr 2022 19:13




Instrument :
 BNA_P
 ClientSampleId :
 SICV622


Tgt Ion: 77 Resp: 306128
 Ion Ratio Lower Upper
 77 100
 123 43.2 42.3 63.5
 65 14.7 5.8 8.8#



#23
 Isophorone
 Concen: 18.228 ng/ul
 RT: 9.722 min Scan# 1145
 Delta R.T. 0.006 min
 Lab File: BP009705.D
 Acq: 07 Apr 2022 19:13

Tgt Ion: 82 Resp: 638988
 Ion Ratio Lower Upper
 82 100
 95 8.4 7.8 11.8
 138 17.7 12.9 19.3









#25
2-Nitrophenol
Concen: 18.820 ng/ul
RT: 9.905 min Scan# 1175
Delta R.T. 0.006 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13




Instrument :
BNA_P
ClientSampleId :
SICV622


Tgt Ion:139 Resp: 145856
Ion Ratio Lower Upper
139 100
65 58.6 49.4 74.2
109 34.1 44.7 67.1#



#26
2,4-Dimethylphenol
Concen: 17.346 ng/ul
RT: 9.963 min Scan# 1186
Delta R.T. 0.006 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13

Tgt Ion:107 Resp: 319026
Ion Ratio Lower Upper
107 100
121 48.6 34.1 51.1
122 79.5 46.3 69.5#









#27
 Bis(2-Chloroethoxy)methane
 Concen: 17.323 ng/ul
 RT: 10.205 min Scan# 1227
 Delta R.T. 0.012 min
 Lab File: BP009705.D
 Acq: 07 Apr 2022 19:13




Instrument :
 BNA_P
 ClientSampleId :
 SICV622


Tgt Ion: 93 Resp: 356540
 Ion Ratio Lower Upper
 93 100
 95 32.1 26.2 39.4
 123 11.4 6.2 9.4#



#29
 2,4-Dichlorophenol
 Concen: 17.491 ng/ul
 RT: 10.440 min Scan# 1267
 Delta R.T. 0.006 min
 Lab File: BP009705.D
 Acq: 07 Apr 2022 19:13

Tgt Ion: 162 Resp: 257840
 Ion Ratio Lower Upper
 162 100
 164 66.3 37.0 55.6#
 98 37.4 31.0 46.6





#30

Naphthalene

Concen: 17.282 ng/ul

RT: 10.846 min Scan# 1335

Delta R.T. 0.006 min

Lab File: BP009705.D

Acq: 07 Apr 2022 19:13

Instrument :

BNA_P

ClientSampleId :

SICV622





Tgt Ion:128 Resp: 816896

Ion Ratio Lower Upper

128 100

129 10.9 8.6 13.0

127 13.1 12.2 18.4



#32

4-Chloroaniline

Concen: 17.422 ng/ul

RT: 10.952 min Scan# 1354

Delta R.T. 0.012 min

Lab File: BP009705.D




Acq: 07 Apr 2022 19:13


Tgt Ion:127 Resp: 373381

Ion Ratio Lower Upper

127 100

129 32.5 24.6 37.0









#33
Hexachlorobutadiene
Concen: 16.984 ng/ul
RT: 11.146 min Scan# 11
Delta R.T. 0.006 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13




Instrument :
BNA_P
ClientSampleId :
SICV622


Tgt Ion:225 Resp: 180317
Ion Ratio Lower Upper
225 100
223 61.6 53.4 80.0
227 61.7 53.8 80.8



#34
Caprolactam
Concen: 11.042 ng/ul
RT: 11.722 min Scan# 1485
Delta R.T. 0.018 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13

Tgt Ion:113 Resp: 53833
Ion Ratio Lower Upper
113 100
55 176.7 58.2 87.2#
56 138.3 68.6 103.0#









#35
4-Chloro-3-methylphenol
Concen: 18.221 ng/ul
RT: 12.069 min Scan# 1542
Delta R.T. 0.012 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13




Instrument :
BNA_P
ClientSampleId :
SICV622


Tgt Ion:107 Resp: 325465
Ion Ratio Lower Upper
107 100
144 24.8 15.8 23.8#
142 74.3 38.9 58.3#

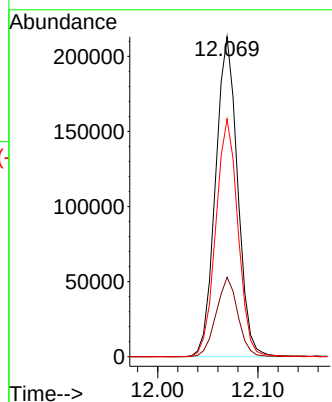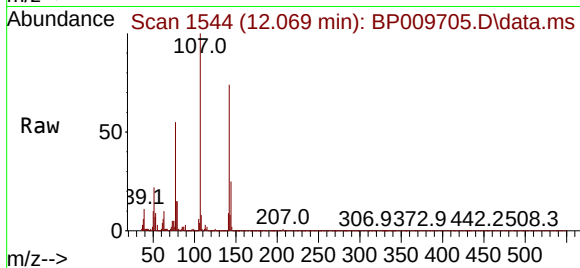

#36
2-Methylnaphthalene
Concen: 17.774 ng/ul
RT: 12.451 min Scan# 1609
Delta R.T. 0.006 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13

Tgt Ion:142 Resp: 613786
Ion Ratio Lower Upper
142 100
141 90.0 64.3 96.5









#37
1-Methylnaphthalene
Concen: 17.019 ng/ul
RT: 12.669 min Scan# 1645
Delta R.T. 0.006 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13




Instrument :
BNA_P
ClientSampleId :
SICV622


Tgt Ion:142 Resp: 593420
Ion Ratio Lower Upper
142 100
141 92.7 69.8 104.8
116 4.1 5.6 8.4#

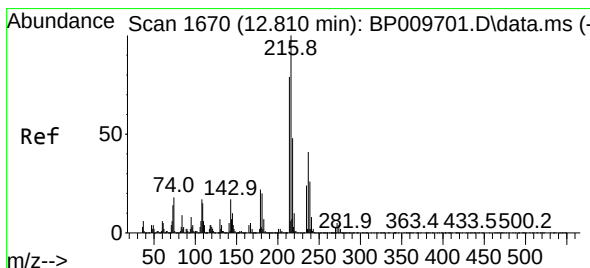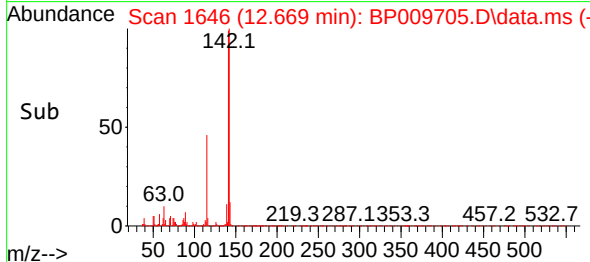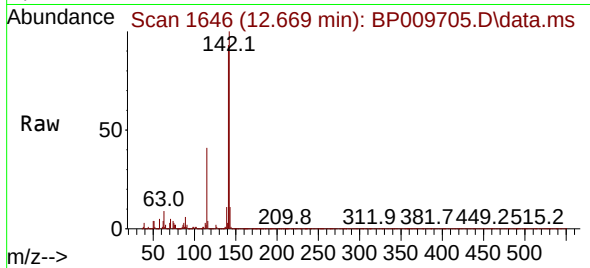

#39
1,2,4,5-Tetrachlorobenzene
Concen: 16.648 ng/ul
RT: 12.822 min Scan# 1672
Delta R.T. 0.012 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13

Tgt Ion:216 Resp: 352004
Ion Ratio Lower Upper
216 100
214 76.7 58.2 87.2
179 21.0 14.2 21.2
108 16.1 15.3 22.9


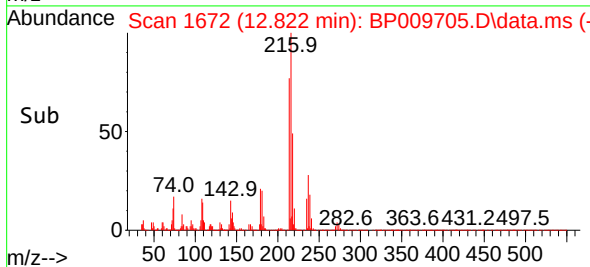

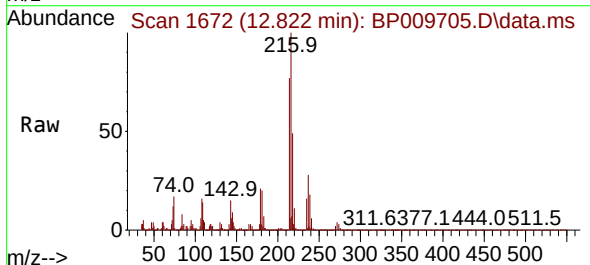




#40
 Hexachlorocyclopentadiene
 Concen: 16.777 ng/ul
 RT: 12.810 min Scan# 1670
 Delta R.T. 0.012 min
 Lab File: BP009705.D
 Acq: 07 Apr 2022 19:13




Instrument :
 BNA_P
 ClientSampleId :
 SICV622


Tgt Ion:237 Resp: 246169
 Ion Ratio Lower Upper
 237 100
 235 63.1 53.2 79.8
 272 11.9 10.8 16.2



#41
 2,4,6-Trichlorophenol
 Concen: 17.443 ng/ul
 RT: 13.051 min Scan# 1711
 Delta R.T. 0.006 min
 Lab File: BP009705.D
 Acq: 07 Apr 2022 19:13

Tgt Ion:196 Resp: 235529
 Ion Ratio Lower Upper
 196 100
 198 97.2 64.1 96.1#
 200 31.5 19.9 29.9#





#42

2,4,5-Trichlorophenol

Concen: 17.545 ng/ul

RT: 13.122 min Scan# 1

Delta R.T. 0.012 min

Lab File: BP009705.D

Acq: 07 Apr 2022 19:13

Instrument :

BNA_P

ClientSampleId :

SICV622





Tgt Ion:196 Resp: 256032

Ion Ratio Lower Upper

196 100

198 100.3 68.6 103.0

200 32.4 32.8 49.2#

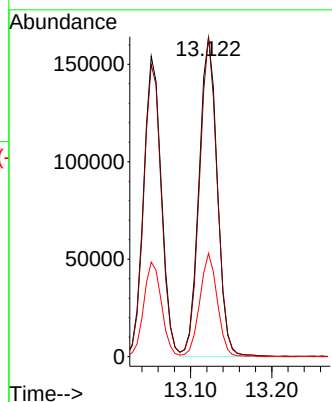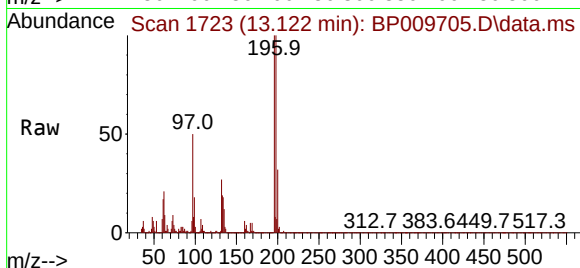

#43

1,1'-Biphenyl

Concen: 16.837 ng/ul

RT: 13.457 min Scan# 1780

Delta R.T. 0.006 min

Lab File: BP009705.D

Acq: 07 Apr 2022 19:13




Tgt Ion:154 Resp: 849002


Ion Ratio Lower Upper

154 100

153 40.7 28.6 43.0

76 12.0 8.5 12.7



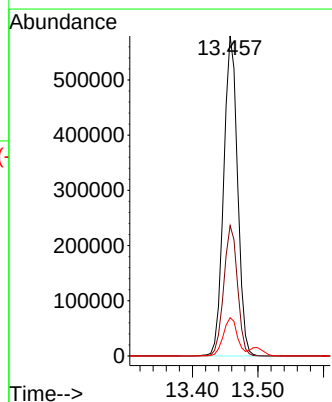





#44
2-Chloronaphthalene
Concen: 16.846 ng/ul
RT: 13.499 min Scan# 11
Delta R.T. 0.012 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13




Instrument :
BNA_P
ClientSampleId :
SICV622


Tgt Ion:162 Resp: 652980
Ion Ratio Lower Upper
162 100
164 33.3 27.5 41.3
127 40.2 37.1 55.7

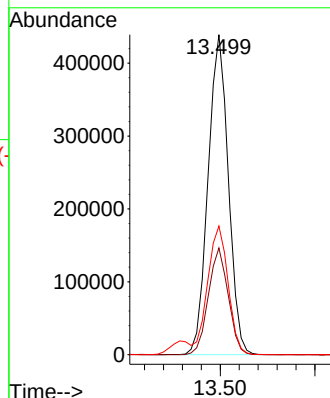

#45
2-Nitroaniline
Concen: 19.642 ng/ul
RT: 13.693 min Scan# 1820
Delta R.T. 0.012 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13

Tgt Ion: 65 Resp: 223117
Ion Ratio Lower Upper
65 100
92 66.0 77.9 116.9#
138 97.1 81.5 122.3



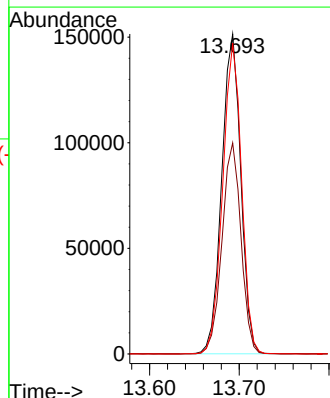





#47
Dimethylphthalate
Concen: 17.645 ng/ul
RT: 14.081 min Scan# 1884
Delta R.T. 0.012 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13




Instrument :
BNA_P
ClientSampleId :
SICV622


Tgt Ion:163 Resp: 921943
Ion Ratio Lower Upper
163 100
194 4.3 4.1 6.1
164 9.8 11.3 16.9#



#48
2,6-Dinitrotoluene
Concen: 20.928 ng/ul
RT: 14.187 min Scan# 1904
Delta R.T. 0.012 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13

Tgt Ion:165 Resp: 201130
Ion Ratio Lower Upper
165 100
89 59.6 51.7 77.5
121 21.2 18.3 27.5









#50
Acenaphthylene
Concen: 17.722 ng/ul
RT: 14.346 min Scan# 1929
Delta R.T. 0.012 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13




Instrument :
BNA_P
ClientSampleId :
SICV622


Tgt Ion:152 Resp: 1124797
Ion Ratio Lower Upper
152 100
151 19.8 18.3 27.5
153 13.0 11.0 16.6

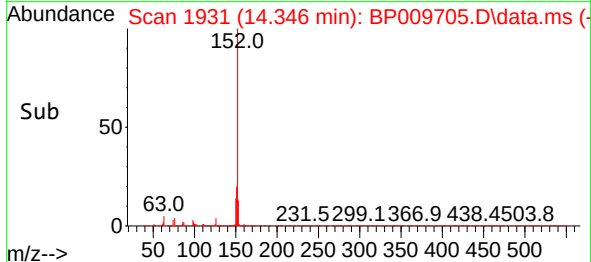

#51
3-Nitroaniline
Concen: 20.651 ng/ul
RT: 14.516 min Scan# 1960
Delta R.T. 0.012 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13

Tgt Ion:138 Resp: 206330
Ion Ratio Lower Upper
138 100
108 12.8 15.8 23.8#
92 122.8 117.1 175.7


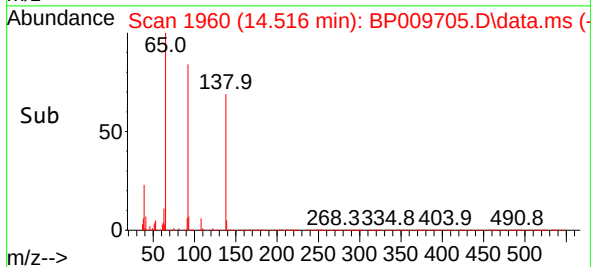

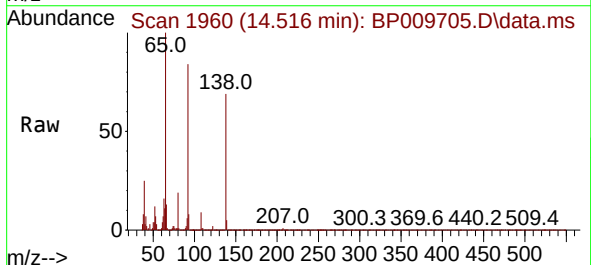




#52
Acenaphthene
Concen: 17.178 ng/ul
RT: 14.687 min Scan# 1989
Delta R.T. 0.012 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13




Instrument :
BNA_P
ClientSampleId :
SICV622


Tgt Ion:153 Resp: 713847
Ion Ratio Lower Upper
153 100
152 46.2 34.3 51.5
154 89.3 70.0 105.0

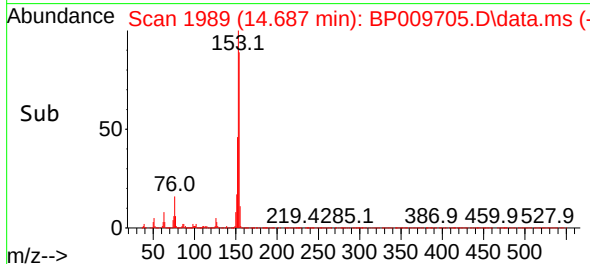

#53
2,4-Dinitrophenol
Concen: 18.964 ng/ul
RT: 14.716 min Scan# 1994
Delta R.T. 0.012 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13

Tgt Ion:184 Resp: 110164
Ion Ratio Lower Upper
184 100
63 71.6 34.6 52.0#
154 71.0 57.7 86.5


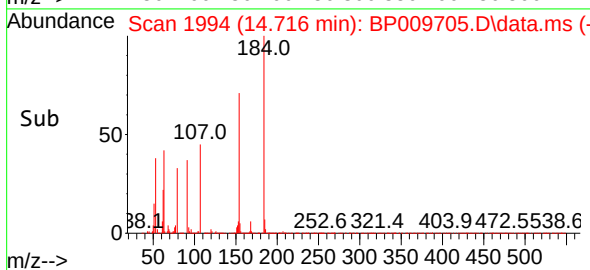

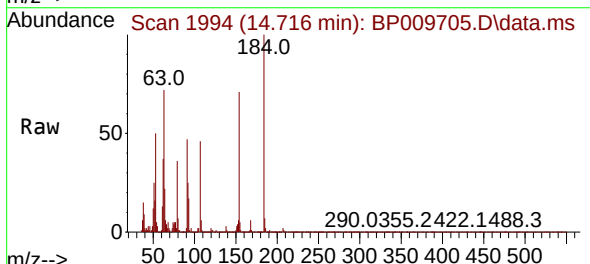




#55
4-Nitrophenol
Concen: 17.939 ng/ul
RT: 14.816 min Scan# 2011
Delta R.T. 0.012 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13




Instrument :
BNA_P
ClientSampleId :
SICV622


Tgt Ion:109 Resp: 162578
Ion Ratio Lower Upper
109 100
139 114.8 61.4 92.2#
65 128.2 65.3 97.9#



#56
Dibenzofuran
Concen: 17.191 ng/ul
RT: 15.022 min Scan# 2046
Delta R.T. 0.012 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13

Tgt Ion:168 Resp: 1051448
Ion Ratio Lower Upper
168 100
139 38.6 30.1 45.1



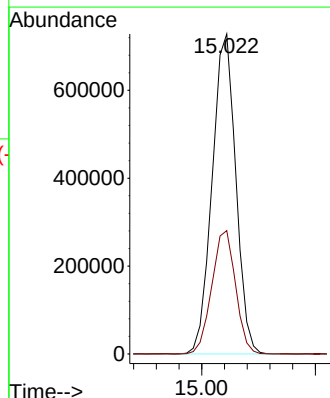





#57
2,4-Dinitrotoluene
Concen: 19.721 ng/ul
RT: 14.975 min Scan# 2038
Delta R.T. 0.012 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13




Instrument :
BNA_P
ClientSampleId :
SICV622


Tgt Ion:165 Resp: 278312
Ion Ratio Lower Upper
165 100
63 45.6 29.5 44.3#
182 3.3 2.8 4.2

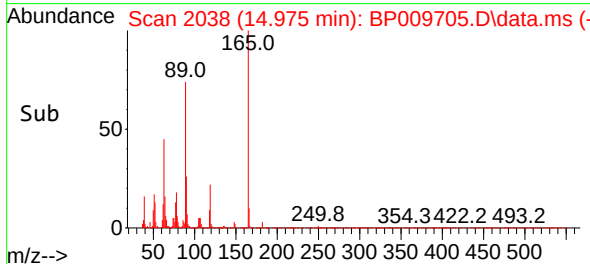

#58
2,3,4,6-Tetrachlorophenol
Concen: 18.523 ng/ul
RT: 15.245 min Scan# 2084
Delta R.T. 0.012 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13

Tgt Ion:232 Resp: 246450
Ion Ratio Lower Upper
232 100
131 41.0 25.4 38.2#
130 2.4 4.2 6.2#
166 29.7 28.1 42.1


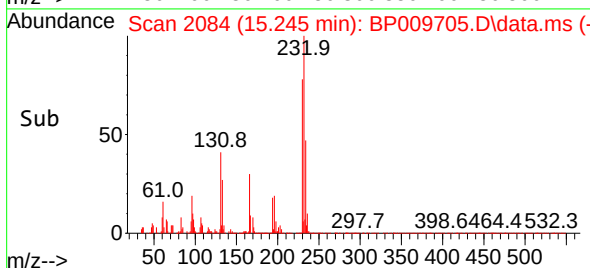
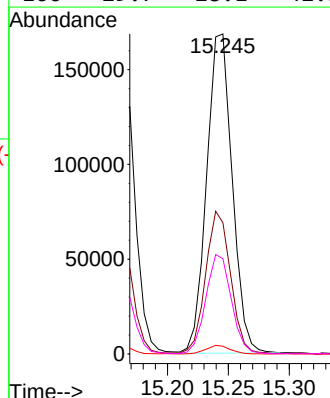
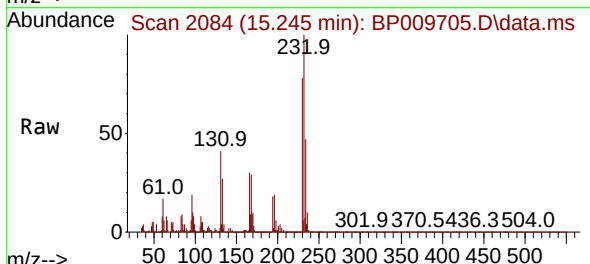




#59
Diethylphthalate
Concen: 17.696 ng/ul
RT: 15.445 min Scan# 2118
Delta R.T. 0.012 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13




Instrument :
BNA_P
ClientSampleId :
SICV622


Tgt Ion:149 Resp: 956865
Ion Ratio Lower Upper
149 100
177 22.2 22.0 33.0
150 12.9 10.2 15.2



#61
Fluorene
Concen: 17.145 ng/ul
RT: 15.669 min Scan# 2156
Delta R.T. 0.006 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13

Tgt Ion:166 Resp: 863735
Ion Ratio Lower Upper
166 100
165 95.7 70.3 105.5
167 13.8 9.5 14.3









#62
4-Chlorophenyl-phenylether
Concen: 17.090 ng/ul
RT: 15.669 min Scan# 2156
Delta R.T. 0.012 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13




Instrument :
BNA_P
ClientSampleId :
SICV622


Tgt Ion:204 Resp: 457773
Ion Ratio Lower Upper
204 100
206 33.6 27.6 41.4
141 58.8 46.6 69.8



#63
4-Nitroaniline
Concen: 22.205 ng/ul
RT: 15.681 min Scan# 2158
Delta R.T. 0.018 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13

Tgt Ion:138 Resp: 222208
Ion Ratio Lower Upper
138 100
92 52.0 41.6 62.4
108 88.0 97.6 146.4#









#66
4,6-Dinitro-2-methylphenol
Concen: 18.309 ng/ul
RT: 15.740 min Scan# 2166
Delta R.T. 0.012 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13




Instrument :
BNA_P
ClientSampleId :
SICV622


Tgt Ion:198 Resp: 170161
Ion Ratio Lower Upper
198 100
182 4.1 6.0 9.0#
77 26.7 17.7 26.5#

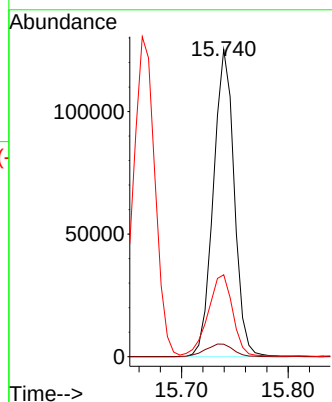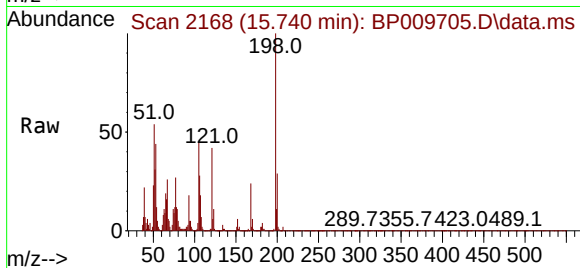

#67
N-Nitrosodiphenylamine
Concen: 17.332 ng/ul
RT: 15.875 min Scan# 2191
Delta R.T. 0.012 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13

Tgt Ion:169 Resp: 783093
Ion Ratio Lower Upper
169 100
168 64.5 48.3 72.5
167 34.0 29.6 44.4









#68
4-Bromophenyl-phenylether
Concen: 17.029 ng/ul
RT: 16.563 min Scan# 21
Delta R.T. 0.012 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13




Instrument :
BNA_P
ClientSampleId :
SICV622


Tgt Ion:248 Resp: 290943
Ion Ratio Lower Upper
248 100
250 97.4 79.4 119.0
141 73.6 67.2 100.8

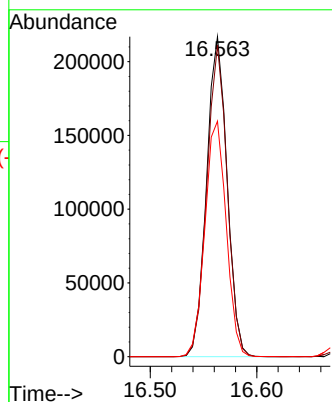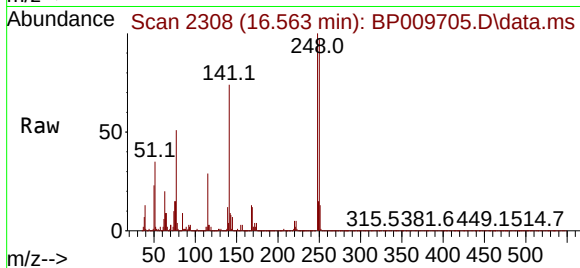

#69
Hexachlorobenzene
Concen: 16.752 ng/ul
RT: 16.681 min Scan# 2328
Delta R.T. 0.012 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13

Tgt Ion:284 Resp: 329090
Ion Ratio Lower Upper
284 100
142 31.6 19.2 28.8#
249 32.1 27.4 41.2


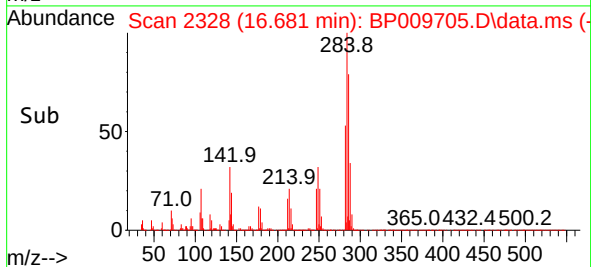
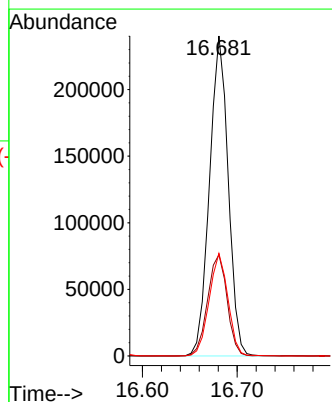
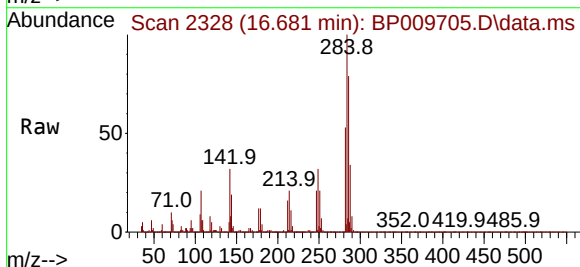




#70
Atrazine
Concen: 16.270 ng/ul
RT: 16.834 min Scan# 21
Delta R.T. 0.012 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13




Instrument :
BNA_P
ClientSampleId :
SICV622


Tgt Ion:200 Resp: 303412
Ion Ratio Lower Upper
200 100
173 27.7 19.2 28.8
215 49.6 32.2 48.4#

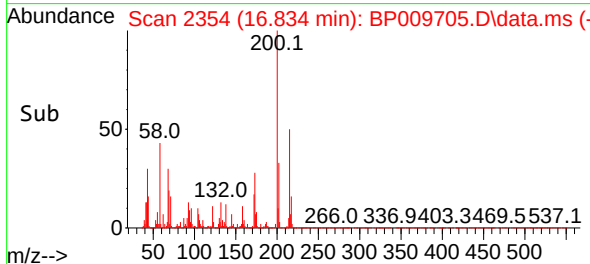

#71
Pentachlorophenol
Concen: 16.792 ng/ul
RT: 17.022 min Scan# 2386
Delta R.T. 0.012 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13

Tgt Ion:266 Resp: 223295
Ion Ratio Lower Upper
266 100
264 63.9 57.3 85.9
268 66.4 65.7 98.5

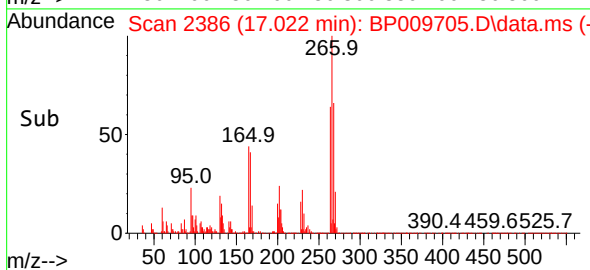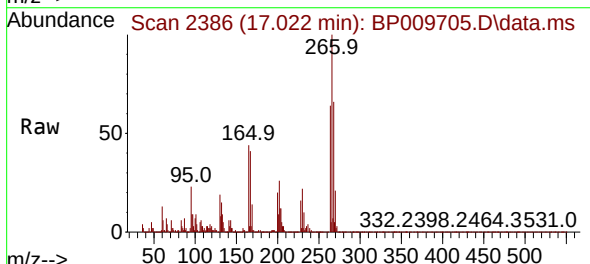



#72

Phenanthrene

Concen: 17.116 ng/ul

RT: 17.416 min Scan# 2453

Delta R.T. 0.012 min

Lab File: BP009705.D

Acq: 07 Apr 2022 19:13

Instrument :

BNA_P

ClientSampleId :

SICV622





Tgt Ion:178 Resp: 1442027

Ion Ratio Lower Upper

178 100

179 15.4 11.7 17.5

176 18.8 14.5 21.7

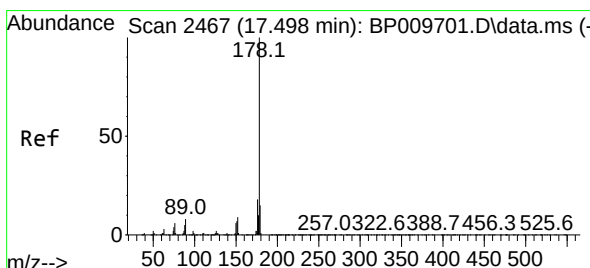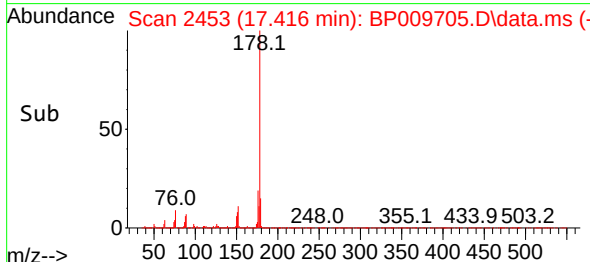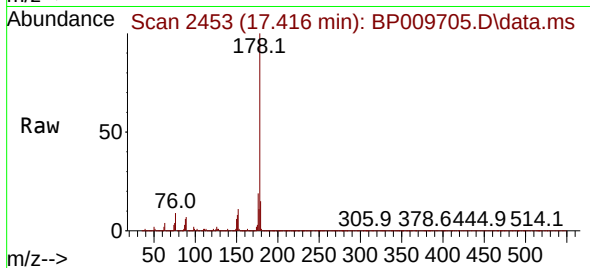

#74

Anthracene

Concen: 17.117 ng/ul

RT: 17.510 min Scan# 2469

Delta R.T. 0.012 min

Lab File: BP009705.D

Acq: 07 Apr 2022 19:13




Tgt Ion:178 Resp: 1462112


Ion Ratio Lower Upper

178 100

179 15.6 12.3 18.5

176 18.1 13.4 20.2

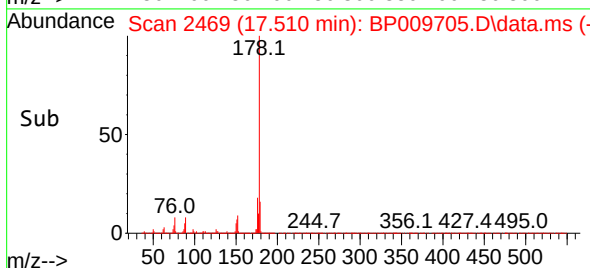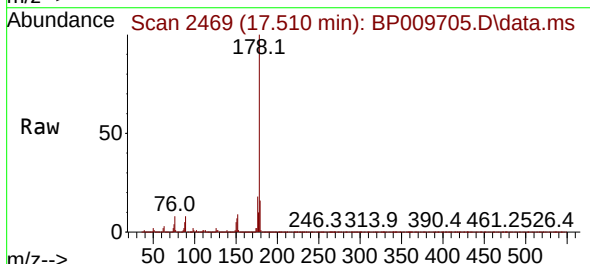



#75

1,2,3,4-Tetrachlorobenzene

Concen: 16.497 ng/uL

RT: 13.422 min Scan# 1774

Delta R.T. 0.006 min

Lab File: BP009705.D

Acq: 07 Apr 2022 19:13

Instrument :

BNA_P

ClientSampleId :

SICV622





Tgt Ion:216 Resp: 376440

Ion Ratio Lower Upper

216 100

214 77.9 50.4 75.6#

218 47.5 35.2 52.8

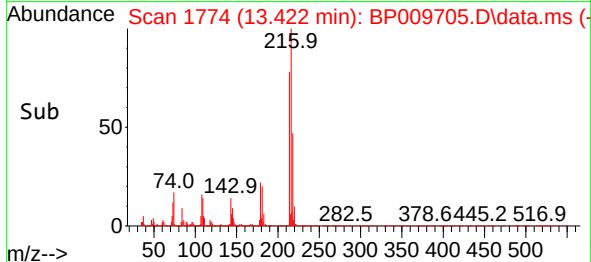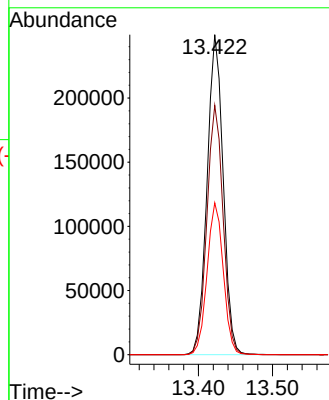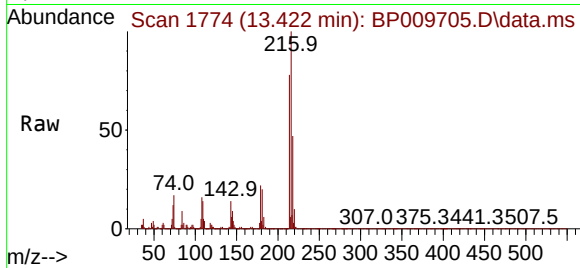

#76

Pentachlorobenzene

Concen: 16.886 ng/uL

RT: 14.945 min Scan# 2033

Delta R.T. 0.012 min

Lab File: BP009705.D

Acq: 07 Apr 2022 19:13




Tgt Ion:250 Resp: 375590


Ion Ratio Lower Upper

250 100

248 61.5 43.5 65.3

252 62.7 46.5 69.7


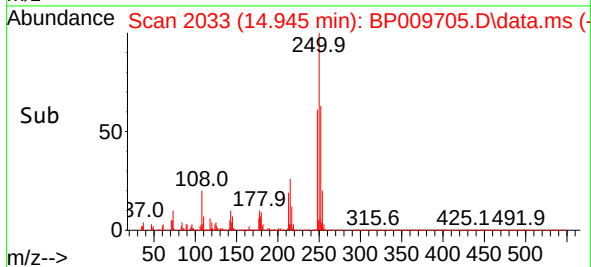
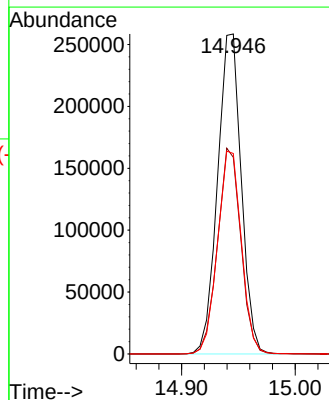
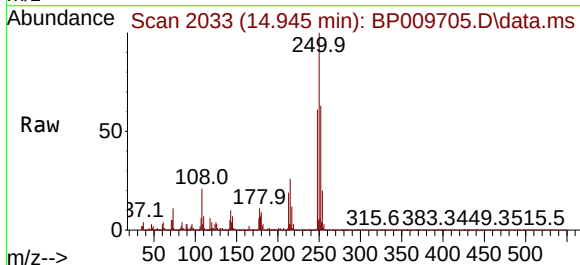




#77
 Carbazole
 Concen: 17.531 ng/ul
 RT: 17.769 min Scan# 2513
 Delta R.T. 0.012 min
 Lab File: BP009705.D
 Acq: 07 Apr 2022 19:13




Instrument :
 BNA_P
 ClientSampleId :
 SICV622


Tgt Ion:167 Resp: 1353260
 Ion Ratio Lower Upper
 167 100
 166 21.5 15.8 23.8
 139 13.3 8.3 12.5#

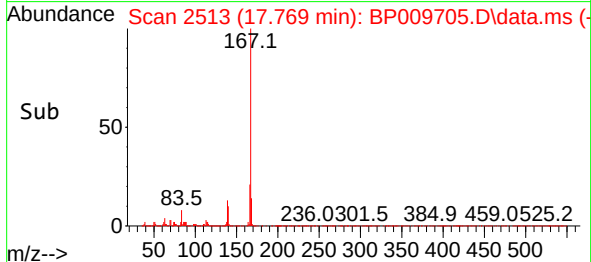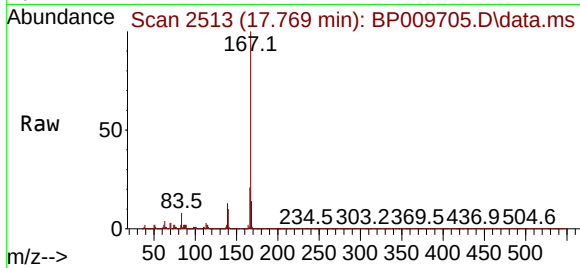

#78
 Di-n-butylphthalate
 Concen: 18.088 ng/ul
 RT: 18.334 min Scan# 2609
 Delta R.T. 0.012 min
 Lab File: BP009705.D
 Acq: 07 Apr 2022 19:13

Tgt Ion:149 Resp: 1716930
 Ion Ratio Lower Upper
 149 100
 150 8.9 9.6 14.4#
 104 5.1 6.2 9.4#


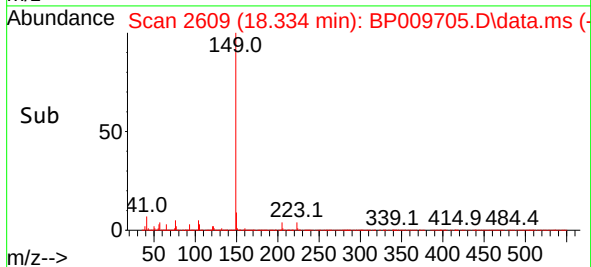

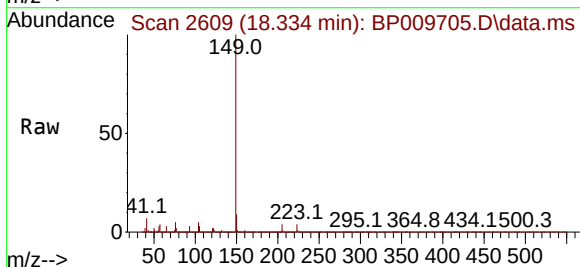




#80
Fluoranthene
Concen: 16.955 ng/ul
RT: 19.375 min Scan# 21
Delta R.T. 0.012 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13




Instrument :
BNA_P
ClientSampleId :
SICV622


Tgt Ion:202 Resp: 1794946
Ion Ratio Lower Upper
202 100
101 9.5 9.6 14.4#
100 7.5 6.3 9.5

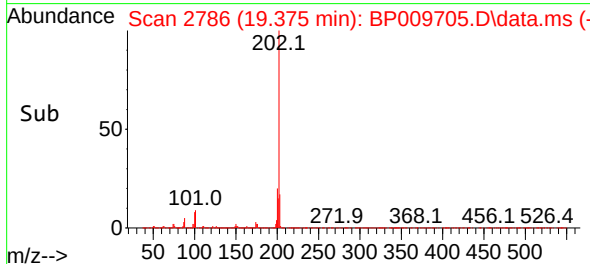

#82
Pyrene
Concen: 17.055 ng/ul
RT: 19.728 min Scan# 2846
Delta R.T. 0.012 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13

Tgt Ion:202 Resp: 1830639
Ion Ratio Lower Upper
202 100
101 11.2 10.6 15.8
100 9.3 9.8 14.6#

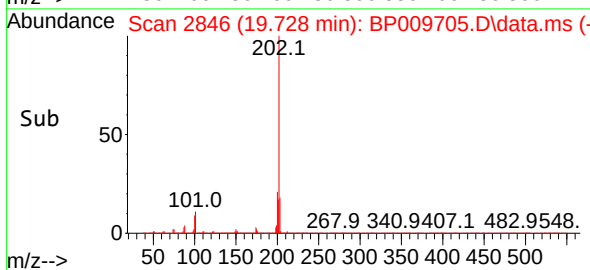



#83

Butylbenzylphthalate

Concen: 18.237 ng/ul

RT: 20.604 min Scan# 2995

Delta R.T. 0.012 min

Lab File: BP009705.D

Acq: 07 Apr 2022 19:13

Instrument :

BNA_P

ClientSampleId :

SICV622





Tgt Ion:149 Resp: 803001

Ion Ratio Lower Upper

149 100

91 69.5 71.1 106.7#

206 22.3 28.8 43.2#

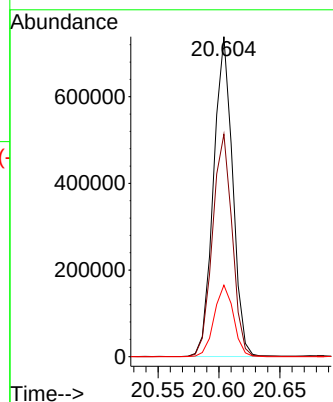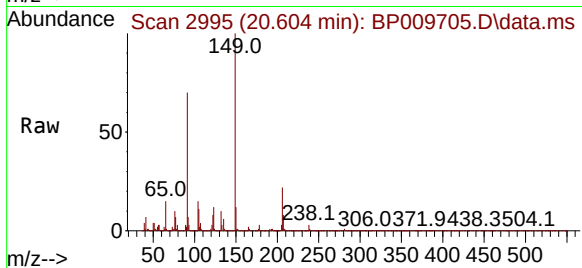

#84

3,3'-Dichlorobenzidine

Concen: 20.260 ng/ul

RT: 21.369 min Scan# 3125

Delta R.T. 0.012 min

Lab File: BP009705.D

Acq: 07 Apr 2022 19:13




Tgt Ion:252 Resp: 727035


Ion Ratio Lower Upper

252 100

254 63.8 49.8 74.6

126 9.2 4.3 6.5#



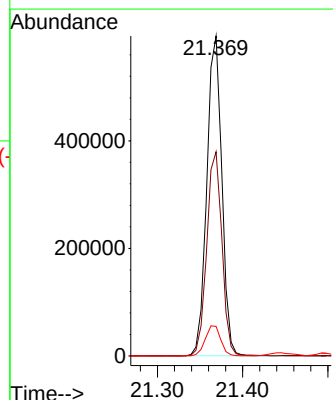
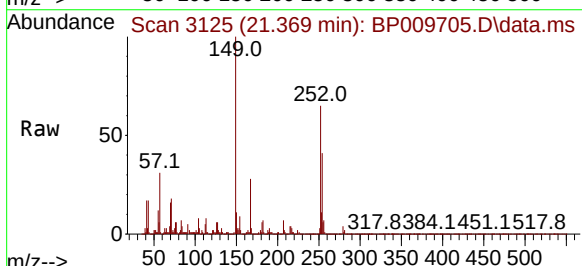




#85
 Benzo(a)anthracene
 Concen: 17.656 ng/ul
 RT: 21.439 min Scan# 3137
 Delta R.T. 0.012 min
 Lab File: BP009705.D
 Acq: 07 Apr 2022 19:13




Instrument :
 BNA_P
 ClientSampleId :
 SICV622


Tgt Ion:228 Resp: 1884937
 Ion Ratio Lower Upper
 228 100
 229 19.7 18.2 27.2
 226 26.0 22.8 34.2

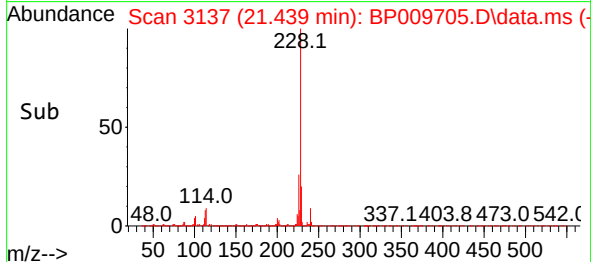

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 18.053 ng/ul
 RT: 21.375 min Scan# 3126
 Delta R.T. 0.012 min
 Lab File: BP009705.D
 Acq: 07 Apr 2022 19:13

Tgt Ion:149 Resp: 1195674
 Ion Ratio Lower Upper
 149 100
 167 28.1 32.8 49.2#
 279 5.2 5.6 8.4#

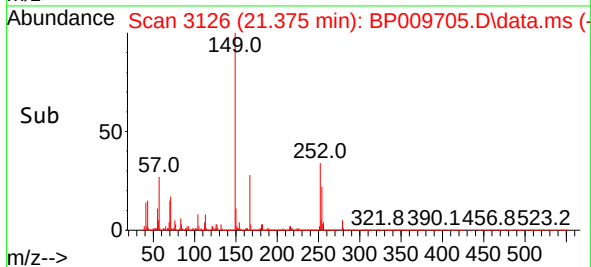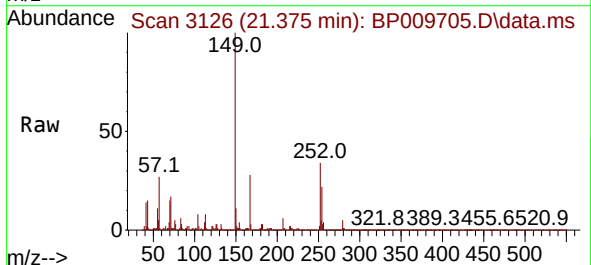



#87

Chrysene

Concen: 16.829 ng/ul

RT: 21.498 min Scan# 3145

Delta R.T. 0.012 min

Lab File: BP009705.D

Acq: 07 Apr 2022 19:13

Instrument :

BNA_P

ClientSampleId :

SICV622





Tgt Ion:228 Resp: 1733458

Ion Ratio Lower Upper

228 100

226 29.3 22.7 34.1

229 20.2 15.2 22.8

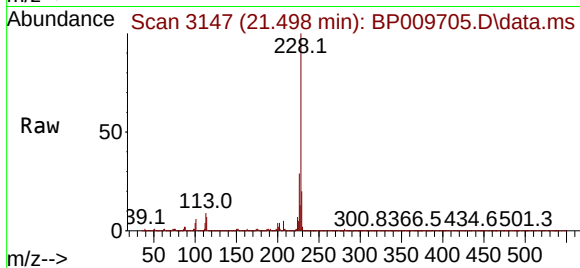

#89

Di-n-octyl phthalate

Concen: 17.543 ng/ul




RT: 22.333 min Scan# 3289


Delta R.T. 0.012 min

Lab File: BP009705.D

Acq: 07 Apr 2022 19:13

Tgt Ion:149 Resp: 1960353









#90
Benzo(b)fluoranthene
Concen: 17.301 ng/ul
RT: 23.180 min Scan# 3431
Delta R.T. 0.012 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13




Instrument :
BNA_P
ClientSampleId :
SICV622


Tgt Ion:252 Resp: 1833308
Ion Ratio Lower Upper
252 100
253 22.0 17.4 26.0
125 8.6 7.3 10.9

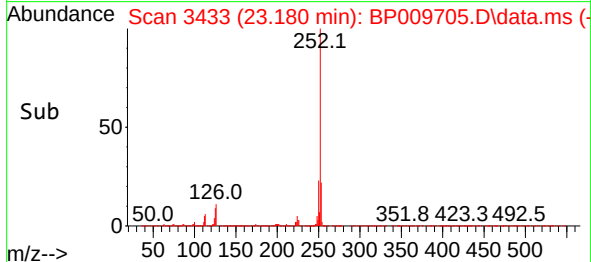

#91
Benzo(k)fluoranthene
Concen: 17.766 ng/ul
RT: 23.233 min Scan# 3442
Delta R.T. 0.018 min
Lab File: BP009705.D
Acq: 07 Apr 2022 19:13

Tgt Ion:252 Resp: 1717883
Ion Ratio Lower Upper
252 100
253 21.8 17.9 26.9
125 8.0 5.1 7.7#

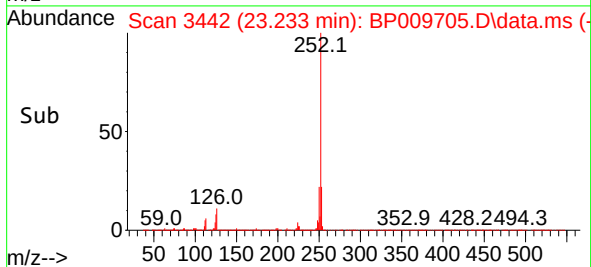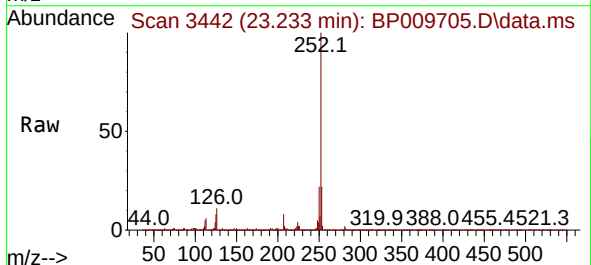



#93

Benzo(a)pyrene

Concen: 17.272 ng/ul

RT: 23.833 min Scan# 3

Delta R.T. 0.018 min

Lab File: BP009705.D

Acq: 07 Apr 2022 19:13

Instrument :

BNA_P

ClientSampleId :

SICV622





Tgt Ion:252 Resp: 1696480

Ion Ratio Lower Upper

252 100

253 21.6 17.5 26.3

125 8.8 6.4 9.6

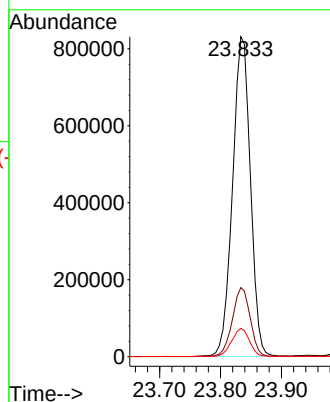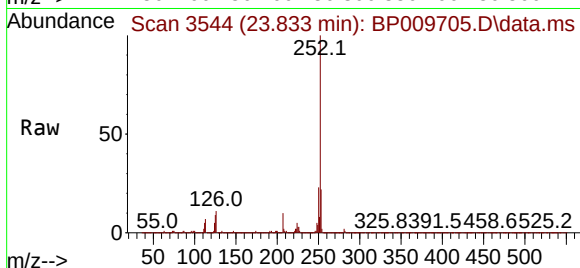

#94

Indeno(1,2,3-cd)pyrene

Concen: 16.310 ng/ul

RT: 26.551 min Scan# 4006

Delta R.T. 0.036 min

Lab File: BP009705.D

Acq: 07 Apr 2022 19:13




Tgt Ion:276 Resp: 1675195


Ion Ratio Lower Upper

276 100

138 18.5 12.3 18.5#

277 25.3 19.3 28.9





#95

Dibenzo(a,h)anthracene

Concen: 16.617 ng/ul

RT: 26.568 min Scan# 4009

Delta R.T. 0.036 min

Lab File: BP009705.D

Acq: 07 Apr 2022 19:13

Instrument :

BNA_P

ClientSampleId :

SICV622





Tgt Ion:278 Resp: 1480006

Ion Ratio Lower Upper

278 100

139 13.0 6.6 10.0#

279 23.5 18.4 27.6

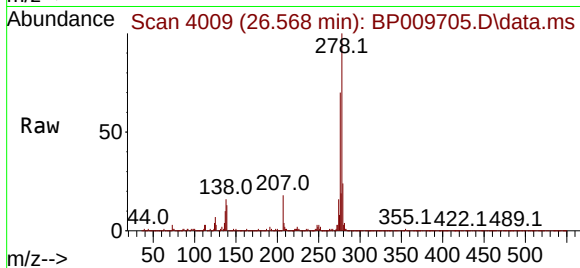

#96

Benzo(g,h,i)perylene

Concen: 16.530 ng/ul

RT: 27.345 min Scan# 4141

Delta R.T. 0.036 min

Lab File: BP009705.D

Acq: 07 Apr 2022 19:13

Tgt Ion:276 Resp: 1399927

Ion Ratio Lower Upper

276 100

138 16.7 11.6 17.4

277 24.1 15.9 23.9#

