

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040821\
 Data File : BP005237.D
 Acq On : 08 Apr 2021 15:51
 Operator : CG/JU
 Sample : M1955-01RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SIDEWALK-206RE

Integration Parameters: rteint.p

Integrator: RTE

Smoother: ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP005237.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.234	190	195	204	rVB	342520	445891	31.37%	6.904%
2	4.834	291	297	303	rVB	538428	740319	52.08%	11.463%
3	5.287	370	374	382	rVB	35211	50813	3.57%	0.787%
4	6.869	637	643	656	rVB	170122	273826	19.26%	4.240%
5	7.687	775	782	788	rBV	85741	127619	8.98%	1.976%
6	8.846	972	979	987	rBV	205777	335928	23.63%	5.201%
7	10.475	1247	1256	1266	rBV	99154	162098	11.40%	2.510%
8	12.963	1672	1679	1685	rBV	497562	731698	51.47%	11.329%
9	13.246	1719	1727	1732	rVB3	11379	18590	1.31%	0.288%
10	13.810	1817	1823	1828	rBV	14016	19576	1.38%	0.303%
11	14.346	1906	1914	1921	rBV	144138	212811	14.97%	3.295%
12	15.740	2142	2151	2160	rBV5	12320	29487	2.07%	0.457%
13	17.110	2378	2384	2390	rBV	187420	258695	18.20%	4.005%
14	17.522	2451	2454	2463	rVB2	8156	14223	1.00%	0.220%
15	18.010	2532	2537	2542	rBV	62917	91989	6.47%	1.424%
16	18.081	2545	2549	2553	rVB	14345	22658	1.59%	0.351%
17	19.134	2724	2728	2732	rBV	14686	18952	1.33%	0.293%
18	19.251	2744	2748	2755	rBV5	24312	36768	2.59%	0.569%
19	19.486	2786	2788	2794	rVB	13012	18812	1.32%	0.291%
20	19.686	2817	2822	2832	rBV	1192939	1421466	100.00%	22.009%
21	20.363	2934	2937	2943	rVB	35335	40235	2.83%	0.623%
22	20.928	3029	3033	3040	rVB3	88797	135333	9.52%	2.095%
23	20.992	3040	3044	3050	rBV	100612	117762	8.28%	1.823%
24	21.122	3063	3066	3074	rVB	63138	96369	6.78%	1.492%
25	21.210	3075	3081	3085	rBV2	317642	432623	30.43%	6.699%
26	21.245	3085	3087	3093	rVB	48623	55877	3.93%	0.865%
27	22.004	3213	3216	3221	rVB	48410	55519	3.91%	0.860%
28	22.792	3346	3350	3354	rBV2	42967	72913	5.13%	1.129%
29	23.486	3462	3468	3475	rVB2	218060	419652	29.52%	6.498%




Sum of corrected areas: 6458502

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040821\
Data File : BP005237.D
Acq On : 08 Apr 2021 15:51
Operator : CG/JU
Sample : M1955-01RE
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SIDEWALK-206RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

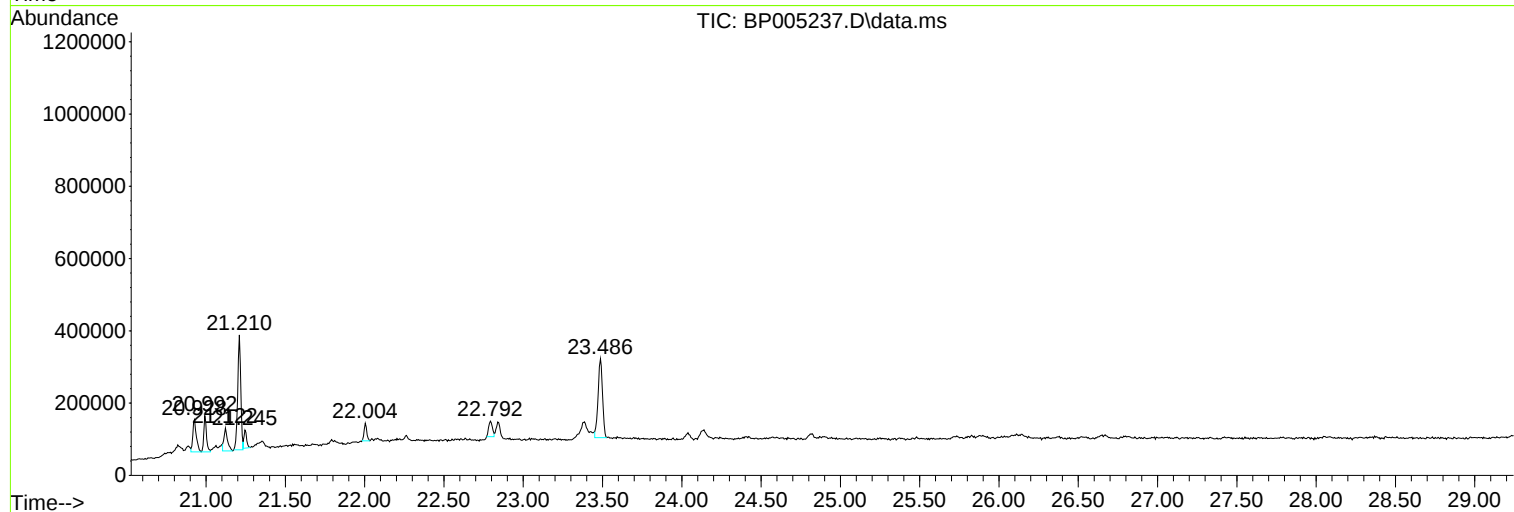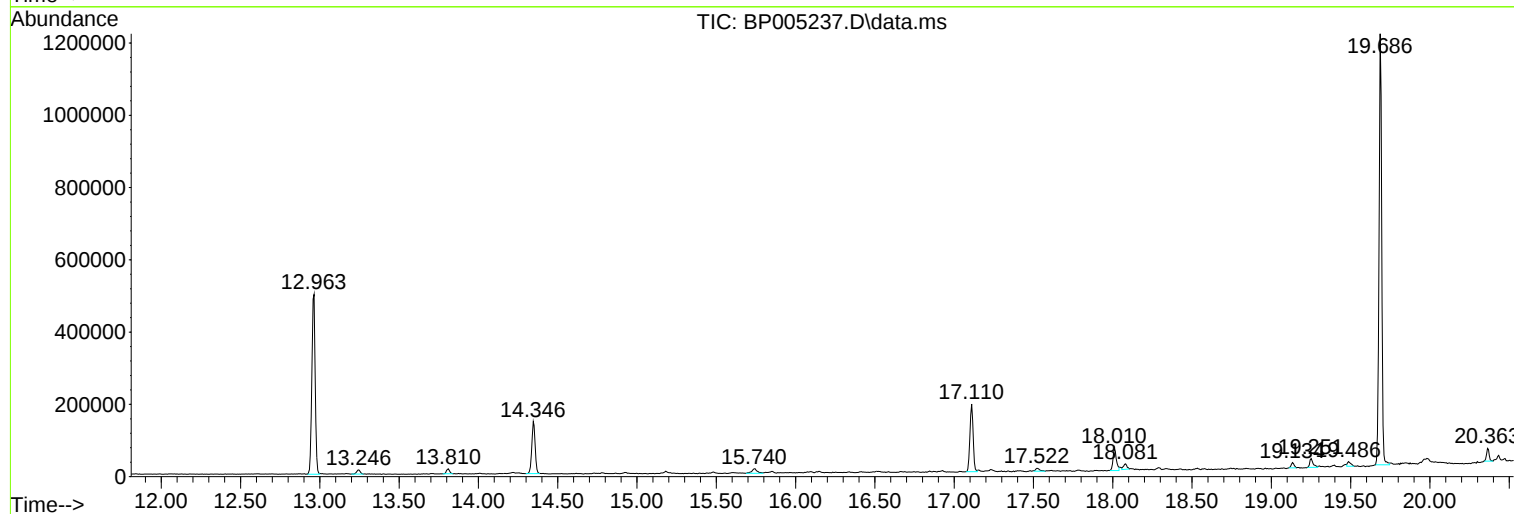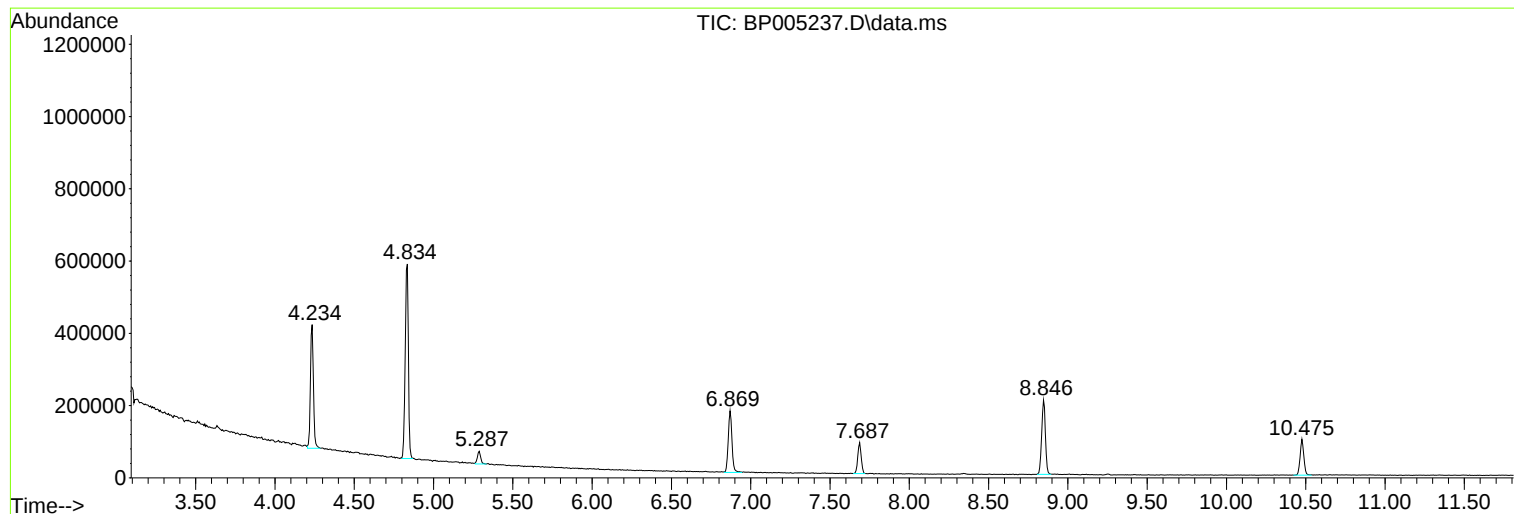

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040821\
Data File : BP005237.D
Acq On : 08 Apr 2021 15:51
Operator : CG/JU
Sample : M1955-01RE
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SIDEWALK-206RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040821\
Data File : BP005237.D
Acq On : 08 Apr 2021 15:51
Operator : CG/JU
Sample : M1955-01RE
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SIDEWALK-206RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------