
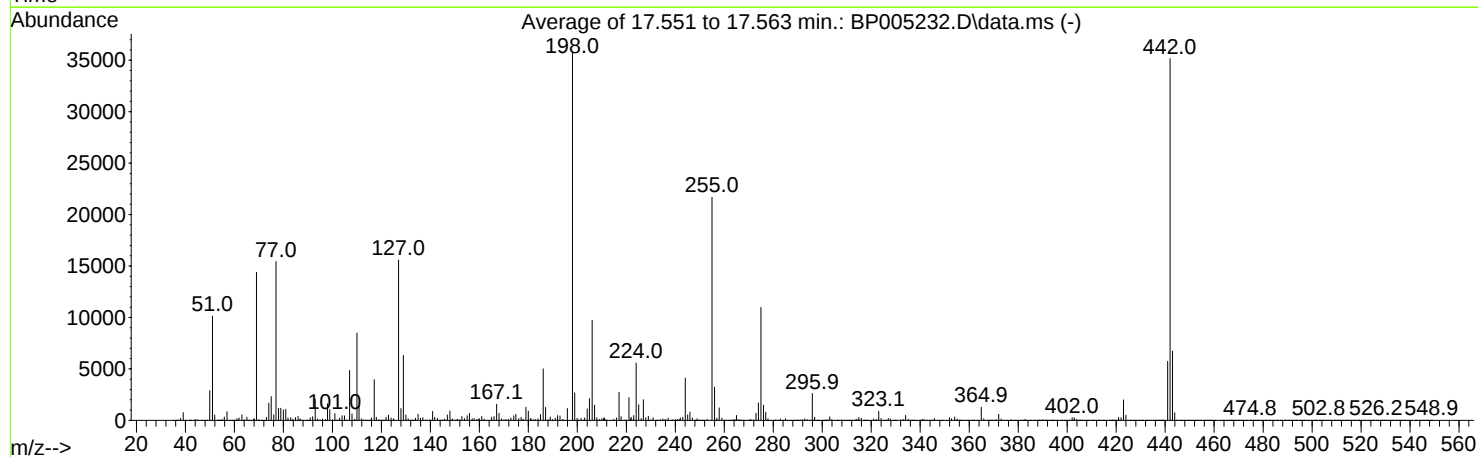


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040821\
 Data File : BP005232.D
 Acq On : 08 Apr 2021 11:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 06 12:33:08 2021

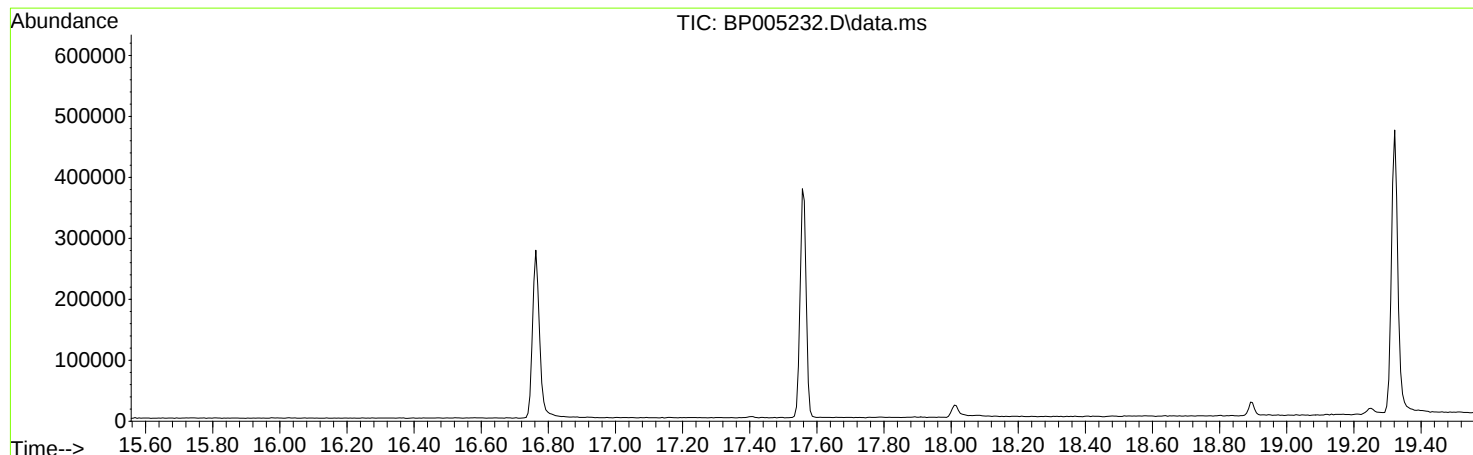

AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.3	10132	PASS
68	69	0.00	2	1.1	154	PASS
69	198	0.00	100	40.3	14391	PASS
70	69	0.00	2	0.4	64	PASS
127	198	10	80	43.6	15582	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	35749	PASS
199	198	5	9	7.5	2669	PASS
275	198	10	60	30.7	10974	PASS
365	198	1	100	3.6	1274	PASS
441	198	0.01	100	16.1	5741	PASS
442	442	100	100	100.0	35155	PASS
443	442	15	24	19.2	6739	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/8/2021	BNA_P	<u>BP005232.D</u>
Compound Name	Response	Retention Time
DDT	152137	20.52
DDD	3686	20.09
DDE	508	19.59
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4194	156331	2.68

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040821\
 Data File : BP005232.D
 Acq On : 08 Apr 2021 11:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Apr 08 12:47:47 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 06 12:33:08 2021
 Response via : Initial Calibration

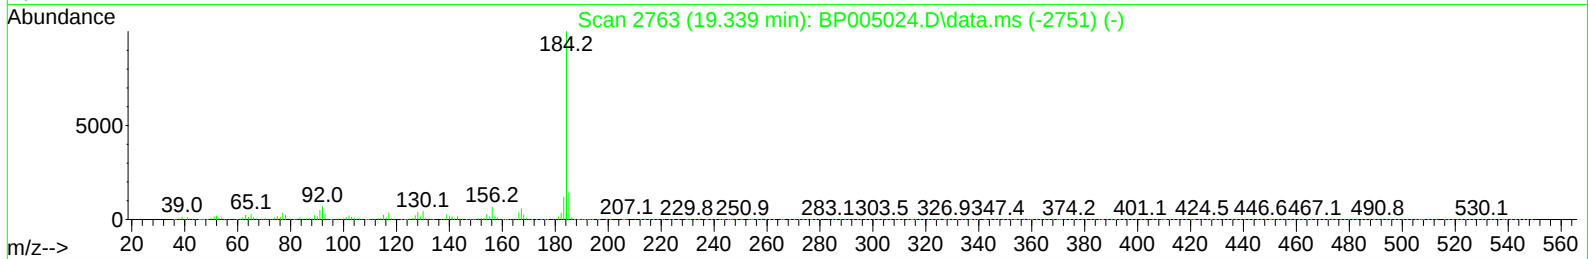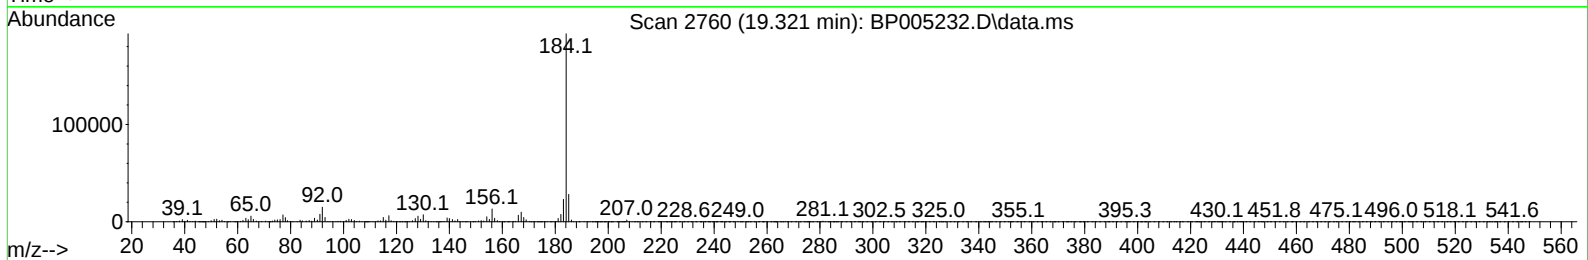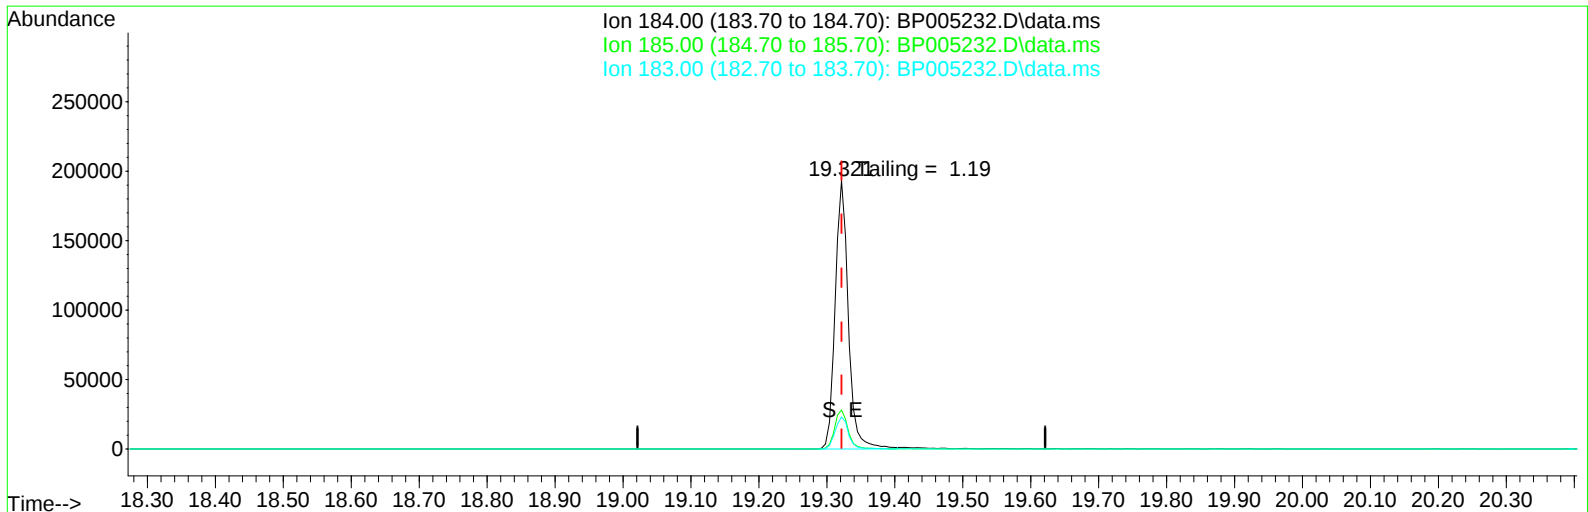

TIC: BP005232.D\data.ms

(77) Benzidine

19.321min (-0.000) 258020.06 ng




response 260407

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.58
183.00	12.00	11.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040821\
 Data File : BP005232.D
 Acq On : 08 Apr 2021 11:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Apr 08 12:47:47 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 06 12:33:08 2021
 Response via : Initial Calibration

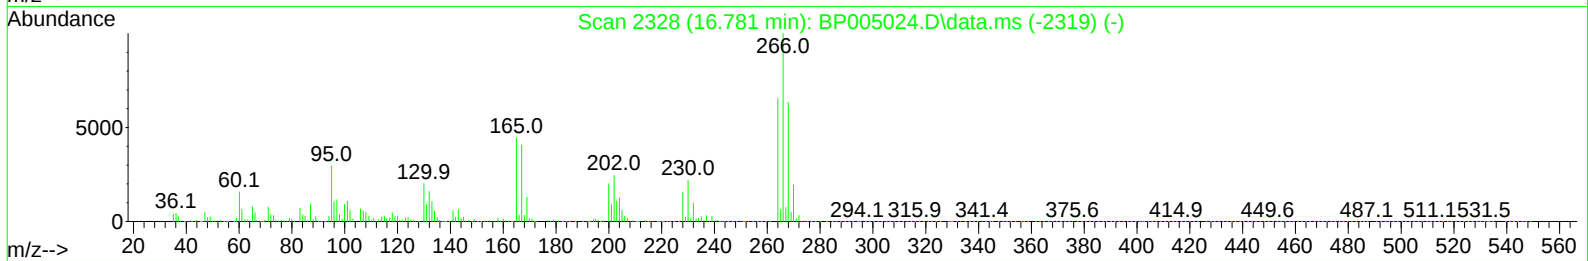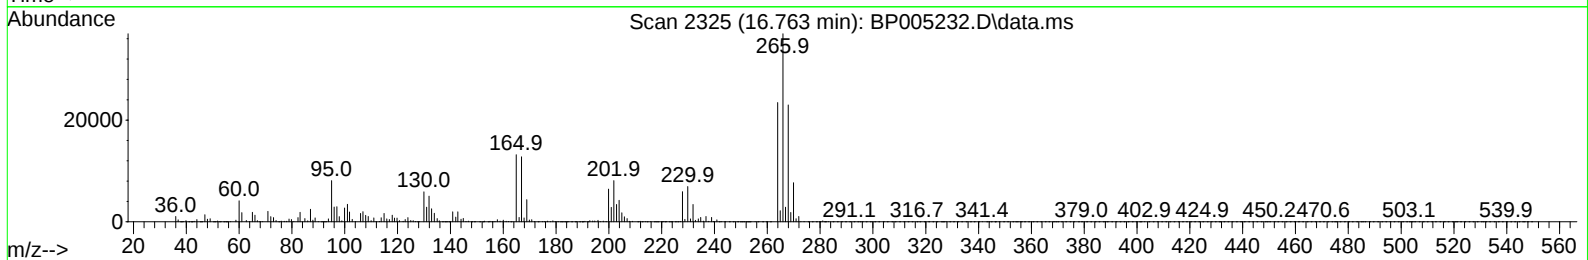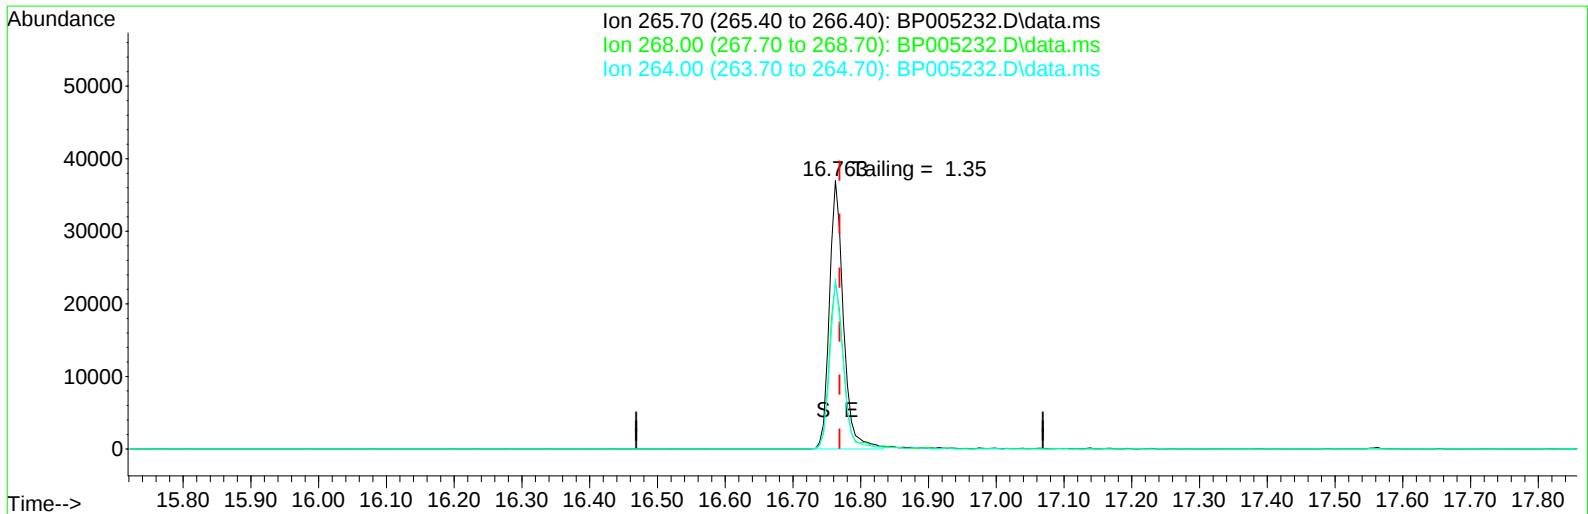

TIC: BP005232.D\data.ms

(70) Pentachlorophenol (C)

16.763min (-0.006) 1038276.17 ng

response 53593

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	62.10
264.00	63.30	63.40
0.00	0.00	0.00