
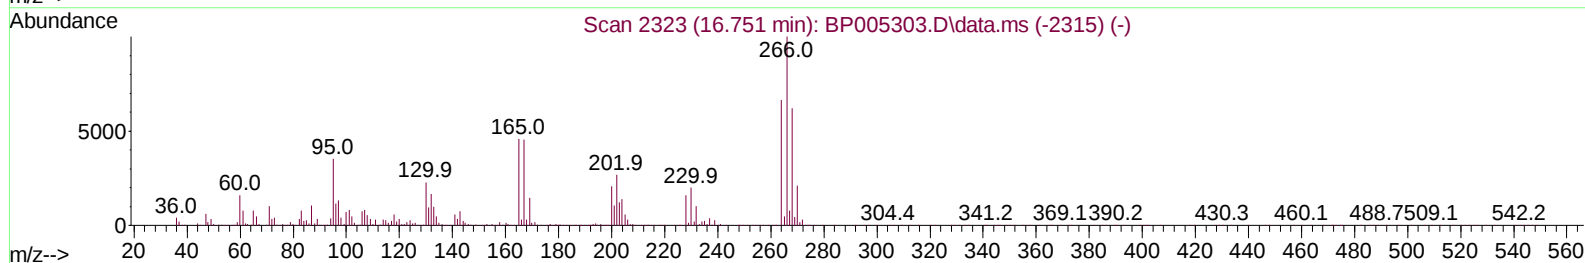
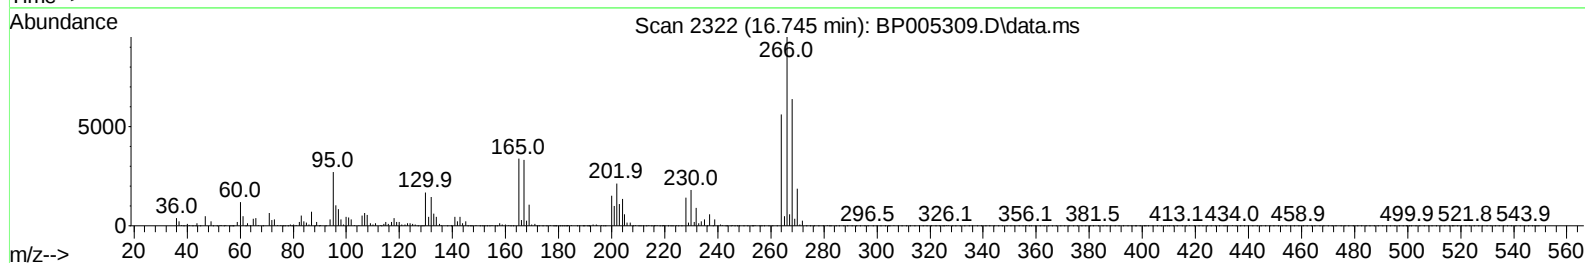


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041621\
Data File : BP005309.D
Acq On : 16 Apr 2021 09:33
Operator : CG/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 16 10:53:21 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 16 06:09:06 2021
Response via : Initial Calibration

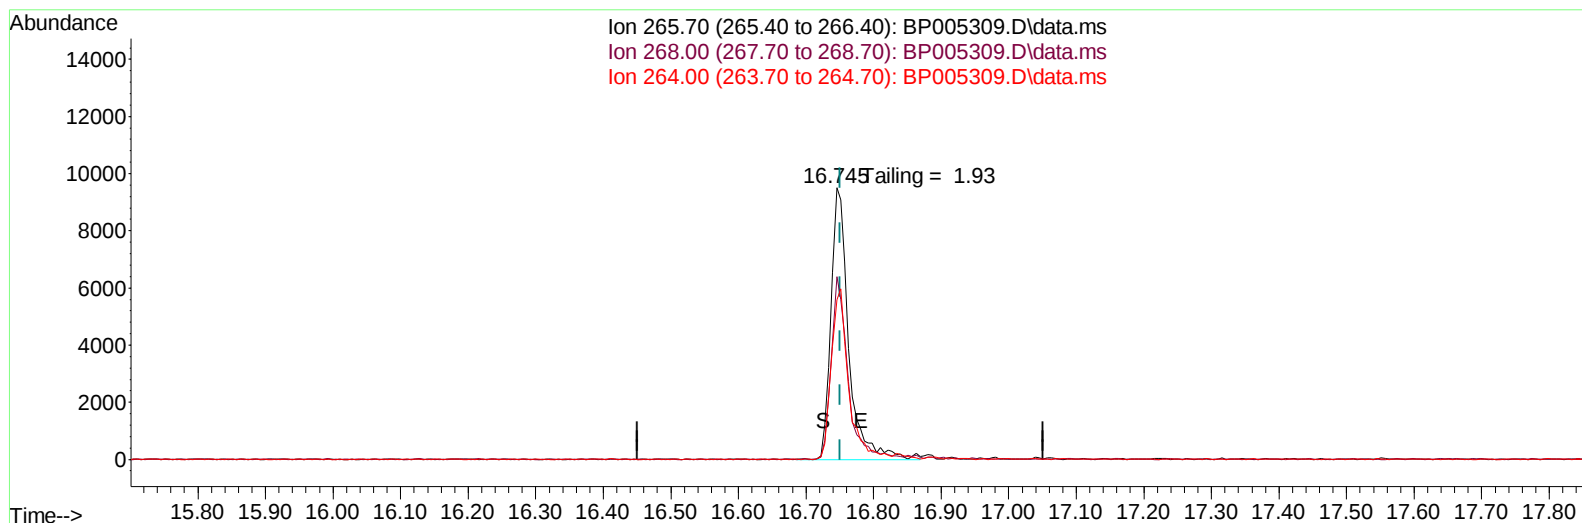

TIC: BP005309.D\data.ms

(70) Pentachlorophenol (C)




16.745min (-0.006) 526343.41 ng

response 17249

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	67.21
264.00	66.60	58.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041621\
Data File : BP005309.D
Acq On : 16 Apr 2021 09:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 16 10:53:21 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 16 06:09:06 2021
Response via : Initial Calibration

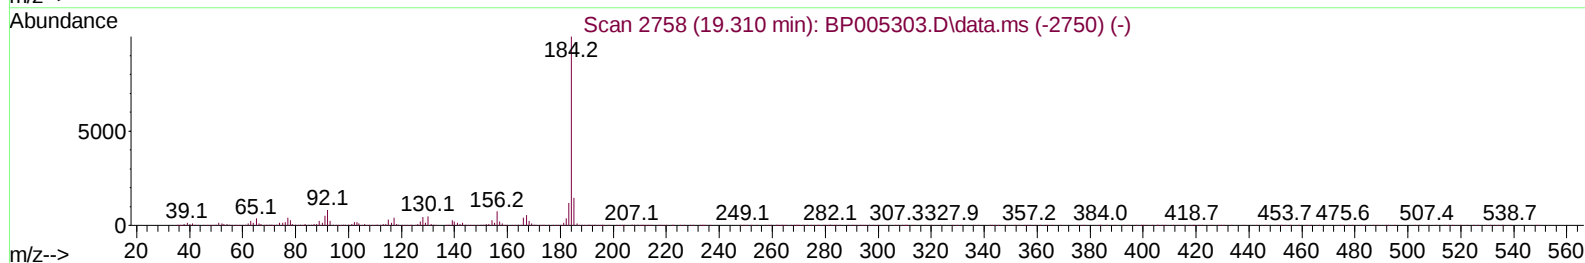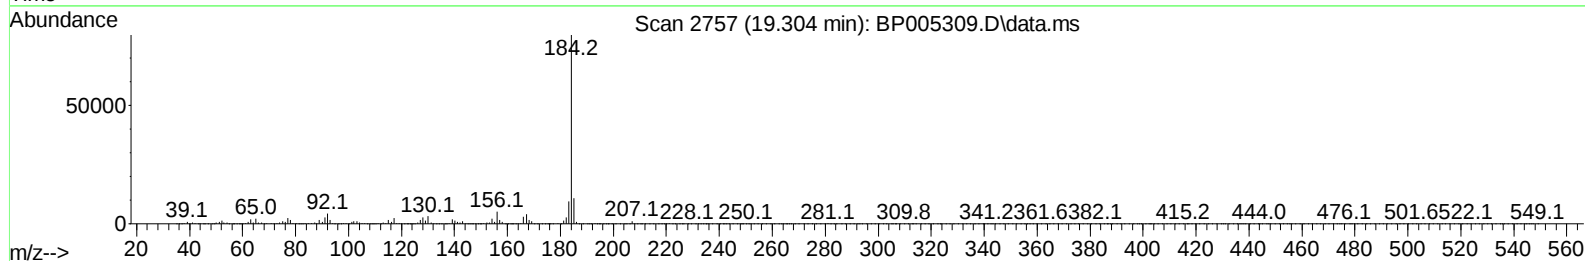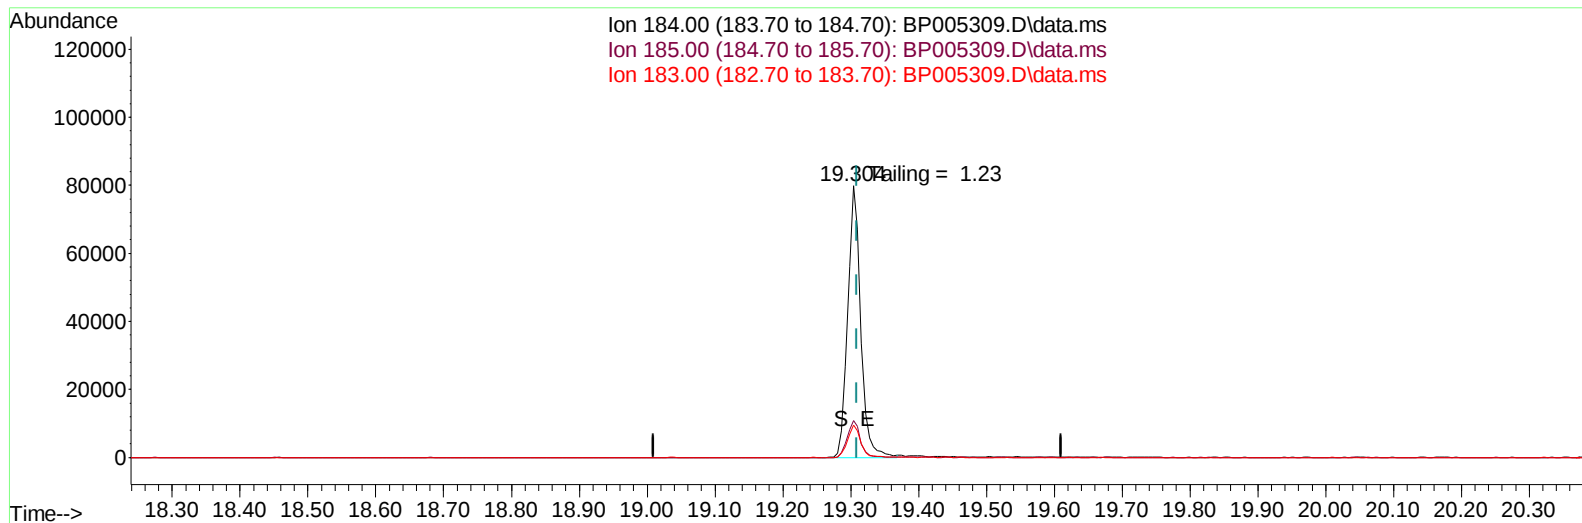

TIC: BP005309.D\data.ms

(77) Benzidine**19.304min (-0.006) 1725685.55 ng****response 106712**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.69
183.00	12.10	11.85
0.00	0.00	0.00