

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041621\
 Data File : BP005311.D
 Acq On : 16 Apr 2021 10:42
 Operator : CG/JU
 Sample : PB135754BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB135754BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP005311.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.263	366	370	377	rVB	545163	737870	53.33%	12.851%
2	6.852	635	640	652	rVB	484703	738797	53.40%	12.867%
3	7.663	773	778	789	rVB2	109730	178168	12.88%	3.103%
4	8.822	968	975	984	rBV	250808	419016	30.29%	7.298%
5	10.457	1246	1253	1264	rBV	74959	127588	9.22%	2.222%
6	12.940	1668	1675	1687	rBV	551272	698209	50.47%	12.160%
7	14.328	1905	1911	1922	rBV	113167	168392	12.17%	2.933%
8	15.833	2160	2167	2187	rBV	304116	443622	32.06%	7.726%
9	17.092	2374	2381	2389	rBV	125201	178991	12.94%	3.117%
10	19.669	2814	2819	2831	rBV	1285332	1383546	100.00%	24.096%
11	21.198	3074	3079	3088	rBV	266588	332099	24.00%	5.784%
12	23.462	3458	3464	3473	rVB	176818	335557	24.25%	5.844%




Sum of corrected areas: 5741855

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041621\
Data File : BP005311.D
Acq On : 16 Apr 2021 10:42
Operator : CG/JU
Sample : PB135754BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB135754BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

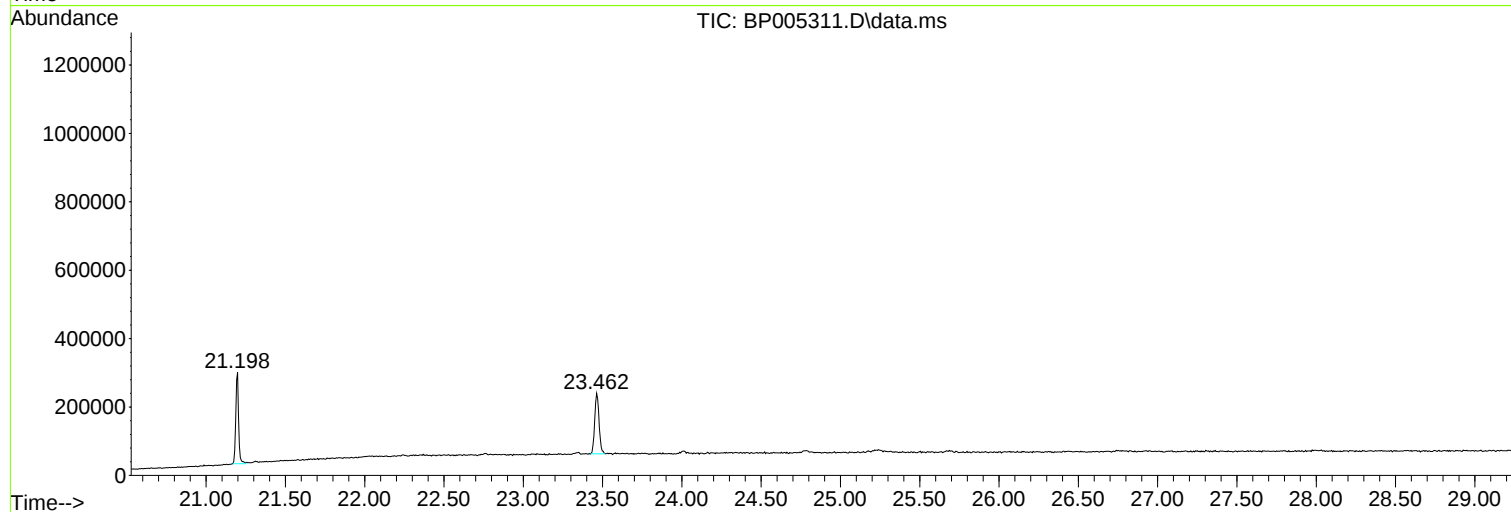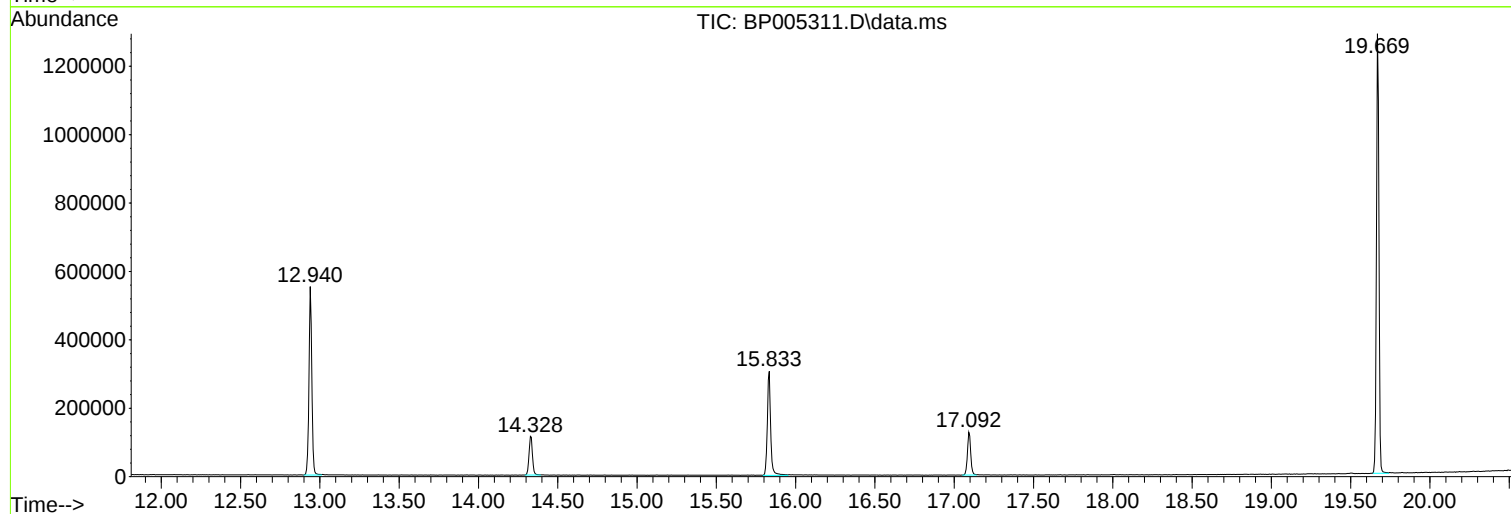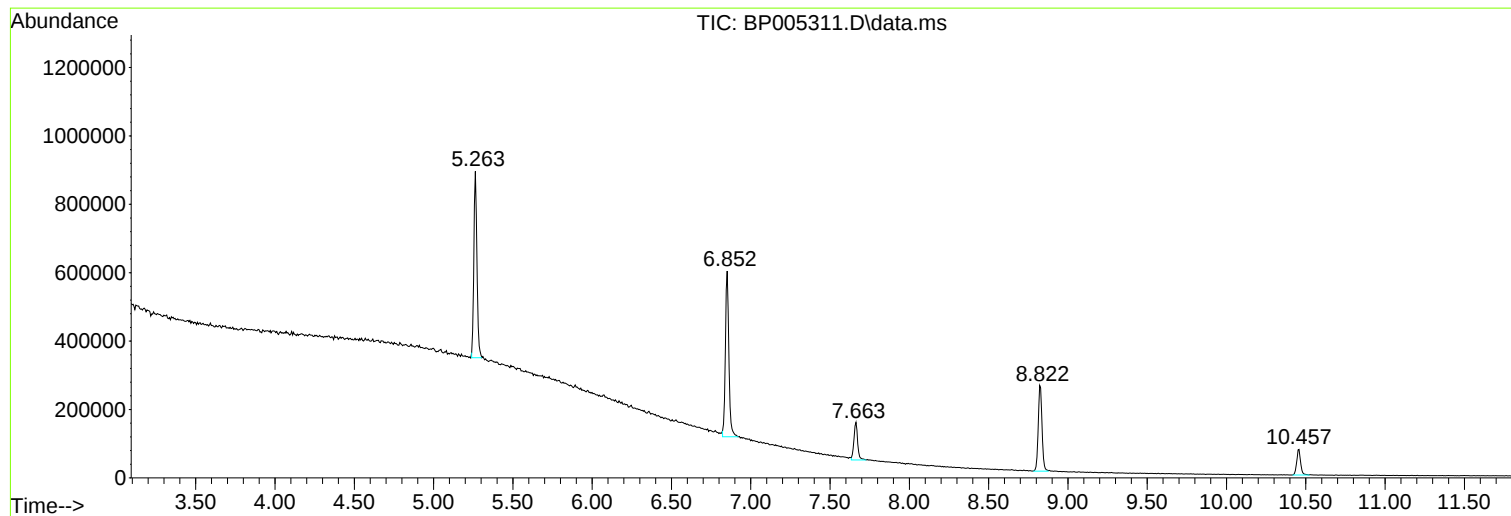

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041621\
Data File : BP005311.D
Acq On : 16 Apr 2021 10:42
Operator : CG/JU
Sample : PB135754BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB135754BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041621\
Data File : BP005311.D
Acq On : 16 Apr 2021 10:42
Operator : CG/JU
Sample : PB135754BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB135754BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------