
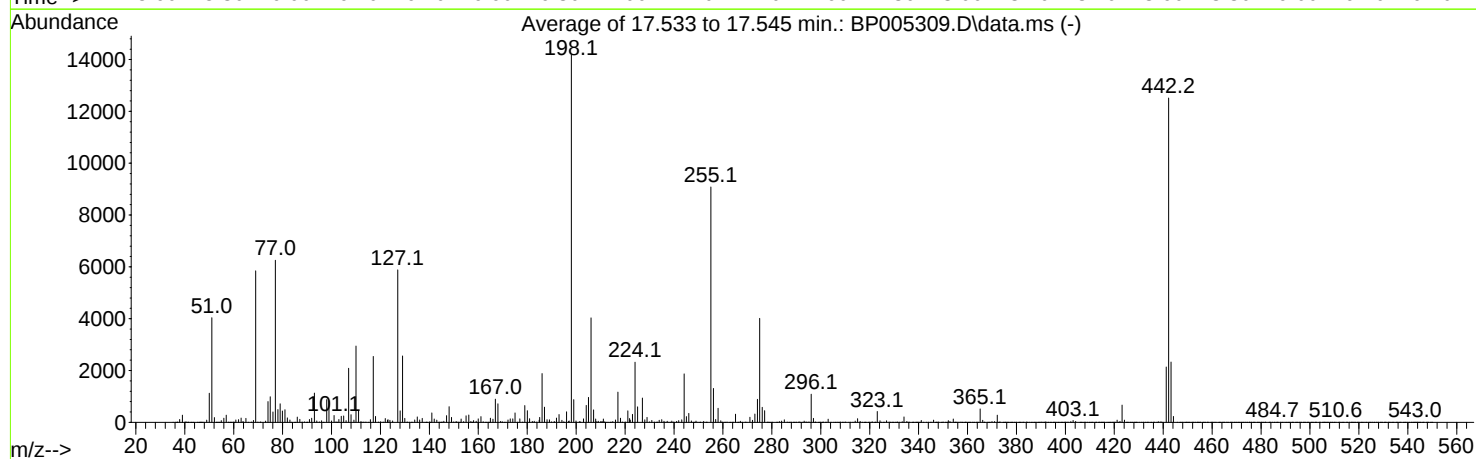


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041621\
 Data File : BP005309.D
 Acq On : 16 Apr 2021 09:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 16 11:02:58 2021

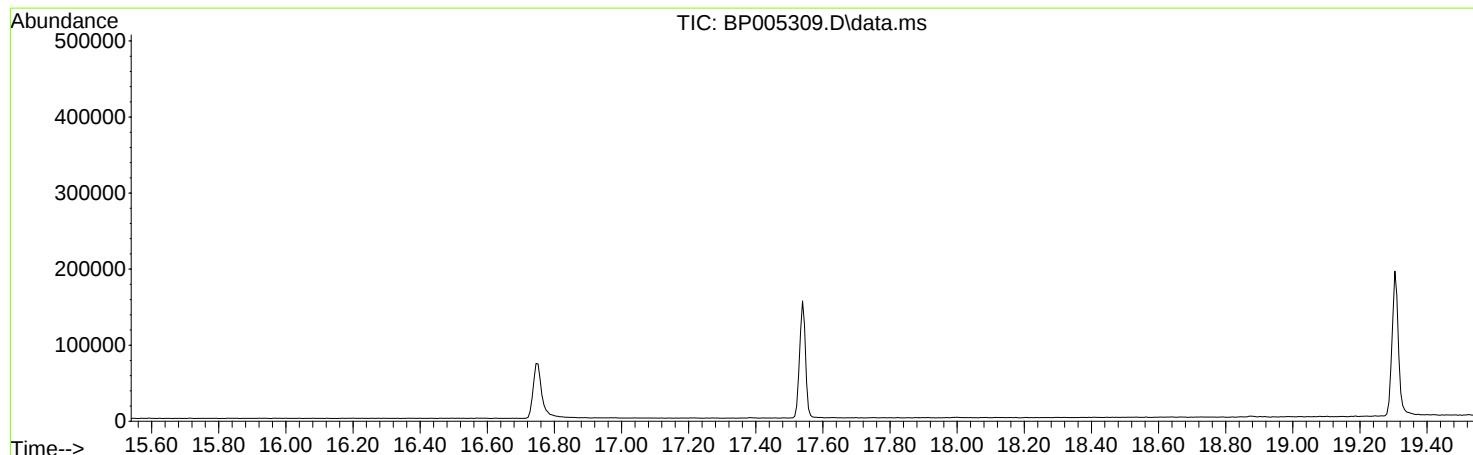

AutoFind: Scans 2456, 2457, 2458; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.5	4039	PASS
68	69	0.00	2	1.3	74	PASS
69	198	0.00	100	41.2	5844	PASS
70	69	0.00	2	0.2	13	PASS
127	198	10	80	41.5	5883	PASS
197	198	0.00	2	0.4	54	PASS
198	198	100	100	100.0	14193	PASS
199	198	5	9	6.2	879	PASS
275	198	10	60	28.3	4012	PASS
365	198	1	100	3.7	519	PASS
441	198	0.01	100	15.0	2136	PASS
442	442	100	100	100.0	12512	PASS
443	442	15	24	18.6	2329	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/16/2021	BNA_P	<u>BP005309.D</u>
Compound Name	Response	Retention Time
DDT	75575	20.504
DDD	752	20.075
DDE	122	19.575
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
874	76449	1.14

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041621\
Data File : BP005309.D
Acq On : 16 Apr 2021 09:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 16 10:53:21 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 16 06:09:06 2021
Response via : Initial Calibration

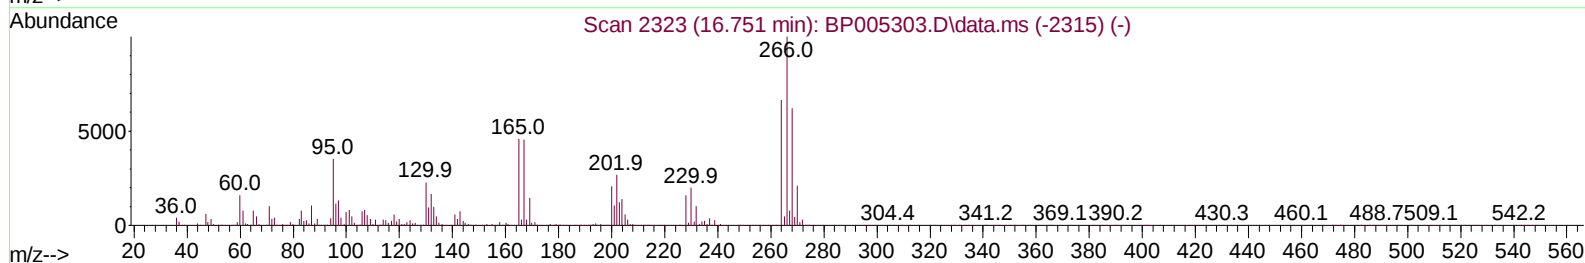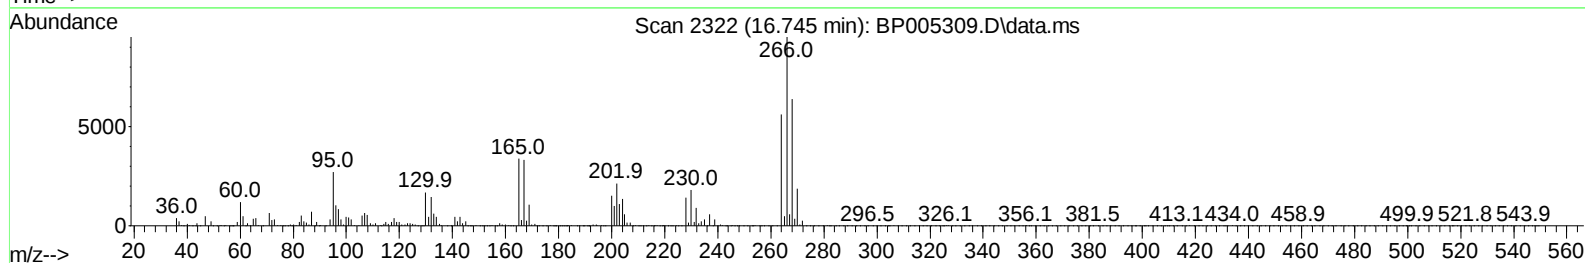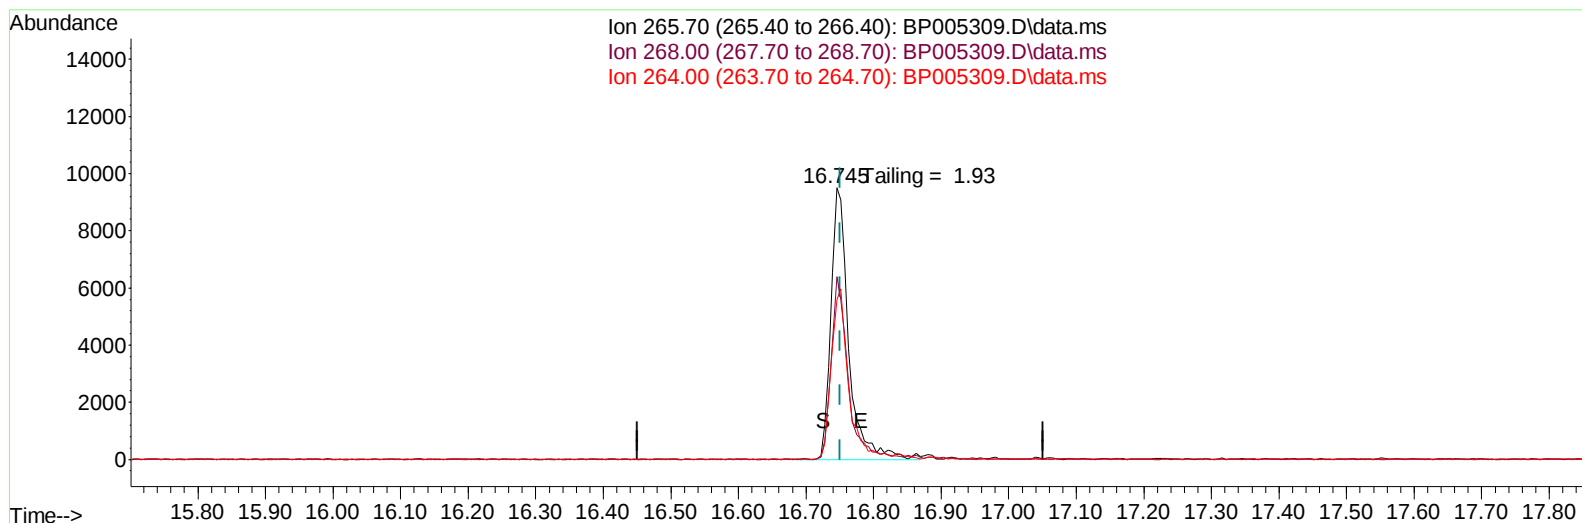

TIC: BP005309.D\data.ms

(70) Pentachlorophenol (C)

16.745min (-0.006) 526343.41 ng




response 17249

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	67.21
264.00	66.60	58.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041621\
Data File : BP005309.D
Acq On : 16 Apr 2021 09:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 16 10:53:21 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 16 06:09:06 2021
Response via : Initial Calibration

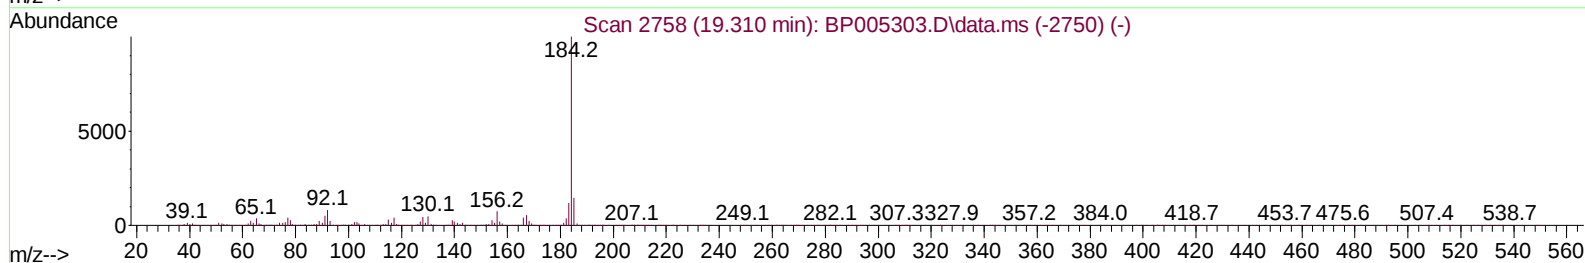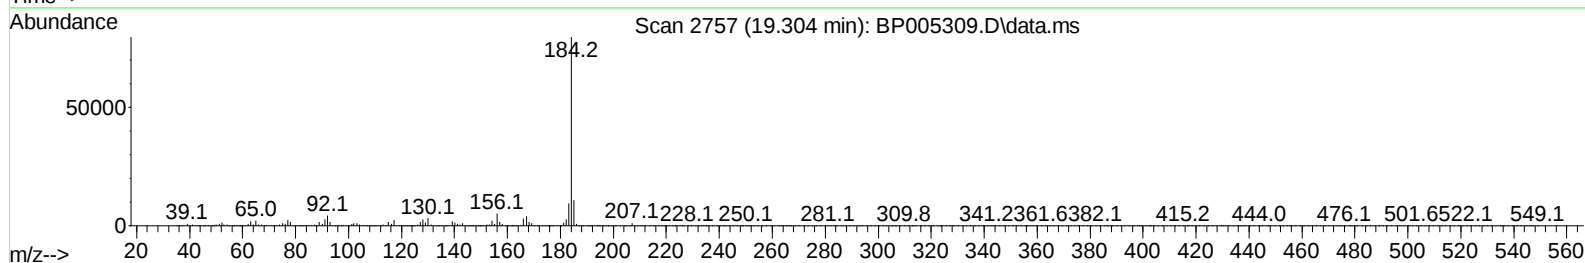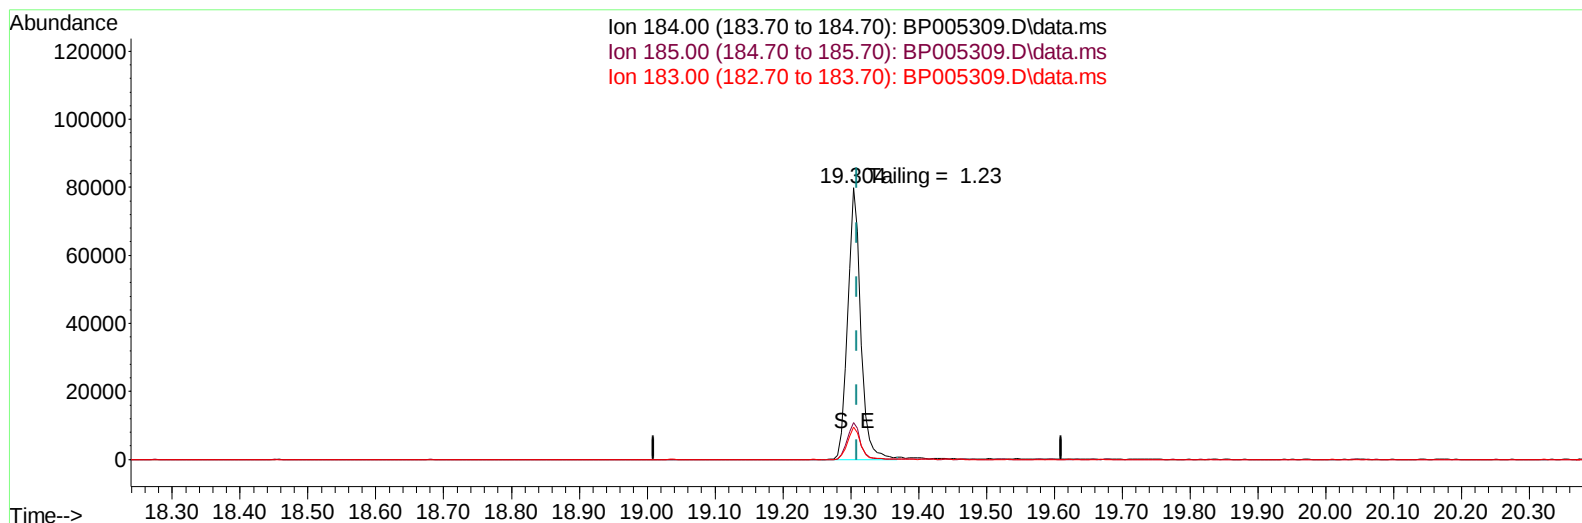

TIC: BP005309.D\data.ms

(77) Benzidine

19.304min (-0.006) 1725685.55 ng

response 106712

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.69
183.00	12.10	11.85
0.00	0.00	0.00