
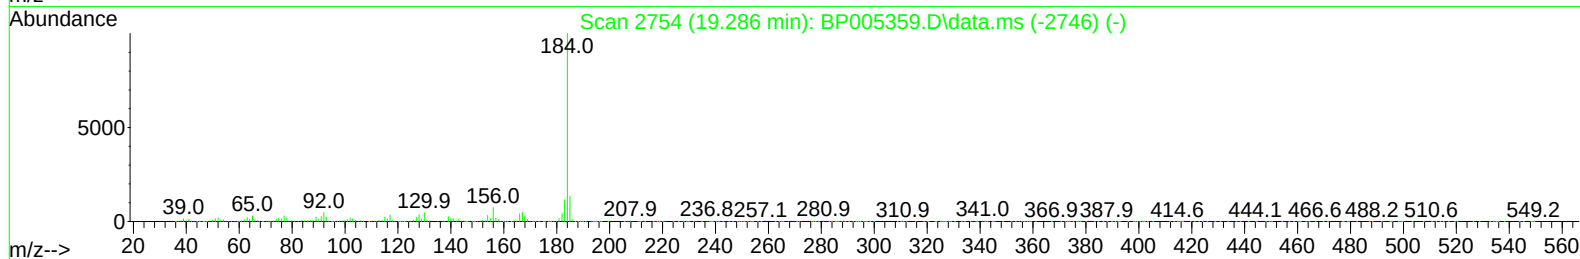
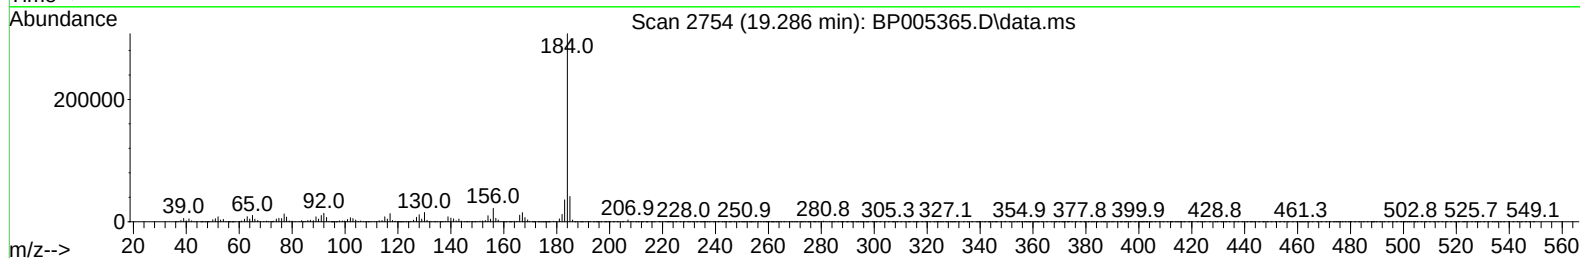


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042221\
 Data File : BP005365.D
 Acq On : 22 Apr 2021 09:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 12:47:39 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 21 17:40:15 2021
 Response via : Initial Calibration

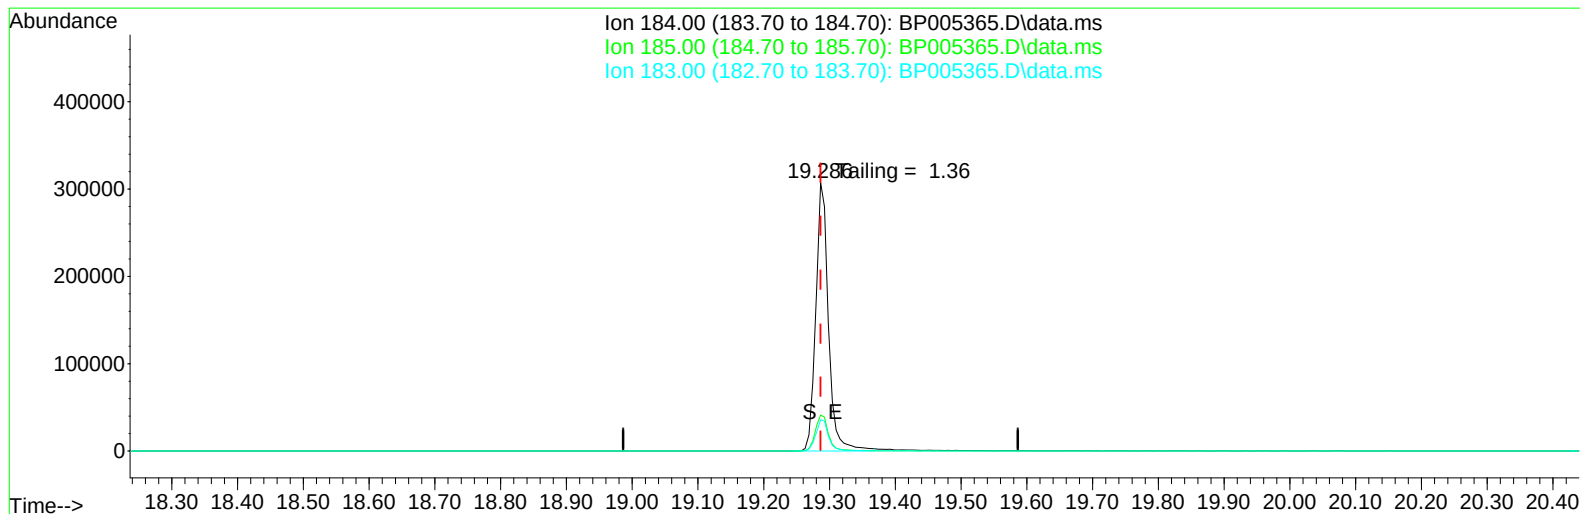




TIC: BP005365.D\data.ms

(77) Benzidine**19.286min (-0.000) 78103.55 ng****response 415890**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.41
183.00	12.30	11.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042221\
 Data File : BP005365.D
 Acq On : 22 Apr 2021 09:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 12:47:39 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 21 17:40:15 2021
 Response via : Initial Calibration

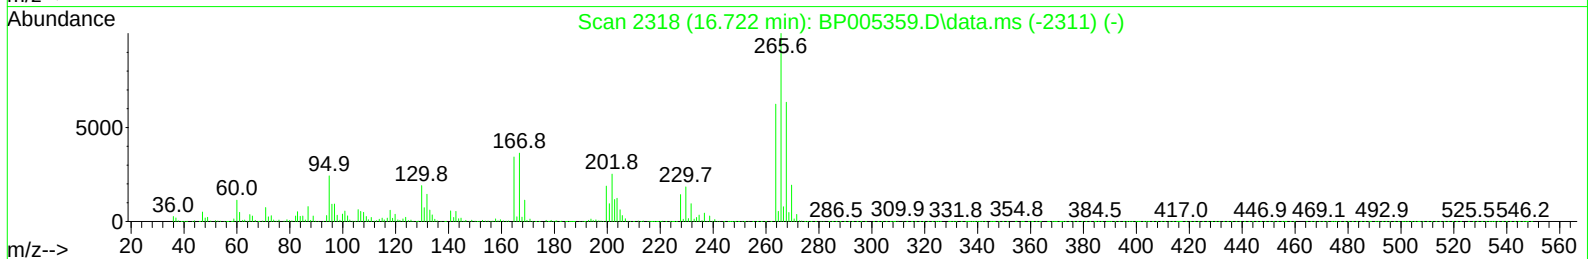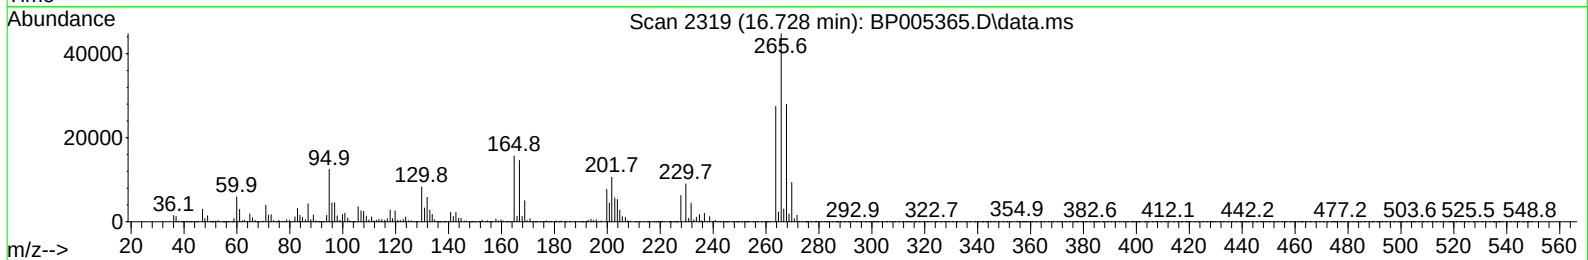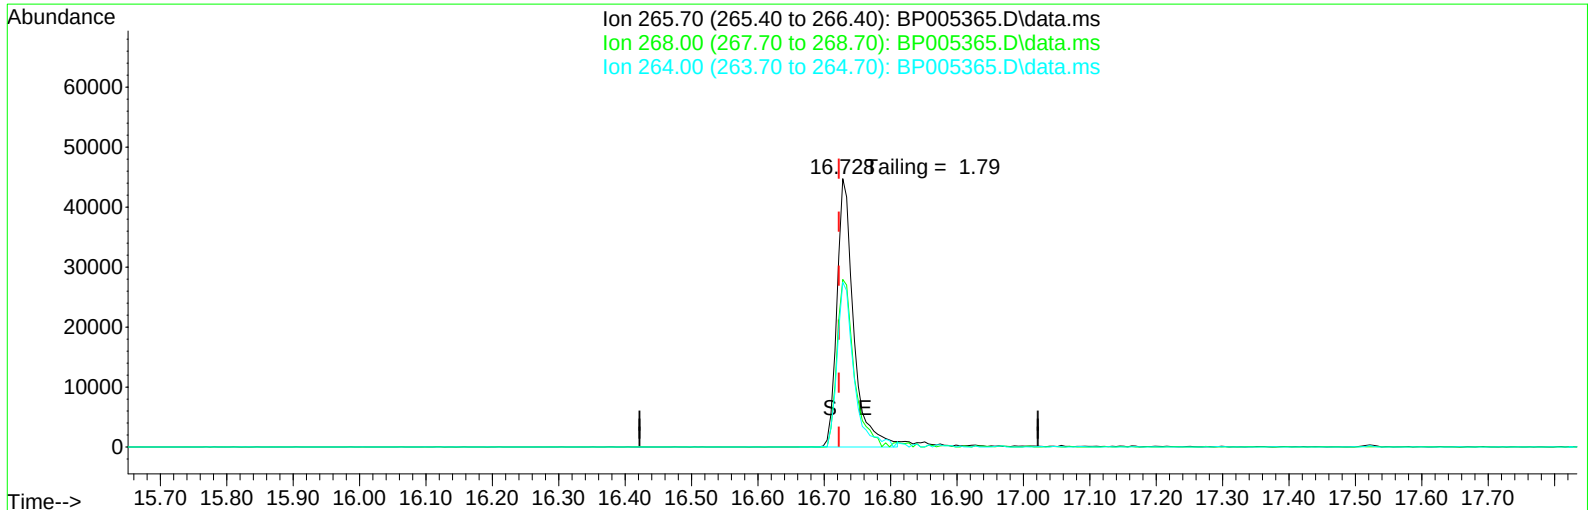

TIC: BP005365.D\data.ms

(70) Pentachlorophenol (C)

16.728min (+ 0.006) 419699.10 ng

response 79552

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	66.60
264.00	67.10	66.49
0.00	0.00	0.00