

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042221\
 Data File : BP005367.D
 Acq On : 22 Apr 2021 10:08
 Operator : CG/JU
 Sample : PB135840BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB135840BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP005367.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.246	361	367	382	rBV	1044490	1454163	40.69%	10.688%
2	6.834	629	637	654	rBV	903098	1428004	39.96%	10.496%
3	7.640	768	774	783	rBV	164397	262801	7.35%	1.932%
4	8.805	965	972	988	rBV	553964	911778	25.52%	6.702%
5	10.428	1242	1248	1265	rBV	160862	299082	8.37%	2.198%
6	12.916	1664	1671	1694	rBV	1394824	1995718	55.85%	14.669%
7	14.304	1900	1907	1921	rBV	254059	382651	10.71%	2.813%
8	15.810	2154	2163	2184	rBV	1118723	1664475	46.58%	12.234%
9	17.069	2370	2377	2391	rBV	303002	470512	13.17%	3.458%
10	19.645	2809	2815	2826	rBV	3089520	3573438	100.00%	26.265%
11	21.169	3069	3074	3088	rBV	414946	607523	17.00%	4.465%
12	23.427	3452	3458	3468	rVB2	283576	555072	15.53%	4.080%




Sum of corrected areas: 13605217

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042221\
Data File : BP005367.D
Acq On : 22 Apr 2021 10:08
Operator : CG/JU
Sample : PB135840BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB135840BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

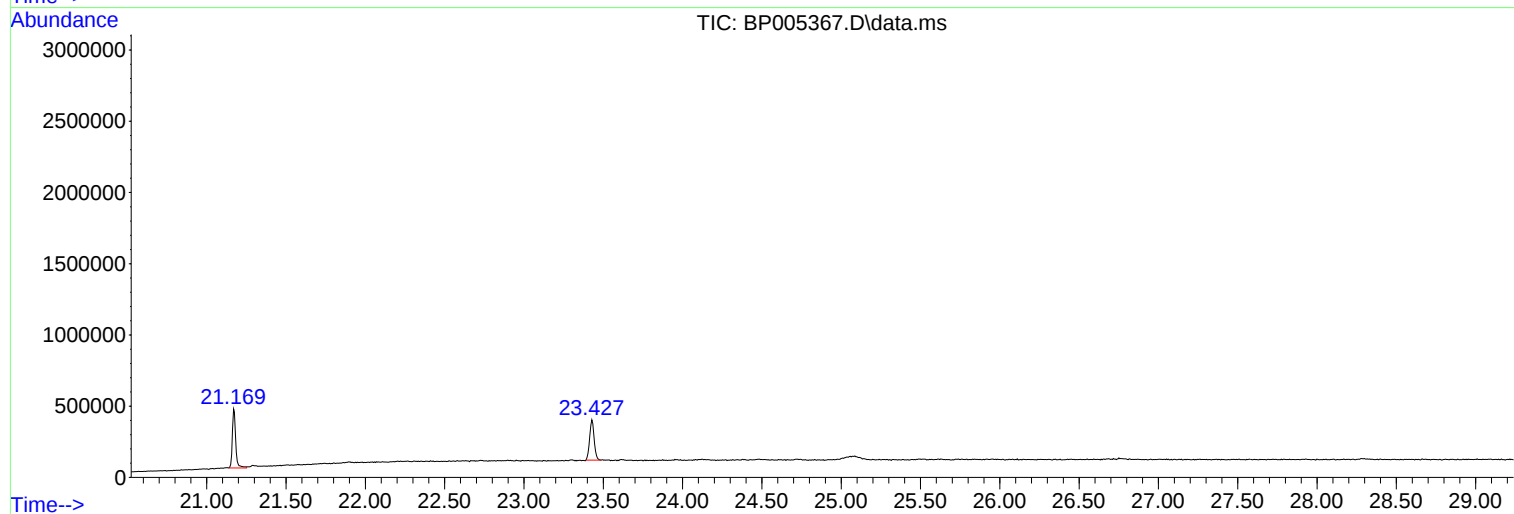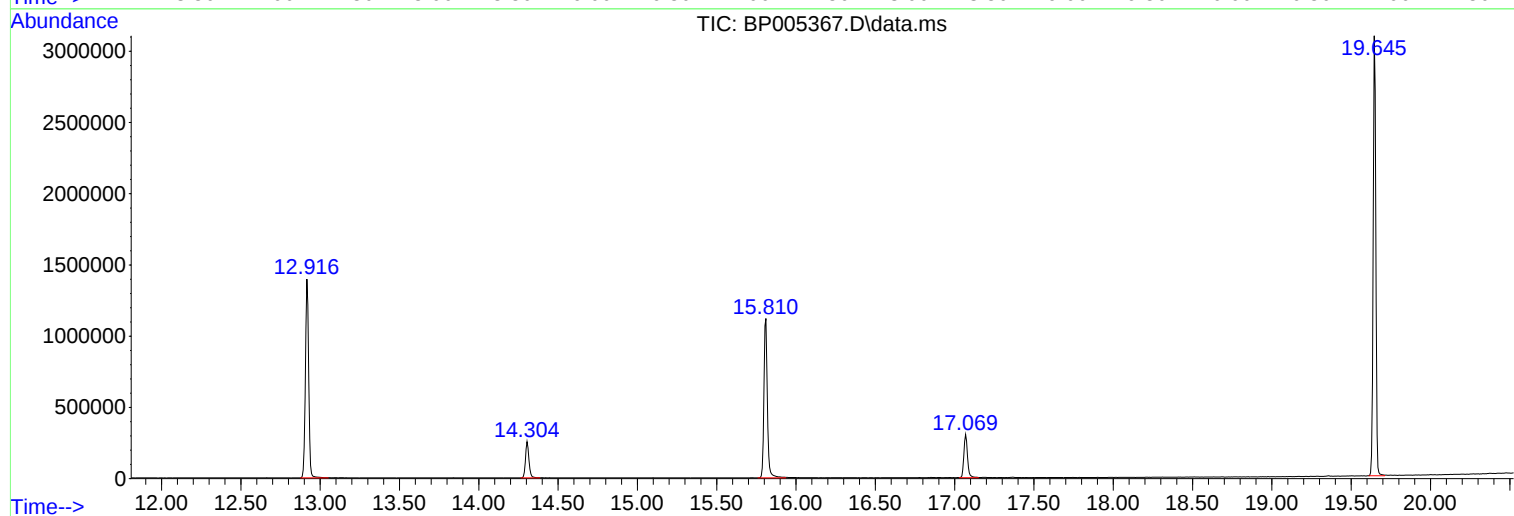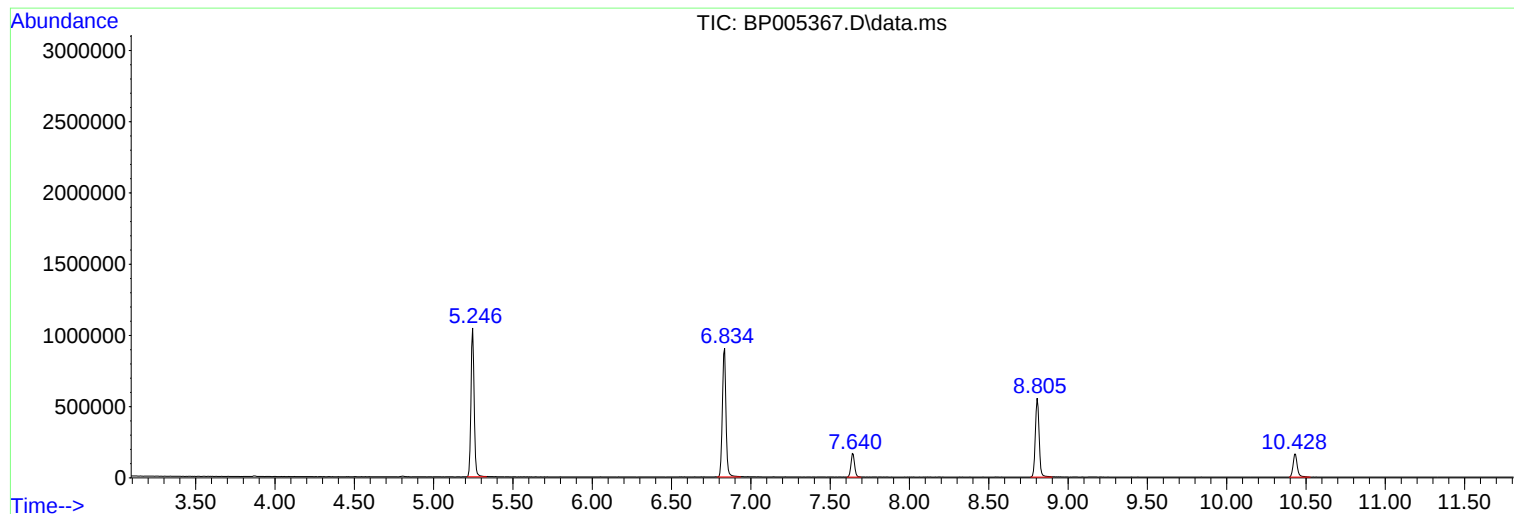

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042221\
Data File : BP005367.D
Acq On : 22 Apr 2021 10:08
Operator : CG/JU
Sample : PB135840BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB135840BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042221\
Data File : BP005367.D
Acq On : 22 Apr 2021 10:08
Operator : CG/JU
Sample : PB135840BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB135840BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------