

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042221\
 Data File : BP005375.D
 Acq On : 22 Apr 2021 14:51
 Operator : CG/JU
 Sample : M2103-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 RO-124030

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP005375.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.246	361	367	384	rBV	766532	1085374	51.25%	9.362%
2	6.834	630	637	650	rBV	715224	1134375	53.57%	9.784%
3	7.640	767	774	782	rBV	147904	237040	11.19%	2.045%
4	8.804	965	972	990	rBV	435830	716961	33.86%	6.184%
5	10.428	1240	1248	1255	rBV	173099	291941	13.79%	2.518%
6	12.916	1664	1671	1687	rBV	910372	1255382	59.28%	10.828%
7	13.769	1809	1816	1824	rBV	43727	66683	3.15%	0.575%
8	14.304	1900	1907	1913	rVV	264035	387315	18.29%	3.341%
9	14.369	1913	1918	1922	rVB2	15977	25059	1.18%	0.216%
10	15.810	2156	2163	2172	rBV	979196	1393769	65.82%	12.022%
11	17.068	2370	2377	2381	rBV	360511	499333	23.58%	4.307%
12	17.110	2381	2384	2391	rVV	39661	59704	2.82%	0.515%
13	17.204	2395	2400	2405	rVB	17460	29166	1.38%	0.252%
14	17.968	2526	2530	2539	rBV2	96273	142126	6.71%	1.226%
15	18.133	2553	2558	2568	rVB3	19095	40100	1.89%	0.346%
16	18.662	2644	2648	2653	rBV3	32893	43864	2.07%	0.378%
17	19.092	2714	2721	2727	rBV	137939	184126	8.69%	1.588%
18	19.145	2727	2730	2736	rVV3	26690	33810	1.60%	0.292%
19	19.210	2737	2741	2751	rVB3	39849	70904	3.35%	0.612%
20	19.421	2773	2777	2778	rBV2	21989	28154	1.33%	0.243%
21	19.445	2778	2781	2789	rVB	95874	133930	6.32%	1.155%
22	19.645	2810	2815	2821	rBV	1767355	2117619	100.00%	18.265%
23	20.886	3022	3026	3034	rVB2	145304	201040	9.49%	1.734%
24	21.080	3057	3059	3064	rVB2	38383	37701	1.78%	0.325%
25	21.168	3069	3074	3079	rBV	533995	720092	34.00%	6.211%
26	23.427	3453	3458	3472	rVB	346156	658400	31.09%	5.679%




Sum of corrected areas: 11593968

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042221\
Data File : BP005375.D
Acq On : 22 Apr 2021 14:51
Operator : CG/JU
Sample : M2103-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
RO-124030

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

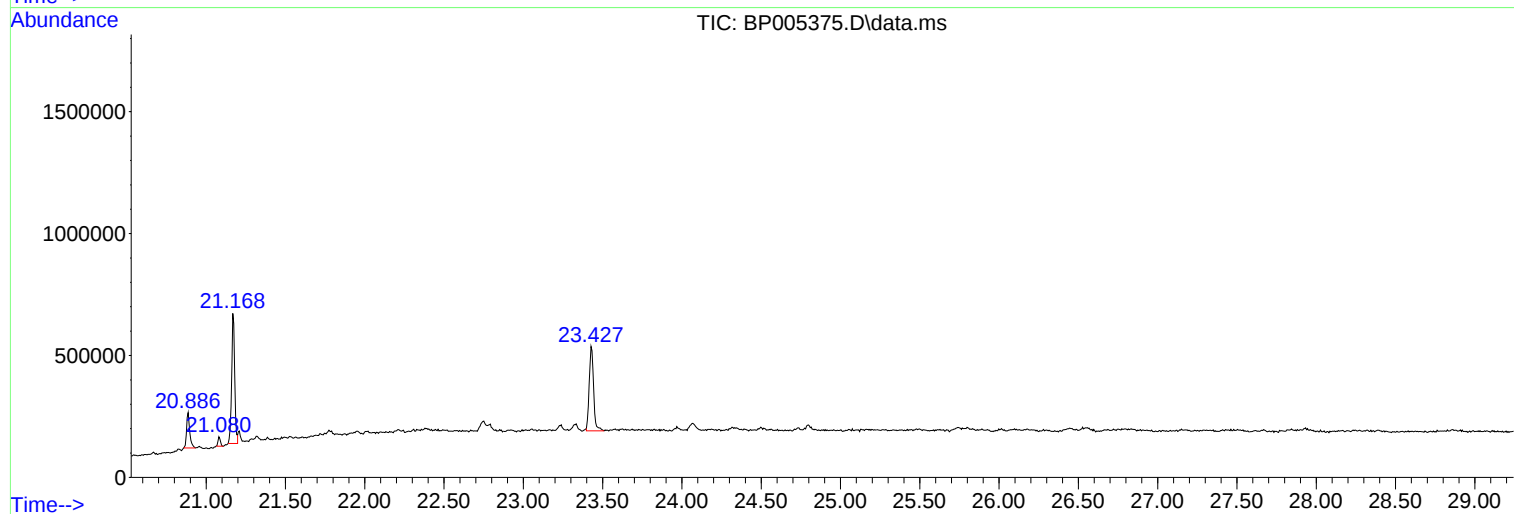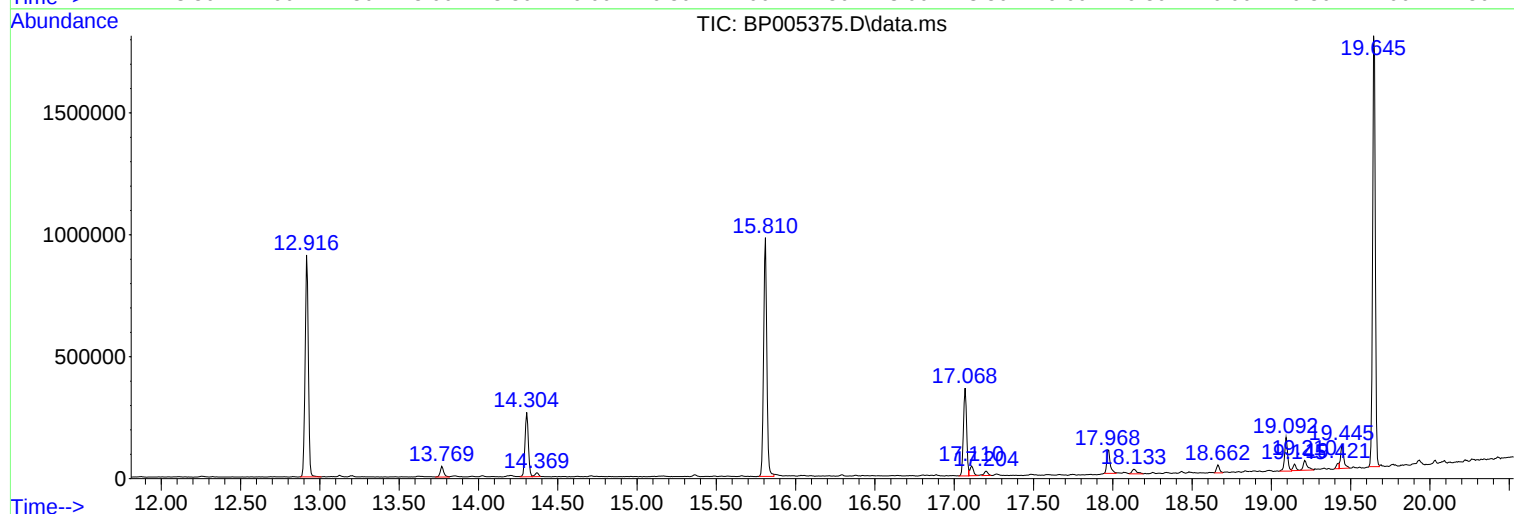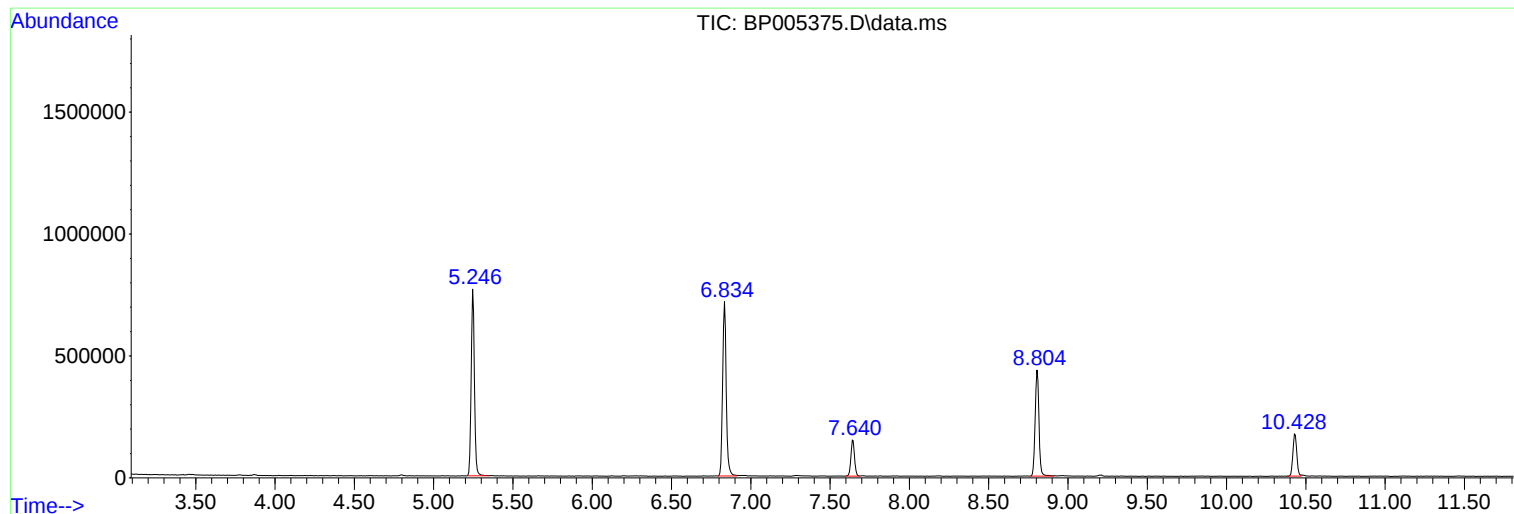

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042221\
Data File : BP005375.D
Acq On : 22 Apr 2021 14:51
Operator : CG/JU
Sample : M2103-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
RO-124030

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042221\
Data File : BP005375.D
Acq On : 22 Apr 2021 14:51
Operator : CG/JU
Sample : M2103-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
RO-124030

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------