

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042221\
 Data File : BP005379.D
 Acq On : 22 Apr 2021 17:06
 Operator : CG/JU
 Sample : M2102-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 RO-124037

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042121.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP005379.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.446	54	61	74	rBV	689134	1083903	54.09%	9.616%
2	5.246	361	367	383	rBV	624041	916809	45.75%	8.134%
3	6.834	629	637	655	rBV	617674	999109	49.86%	8.864%
4	7.640	767	774	783	rBV	156798	251528	12.55%	2.232%
5	8.804	964	972	984	rBV	366307	611800	30.53%	5.428%
6	10.428	1241	1248	1257	rBV	180070	308594	15.40%	2.738%
7	12.916	1663	1671	1682	rBV	847877	1212339	60.50%	10.756%
8	13.769	1811	1816	1824	rVB	20910	32790	1.64%	0.291%
9	14.304	1901	1907	1914	rBV	266973	396838	19.80%	3.521%
10	15.810	2154	2163	2176	rBV	755270	1106066	55.19%	9.813%
11	17.069	2370	2377	2382	rBV	353978	495417	24.72%	4.395%
12	17.110	2382	2384	2389	rVV	20543	26153	1.31%	0.232%
13	17.198	2391	2399	2406	rVB2	10035	20771	1.04%	0.184%
14	17.968	2523	2530	2540	rBV2	74667	117947	5.89%	1.046%
15	19.092	2715	2721	2727	rBV	58569	84755	4.23%	0.752%
16	19.210	2737	2741	2750	rBV4	32443	58406	2.91%	0.518%
17	19.445	2774	2781	2790	rBV	47018	90860	4.53%	0.806%
18	19.645	2810	2815	2820	rBV	1751910	2003949	100.00%	17.779%
19	20.886	3022	3026	3034	rVB2	99964	139352	6.95%	1.236%
20	21.168	3069	3074	3079	rBV	505163	674970	33.68%	5.988%
21	23.427	3452	3458	3474	rVB	325004	639258	31.90%	5.671%




Sum of corrected areas: 11271614

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042221\
Data File : BP005379.D
Acq On : 22 Apr 2021 17:06
Operator : CG/JU
Sample : M2102-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
RO-124037

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

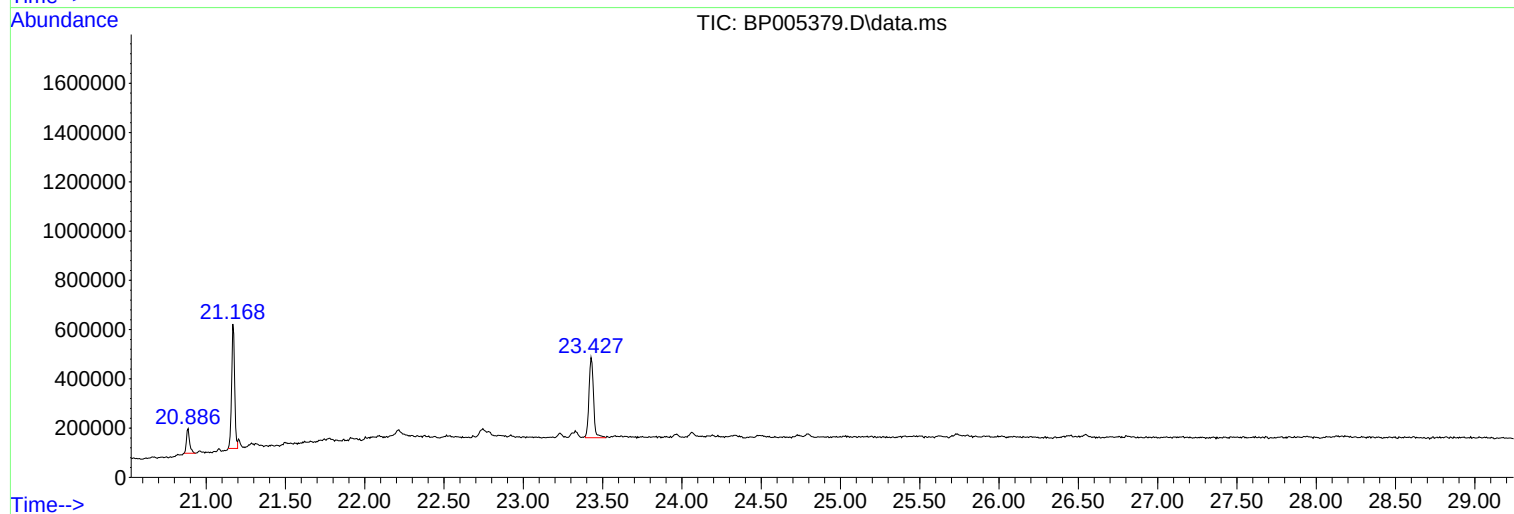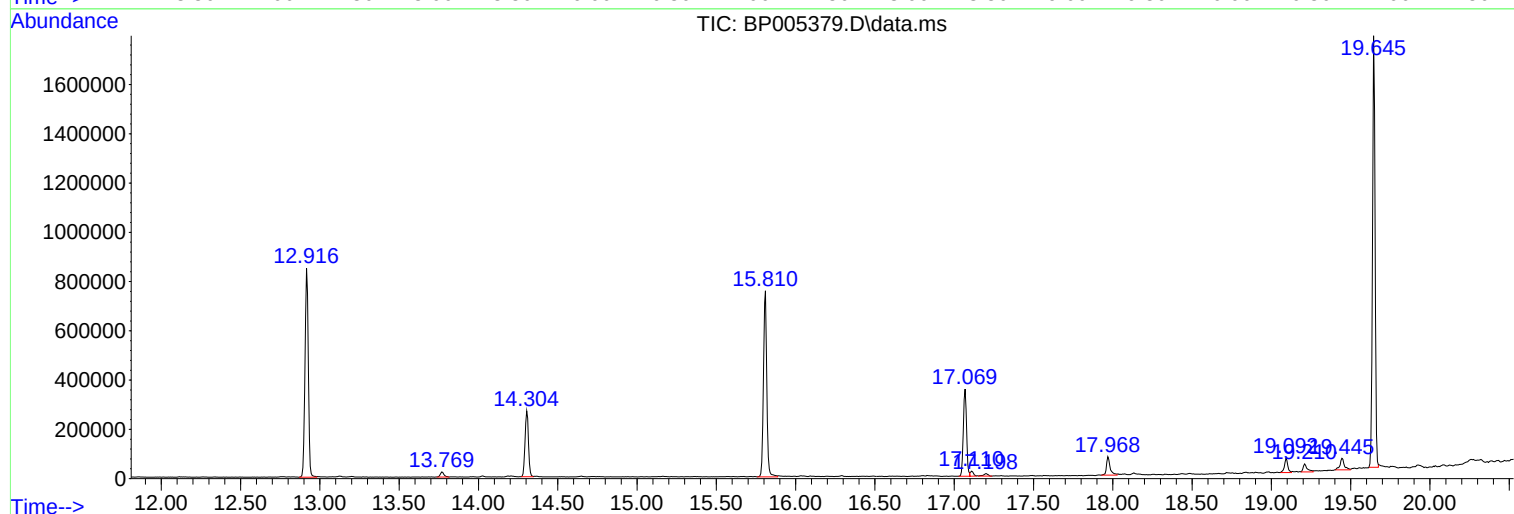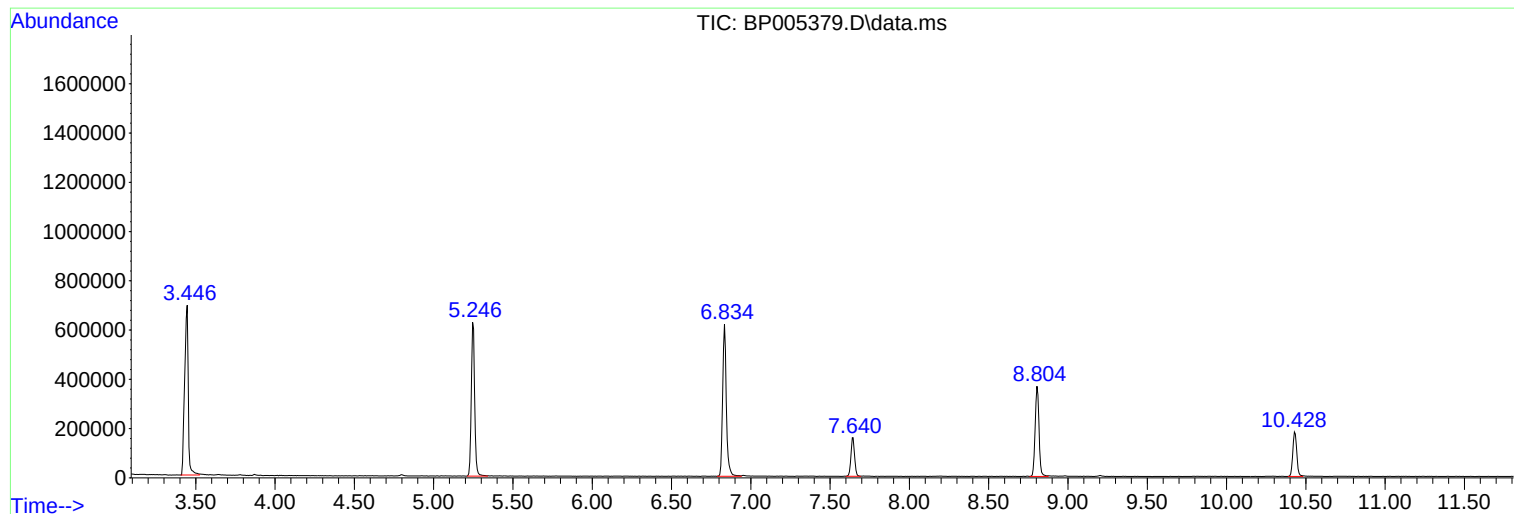

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042221\
Data File : BP005379.D
Acq On : 22 Apr 2021 17:06
Operator : CG/JU
Sample : M2102-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
RO-124037

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042221\
Data File : BP005379.D
Acq On : 22 Apr 2021 17:06
Operator : CG/JU
Sample : M2102-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
RO-124037

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------