
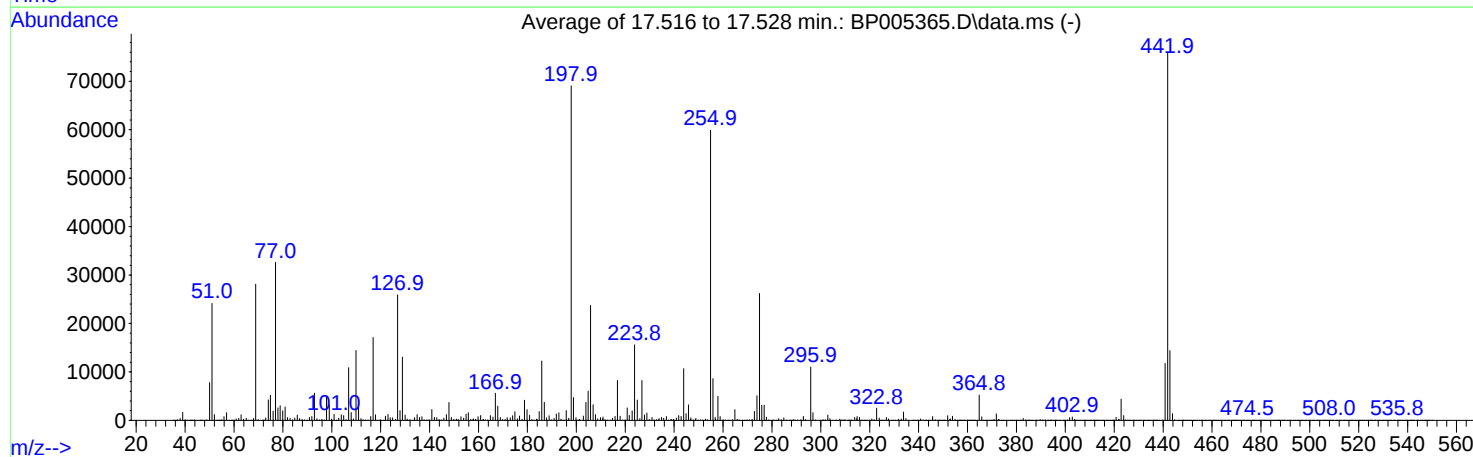


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042221\
 Data File : BP005365.D
 Acq On : 22 Apr 2021 09:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 21 17:40:15 2021

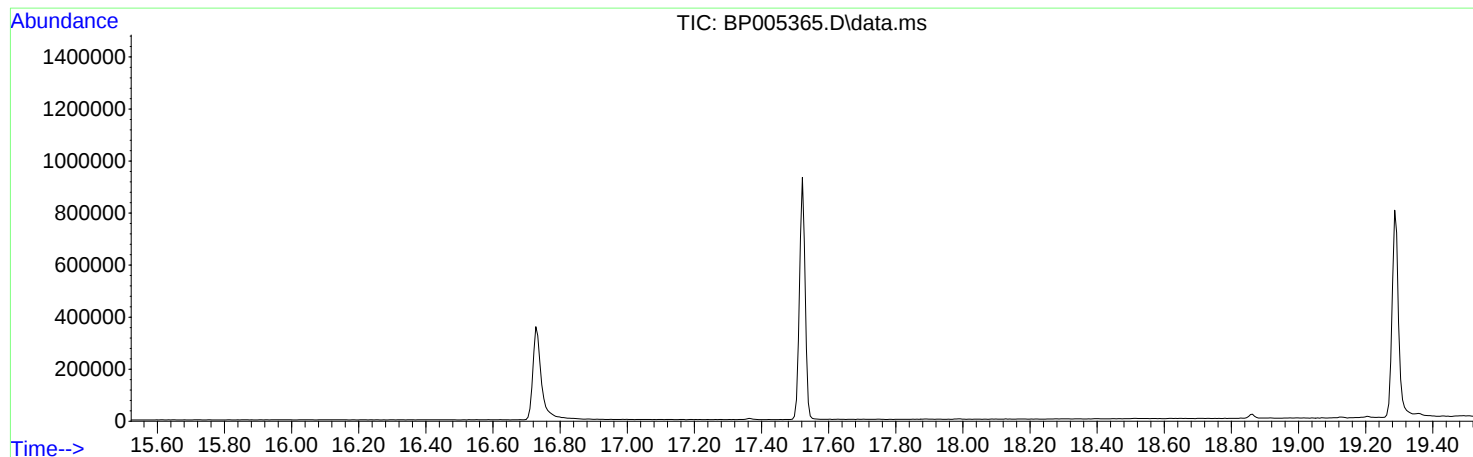




AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	24157	PASS
68	69	0.00	2	1.5	415	PASS
69	198	0.00	100	40.7	28108	PASS
70	69	0.00	2	0.6	163	PASS
127	198	10	80	37.5	25896	PASS
197	198	0.00	2	0.6	446	PASS
198	198	100	100	100.0	69044	PASS
199	198	5	9	6.9	4732	PASS
275	198	10	60	37.9	26179	PASS
365	198	1	100	7.5	5204	PASS
441	198	0.01	100	17.0	11768	PASS
442	442	100	100	100.0	75931	PASS
443	442	15	24	19.0	14407	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042221\
Data File : BP005365.D
Acq On : 22 Apr 2021 09:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 22 12:47:39 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 21 17:40:15 2021
Response via : Initial Calibration

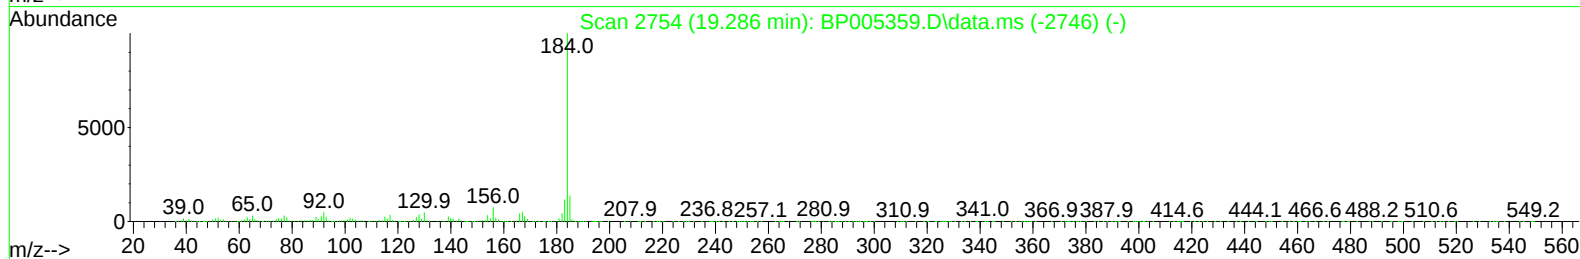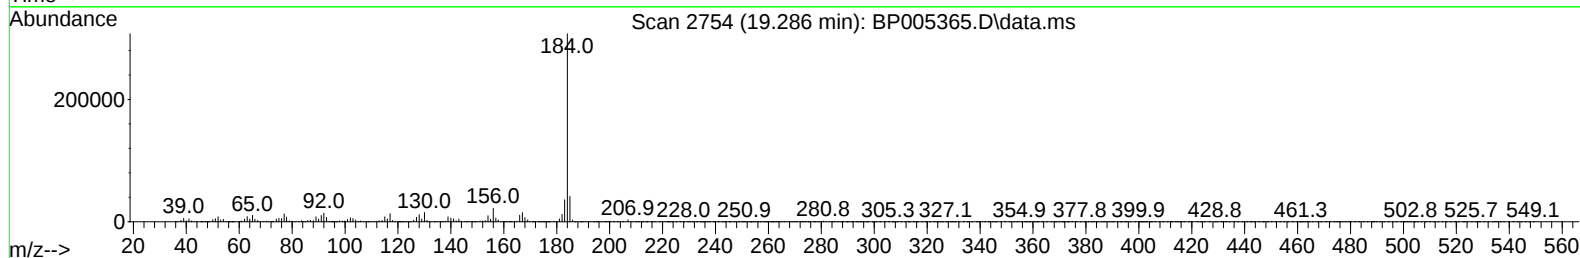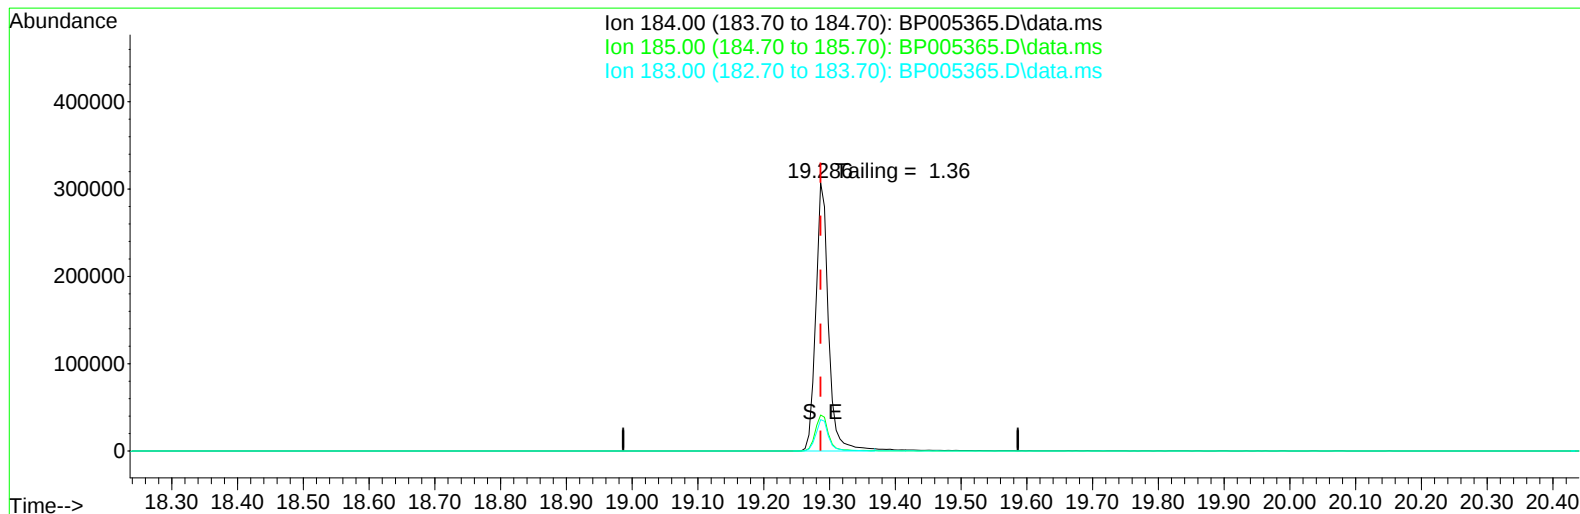

TIC: BP005365.D\data.ms

(77) Benzidine

19.286min (-0.000) 78103.55 ng




response 415890

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.41
183.00	12.30	11.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042221\
 Data File : BP005365.D
 Acq On : 22 Apr 2021 09:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Apr 22 12:47:39 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 21 17:40:15 2021
 Response via : Initial Calibration

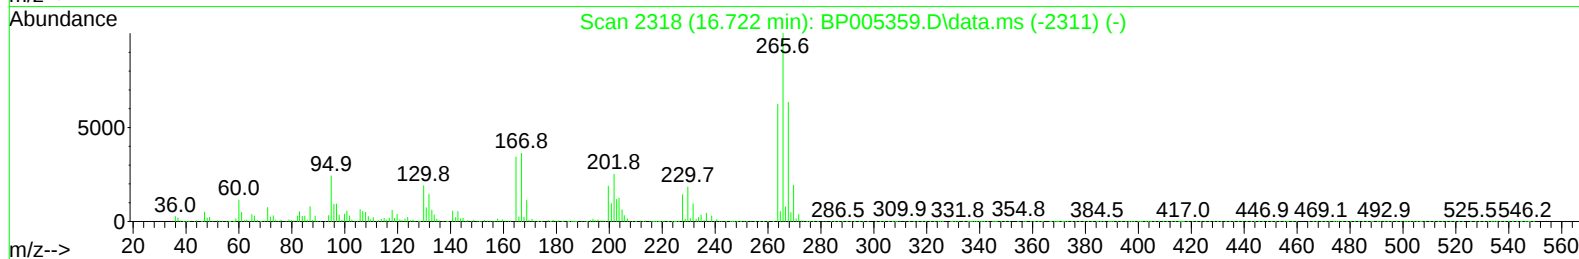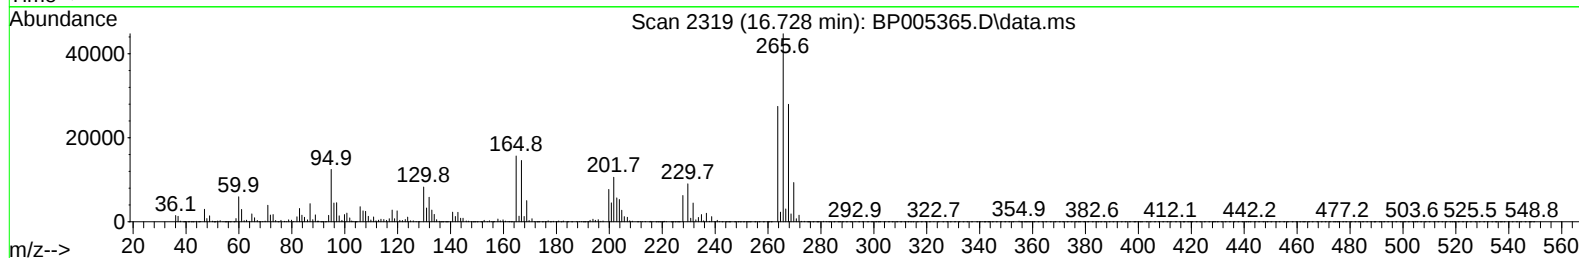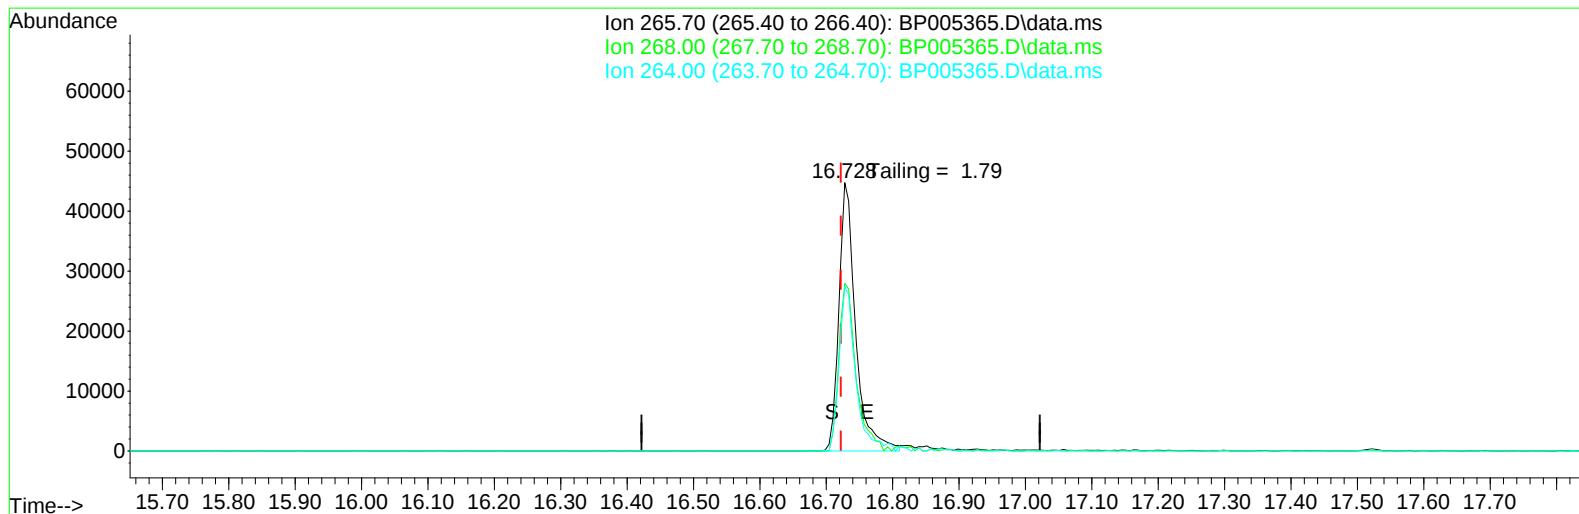

TIC: BP005365.D\data.ms

(70) Pentachlorophenol (C)

16.728min (+ 0.006) 419699.10 ng

response 79552

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	66.60
264.00	67.10	66.49
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
22/4/2021	BNA_P	BP005365.D
Compound Name	Response	Retention Time
DDT	290231	20.48
DDD	1307	20.06
DDE	668	19.56
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1975	292206	0.68